

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102620\
 Data File : PP030851.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Oct 2020 11:00
 Operator : DD\AJ
 Sample : MDL-PCB-BL-S-3
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-S-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:46:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1232PP102520.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 26 04:46:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.804	4.082	1136584	1027543	16.955	16.525
2)	SA Decachlor...	10.686	9.417	660103	676252	17.973	17.092

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102620\
Data File : PP030851.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Oct 2020 11:00
Operator : DD\AJ
Sample : MDL-PCB-BL-S-3
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:46:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1232PP102520.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 26 04:46:19 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

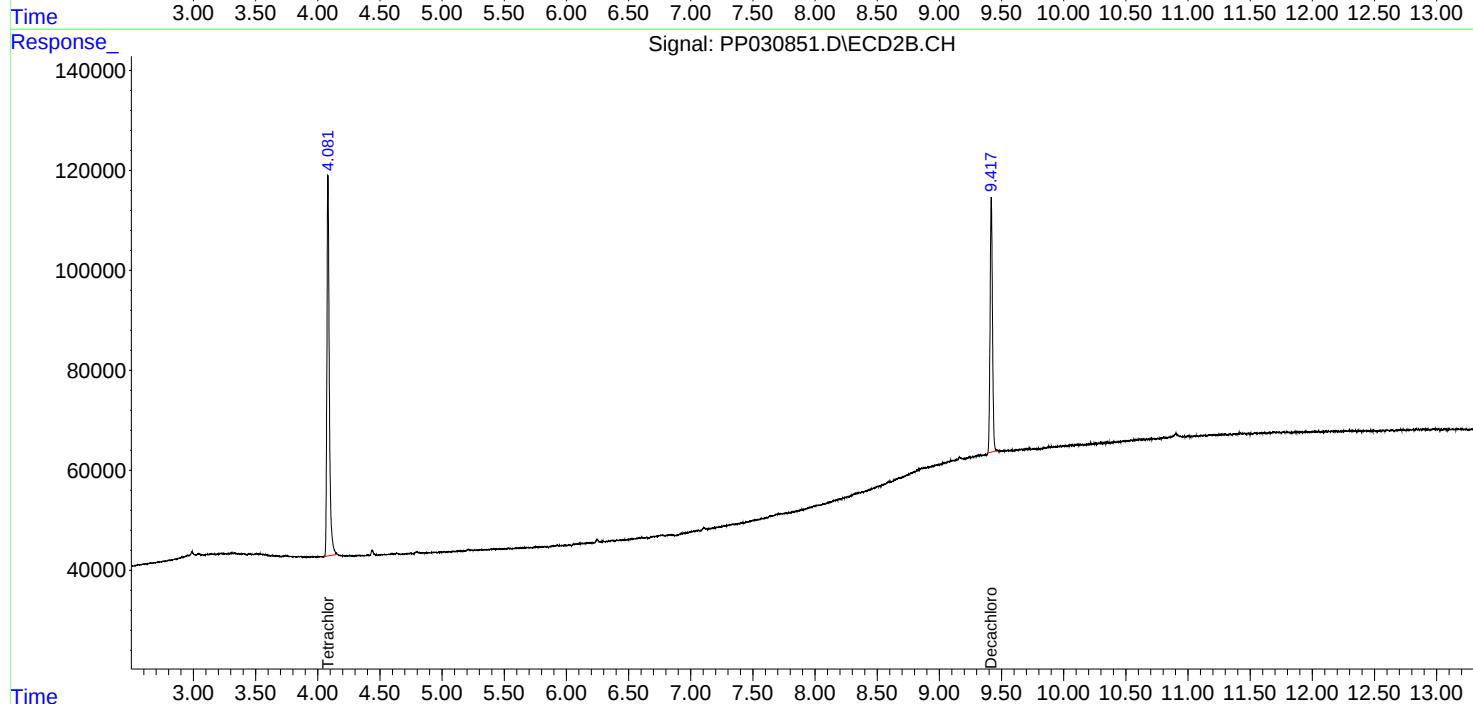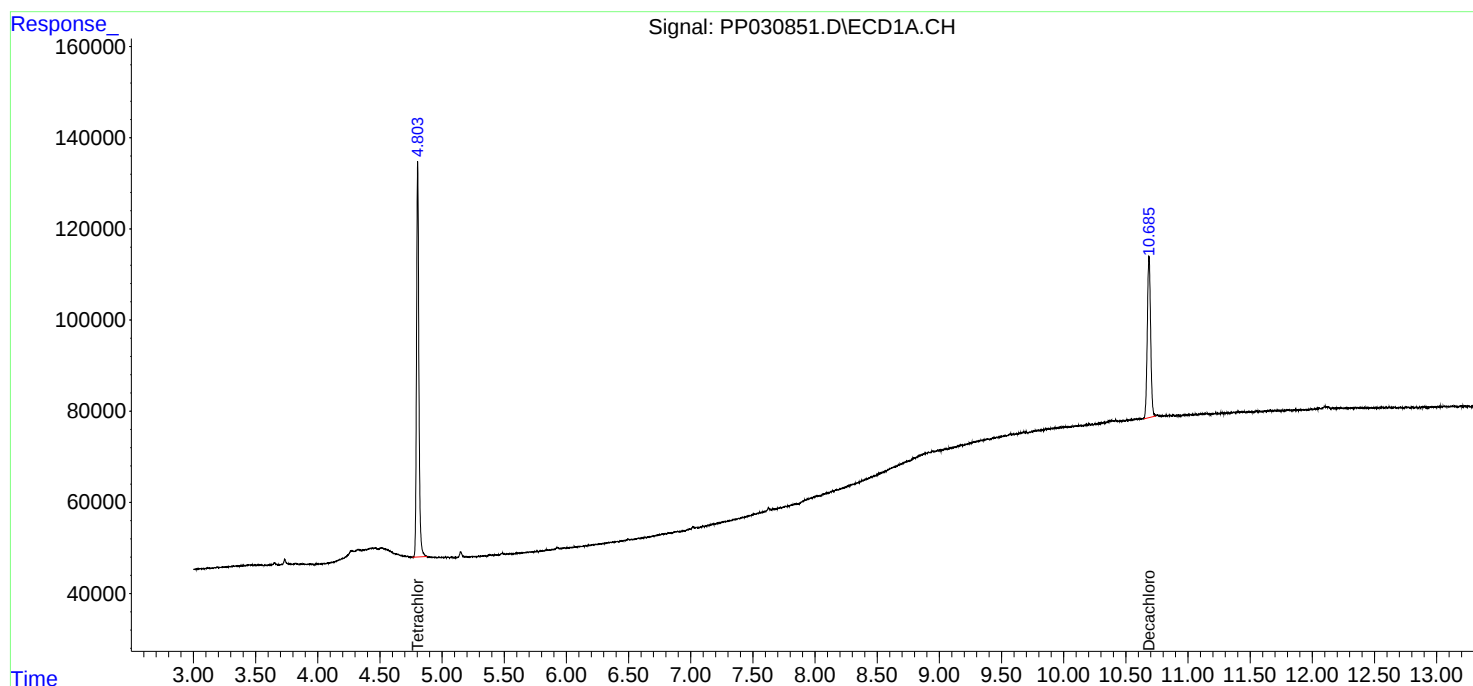


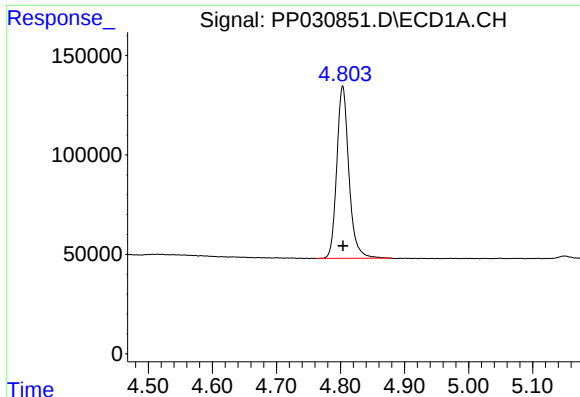

#1 Tetrachloro-m-xylene


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 1136584
Conc: 16.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-3

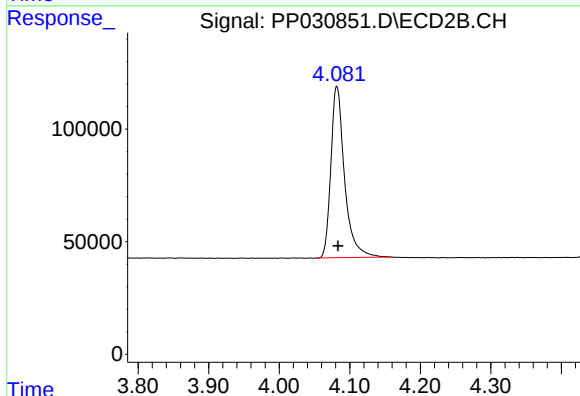


#1 Tetrachloro-m-xylene

R.T.: 4.082 min
Delta R.T.: -0.002 min
Response: 1027543
Conc: 16.53 ng/ml

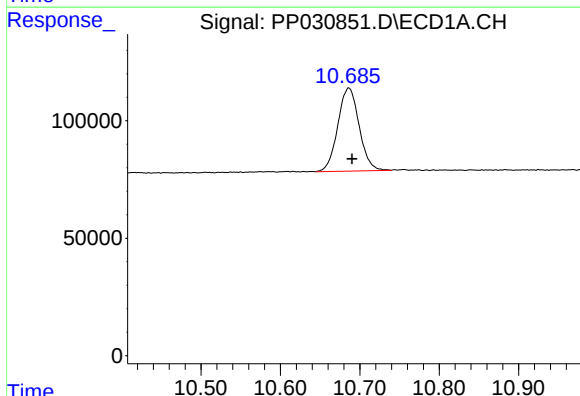

#2 Decachlorobiphenyl

R.T.: 10.686 min
Delta R.T.: -0.004 min
Response: 660103
Conc: 17.97 ng/ml

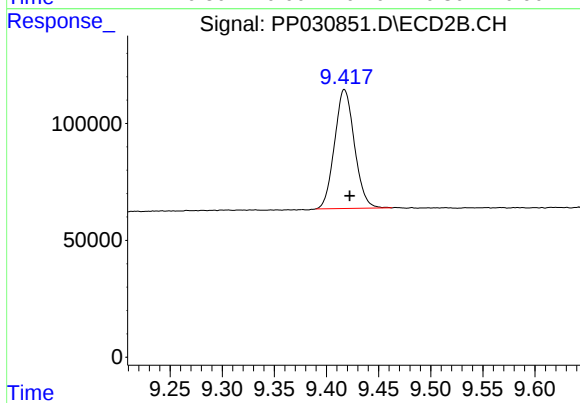

#2 Decachlorobiphenyl

R.T.: 9.417 min
Delta R.T.: -0.005 min
Response: 676252
Conc: 17.09 ng/ml