

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102621\
 Data File : PP040424.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2021 10:38
 Operator : AJ\MA
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 10/27/2021
 Supervised By :mohammad ahmed 10/28/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 11:54:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 27 11:53:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.751	3.773	216803	132084	5.063	4.583
2)	SA Decachlor...	10.688	9.066	175916	157676	5.654	5.641
Target Compounds							
21)	L5 AR-1248-1	6.075	5.026	39223	28496	51.814	53.641
22)	L5 AR-1248-2	6.368	5.291	56520	47702	54.552	61.156
23)	L5 AR-1248-3	6.584	5.337	75928	31589	59.853	41.726 #
24)	L5 AR-1248-4	7.016	5.517	92764	37386	63.167	46.044m#
25)	L5 AR-1248-5	7.055	5.942	86224	65794	60.087	68.345

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102621\
Data File : PP040424.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2021 10:38
Operator : AJ\MA
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/27/2021
Supervised By :mohammad ahmed 10/28/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 11:54:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 27 11:53:31 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

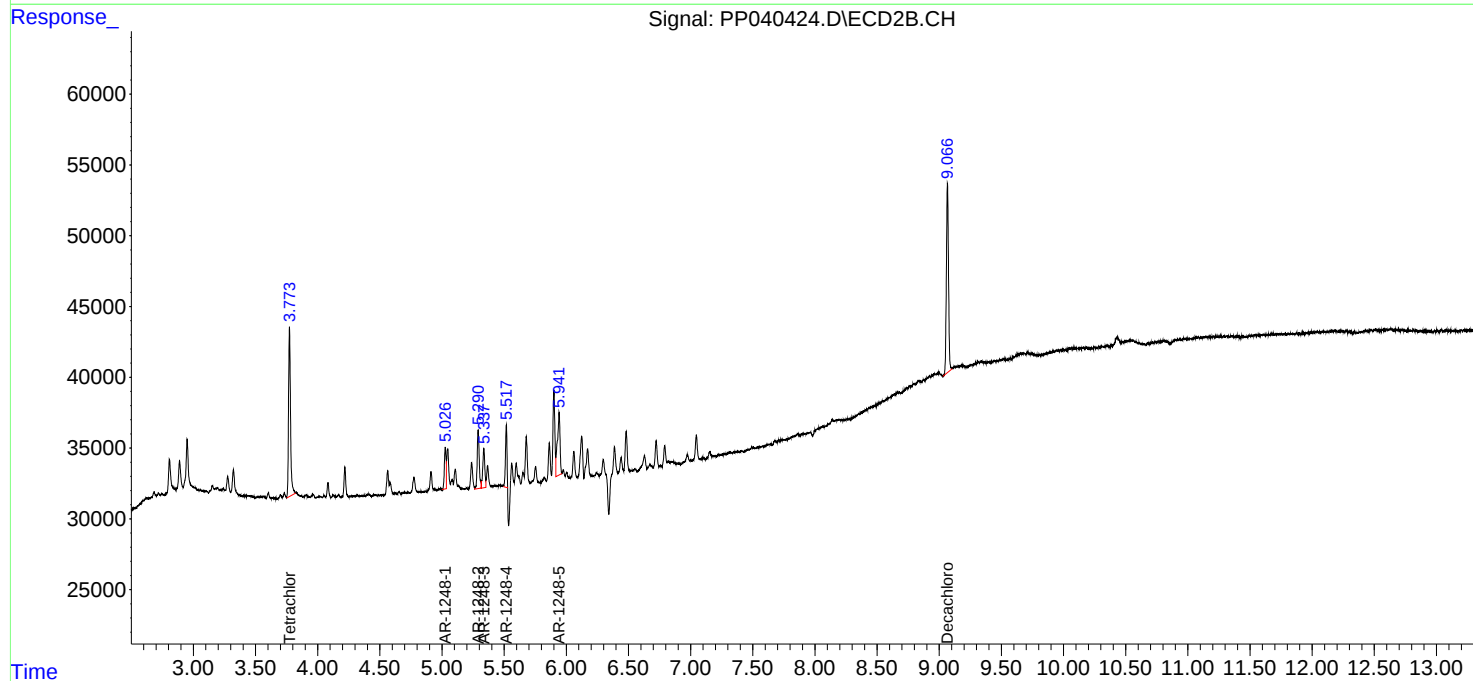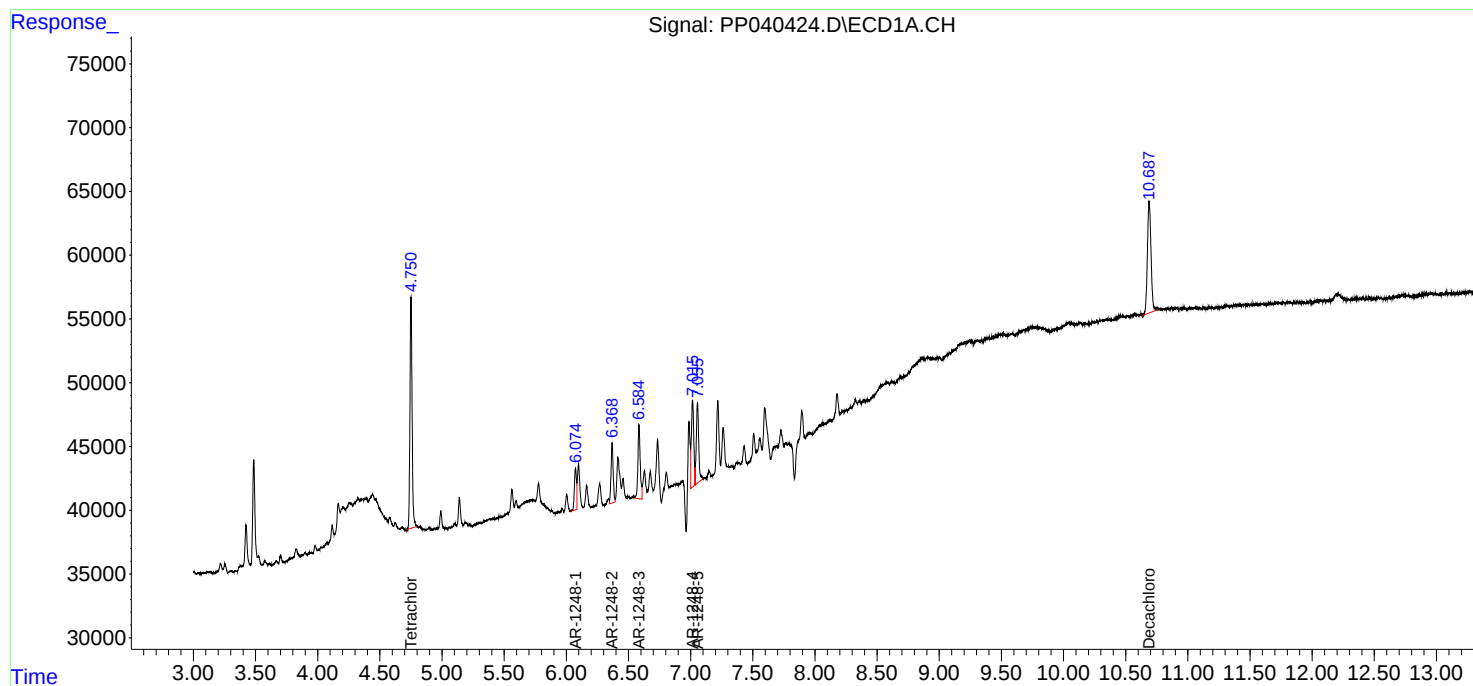

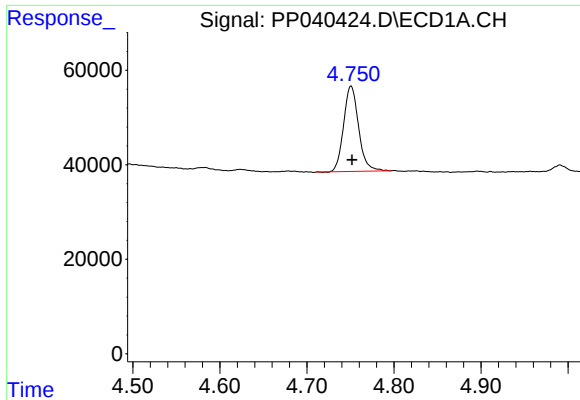


#1 Tetrachloro-m-xylene

R.T.: 4.751 min
Delta R.T.: -0.001 min
Response: 216803
Conc: 5.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/27/2021
Supervised By :mohammad ahmed 10/28/2021

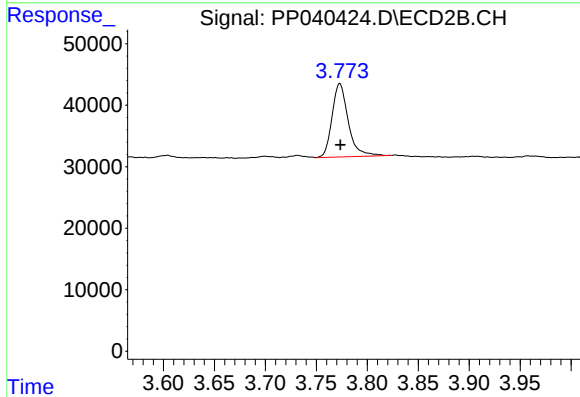


#1 Tetrachloro-m-xylene

R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 132084
Conc: 4.58 ng/ml

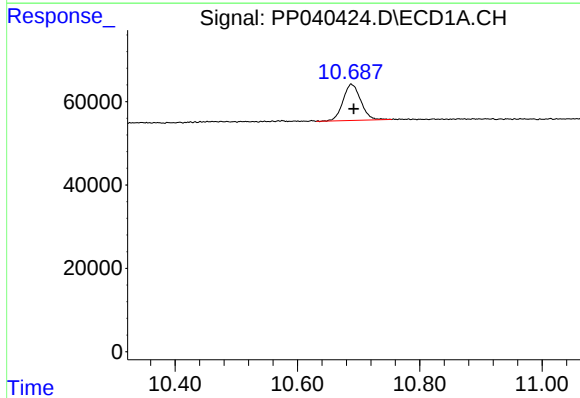


#2 Decachlorobiphenyl

R.T.: 10.688 min
Delta R.T.: -0.004 min
Response: 175916
Conc: 5.65 ng/ml

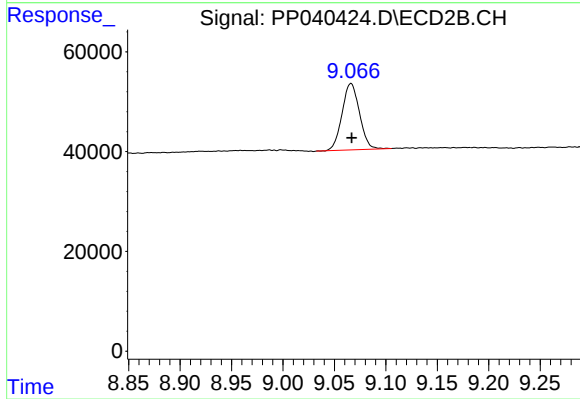

#2 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.000 min
Response: 157676
Conc: 5.64 ng/ml

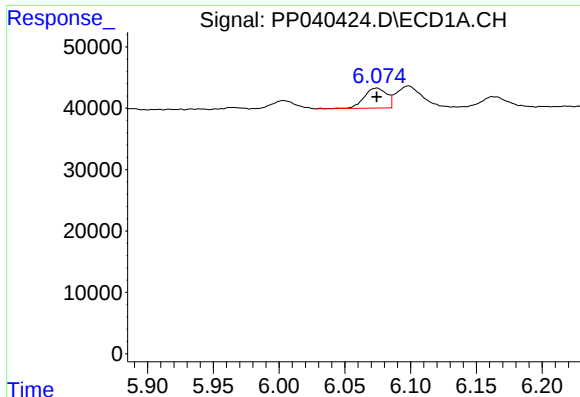


#21 AR-1248-1

R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 39223
Conc: 51.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/27/2021
Supervised By :mohammad ahmed 10/28/2021

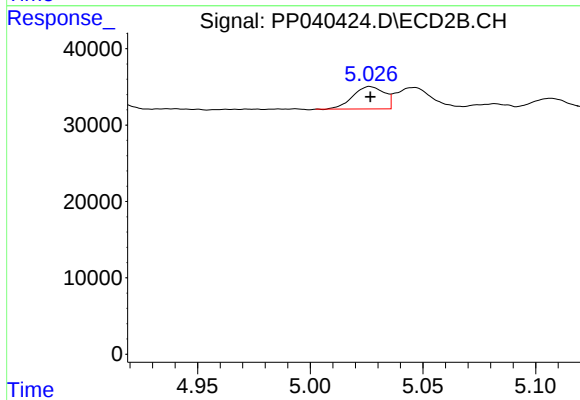


#21 AR-1248-1

R.T.: 5.026 min
Delta R.T.: 0.000 min
Response: 28496
Conc: 53.64 ng/ml

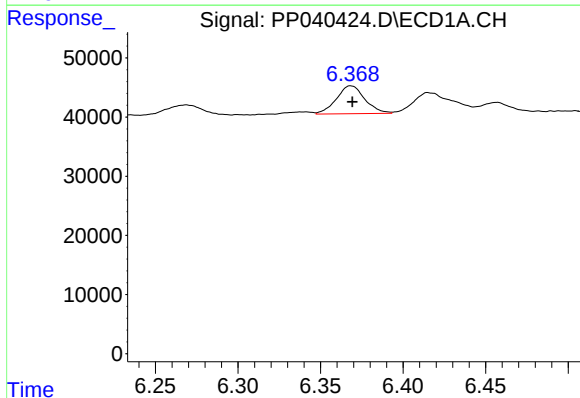


#22 AR-1248-2

R.T.: 6.368 min
Delta R.T.: 0.000 min
Response: 56520
Conc: 54.55 ng/ml

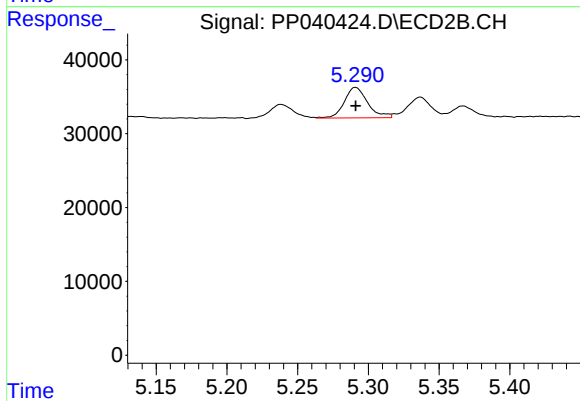

#22 AR-1248-2

R.T.: 5.291 min
Delta R.T.: 0.000 min
Response: 47702
Conc: 61.16 ng/ml

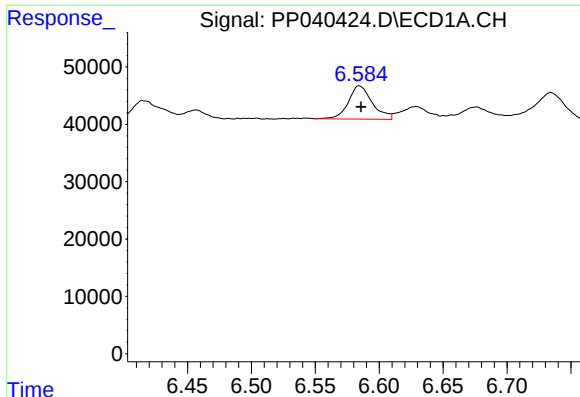


#23 AR-1248-3

R.T.: 6.584 min
Delta R.T.: -0.002 min
Response: 75928
Conc: 59.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/27/2021
Supervised By :mohammad ahmed 10/28/2021

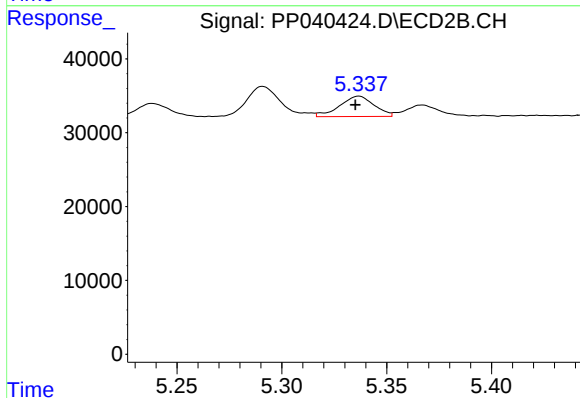


#23 AR-1248-3

R.T.: 5.337 min
Delta R.T.: 0.002 min
Response: 31589
Conc: 41.73 ng/ml

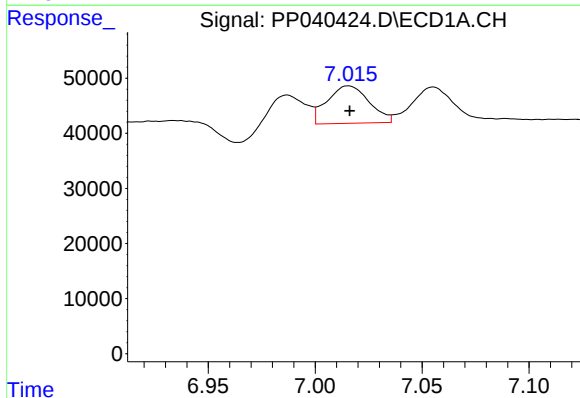


#24 AR-1248-4

R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 92764
Conc: 63.17 ng/ml

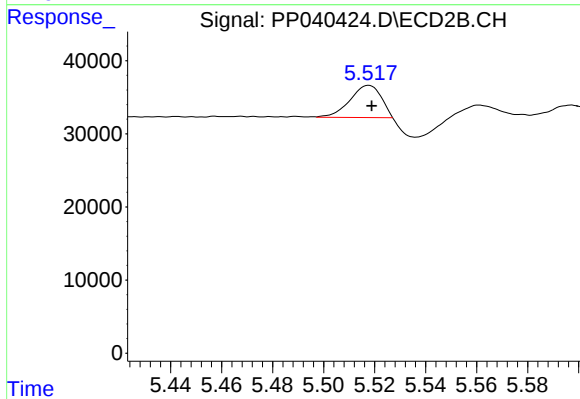

#24 AR-1248-4

R.T.: 5.517 min
Delta R.T.: -0.002 min
Response: 37386
Conc: 46.04 ng/ml m

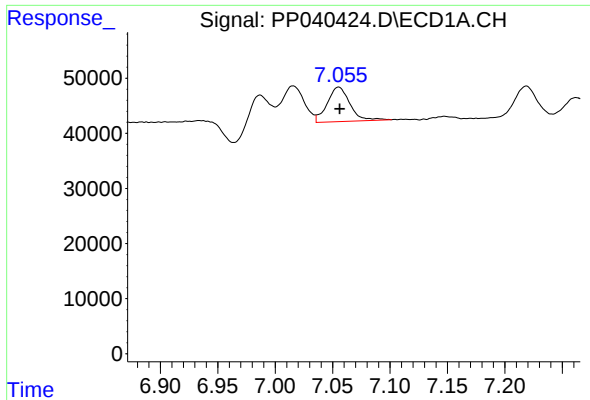


#25 AR-1248-5

R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 86224
Conc: 60.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/27/2021
Supervised By :mohammad ahmed 10/28/2021

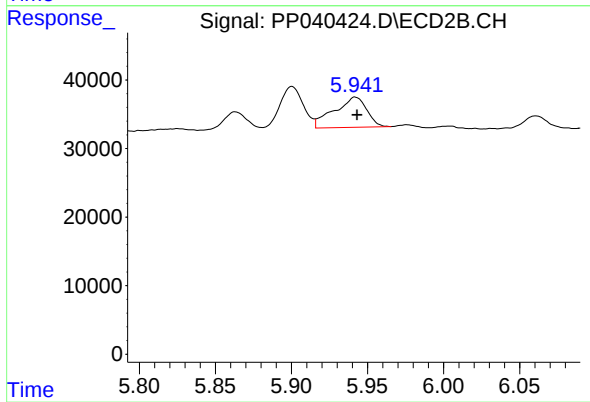

#25 AR-1248-5

R.T.: 5.942 min
Delta R.T.: -0.001 min
Response: 65794
Conc: 68.35 ng/ml