

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102721\
 Data File : PP040466.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2021 22:43
 Operator : AJ\MA
 Sample : PB140286BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB140286BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:03:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 27 13:26:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.750	3.772	905694	515441	22.236	18.920
2)	SA Decachlor...	10.688	9.062	639013	550346	21.092	19.616

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102721\
Data File : PP040466.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2021 22:43
Operator : AJ\MA
Sample : PB140286BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB140286BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:03:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 27 13:26:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

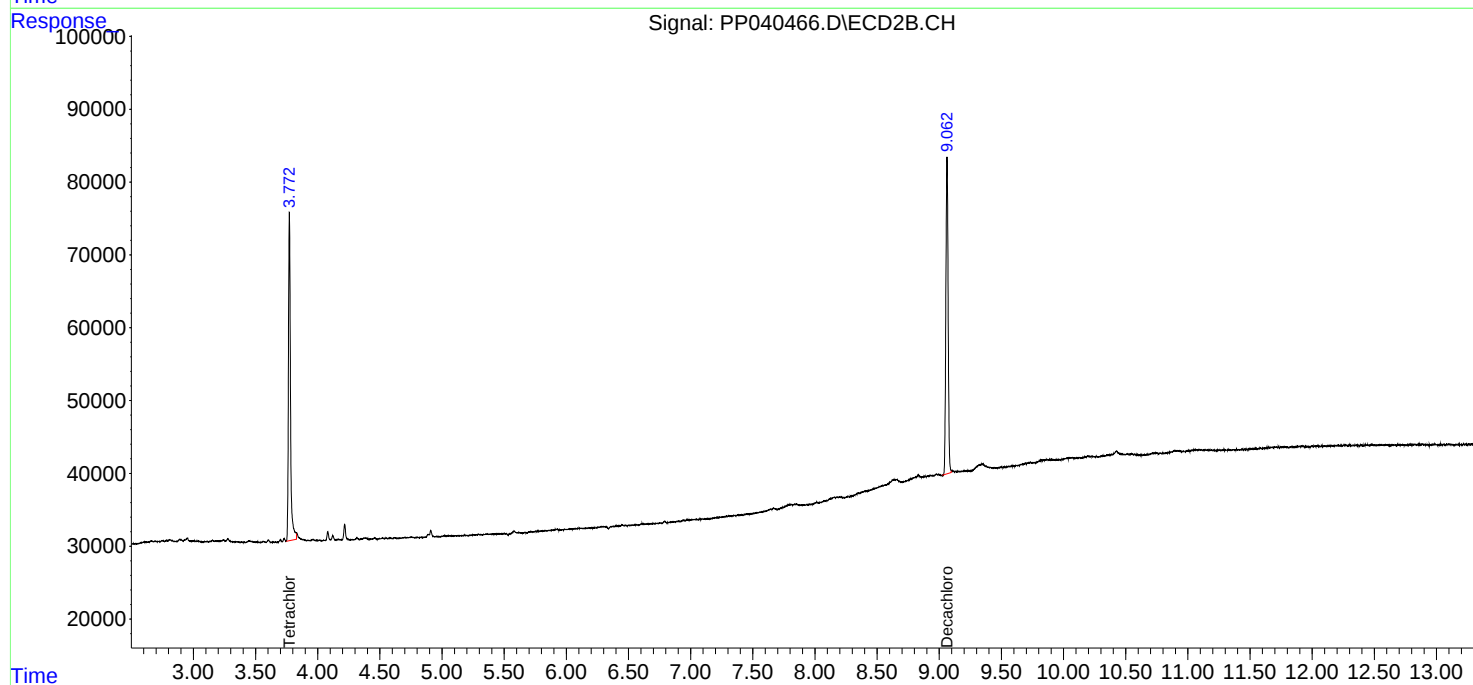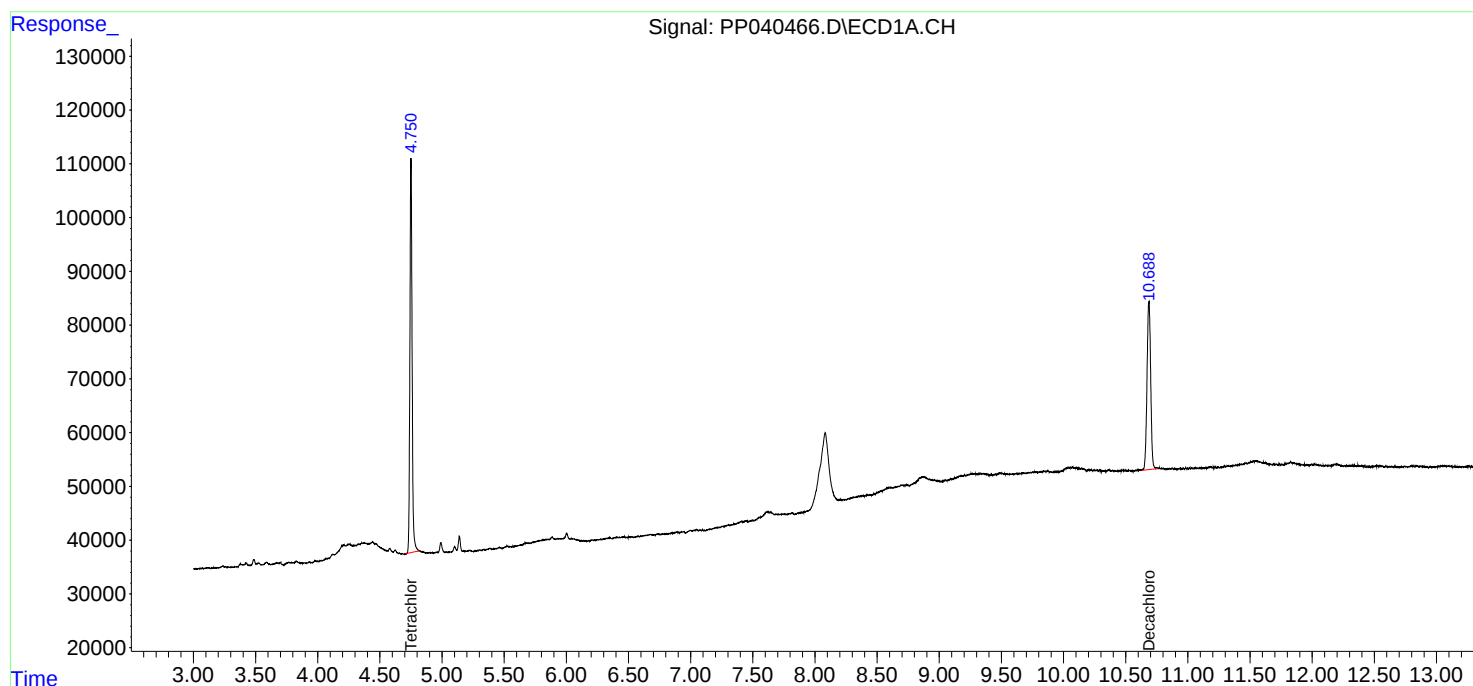


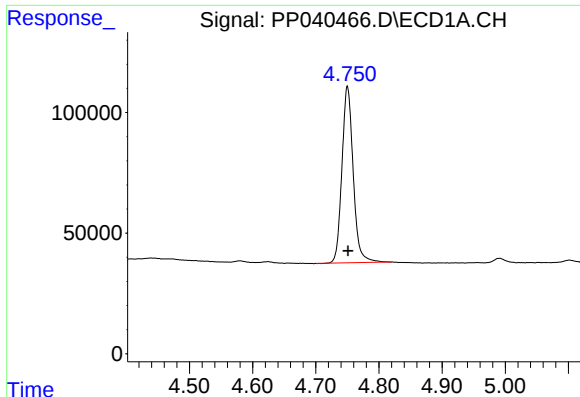

#1 Tetrachloro-m-xylene


R.T.: 4.750 min
Delta R.T.: 0.000 min
Response: 905694
Conc: 22.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB140286BL

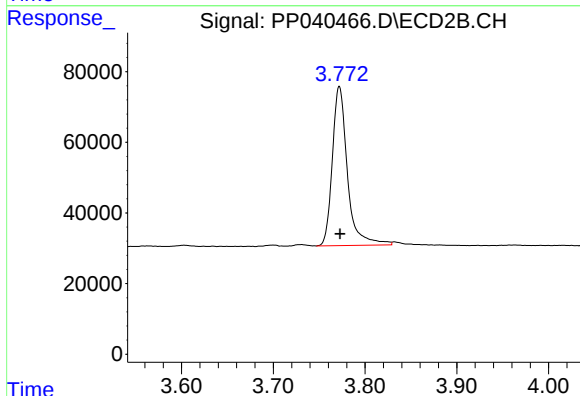


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
Delta R.T.: 0.000 min
Response: 515441
Conc: 18.92 ng/ml

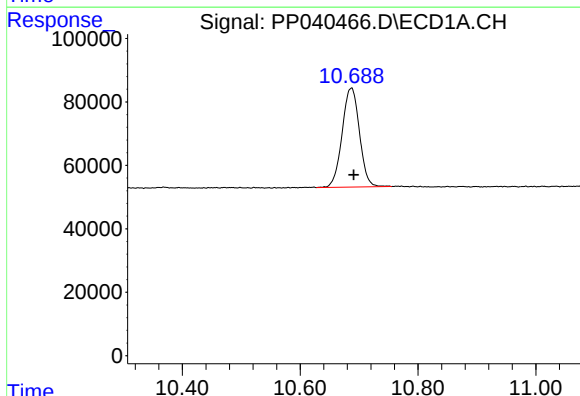

#2 Decachlorobiphenyl

R.T.: 10.688 min
Delta R.T.: -0.004 min
Response: 639013
Conc: 21.09 ng/ml

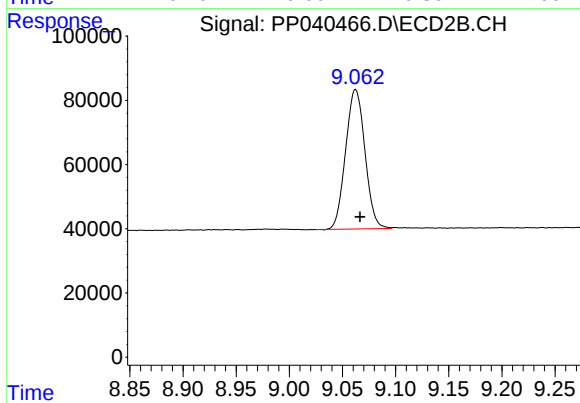

#2 Decachlorobiphenyl

R.T.: 9.062 min
Delta R.T.: -0.004 min
Response: 550346
Conc: 19.62 ng/ml