

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102721\
Data File : PP040473.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 1:08
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:48:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 27 13:26:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.751	3.772	877067	472967	21.533	17.361
2) SA Decachlor...	10.685	9.061	636654	519173	21.014	18.505

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102721\
Data File : PP040473.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 1:08
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:48:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 27 13:26:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

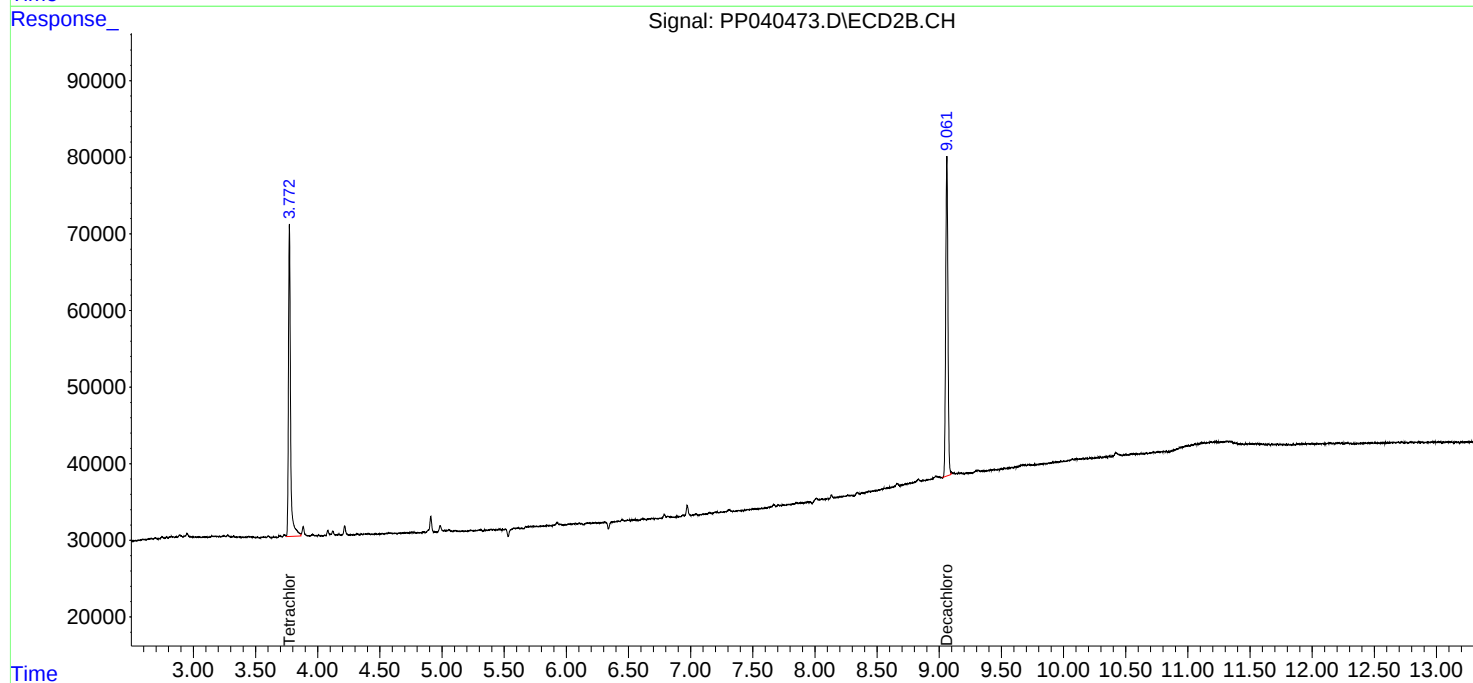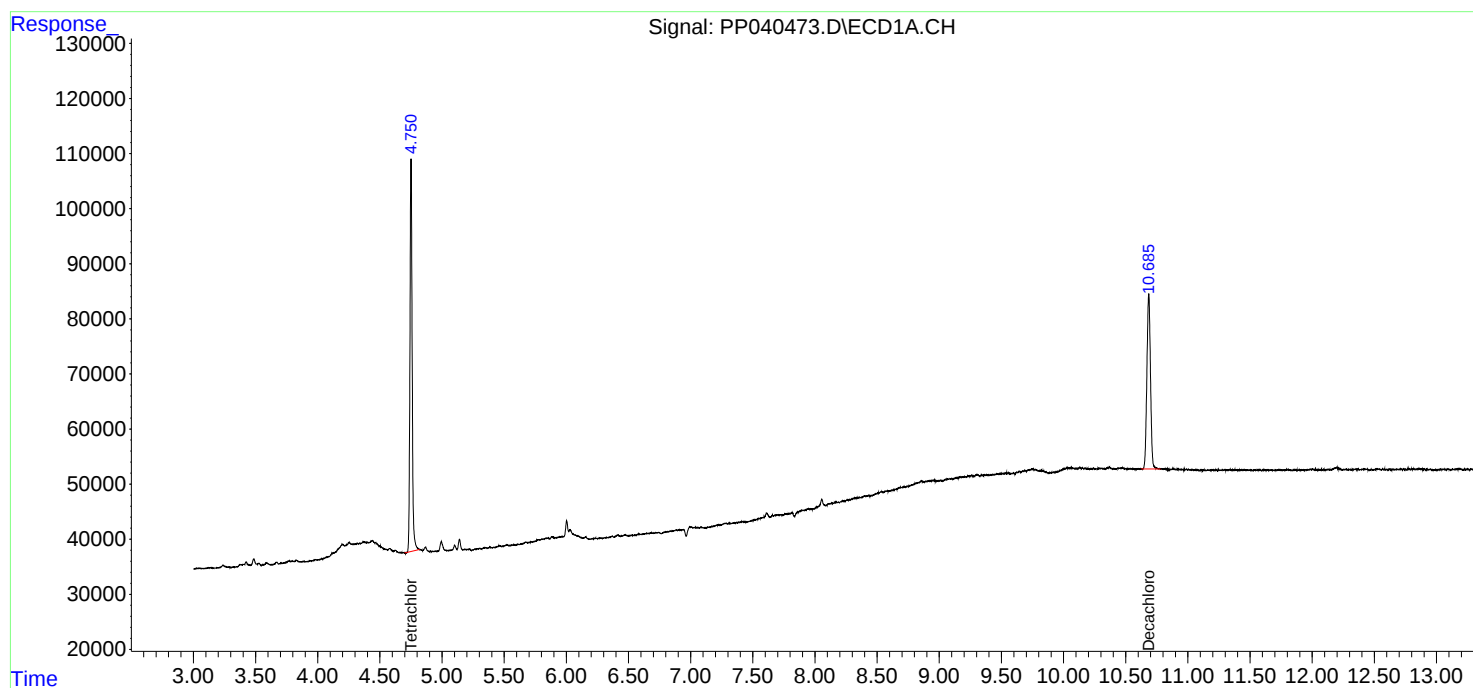


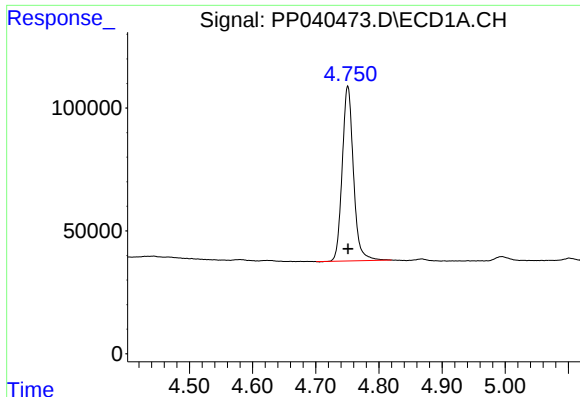

#1 Tetrachloro-m-xylene


R.T.: 4.751 min
Delta R.T.: 0.000 min
Response: 877067
Conc: 21.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

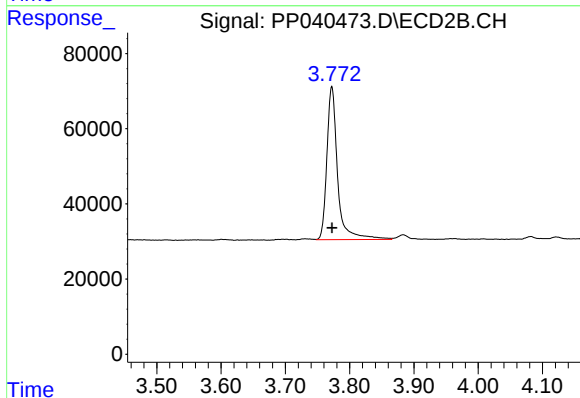


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
Delta R.T.: 0.000 min
Response: 472967
Conc: 17.36 ng/ml

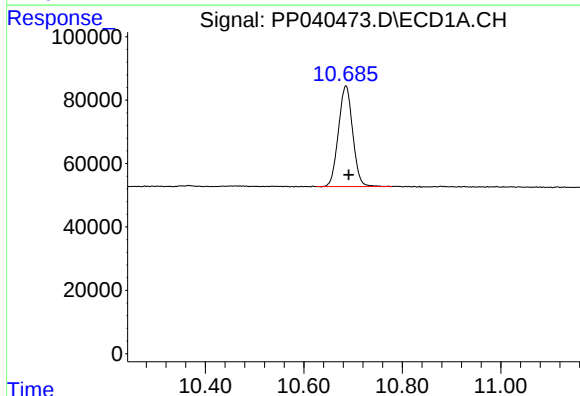

#2 Decachlorobiphenyl

R.T.: 10.685 min
Delta R.T.: -0.006 min
Response: 636654
Conc: 21.01 ng/ml

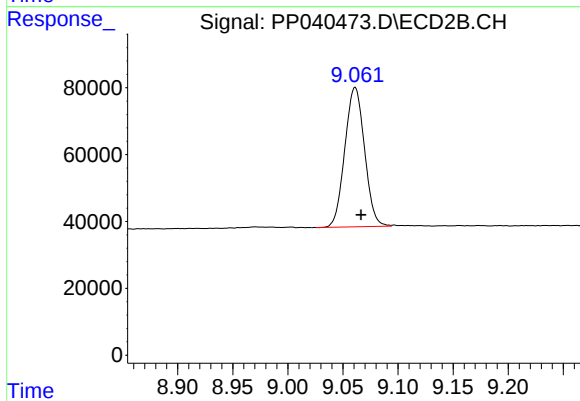

#2 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: -0.005 min
Response: 519173
Conc: 18.51 ng/ml