

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102721\
 Data File : PP040480.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 3:05
 Operator : AJ\MA
 Sample : M4370-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 33501-33503

Manual Integrations
 APPROVED

mohammad
 10/28/2021 1:35:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 07:19:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 27 13:26:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.763	3.774	1195275	336102	29.346m	12.337 #
2) SA Decachlor...	10.684	9.060	460979	352214	15.216	12.554

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102721\
Data File : PP040480.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 3:05
Operator : AJ\MA
Sample : M4370-03
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
33501-33503


Manual Integrations
APPROVED

mohammad
10/28/2021 1:35:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 07:19:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 27 13:26:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

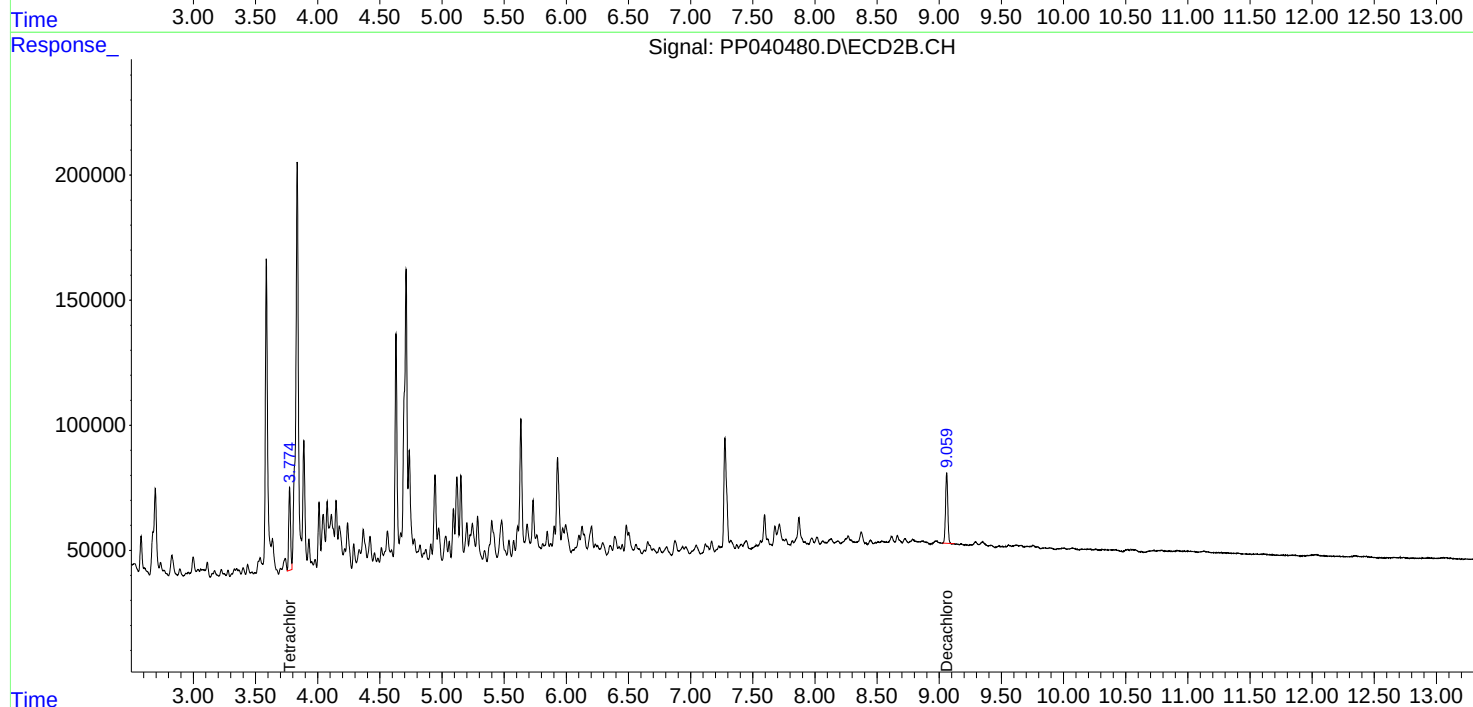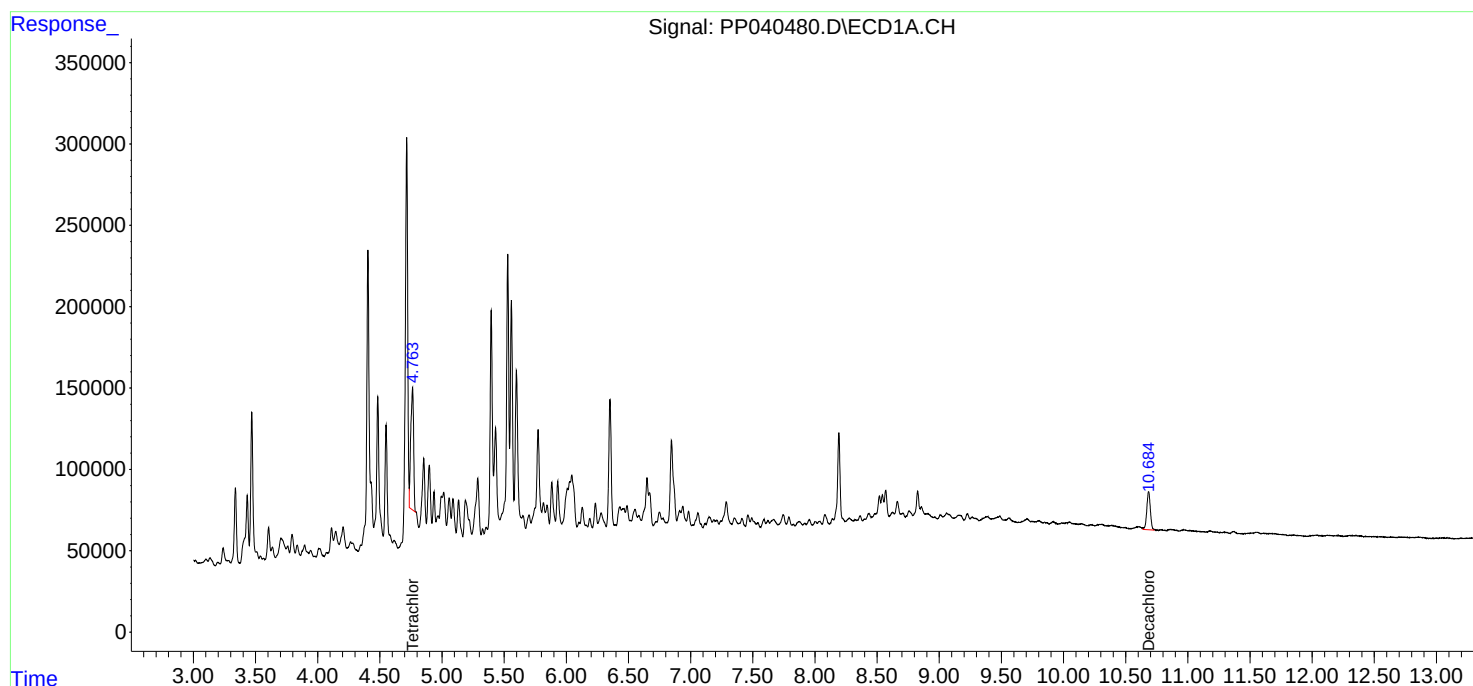

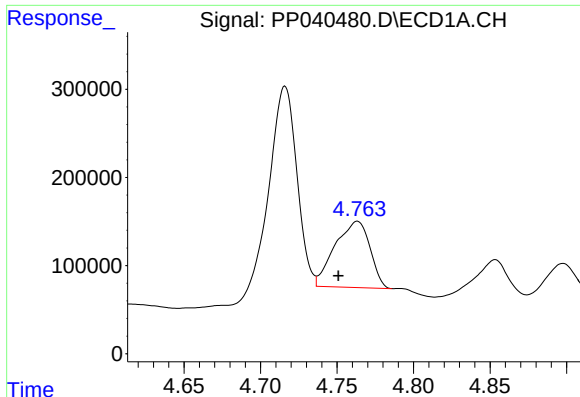


#1 Tetrachloro-m-xylene

R.T.: 4.763 min
Delta R.T.: 0.012 min
Response: 1195275
Conc: 29.35 ng/ml m

Instrument :
ECD_P
ClientSampleId :
33501-33503


Manual Integrations
APPROVED

mohammad
10/28/2021 1:35:29 PM

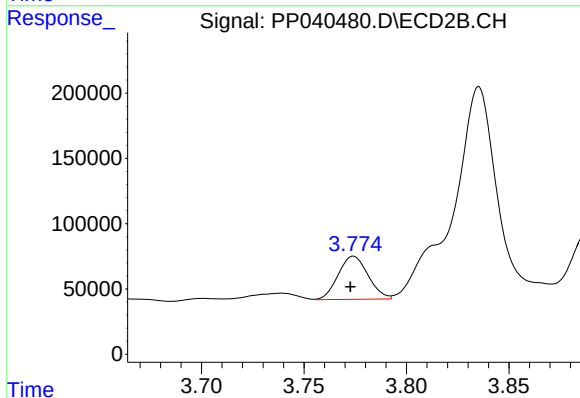


#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: 0.002 min
Response: 336102
Conc: 12.34 ng/ml

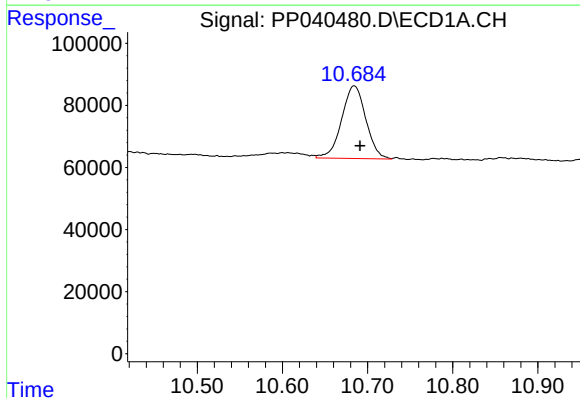

#2 Decachlorobiphenyl

R.T.: 10.684 min
Delta R.T.: -0.007 min
Response: 460979
Conc: 15.22 ng/ml

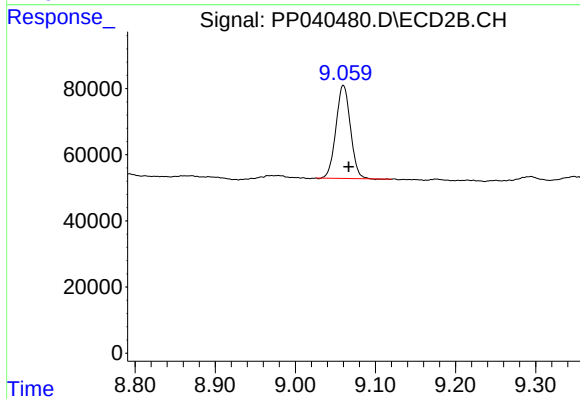

#2 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: -0.006 min
Response: 352214
Conc: 12.55 ng/ml