

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2022 11:10
 Operator : YP\AJ
 Sample : N5265-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CONCRETE-72-11976

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 12:08:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.409	3.653	43242715	39580900	19.569	21.062
2)	SA Decachlor...	10.223	8.742	26132747	36710399	20.588	21.889
Target Compounds							
3)	L1 AR-1016-1	5.605f	0.000	243592	0	3.633	N.D. #
4)	L1 AR-1016-2	5.605	0.000	243592	0	2.439	N.D. #
5)	L1 AR-1016-3	5.662	0.000	288641	0	4.743	N.D. #
6)	L1 AR-1016-4	5.762	0.000	81008	0	1.673	N.D. #
7)	L1 AR-1016-5	6.057	0.000	37320	0	0.775	N.D. #
8)	L2 AR-1221-1	4.617	0.000	179216	0	6.989	N.D. #
9)	L2 AR-1221-2	4.717	3.957	563312	696558	29.612	39.791 #
10)	L2 AR-1221-3	4.785	0.000	102238	0	1.794	N.D. #
11)	L3 AR-1232-1	4.785	0.000	102238	0	2.356	N.D. #
12)	L3 AR-1232-2	5.341f	0.000	642591	0	25.899	N.D. #
13)	L3 AR-1232-3	5.605	0.000	243592	0	5.565	N.D. #
14)	L3 AR-1232-4	5.762	0.000	81008	0	3.795	N.D. #
15)	L3 AR-1232-5	5.854	0.000	28078	0	1.631	N.D. #
16)	L4 AR-1242-1	5.605f	0.000	243592	0	4.328	N.D. #
17)	L4 AR-1242-2	5.605	0.000	243592	0	2.949	N.D. #
18)	L4 AR-1242-3	5.662	0.000	288641	0	5.675	N.D. #
19)	L4 AR-1242-4	5.762	0.000	81008	0	2.000	N.D. #
20)	L4 AR-1242-5	6.515	0.000	104547	0	2.622	N.D. #
21)	L5 AR-1248-1	5.605f	0.000	243592	0	5.997	N.D. #
22)	L5 AR-1248-2	5.854	0.000	28078	0	0.472	N.D. #
23)	L5 AR-1248-3	6.057	0.000	37320	0	0.575	N.D. #
24)	L5 AR-1248-4	6.485	0.000	311628	0	4.839	N.D. #
25)	L5 AR-1248-5	6.515	0.000	104547	0	1.650	N.D. #
26)	L6 AR-1254-1	6.449	0.000	344120	0	4.533	N.D. #
27)	L6 AR-1254-2	6.677	0.000	246846	0	2.209	N.D. #
28)	L6 AR-1254-3	7.035	0.000	583111	0	5.239	N.D. #
29)	L6 AR-1254-4	7.314	0.000	21245543	0	301.696	N.D. #
30)	L6 AR-1254-5	7.763f	6.782	332687	168318	4.226	1.210 #
32)	L7 AR-1260-2	7.470	6.436	10432436	371849	111.719	3.058 #
33)	L7 AR-1260-3	0.000	6.586f	0	17958437	N.D.	153.955 #
34)	L7 AR-1260-4	8.028f	7.086	328598	45201	4.589	0.502 #
35)	L7 AR-1260-5	0.000	7.324	0	103268	N.D.	0.504 #
36)	L8 AR-1262-1	0.000	6.869	0	17477	N.D.	0.305 #
37)	L8 AR-1262-2	0.000	7.086	0	45201	N.D.	0.365 #
38)	L8 AR-1262-3	0.000	7.620	0	896089	N.D.	8.879 #
39)	L8 AR-1262-4	0.000	7.681	0	91935	N.D.	0.514 #
40)	L8 AR-1262-5	9.461	8.183	166408	61690	3.636	0.824 #
41)	L9 AR-1268-1	0.000	7.620	0	896089	N.D.	2.923 #
42)	L9 AR-1268-2	0.000	7.681	0	91935	N.D.	0.339 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2022 11:10
Operator : YP\AJ
Sample : N5265-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 12:08:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	0.000	7.885	0	198361	N.D.	0.846 #
44)	L9 AR-1268-4	9.461	8.183	166408	61690	3.272	0.726 #
45)	L9 AR-1268-5	9.877	8.482	260209	137069	0.606	0.209 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2022 11:10
Operator : YP\AJ
Sample : N5265-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 12:08:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

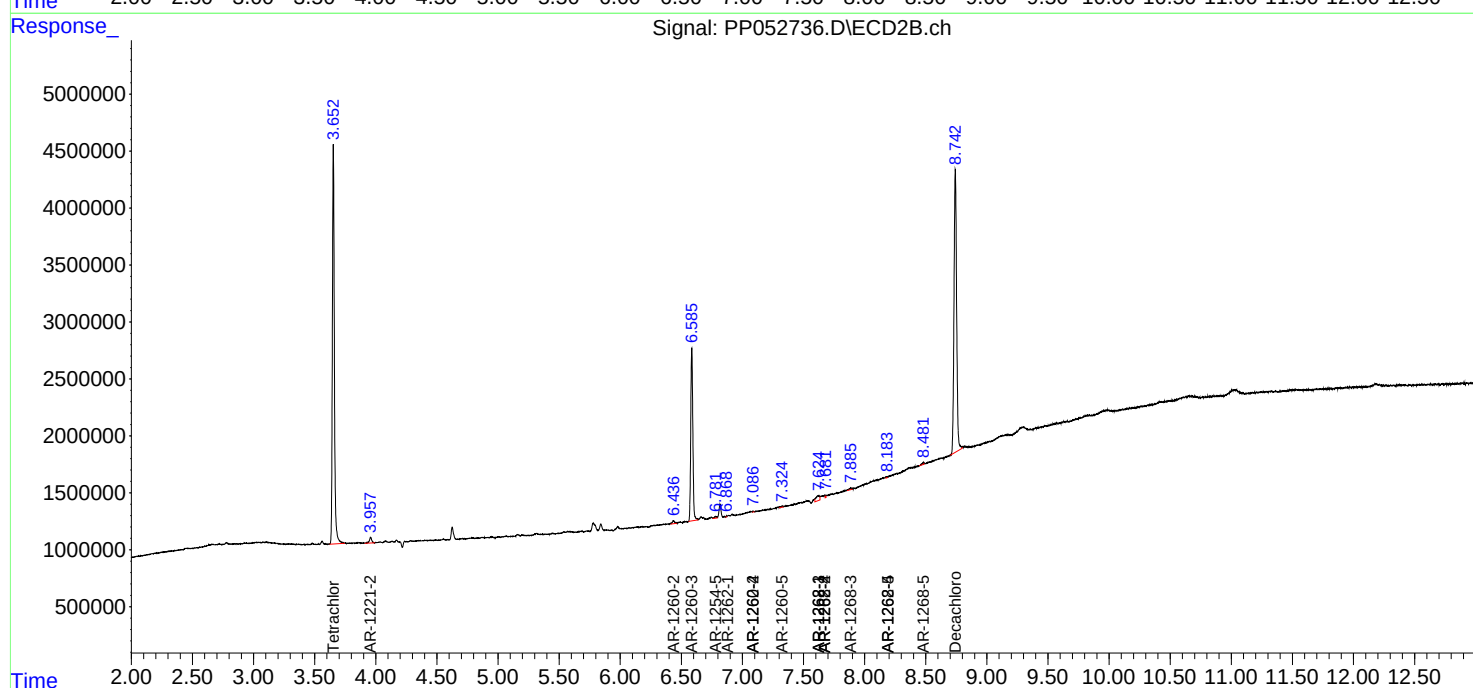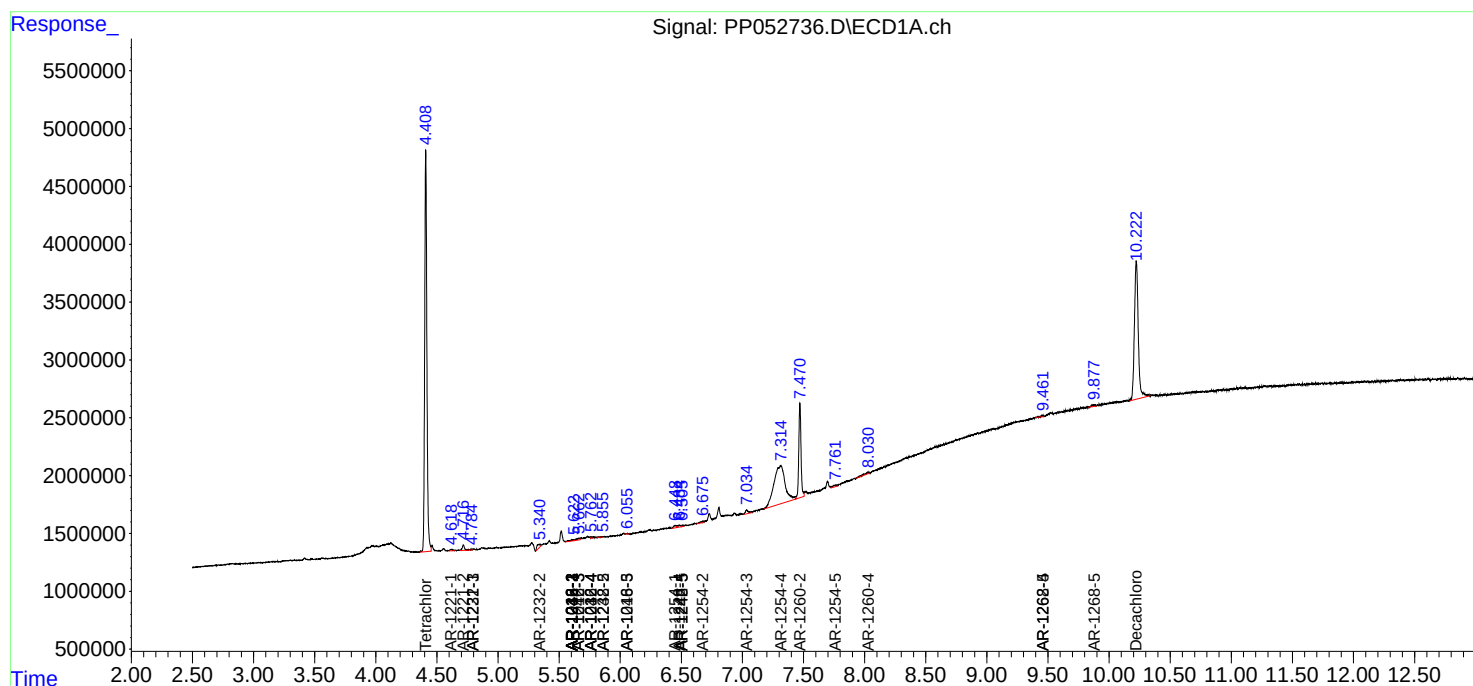


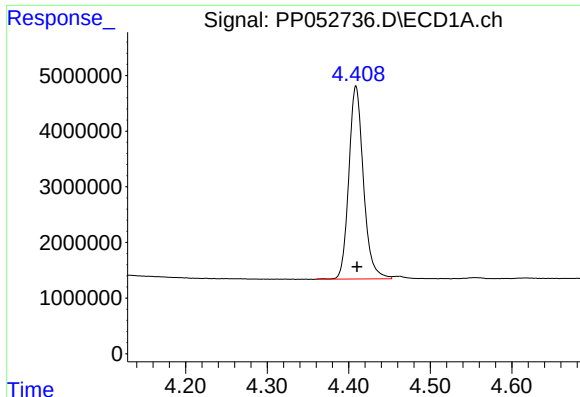

#1 Tetrachloro-m-xylene


R.T.: 4.409 min
Delta R.T.: -0.001 min
Response: 43242715
Conc: 19.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

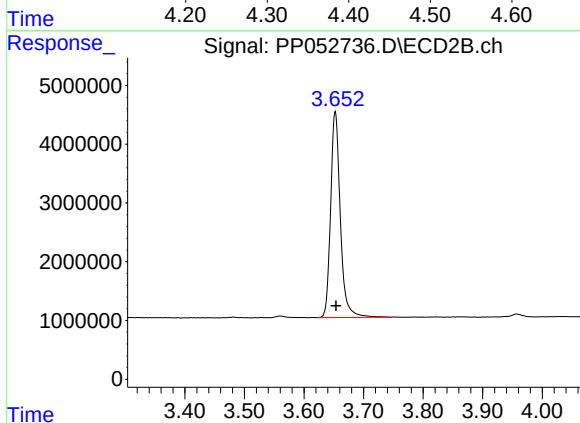


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.001 min
Response: 39580900
Conc: 21.06 ng/ml

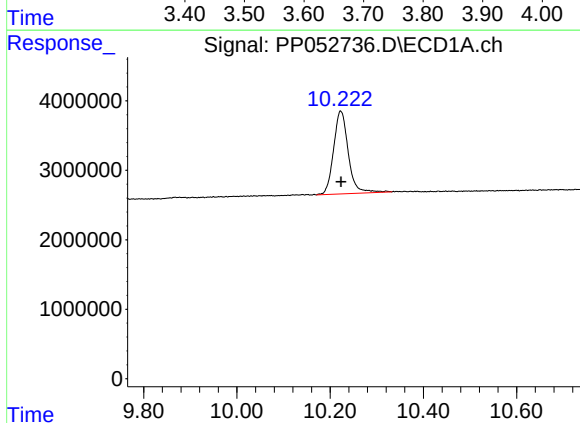


#2 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: 0.000 min
Response: 26132747
Conc: 20.59 ng/ml

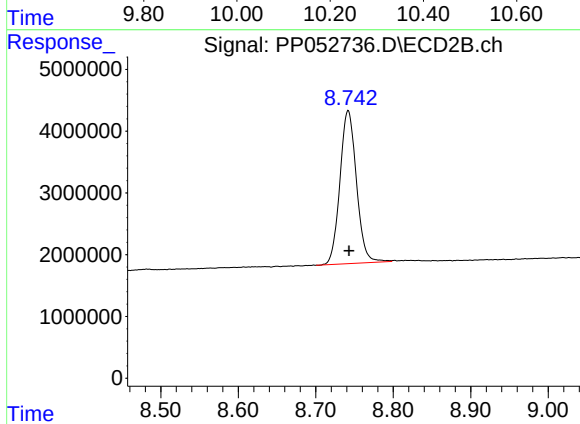

#2 Decachlorobiphenyl


R.T.: 8.742 min
Delta R.T.: 0.000 min
Response: 36710399
Conc: 21.89 ng/ml

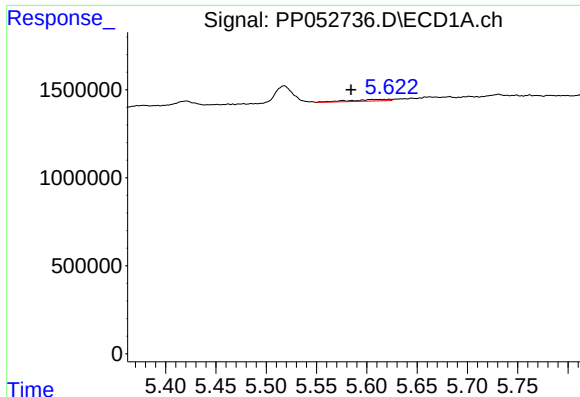

#3 AR-1016-1


R.T.: 5.605 min
Delta R.T.: 0.021 min
Response: 243592
Conc: 3.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

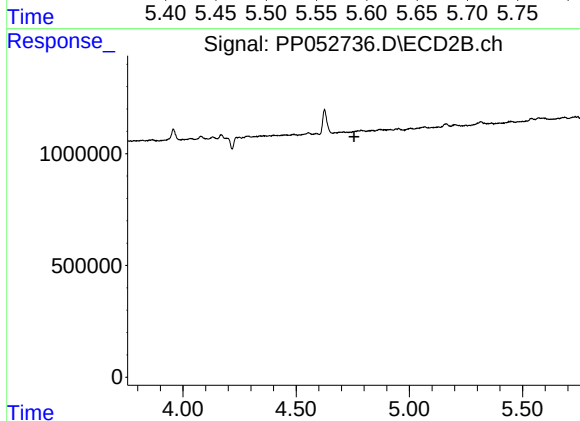


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.755 min
Response: 0
Conc: N.D.

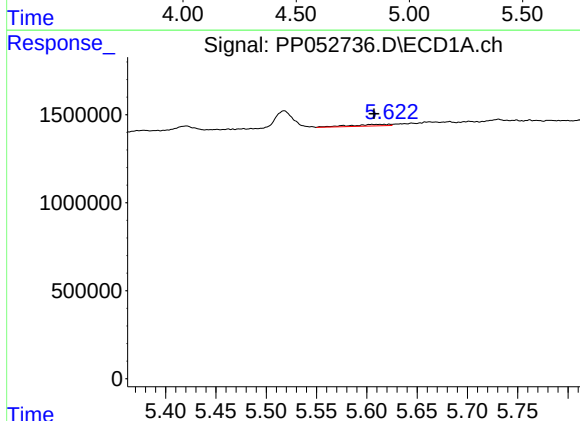


#4 AR-1016-2

R.T.: 5.605 min
Delta R.T.: -0.002 min
Response: 243592
Conc: 2.44 ng/ml

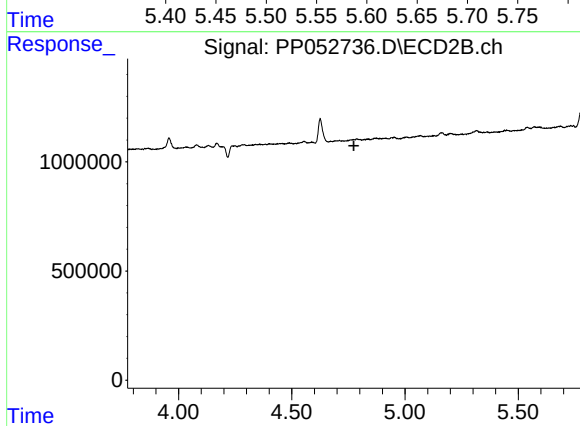

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.774 min
Response: 0
Conc: N.D.

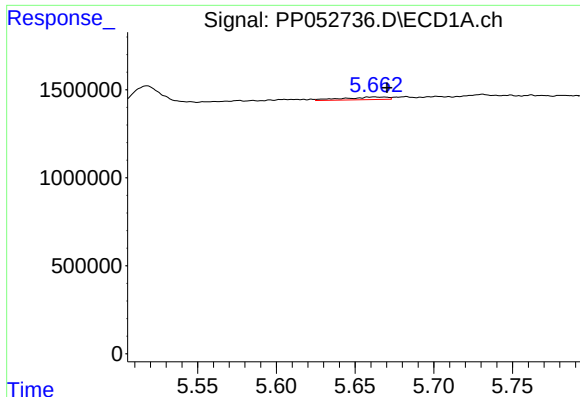

#5 AR-1016-3


R.T.: 5.662 min
Delta R.T.: -0.008 min
Response: 288641
Conc: 4.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

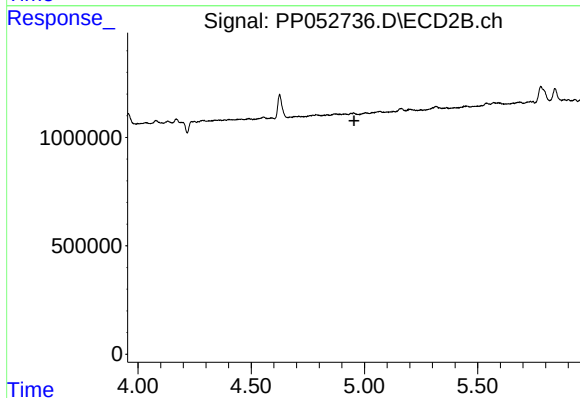


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

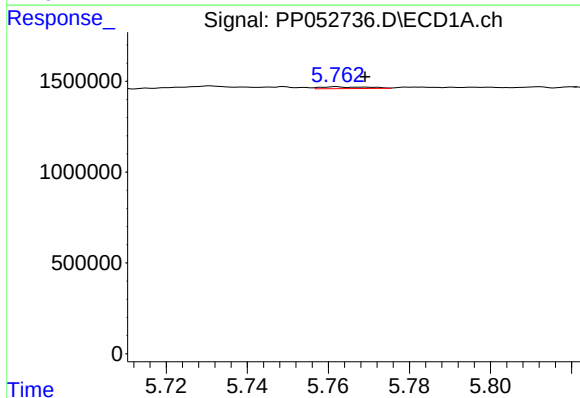


#6 AR-1016-4

R.T.: 5.762 min
Delta R.T.: -0.007 min
Response: 81008
Conc: 1.67 ng/ml

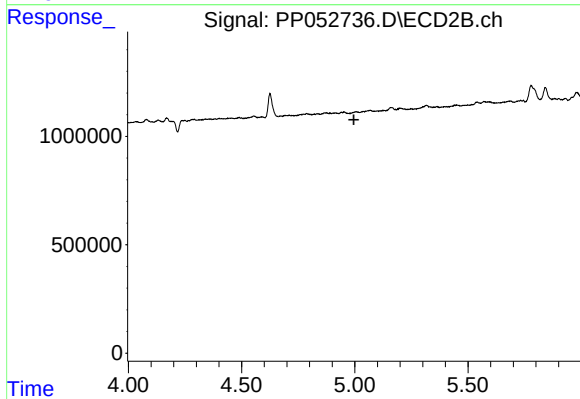

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.996 min
Response: 0
Conc: N.D.

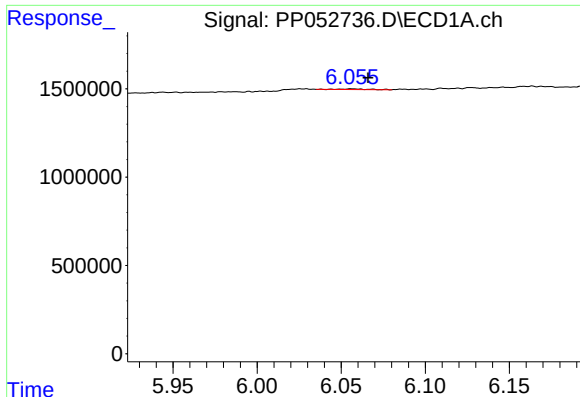

#7 AR-1016-5


R.T.: 6.057 min
Delta R.T.: -0.009 min
Response: 37320
Conc: 0.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

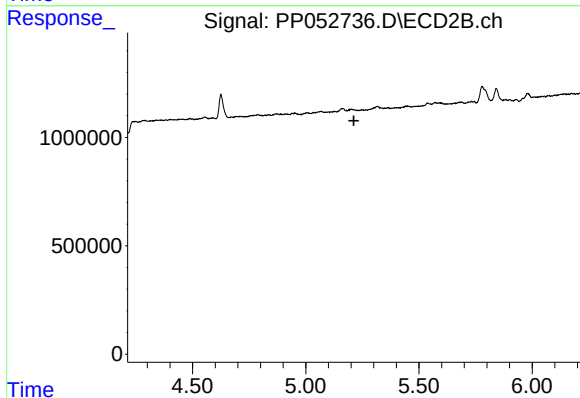


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

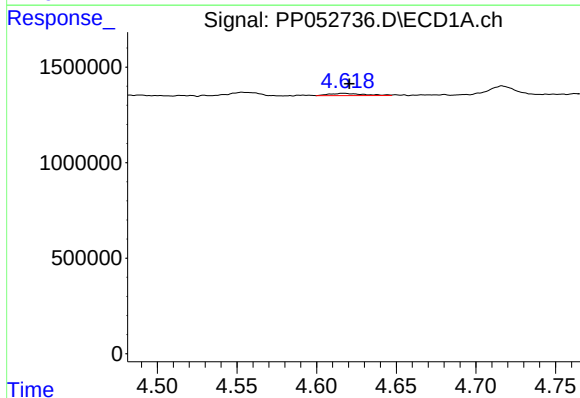


#8 AR-1221-1

R.T.: 4.617 min
Delta R.T.: -0.003 min
Response: 179216
Conc: 6.99 ng/ml

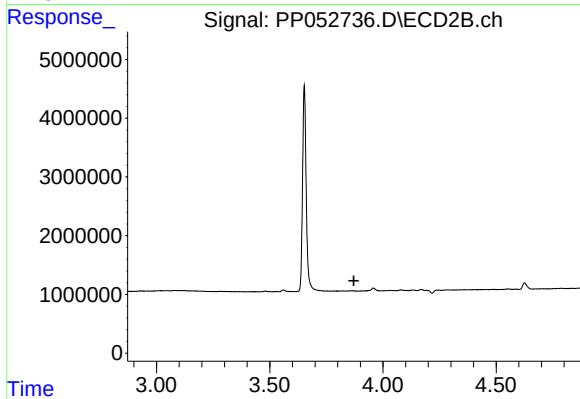

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.872 min
Response: 0
Conc: N.D.

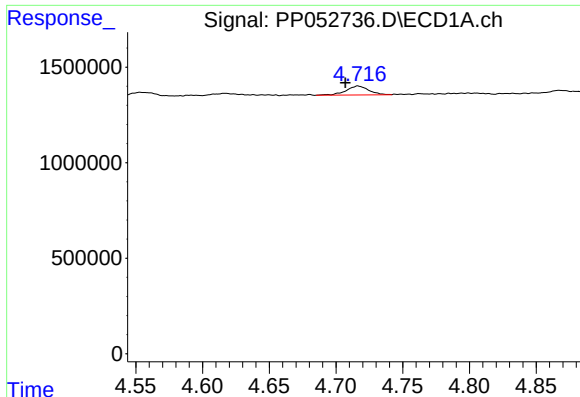

#9 AR-1221-2


R.T.: 4.717 min
Delta R.T.: 0.009 min
Response: 563312
Conc: 29.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

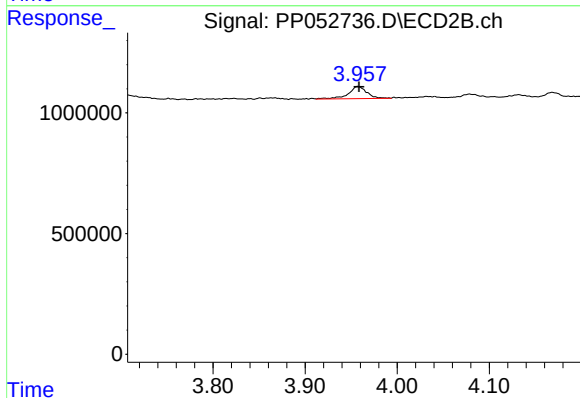


#9 AR-1221-2

R.T.: 3.957 min
Delta R.T.: -0.001 min
Response: 696558
Conc: 39.79 ng/ml

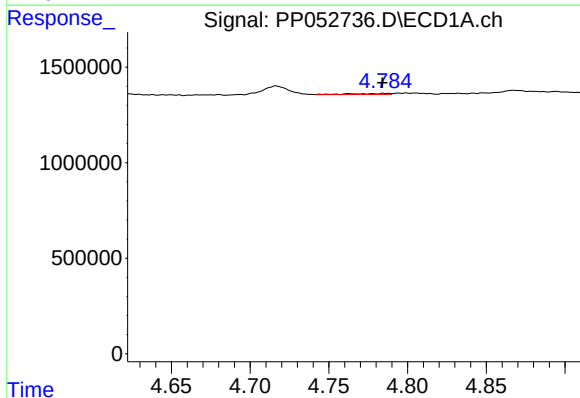


#10 AR-1221-3

R.T.: 4.785 min
Delta R.T.: 0.001 min
Response: 102238
Conc: 1.79 ng/ml

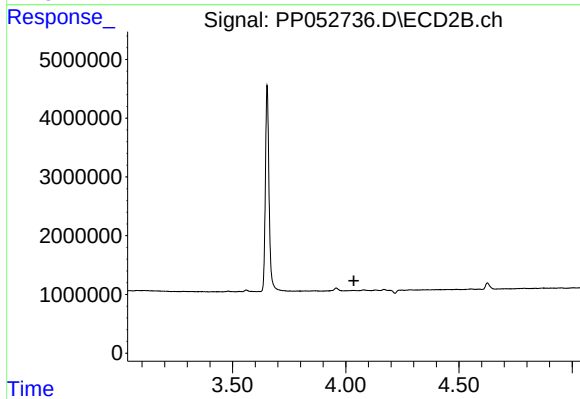

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.036 min
Response: 0
Conc: N.D.

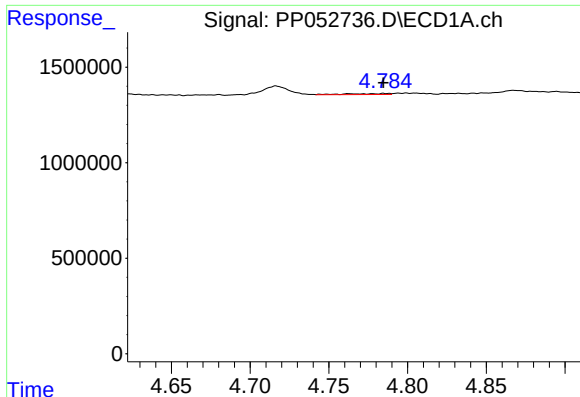

#11 AR-1232-1


R.T.: 4.785 min
Delta R.T.: 0.000 min
Response: 102238
Conc: 2.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

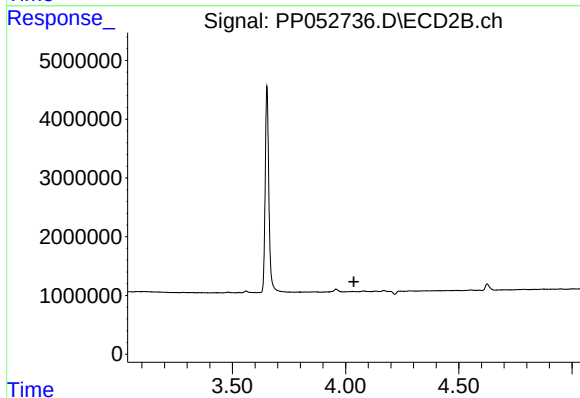


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.036 min
Response: 0
Conc: N.D.

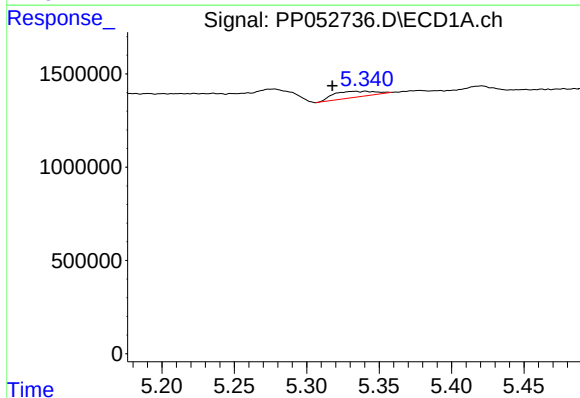


#12 AR-1232-2

R.T.: 5.341 min
Delta R.T.: 0.023 min
Response: 642591
Conc: 25.90 ng/ml

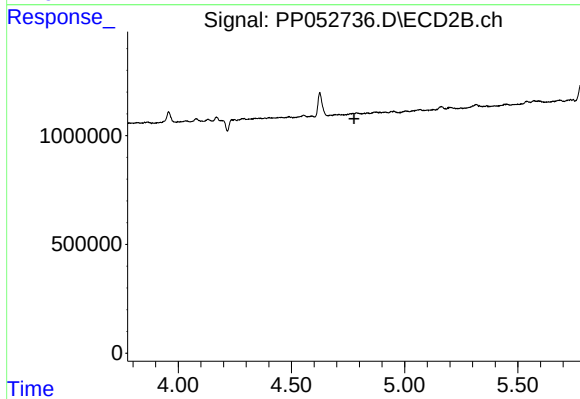

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.776 min
Response: 0
Conc: N.D.

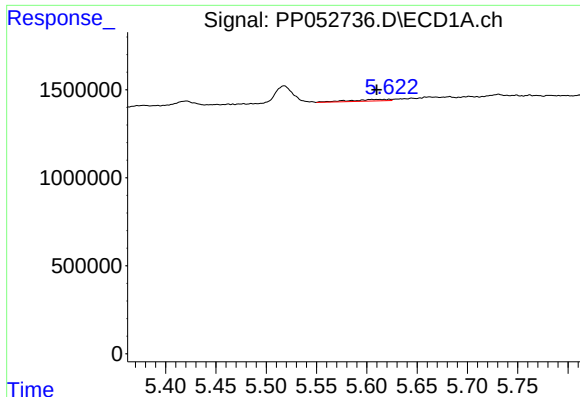

#13 AR-1232-3


R.T.: 5.605 min
Delta R.T.: -0.004 min
Response: 243592
Conc: 5.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

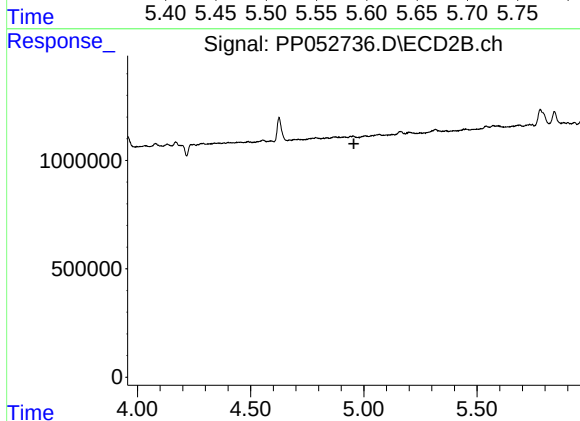


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.955 min
Response: 0
Conc: N.D.

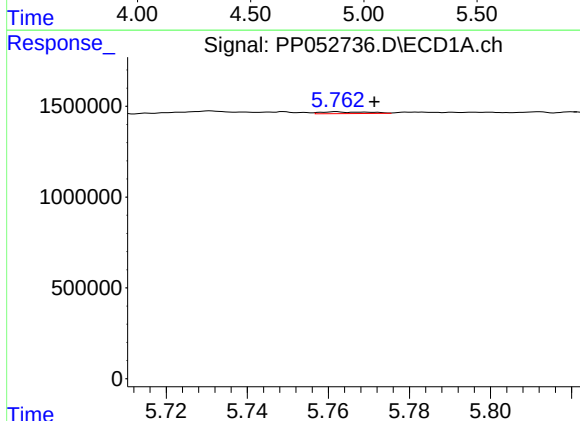


#14 AR-1232-4

R.T.: 5.762 min
Delta R.T.: -0.010 min
Response: 81008
Conc: 3.80 ng/ml

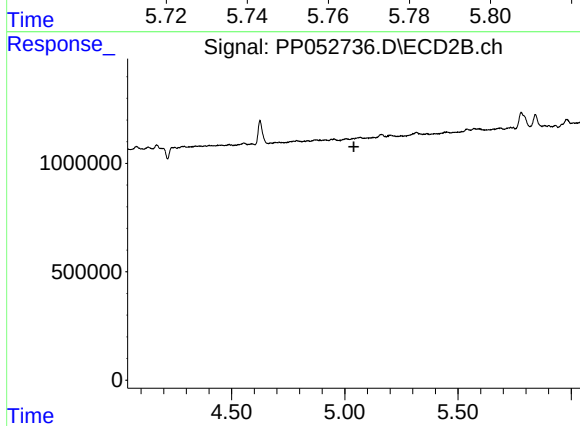

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.040 min
Response: 0
Conc: N.D.

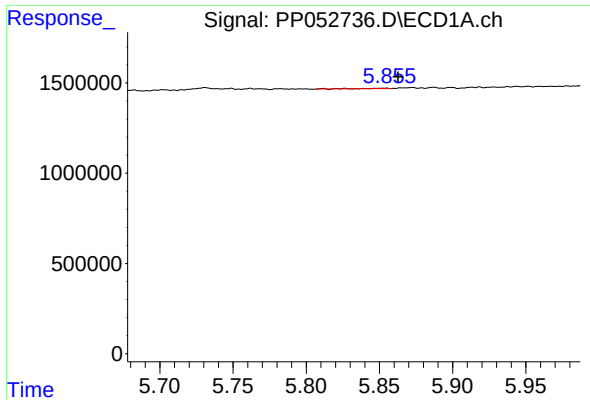

#15 AR-1232-5


R.T.: 5.854 min
Delta R.T.: -0.009 min
Response: 28078
Conc: 1.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

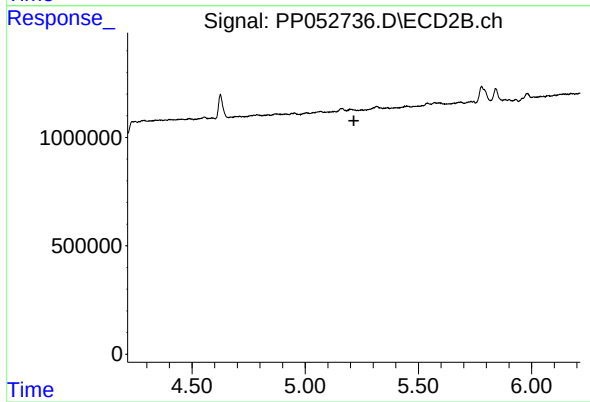


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.215 min
Response: 0
Conc: N.D.

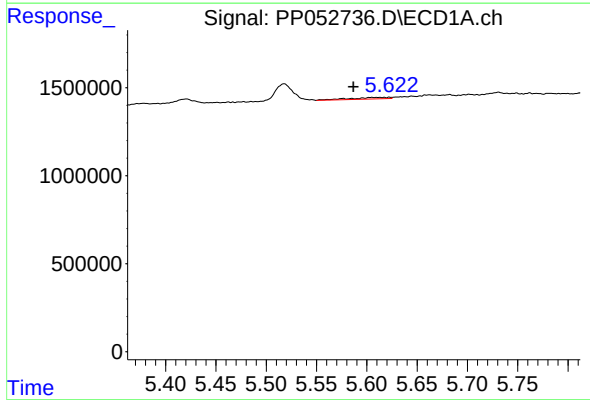


#16 AR-1242-1

R.T.: 5.605 min
Delta R.T.: 0.019 min
Response: 243592
Conc: 4.33 ng/ml

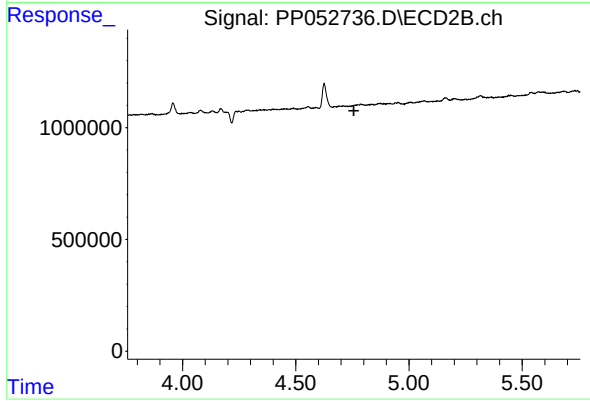

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.757 min
Response: 0
Conc: N.D.

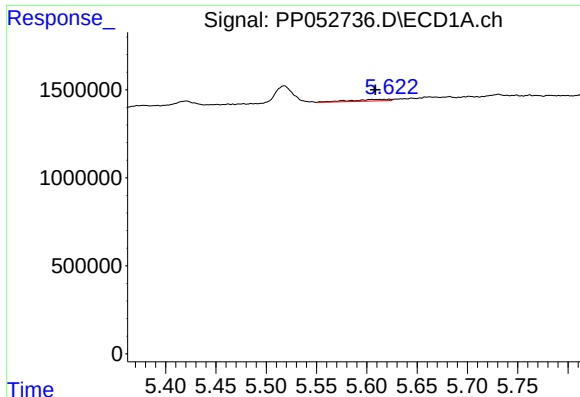

#17 AR-1242-2


R.T.: 5.605 min
Delta R.T.: -0.003 min
Response: 243592
Conc: 2.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

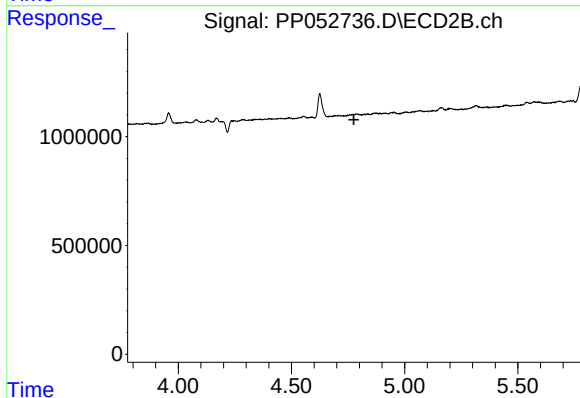


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.776 min
Response: 0
Conc: N.D.

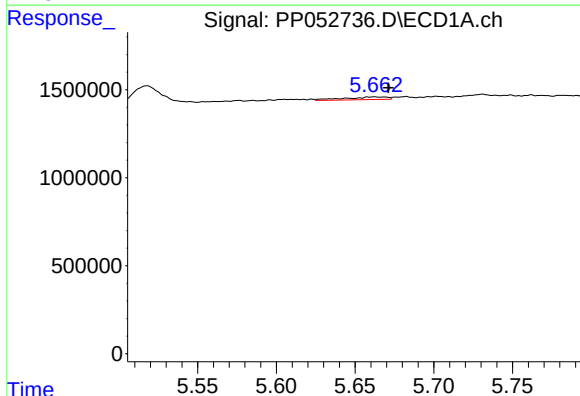


#18 AR-1242-3

R.T.: 5.662 min
Delta R.T.: -0.009 min
Response: 288641
Conc: 5.68 ng/ml

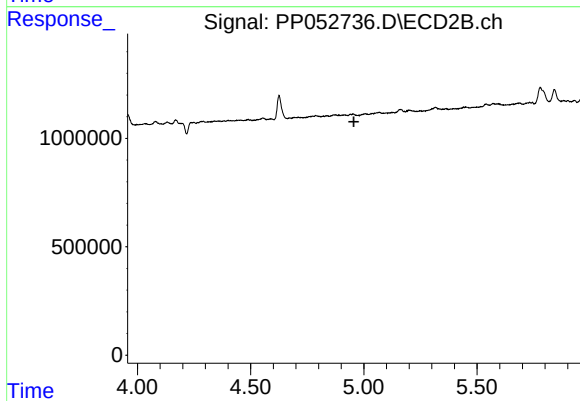

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

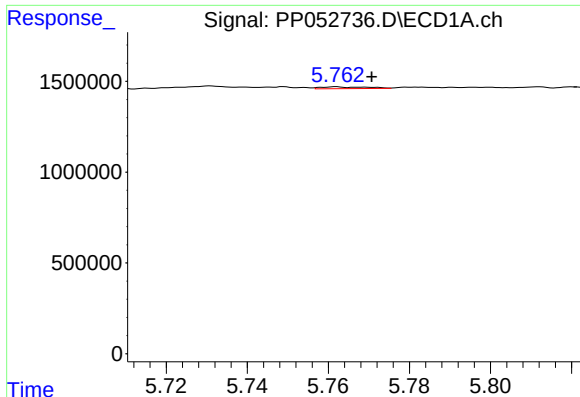

#19 AR-1242-4


R.T.: 5.762 min
Delta R.T.: -0.009 min
Response: 81008
Conc: 2.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

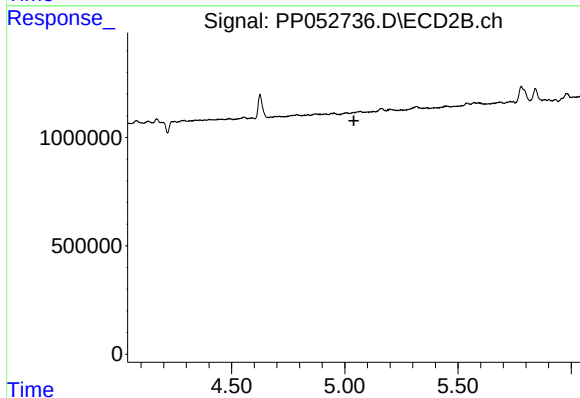


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.040 min
Response: 0
Conc: N.D.

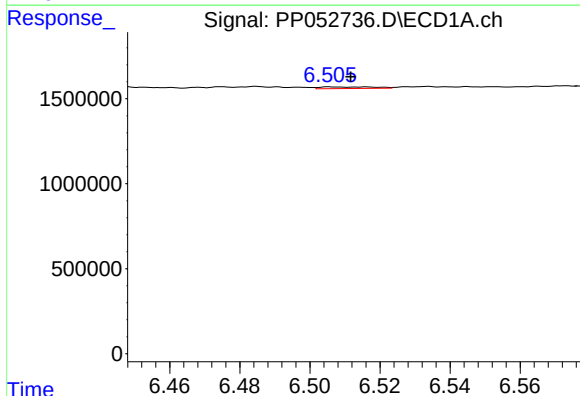


#20 AR-1242-5

R.T.: 6.515 min
Delta R.T.: 0.004 min
Response: 104547
Conc: 2.62 ng/ml

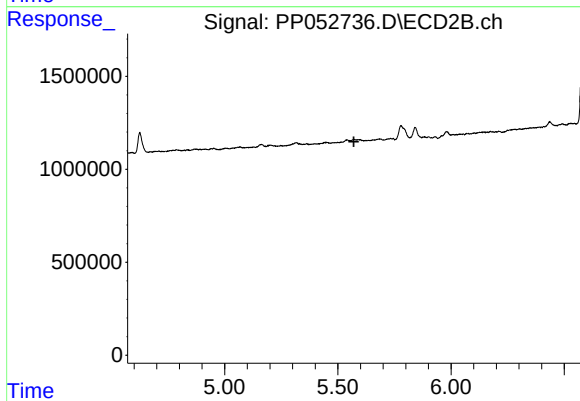

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.571 min
Response: 0
Conc: N.D.

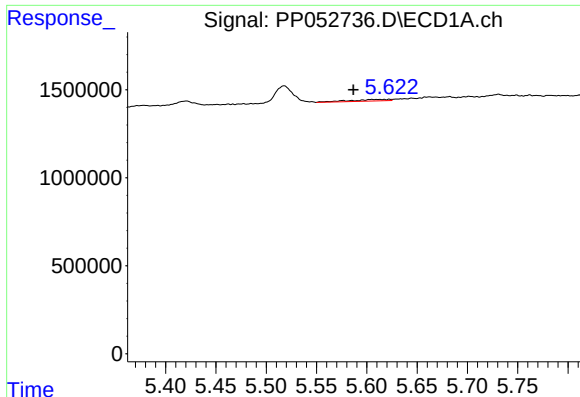

#21 AR-1248-1


R.T.: 5.605 min
Delta R.T.: 0.019 min
Response: 243592
Conc: 6.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

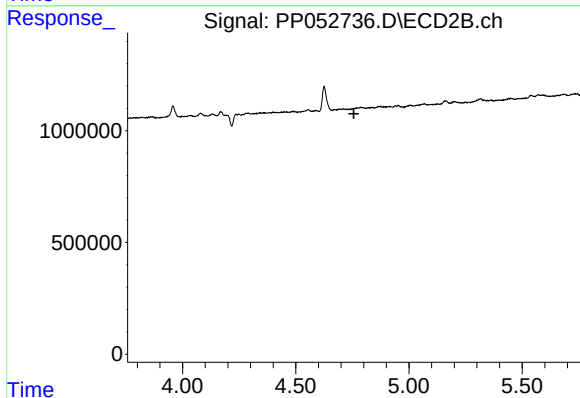


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.757 min
Response: 0
Conc: N.D.

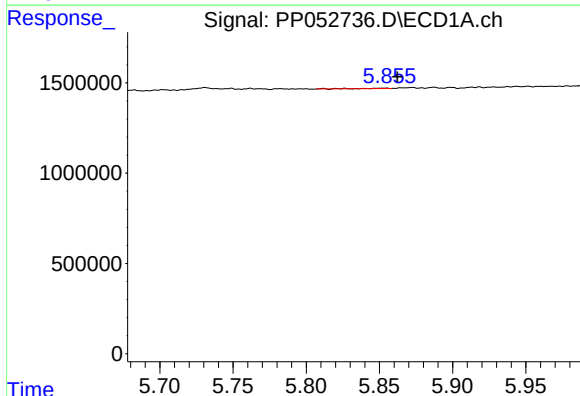


#22 AR-1248-2

R.T.: 5.854 min
Delta R.T.: -0.008 min
Response: 28078
Conc: 0.47 ng/ml

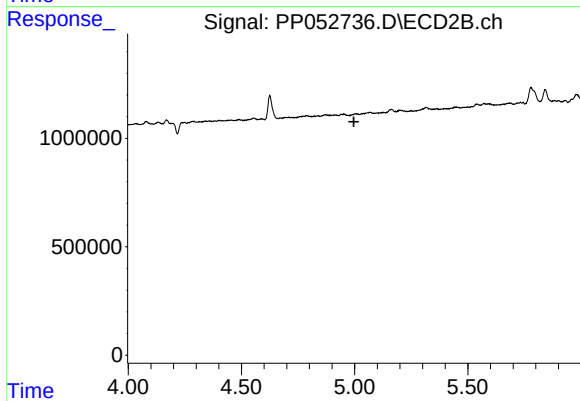

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

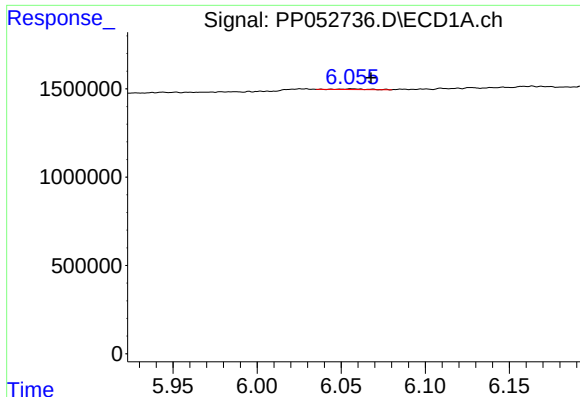

#23 AR-1248-3


R.T.: 6.057 min
Delta R.T.: -0.011 min
Response: 37320
Conc: 0.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

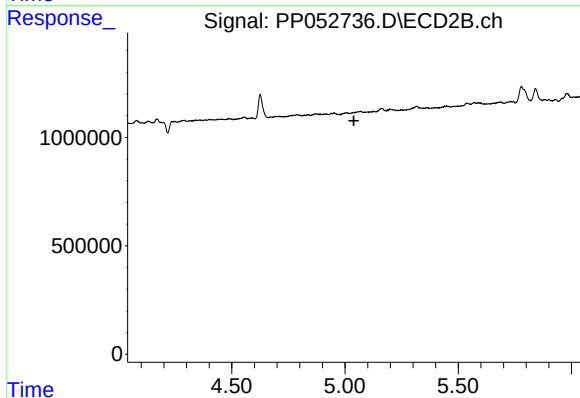


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.039 min
Response: 0
Conc: N.D.

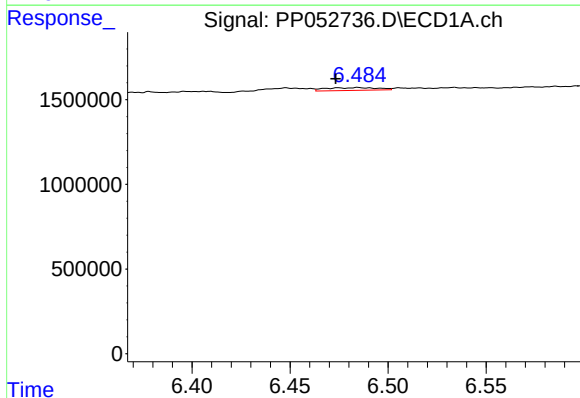


#24 AR-1248-4

R.T.: 6.485 min
Delta R.T.: 0.012 min
Response: 311628
Conc: 4.84 ng/ml

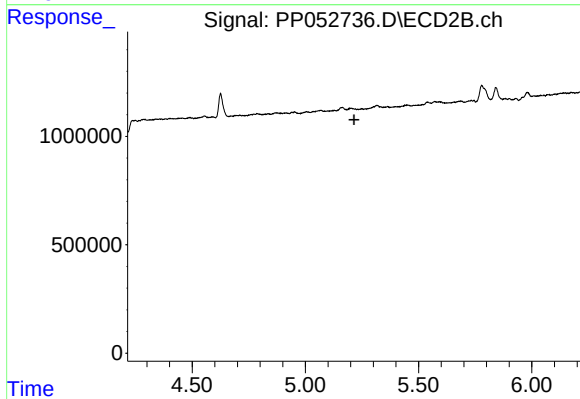

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.215 min
Response: 0
Conc: N.D.

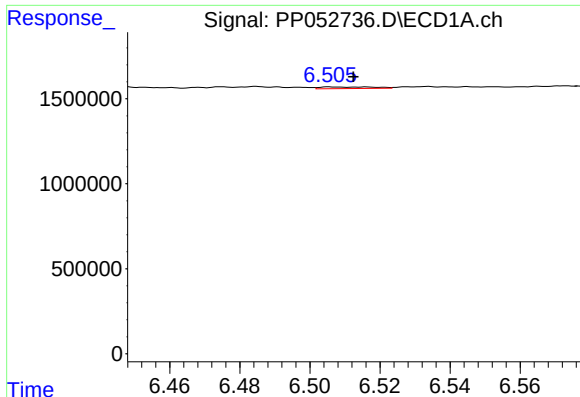

#25 AR-1248-5


R.T.: 6.515 min
Delta R.T.: 0.003 min
Response: 104547
Conc: 1.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

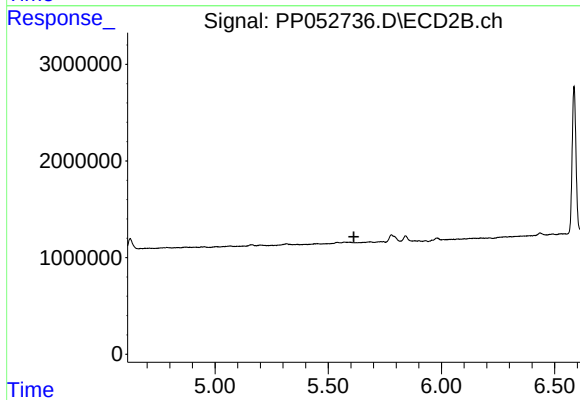


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.613 min
Response: 0
Conc: N.D.

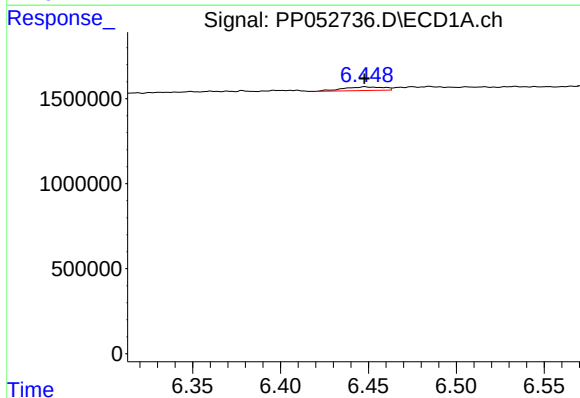


#26 AR-1254-1

R.T.: 6.449 min
Delta R.T.: 0.001 min
Response: 344120
Conc: 4.53 ng/ml

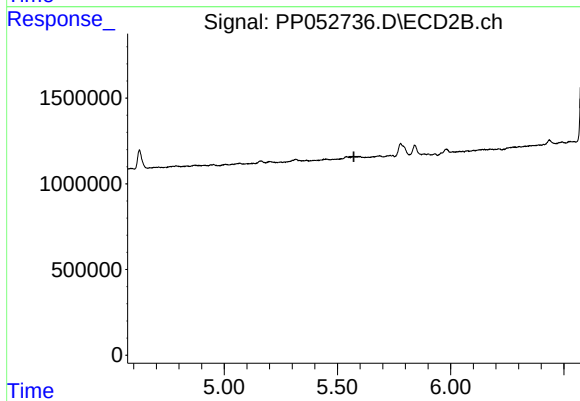

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.572 min
Response: 0
Conc: N.D.

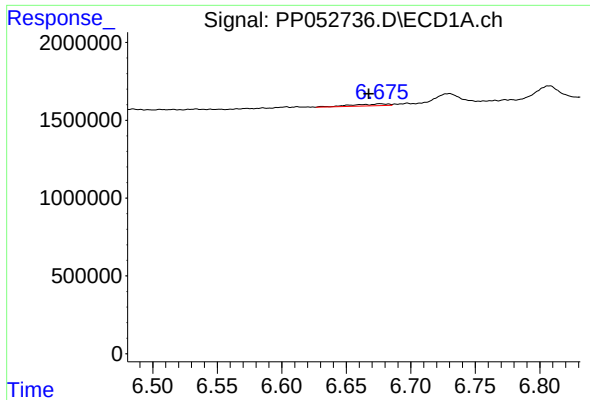

#27 AR-1254-2


R.T.: 6.677 min
Delta R.T.: 0.010 min
Response: 246846
Conc: 2.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

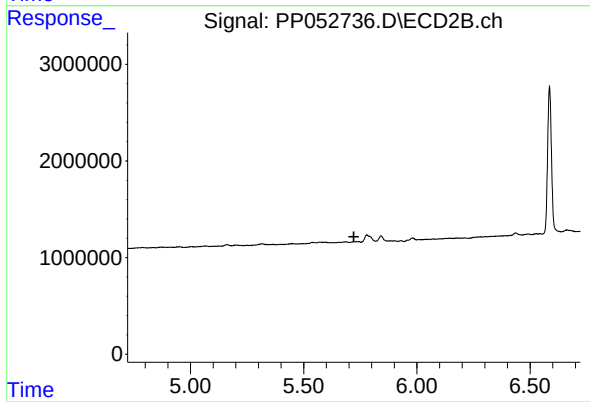


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.722 min
Response: 0
Conc: N.D.

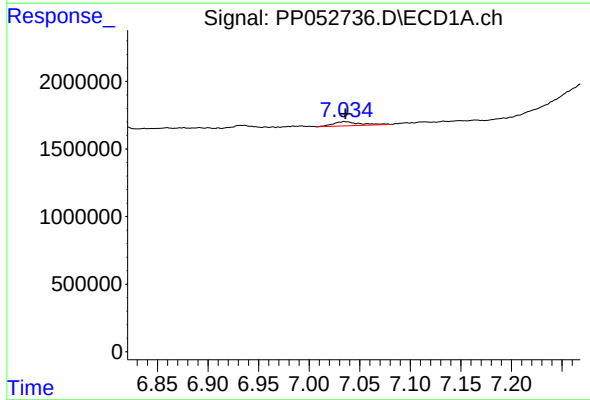


#28 AR-1254-3

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 583111
Conc: 5.24 ng/ml

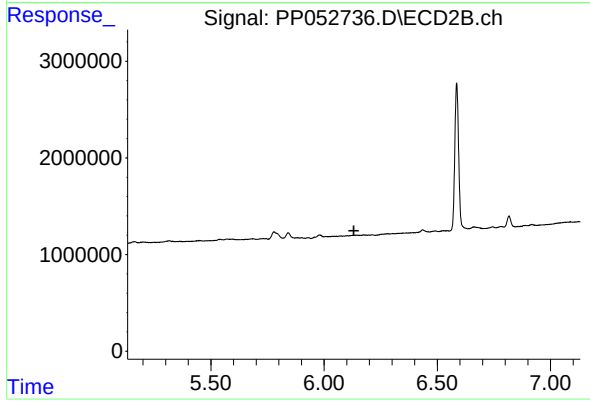

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.131 min
Response: 0
Conc: N.D.

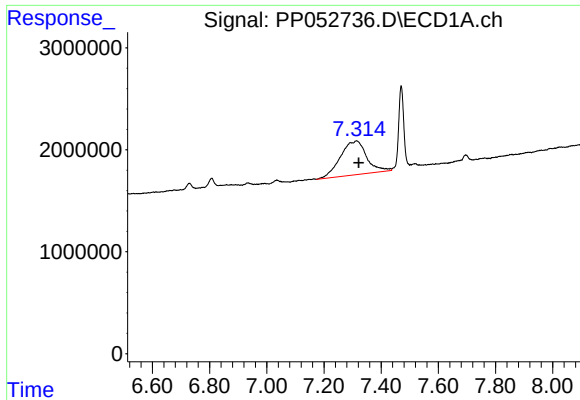

#29 AR-1254-4


R.T.: 7.314 min
Delta R.T.: -0.008 min
Response: 21245543
Conc: 301.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

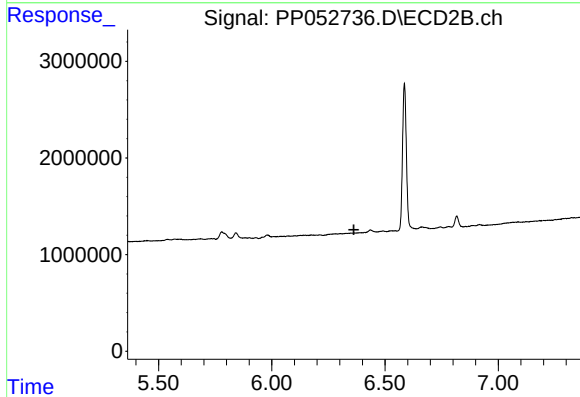


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

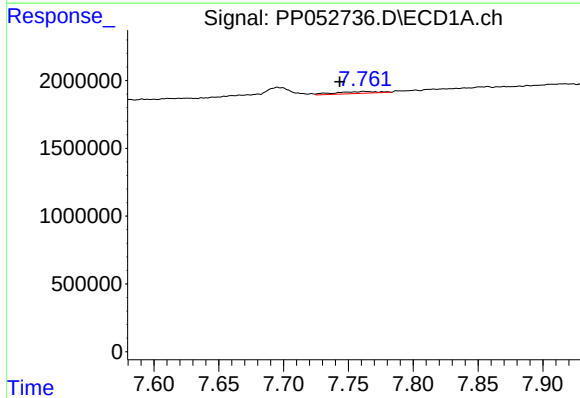


#30 AR-1254-5

R.T.: 7.763 min
Delta R.T.: 0.019 min
Response: 332687
Conc: 4.23 ng/ml

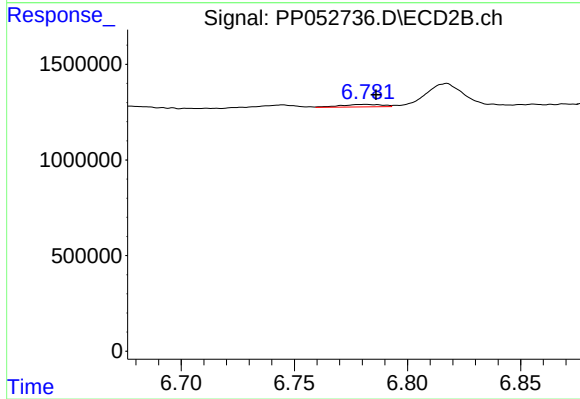

#30 AR-1254-5


R.T.: 6.782 min
Delta R.T.: -0.004 min
Response: 168318
Conc: 1.21 ng/ml

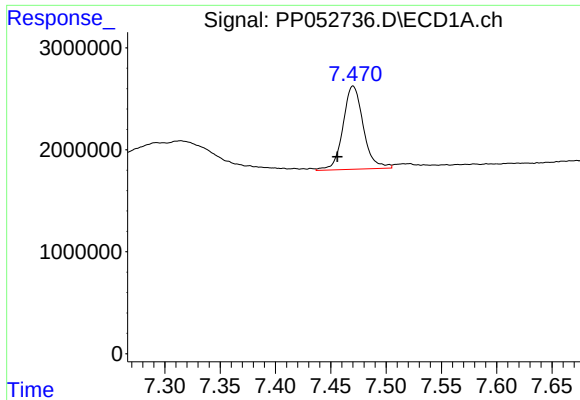

#32 AR-1260-2


R.T.: 7.470 min
Delta R.T.: 0.014 min
Response: 10432436
Conc: 111.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

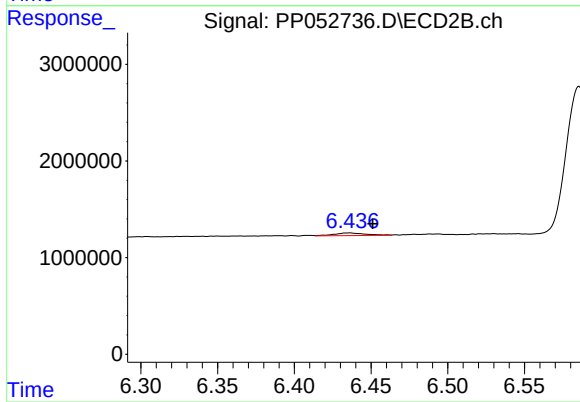


#32 AR-1260-2

R.T.: 6.436 min
Delta R.T.: -0.015 min
Response: 371849
Conc: 3.06 ng/ml

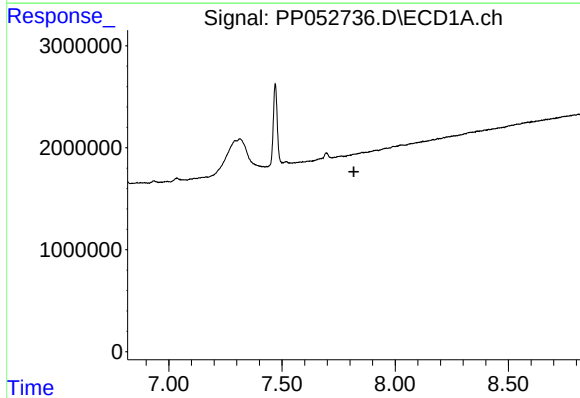


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.817 min
Response: 0
Conc: N.D.

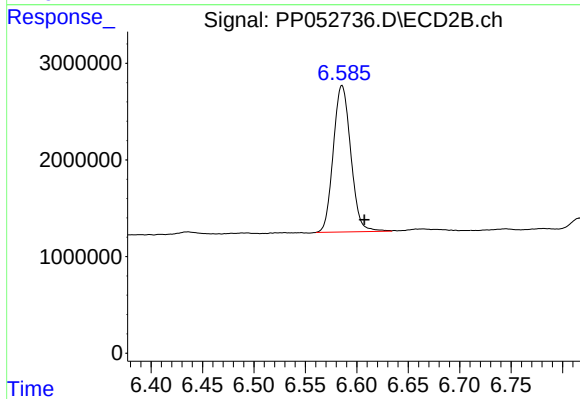

#33 AR-1260-3


R.T.: 6.586 min
Delta R.T.: -0.022 min
Response: 17958437
Conc: 153.96 ng/ml

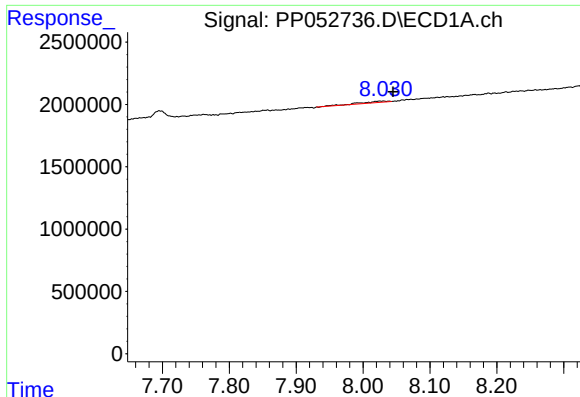

#34 AR-1260-4


R.T.: 8.028 min
Delta R.T.: -0.017 min
Response: 328598
Conc: 4.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

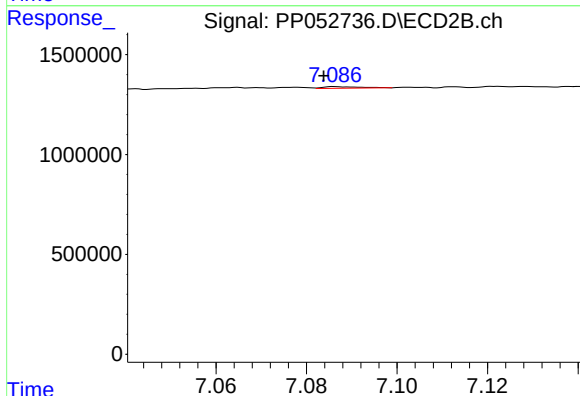


#34 AR-1260-4

R.T.: 7.086 min
Delta R.T.: 0.002 min
Response: 45201
Conc: 0.50 ng/ml

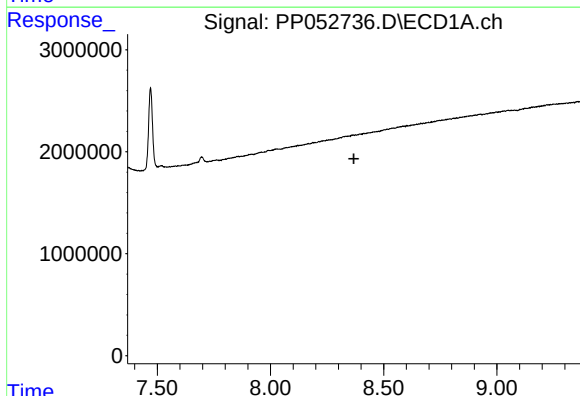


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.368 min
Response: 0
Conc: N.D.

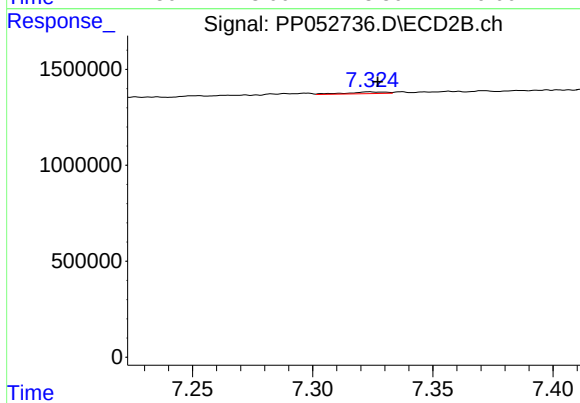

#35 AR-1260-5


R.T.: 7.324 min
Delta R.T.: -0.003 min
Response: 103268
Conc: 0.50 ng/ml

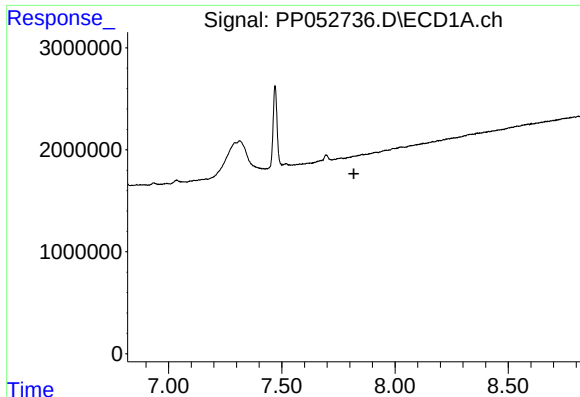

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.818 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

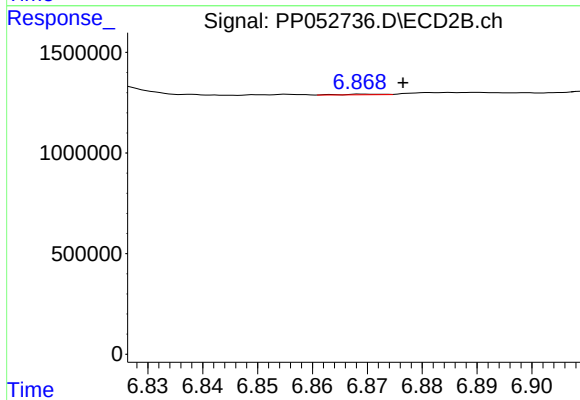


#36 AR-1262-1

R.T.: 6.869 min
Delta R.T.: -0.008 min
Response: 17477
Conc: 0.31 ng/ml

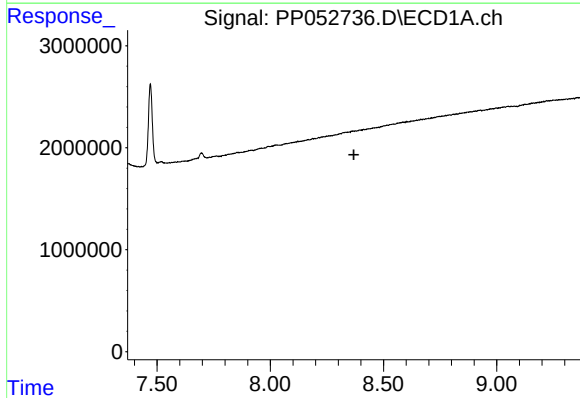


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.369 min
Response: 0
Conc: N.D.

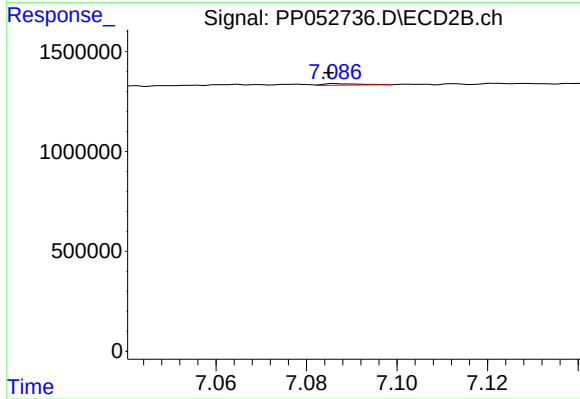

#37 AR-1262-2


R.T.: 7.086 min
Delta R.T.: 0.001 min
Response: 45201
Conc: 0.37 ng/ml

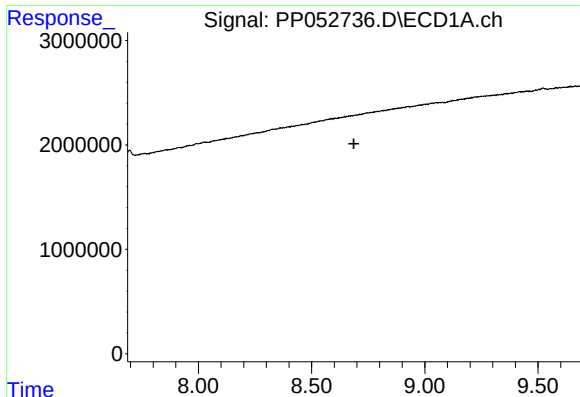

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.687 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

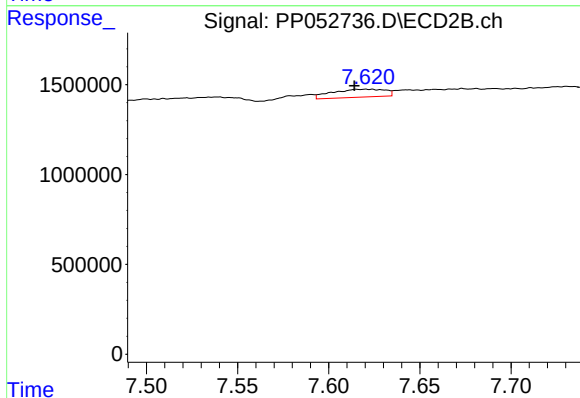


#38 AR-1262-3

R.T.: 7.620 min
Delta R.T.: 0.006 min
Response: 896089
Conc: 8.88 ng/ml

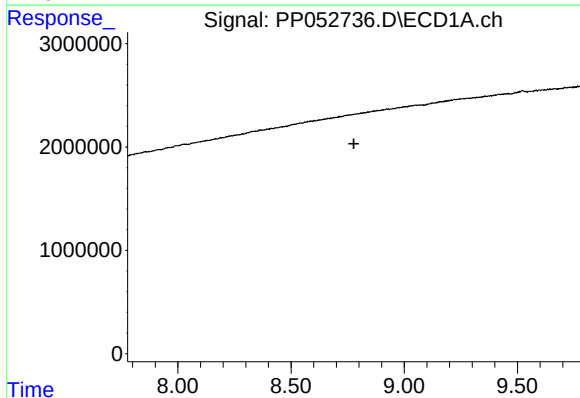


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.777 min
Response: 0
Conc: N.D.

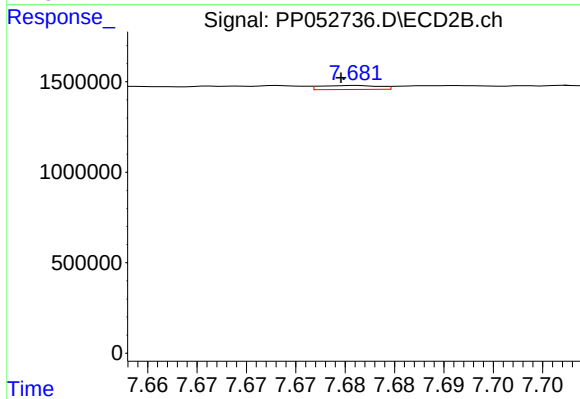

#39 AR-1262-4


R.T.: 7.681 min
Delta R.T.: 0.002 min
Response: 91935
Conc: 0.51 ng/ml

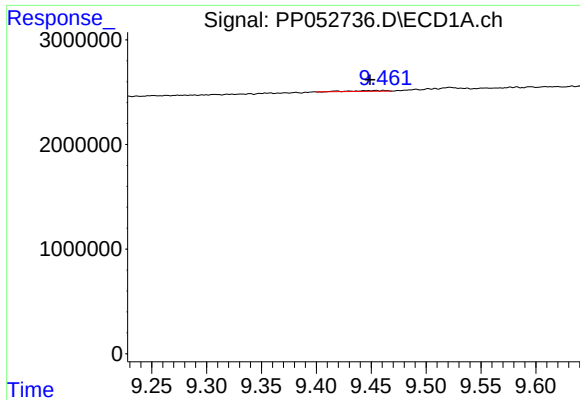

#40 AR-1262-5


R.T.: 9.461 min
Delta R.T.: 0.012 min
Response: 166408
Conc: 3.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

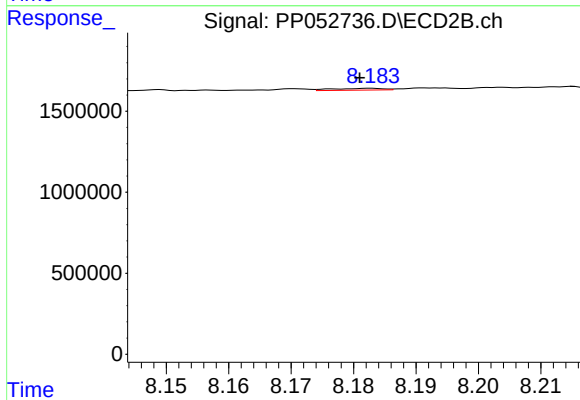


#40 AR-1262-5

R.T.: 8.183 min
Delta R.T.: 0.002 min
Response: 61690
Conc: 0.82 ng/ml

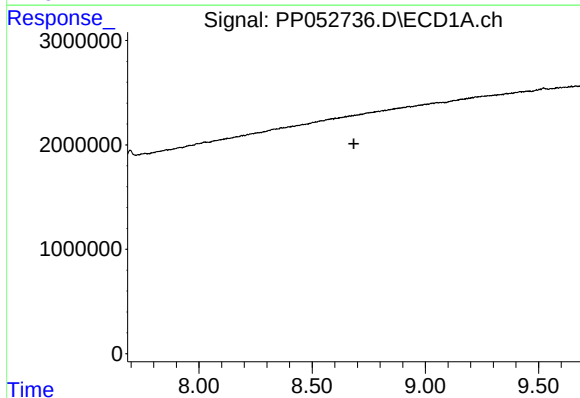


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.684 min
Response: 0
Conc: N.D.

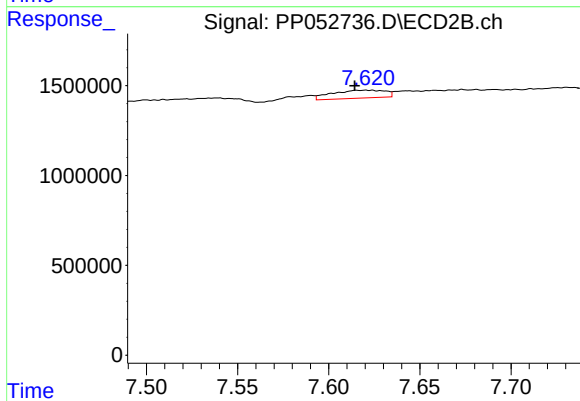

#41 AR-1268-1


R.T.: 7.620 min
Delta R.T.: 0.006 min
Response: 896089
Conc: 2.92 ng/ml

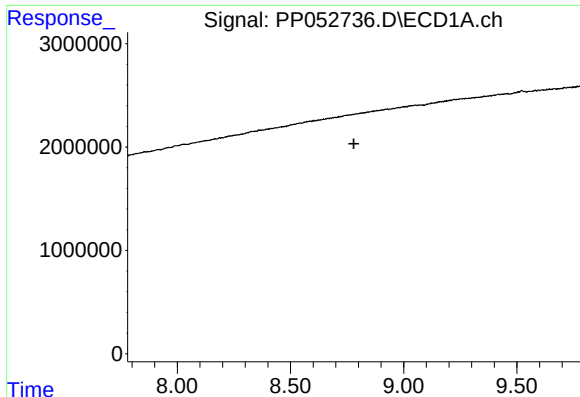

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

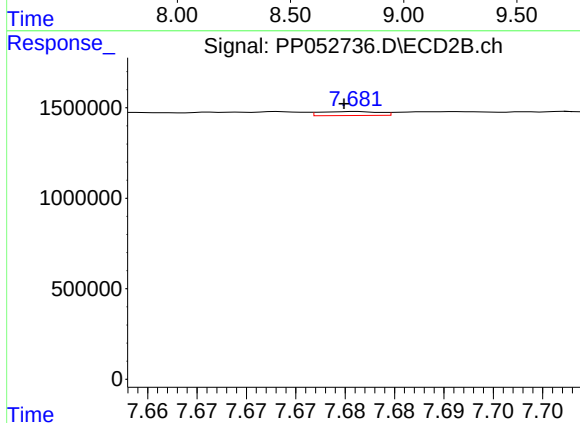


#42 AR-1268-2

R.T.: 7.681 min
Delta R.T.: 0.001 min
Response: 91935
Conc: 0.34 ng/ml

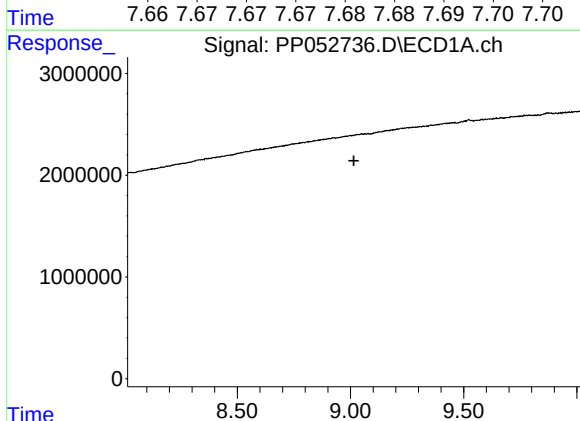


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.015 min
Response: 0
Conc: N.D.

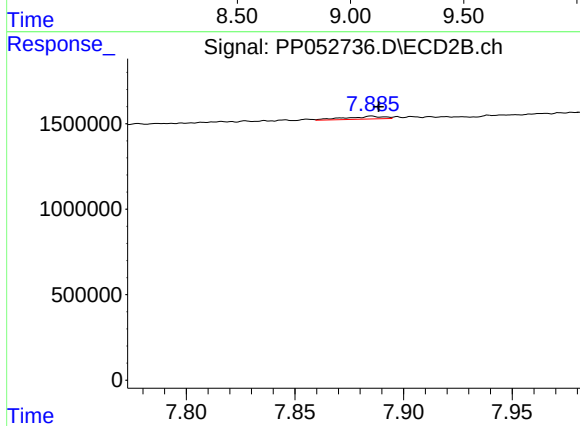

#43 AR-1268-3


R.T.: 7.885 min
Delta R.T.: -0.003 min
Response: 198361
Conc: 0.85 ng/ml

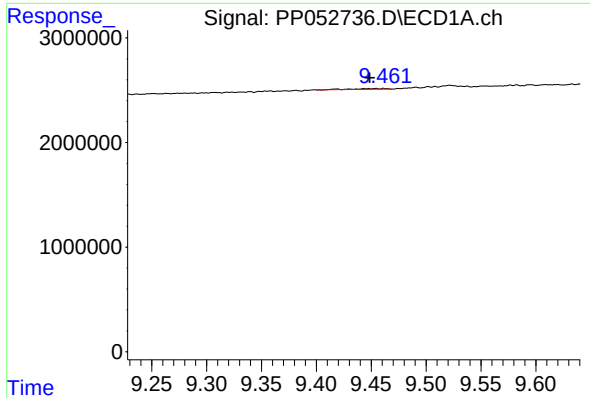

#44 AR-1268-4


R.T.: 9.461 min
Delta R.T.: 0.012 min
Response: 166408
Conc: 3.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
CONCRETE-72-11976

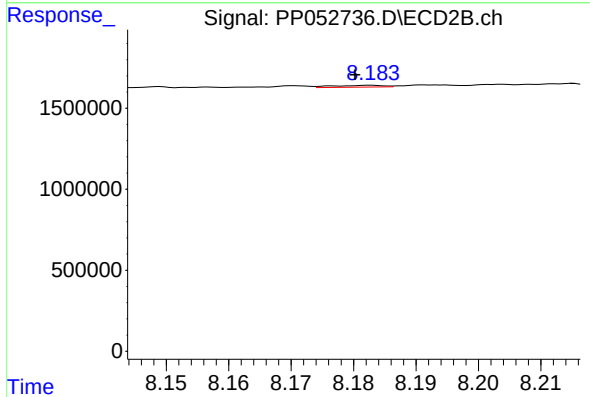


#44 AR-1268-4

R.T.: 8.183 min
Delta R.T.: 0.003 min
Response: 61690
Conc: 0.73 ng/ml

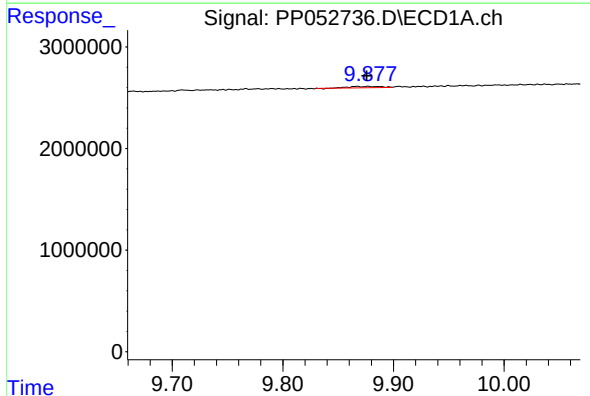

#45 AR-1268-5

R.T.: 9.877 min
Delta R.T.: 0.001 min
Response: 260209
Conc: 0.61 ng/ml

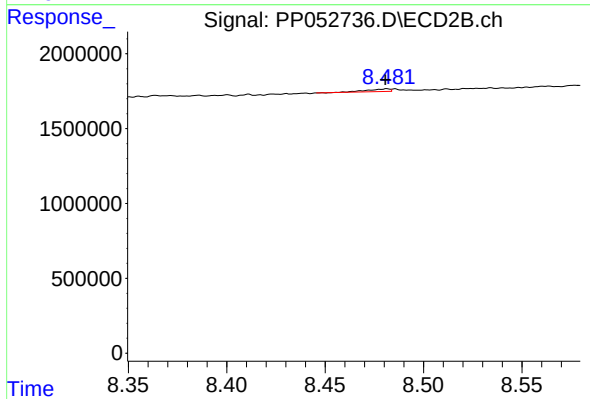

#45 AR-1268-5

R.T.: 8.482 min
Delta R.T.: 0.000 min
Response: 137069
Conc: 0.21 ng/ml