

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2022 15:19
 Operator : YP\AJ
 Sample : N5257-01MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HOLLAND-RD-COMP-1MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:16:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.408	3.652	40735299	33794270	18.435	17.983
2)	SA Decachlor...	10.217	8.741	17670927	22400203	13.922	13.356
Target Compounds							
3)	L1 AR-1016-1	5.583	4.754	31369751	32797487	467.898	498.260
4)	L1 AR-1016-2	5.605	4.773	46393411	45132072	464.472	491.615
5)	L1 AR-1016-3	5.668	4.952	28306670	24347637	465.105	500.773
6)	L1 AR-1016-4	5.767	4.994	22692049	19636017	468.586	504.010
7)	L1 AR-1016-5	6.064	5.211	21893172	24623639	454.547	490.062
8)	L2 AR-1221-1	4.615	3.868	4804947	3382256	187.389	144.084
9)	L2 AR-1221-2	4.704	3.956	4377360	5447104	230.111	311.163 #
10)	L2 AR-1221-3	4.781	4.033	19937539	18349933	349.775	338.059
11)	L3 AR-1232-1	4.781	4.033	19937539	18349933	459.484	440.099
12)	L3 AR-1232-2	5.314	4.773	24821660	45132072	1000.430	1088.660
13)	L3 AR-1232-3	5.605	4.952	46393411	24347637	1059.800	1101.689
14)	L3 AR-1232-4	5.767	5.037	22692049	23431478	1063.067	1140.087
15)	L3 AR-1232-5	5.859	5.211	19650256	24623639	1141.617	1060.607
16)	L4 AR-1242-1	5.583	4.754	31369751	32797487	557.380	587.690
17)	L4 AR-1242-2	5.605	4.773	46393411	45132072	561.612	585.163
18)	L4 AR-1242-3	5.668	4.952	28306670	24347637	556.588	593.439
19)	L4 AR-1242-4	5.767	5.037	22692049	23431478	560.165	552.460
20)	L4 AR-1242-5	6.509	5.569	3748336	20032432	94.019	396.300 #
21)	L5 AR-1248-1	5.583	4.754	31369751	32797487	772.335	819.441
22)	L5 AR-1248-2	5.859	4.994	19650256	19636017	330.150	346.797
23)	L5 AR-1248-3	6.064	5.037	21893172	23431478	337.240	399.091
24)	L5 AR-1248-4	0.000	5.211	0	24623639	N.D.	353.620 #
25)	L5 AR-1248-5	6.509	5.610	3748336	2747835	59.170	43.313 #
26)	L6 AR-1254-1	6.443	5.569	20142884	20032432	265.365	186.550 #
27)	L6 AR-1254-2	6.662	5.718	17878530	20233745	159.964	211.685 #
28)	L6 AR-1254-3	7.031	6.142	10366658	33978284	93.133	222.393 #
29)	L6 AR-1254-4	7.317	6.358	5964030	4706295	84.692	51.835 #
30)	L6 AR-1254-5	7.738	6.781	61501481	71625114	781.138	514.810 #
31)	L7 AR-1260-1	7.196	6.259	36336927	44819736	425.364	440.654
32)	L7 AR-1260-2	7.453	6.449	41322923	52115674	442.518	428.535
33)	L7 AR-1260-3	7.815	6.604	24671855	48931802	390.466	419.485
34)	L7 AR-1260-4	8.041	7.082	30609860	35354408	427.499	392.651
35)	L7 AR-1260-5	8.365	7.325	54150163	82084049	426.025	400.708
36)	L8 AR-1262-1	7.815	6.874	24671855	19251202	257.387	336.134 #
37)	L8 AR-1262-2	8.365	7.082	54150163	35354408	364.021	285.501
38)	L8 AR-1262-3	8.695	7.612	33896625	15723090	341.612	155.799 #
39)	L8 AR-1262-4	8.752f	7.675	18302323	57263135	392.837	320.043
40)	L8 AR-1262-5	9.444	8.177	11049604	16243571	241.459	216.900
41)	L9 AR-1268-1	8.695	7.612	33896625	15723090	180.216	51.292 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2022 15:19
 Operator : YP\AJ
 Sample : N5257-01MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HOLLAND-RD-COMP-1MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:16:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.752f	7.675	18302323	57263135	111.827	211.126 #
43) L9	AR-1268-3	9.012	7.886	945516	1596725	6.240	6.811
44) L9	AR-1268-4	9.444	8.177	11049604	16243571	217.269	191.228
45) L9	AR-1268-5	9.869	8.477	3667910	5038487	8.538	7.684



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2022 15:19
Operator : YP\AJ
Sample : N5257-01MSD
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:16:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

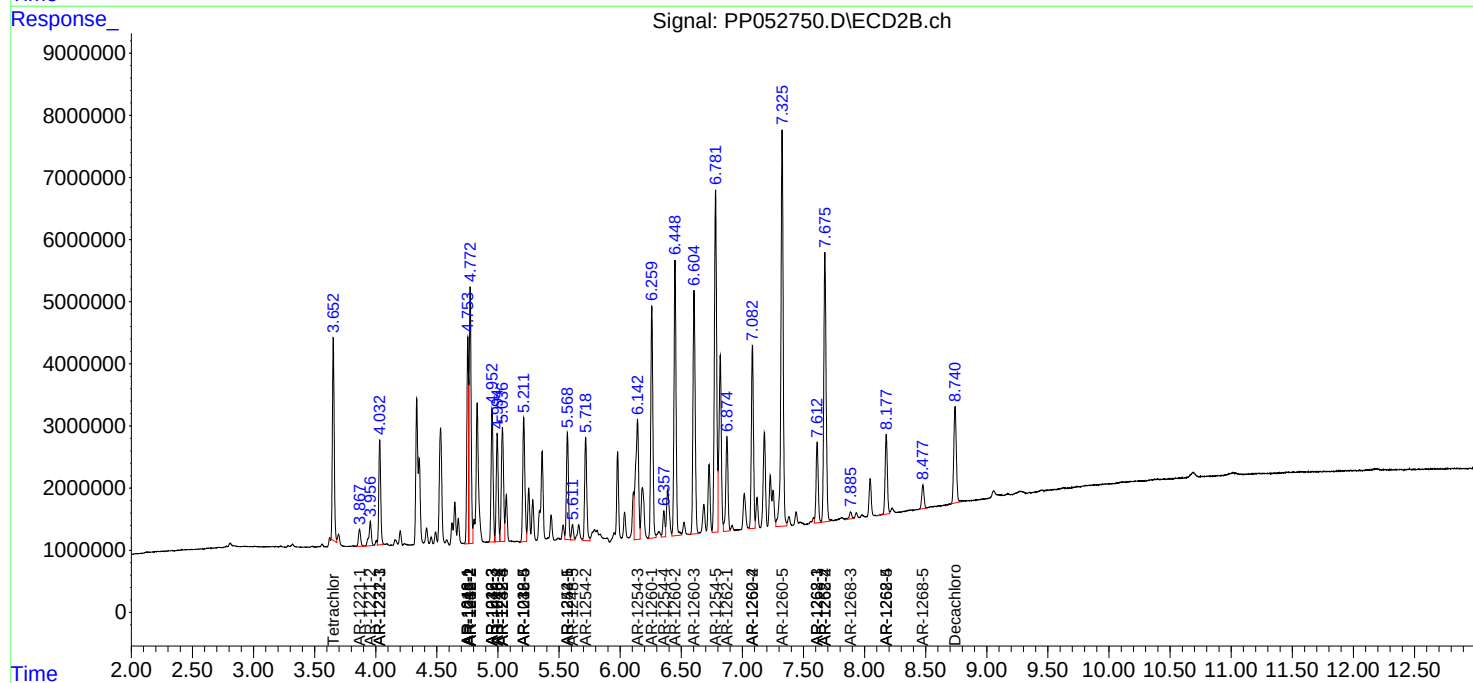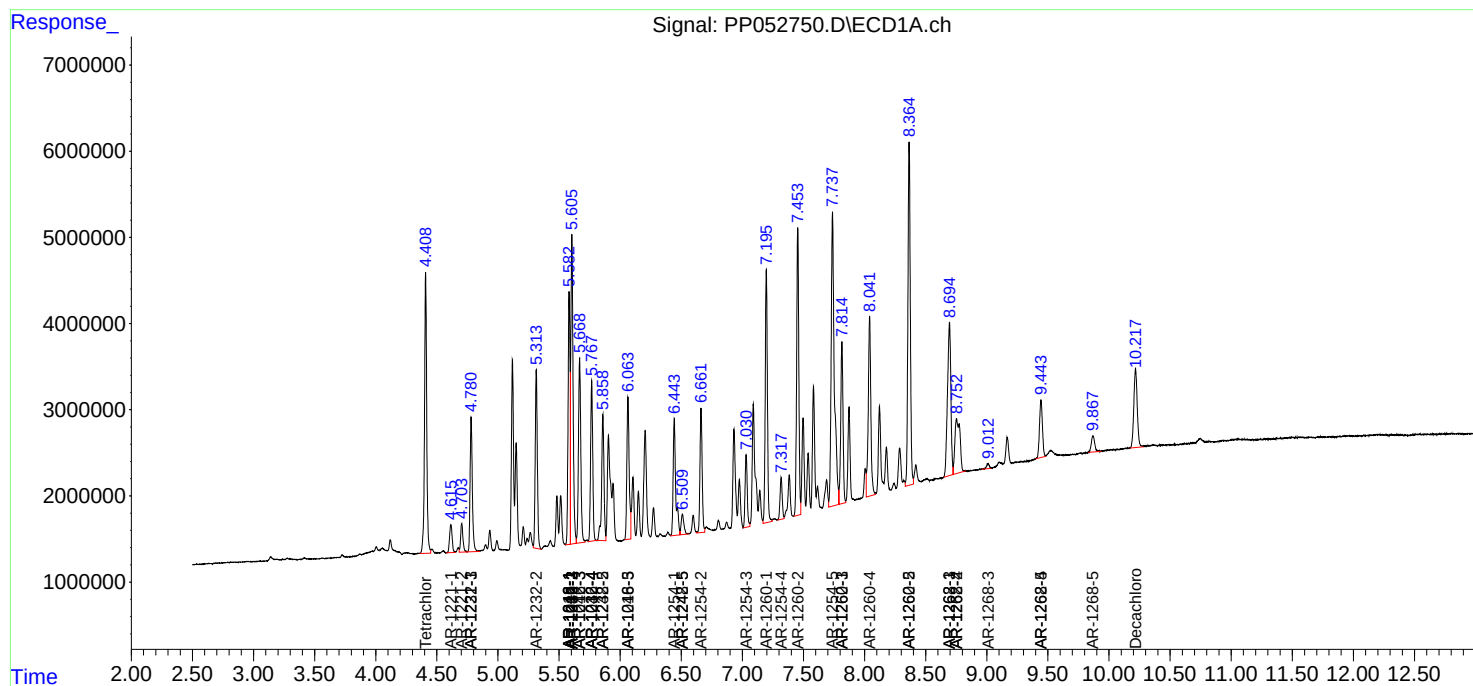


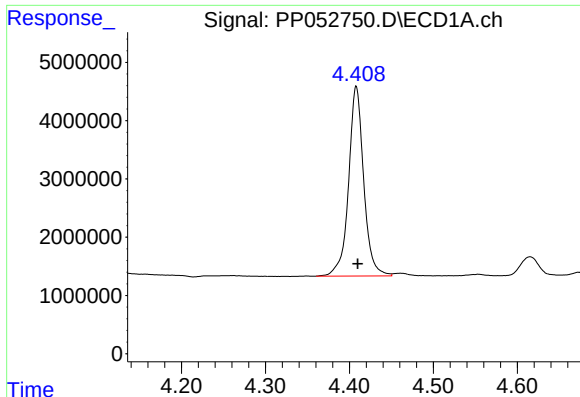

#1 Tetrachloro-m-xylene


R.T.: 4.408 min
Delta R.T.: -0.002 min
Response: 40735299
Conc: 18.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

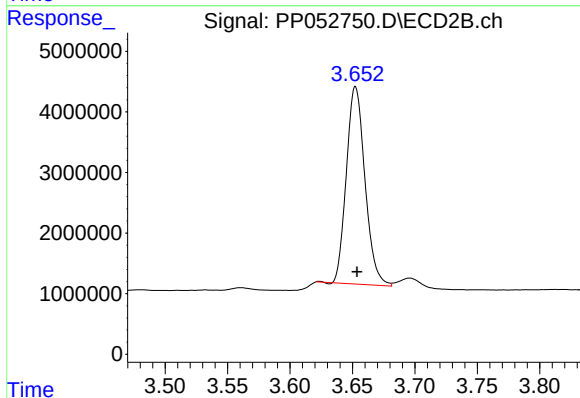


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.001 min
Response: 33794270
Conc: 17.98 ng/ml

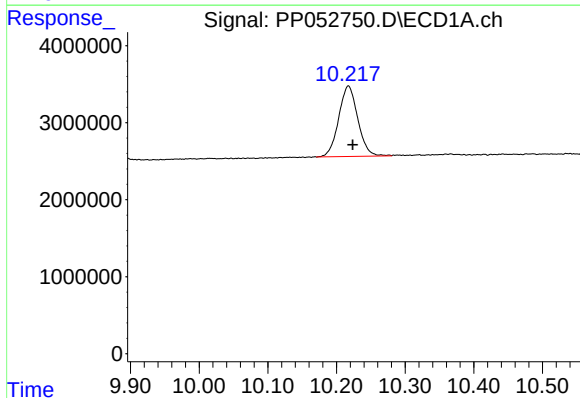


#2 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.006 min
Response: 17670927
Conc: 13.92 ng/ml

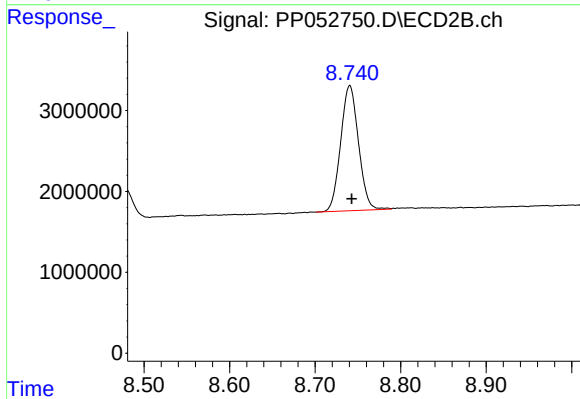

#2 Decachlorobiphenyl


R.T.: 8.741 min
Delta R.T.: -0.002 min
Response: 22400203
Conc: 13.36 ng/ml

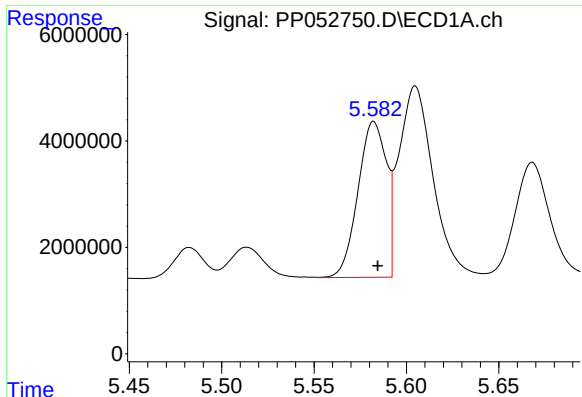

#3 AR-1016-1


R.T.: 5.583 min
Delta R.T.: -0.002 min
Response: 31369751
Conc: 467.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

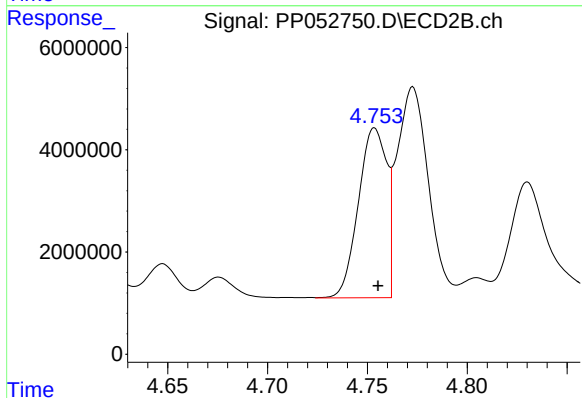


#3 AR-1016-1

R.T.: 4.754 min
Delta R.T.: -0.002 min
Response: 32797487
Conc: 498.26 ng/ml

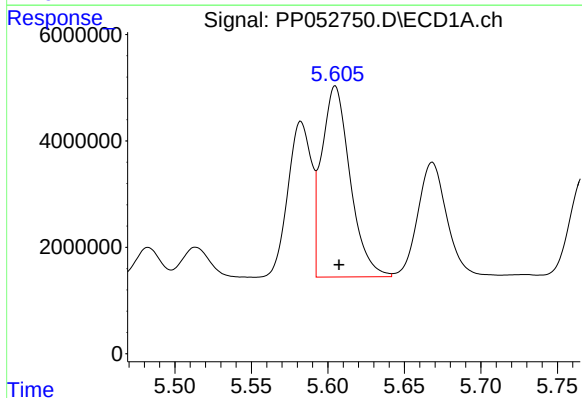


#4 AR-1016-2

R.T.: 5.605 min
Delta R.T.: -0.003 min
Response: 46393411
Conc: 464.47 ng/ml

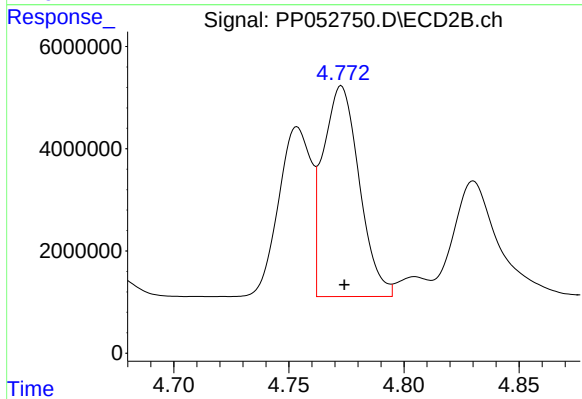

#4 AR-1016-2


R.T.: 4.773 min
Delta R.T.: -0.001 min
Response: 45132072
Conc: 491.62 ng/ml

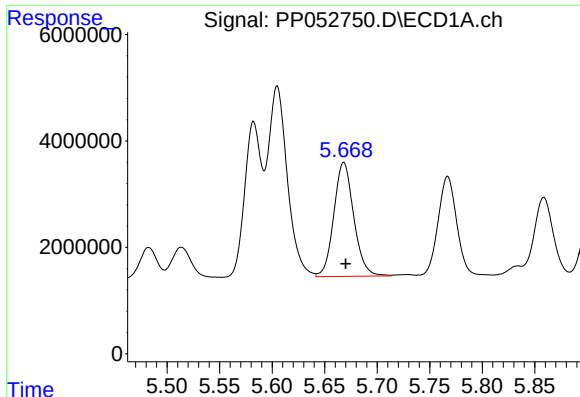

#5 AR-1016-3


R.T.: 5.668 min
Delta R.T.: -0.002 min
Response: 28306670
Conc: 465.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

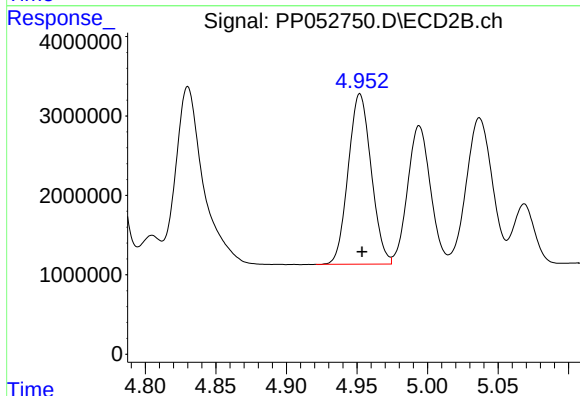


#5 AR-1016-3

R.T.: 4.952 min
Delta R.T.: -0.002 min
Response: 24347637
Conc: 500.77 ng/ml

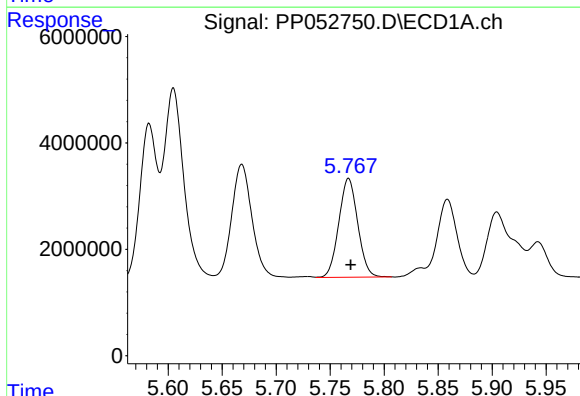


#6 AR-1016-4

R.T.: 5.767 min
Delta R.T.: -0.002 min
Response: 22692049
Conc: 468.59 ng/ml

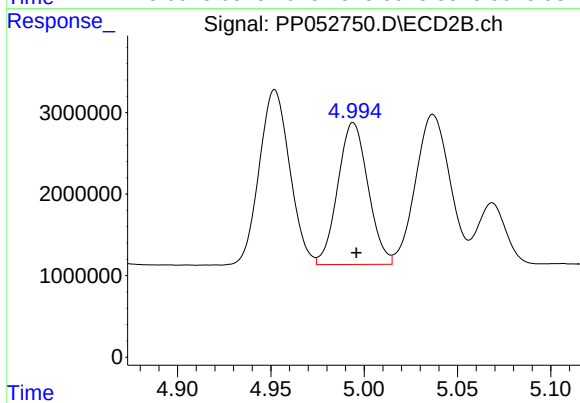

#6 AR-1016-4


R.T.: 4.994 min
Delta R.T.: -0.002 min
Response: 19636017
Conc: 504.01 ng/ml

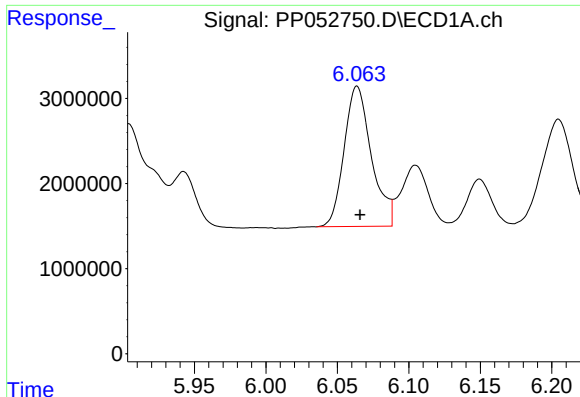

#7 AR-1016-5


R.T.: 6.064 min
Delta R.T.: -0.002 min
Response: 21893172
Conc: 454.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

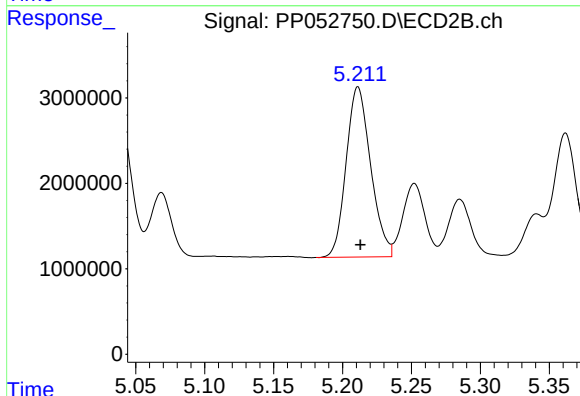


#7 AR-1016-5

R.T.: 5.211 min
Delta R.T.: -0.002 min
Response: 24623639
Conc: 490.06 ng/ml

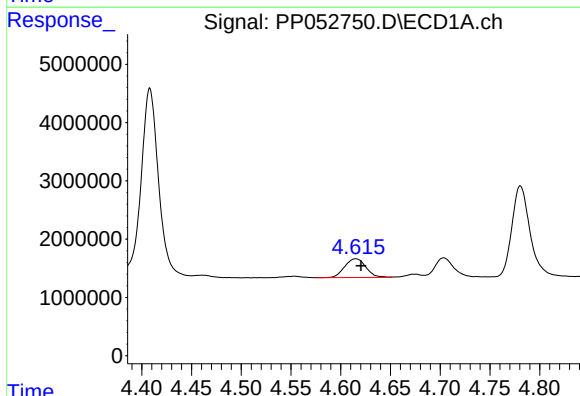


#8 AR-1221-1

R.T.: 4.615 min
Delta R.T.: -0.005 min
Response: 4804947
Conc: 187.39 ng/ml

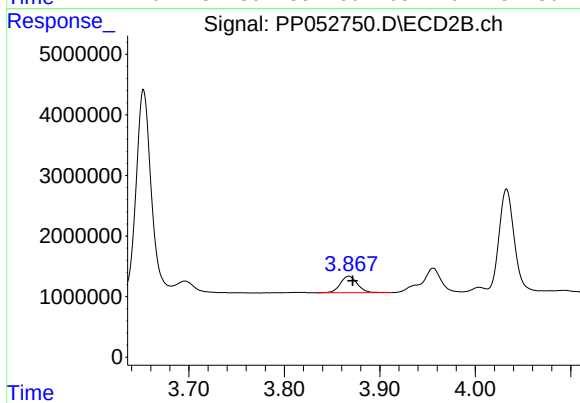

#8 AR-1221-1


R.T.: 3.868 min
Delta R.T.: -0.004 min
Response: 3382256
Conc: 144.08 ng/ml

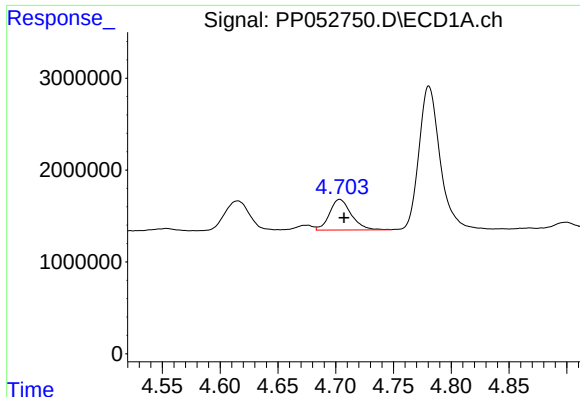

#9 AR-1221-2


R.T.: 4.704 min
Delta R.T.: -0.004 min
Response: 4377360
Conc: 230.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

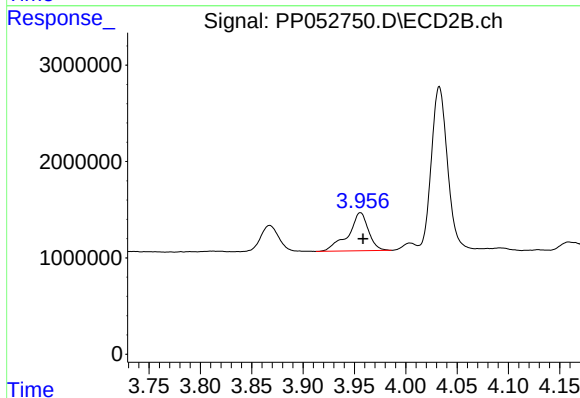


#9 AR-1221-2

R.T.: 3.956 min
Delta R.T.: -0.003 min
Response: 5447104
Conc: 311.16 ng/ml

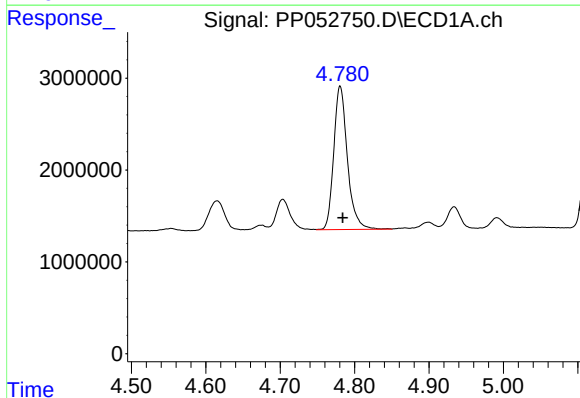


#10 AR-1221-3

R.T.: 4.781 min
Delta R.T.: -0.003 min
Response: 19937539
Conc: 349.78 ng/ml

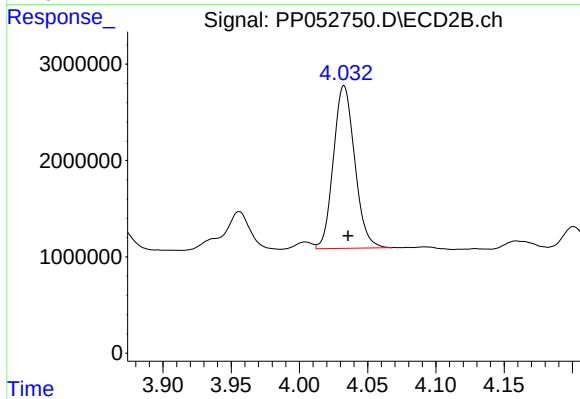

#10 AR-1221-3


R.T.: 4.033 min
Delta R.T.: -0.003 min
Response: 18349933
Conc: 338.06 ng/ml

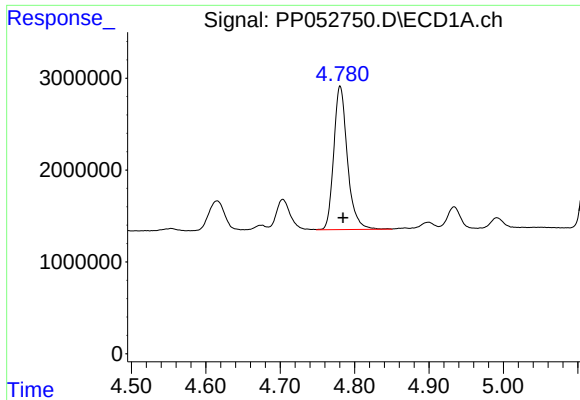

#11 AR-1232-1


R.T.: 4.781 min
Delta R.T.: -0.004 min
Response: 19937539
Conc: 459.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

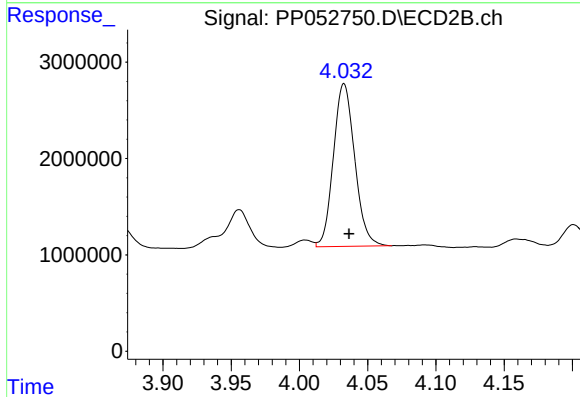


#11 AR-1232-1

R.T.: 4.033 min
Delta R.T.: -0.004 min
Response: 18349933
Conc: 440.10 ng/ml

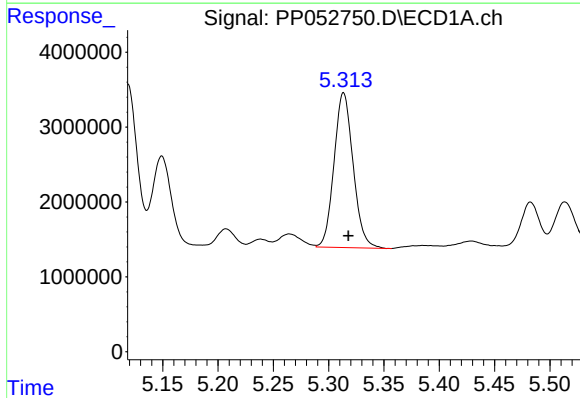


#12 AR-1232-2

R.T.: 5.314 min
Delta R.T.: -0.004 min
Response: 24821660
Conc: 1000.43 ng/ml

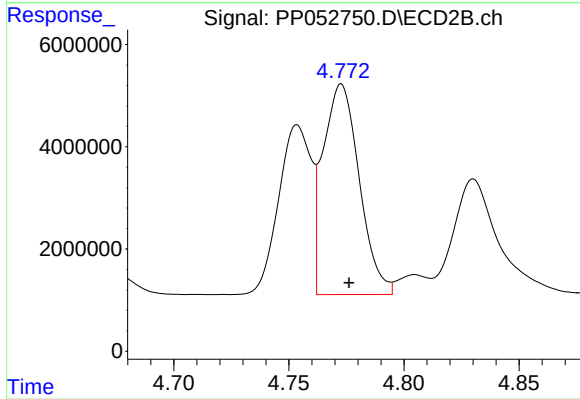

#12 AR-1232-2


R.T.: 4.773 min
Delta R.T.: -0.003 min
Response: 45132072
Conc: 1088.66 ng/ml

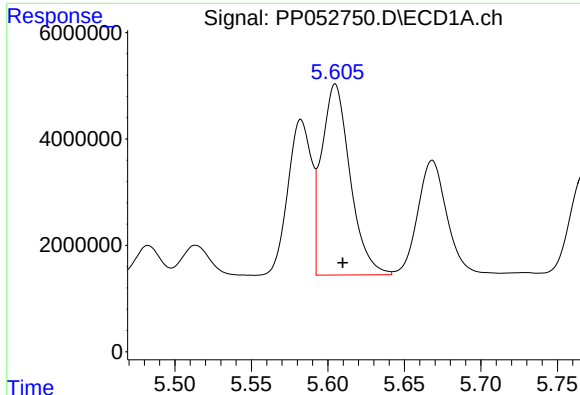

#13 AR-1232-3


R.T.: 5.605 min
Delta R.T.: -0.005 min
Response: 46393411
Conc: 1059.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

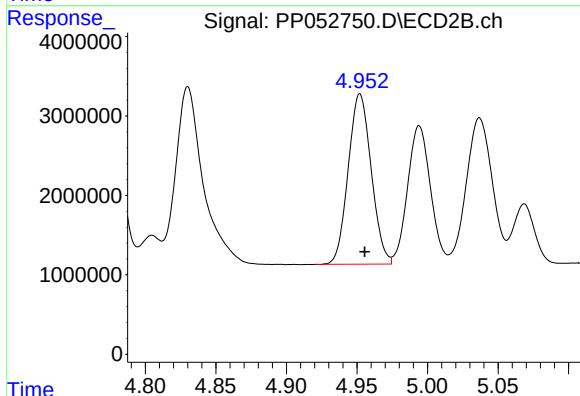


#13 AR-1232-3

R.T.: 4.952 min
Delta R.T.: -0.003 min
Response: 24347637
Conc: 1101.69 ng/ml

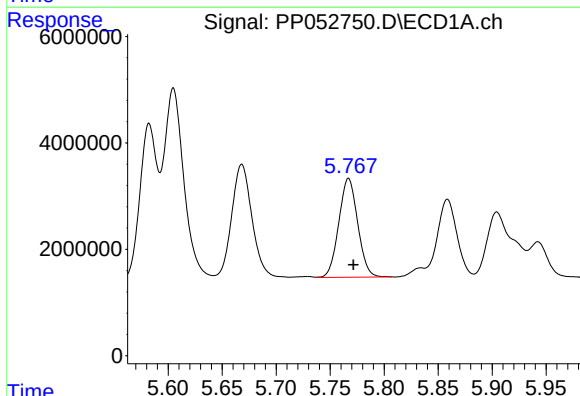


#14 AR-1232-4

R.T.: 5.767 min
Delta R.T.: -0.004 min
Response: 22692049
Conc: 1063.07 ng/ml

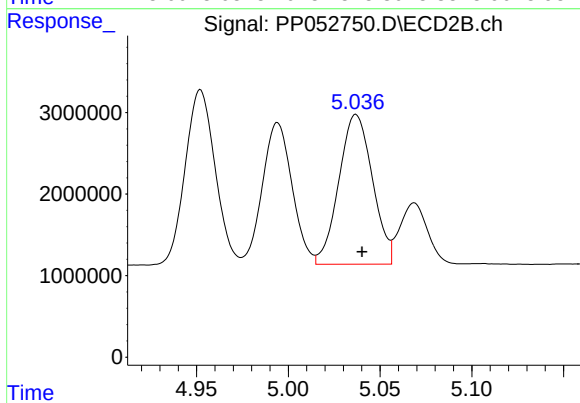

#14 AR-1232-4


R.T.: 5.037 min
Delta R.T.: -0.003 min
Response: 23431478
Conc: 1140.09 ng/ml

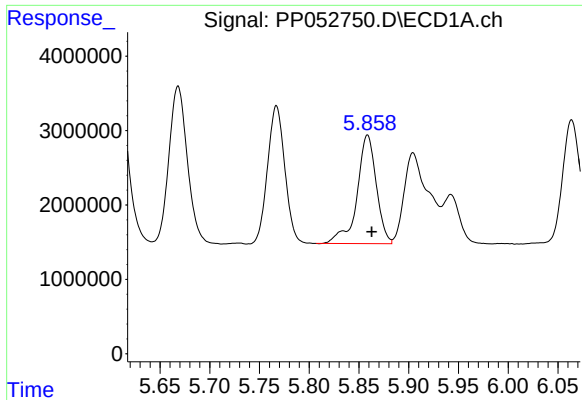

#15 AR-1232-5


R.T.: 5.859 min
Delta R.T.: -0.004 min
Response: 19650256
Conc: 1141.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

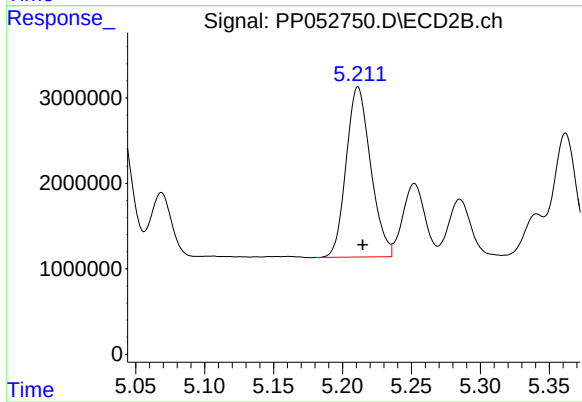


#15 AR-1232-5

R.T.: 5.211 min
Delta R.T.: -0.004 min
Response: 24623639
Conc: 1060.61 ng/ml

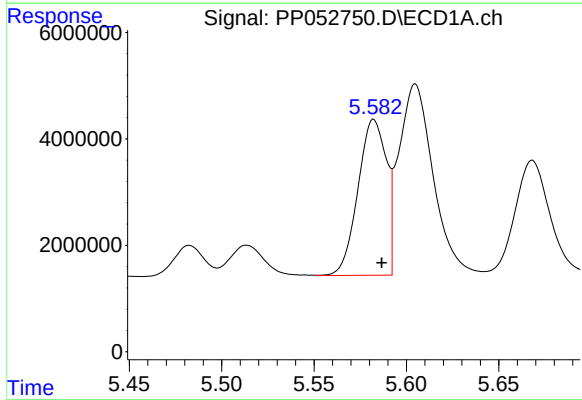


#16 AR-1242-1

R.T.: 5.583 min
Delta R.T.: -0.004 min
Response: 31369751
Conc: 557.38 ng/ml

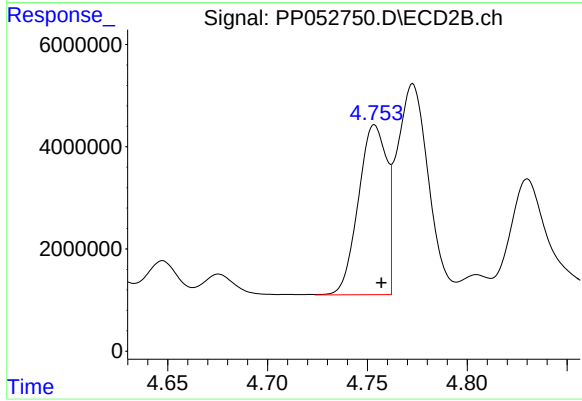

#16 AR-1242-1


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 32797487
Conc: 587.69 ng/ml

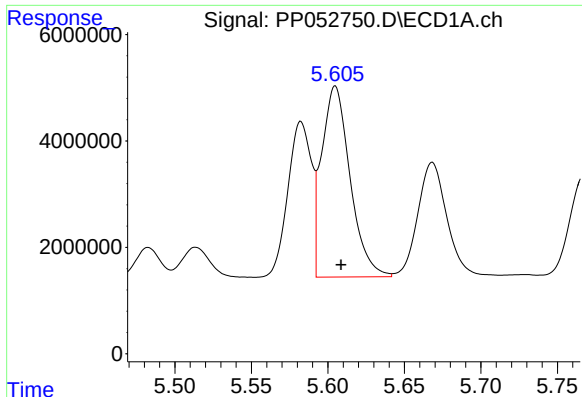

#17 AR-1242-2


R.T.: 5.605 min
Delta R.T.: -0.004 min
Response: 46393411
Conc: 561.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

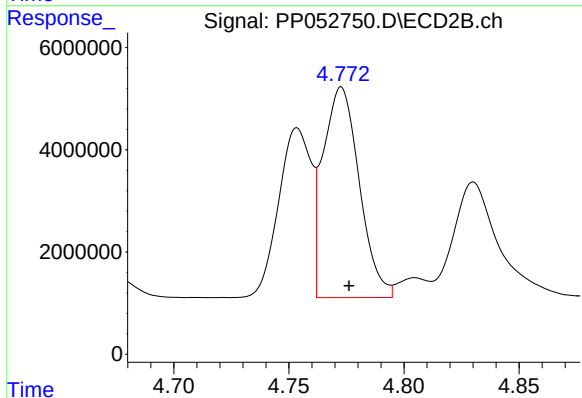


#17 AR-1242-2

R.T.: 4.773 min
Delta R.T.: -0.003 min
Response: 45132072
Conc: 585.16 ng/ml

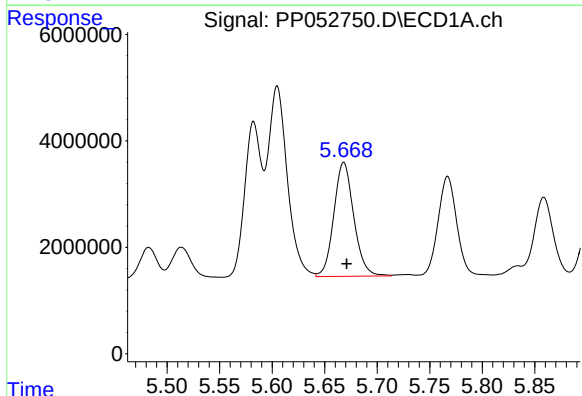


#18 AR-1242-3

R.T.: 5.668 min
Delta R.T.: -0.003 min
Response: 28306670
Conc: 556.59 ng/ml

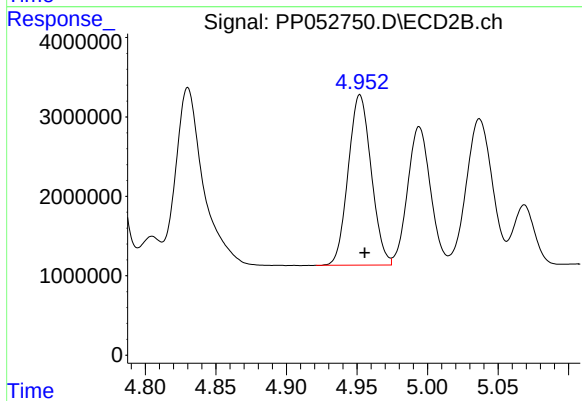

#18 AR-1242-3


R.T.: 4.952 min
Delta R.T.: -0.003 min
Response: 24347637
Conc: 593.44 ng/ml

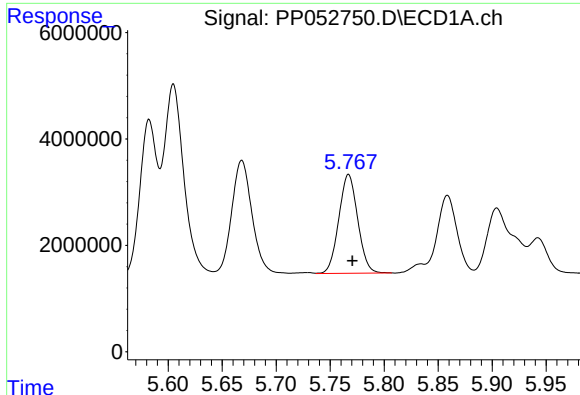

#19 AR-1242-4


R.T.: 5.767 min
Delta R.T.: -0.004 min
Response: 22692049
Conc: 560.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

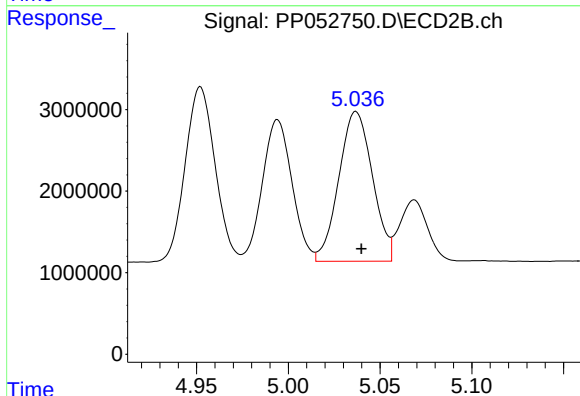


#19 AR-1242-4

R.T.: 5.037 min
Delta R.T.: -0.003 min
Response: 23431478
Conc: 552.46 ng/ml

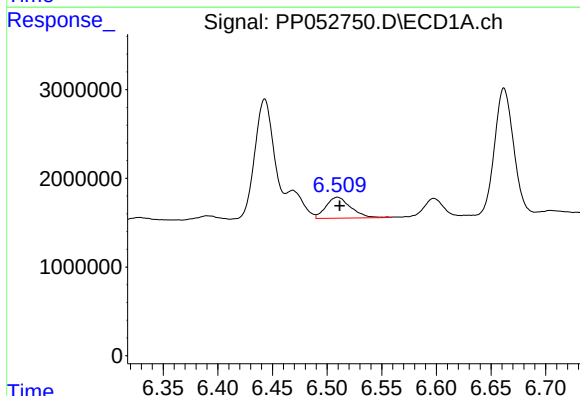


#20 AR-1242-5

R.T.: 6.509 min
Delta R.T.: -0.002 min
Response: 3748336
Conc: 94.02 ng/ml

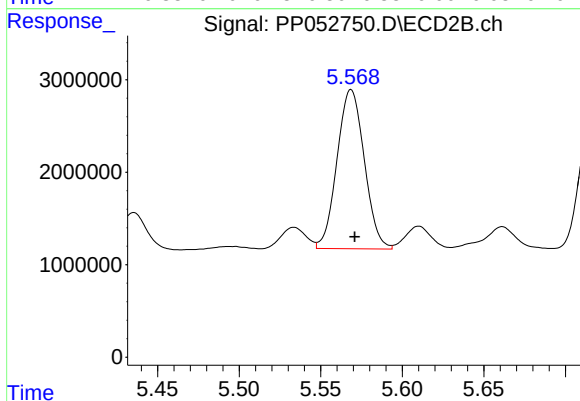

#20 AR-1242-5


R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 20032432
Conc: 396.30 ng/ml

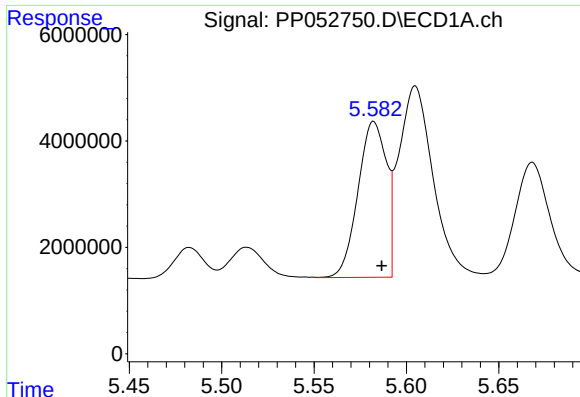

#21 AR-1248-1


R.T.: 5.583 min
Delta R.T.: -0.004 min
Response: 31369751
Conc: 772.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

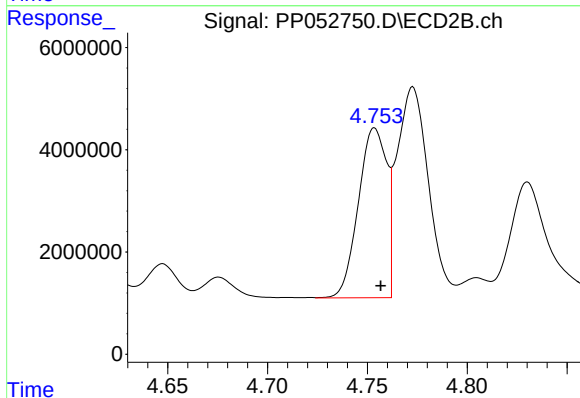


#21 AR-1248-1

R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 32797487
Conc: 819.44 ng/ml

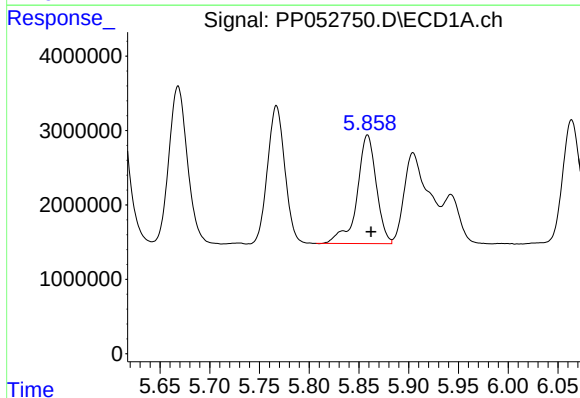


#22 AR-1248-2

R.T.: 5.859 min
Delta R.T.: -0.004 min
Response: 19650256
Conc: 330.15 ng/ml

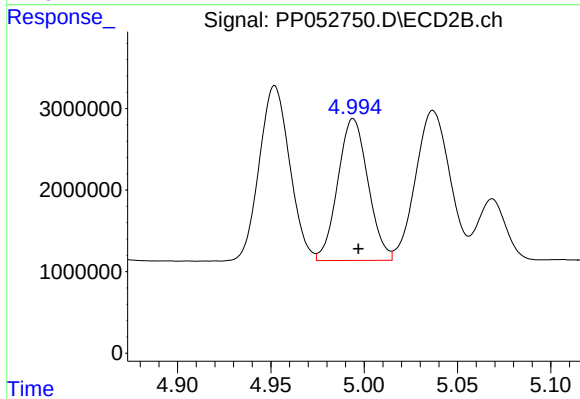

#22 AR-1248-2


R.T.: 4.994 min
Delta R.T.: -0.003 min
Response: 19636017
Conc: 346.80 ng/ml

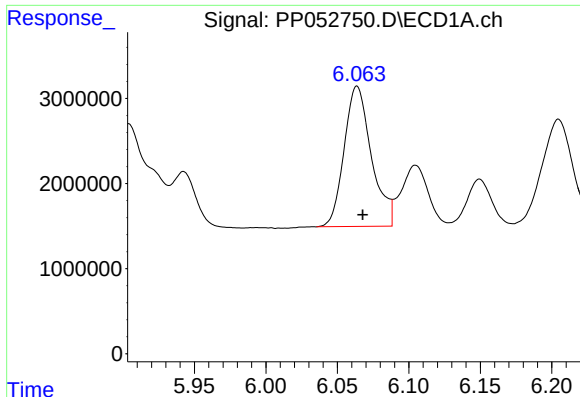

#23 AR-1248-3


R.T.: 6.064 min
Delta R.T.: -0.004 min
Response: 21893172
Conc: 337.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

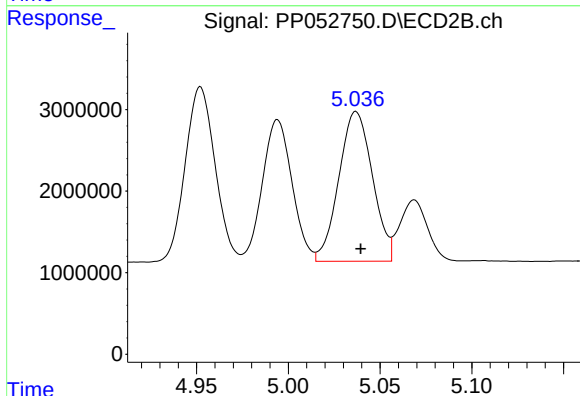


#23 AR-1248-3

R.T.: 5.037 min
Delta R.T.: -0.003 min
Response: 23431478
Conc: 399.09 ng/ml

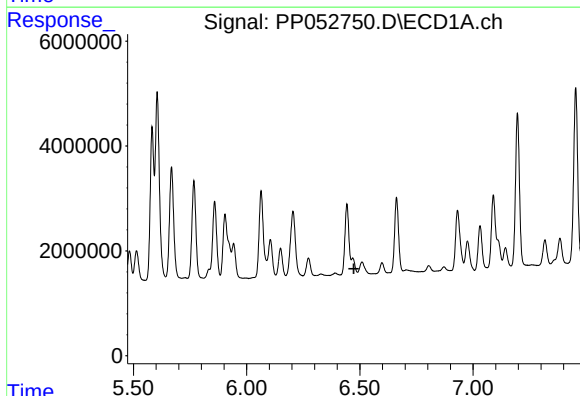


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.473 min
Response: 0
Conc: N.D.

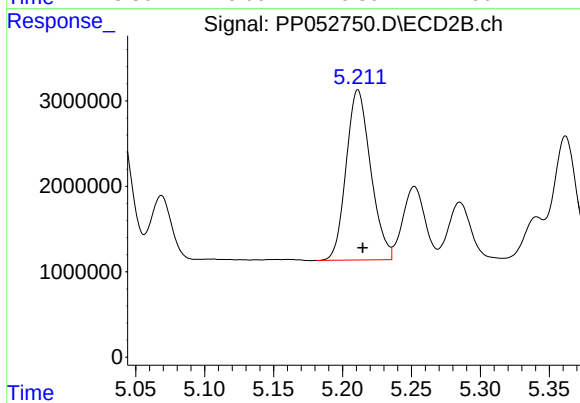

#24 AR-1248-4


R.T.: 5.211 min
Delta R.T.: -0.003 min
Response: 24623639
Conc: 353.62 ng/ml

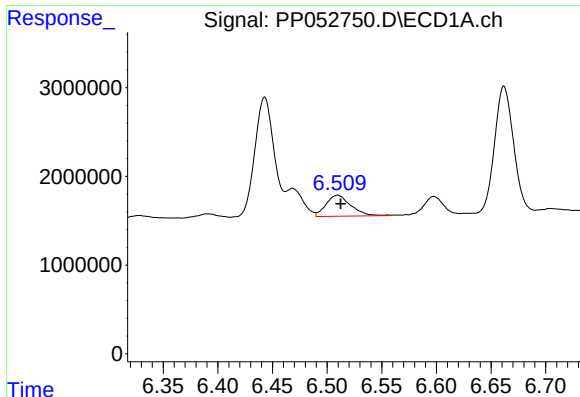

#25 AR-1248-5


R.T.: 6.509 min
Delta R.T.: -0.003 min
Response: 3748336
Conc: 59.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

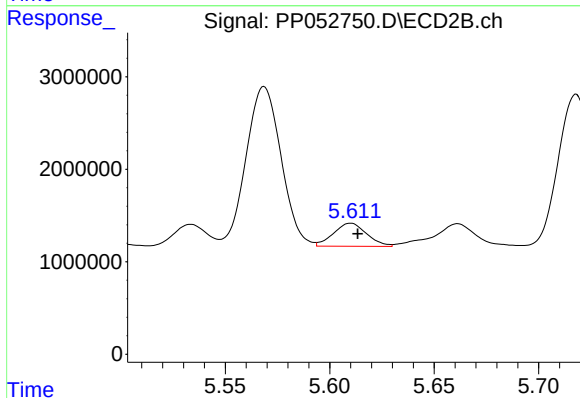


#25 AR-1248-5

R.T.: 5.610 min
Delta R.T.: -0.003 min
Response: 2747835
Conc: 43.31 ng/ml

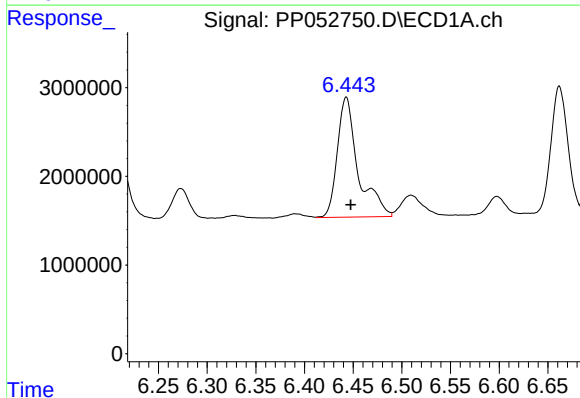


#26 AR-1254-1

R.T.: 6.443 min
Delta R.T.: -0.005 min
Response: 20142884
Conc: 265.36 ng/ml

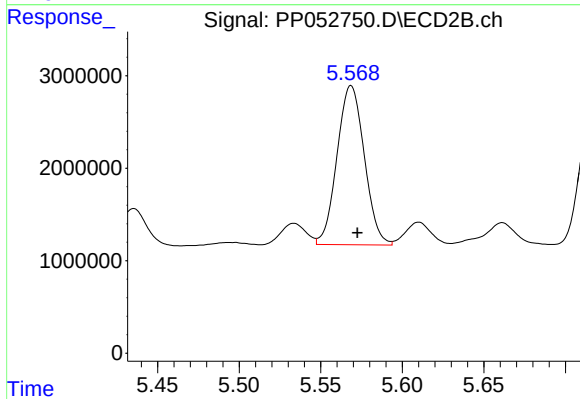

#26 AR-1254-1


R.T.: 5.569 min
Delta R.T.: -0.004 min
Response: 20032432
Conc: 186.55 ng/ml

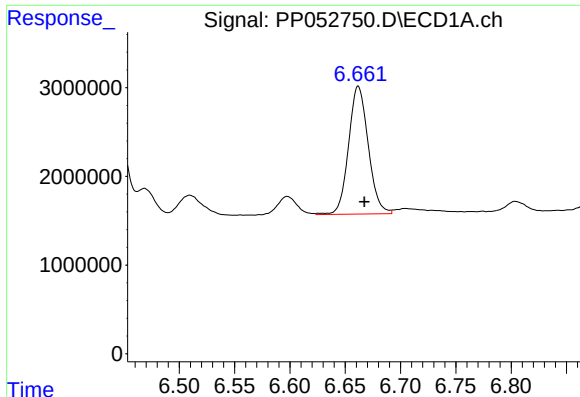

#27 AR-1254-2


R.T.: 6.662 min
Delta R.T.: -0.005 min
Response: 17878530
Conc: 159.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

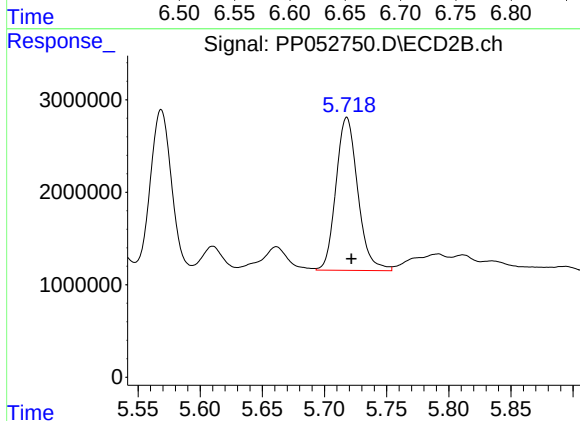


#27 AR-1254-2

R.T.: 5.718 min
Delta R.T.: -0.004 min
Response: 20233745
Conc: 211.69 ng/ml

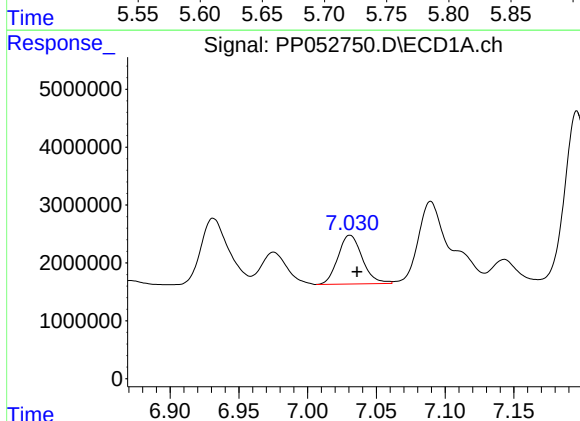


#28 AR-1254-3

R.T.: 7.031 min
Delta R.T.: -0.005 min
Response: 10366658
Conc: 93.13 ng/ml

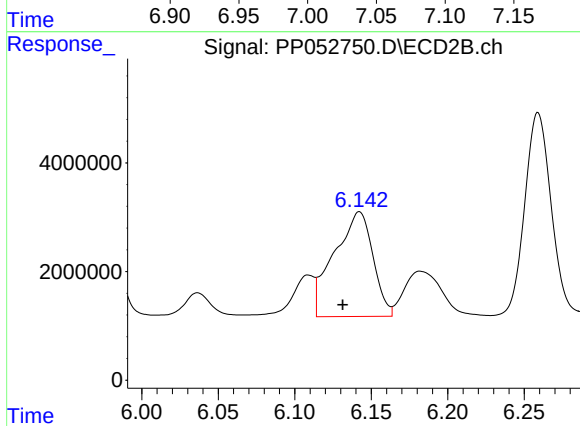

#28 AR-1254-3


R.T.: 6.142 min
Delta R.T.: 0.011 min
Response: 33978284
Conc: 222.39 ng/ml

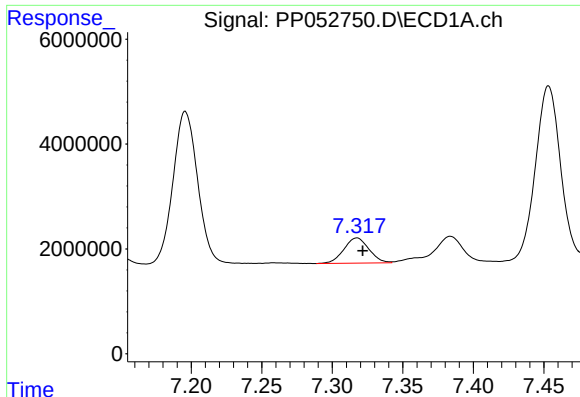

#29 AR-1254-4


R.T.: 7.317 min
Delta R.T.: -0.004 min
Response: 5964030
Conc: 84.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

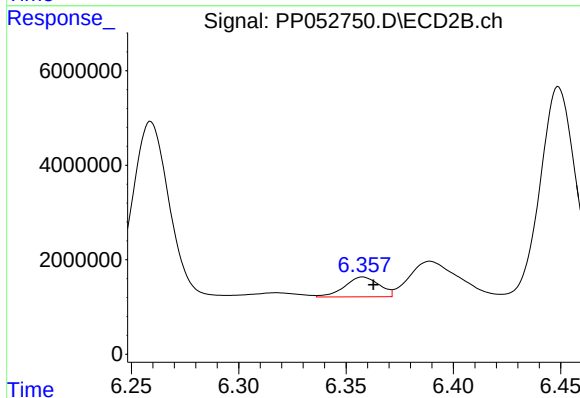


#29 AR-1254-4

R.T.: 6.358 min
Delta R.T.: -0.005 min
Response: 4706295
Conc: 51.83 ng/ml

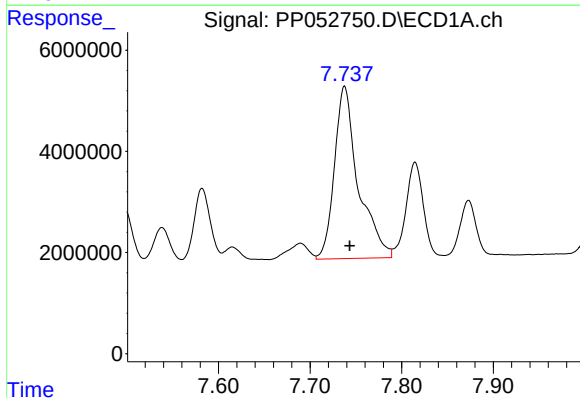


#30 AR-1254-5

R.T.: 7.738 min
Delta R.T.: -0.006 min
Response: 61501481
Conc: 781.14 ng/ml

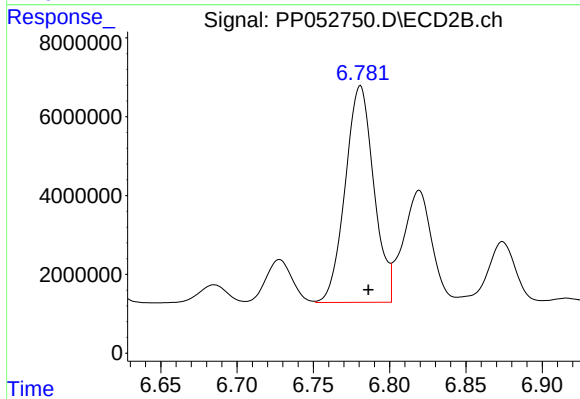

#30 AR-1254-5


R.T.: 6.781 min
Delta R.T.: -0.005 min
Response: 71625114
Conc: 514.81 ng/ml

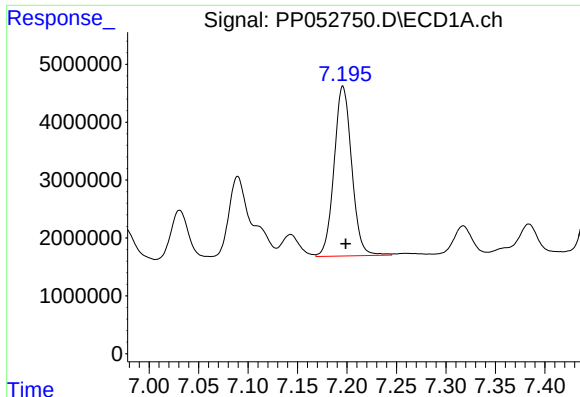

#31 AR-1260-1


R.T.: 7.196 min
Delta R.T.: -0.003 min
Response: 36336927
Conc: 425.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

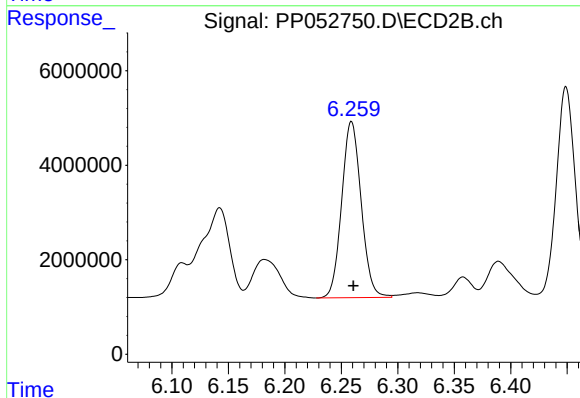


#31 AR-1260-1

R.T.: 6.259 min
Delta R.T.: -0.002 min
Response: 44819736
Conc: 440.65 ng/ml

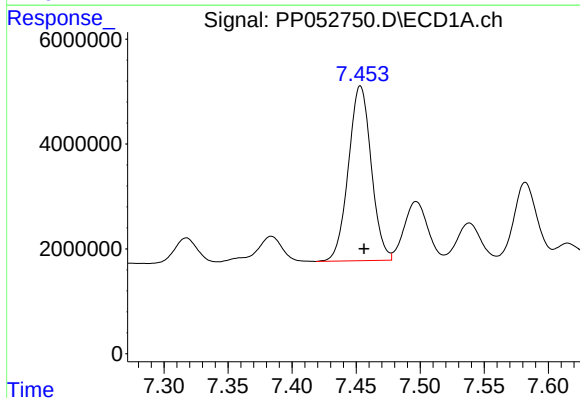


#32 AR-1260-2

R.T.: 7.453 min
Delta R.T.: -0.003 min
Response: 41322923
Conc: 442.52 ng/ml

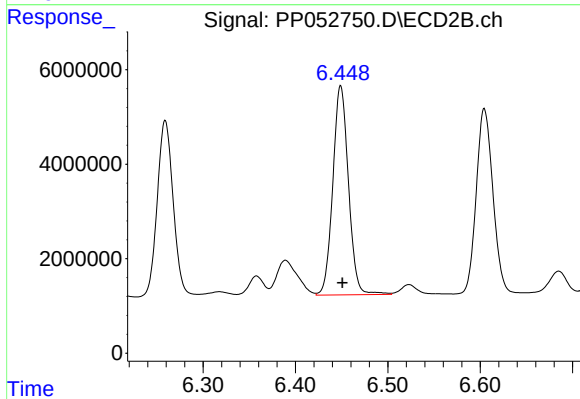

#32 AR-1260-2


R.T.: 6.449 min
Delta R.T.: -0.002 min
Response: 52115674
Conc: 428.54 ng/ml

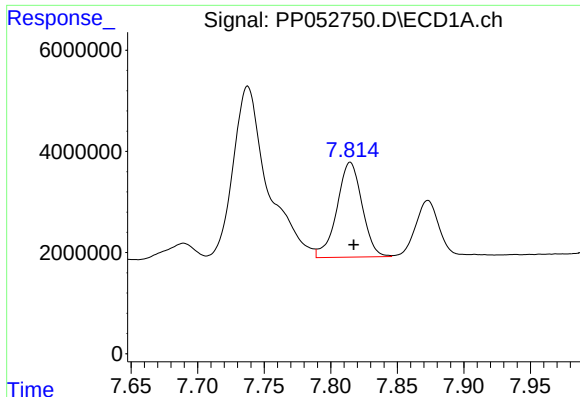

#33 AR-1260-3


R.T.: 7.815 min
Delta R.T.: -0.003 min
Response: 24671855
Conc: 390.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

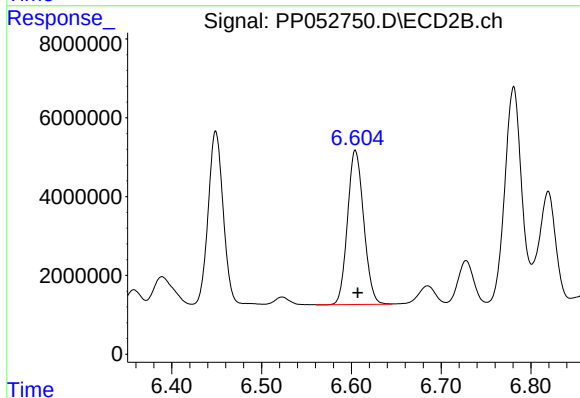


#33 AR-1260-3

R.T.: 6.604 min
Delta R.T.: -0.003 min
Response: 48931802
Conc: 419.49 ng/ml

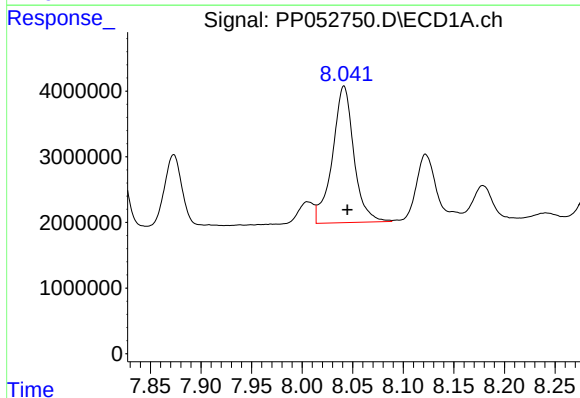


#34 AR-1260-4

R.T.: 8.041 min
Delta R.T.: -0.004 min
Response: 30609860
Conc: 427.50 ng/ml

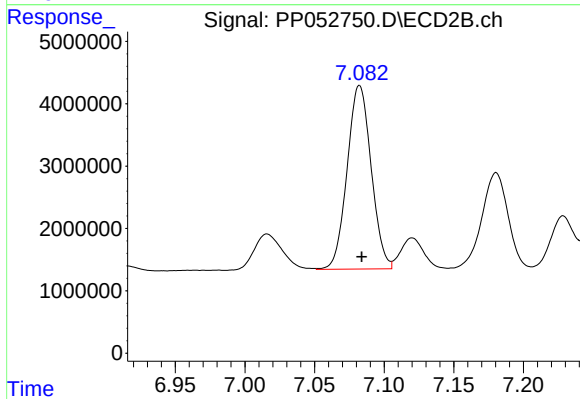

#34 AR-1260-4


R.T.: 7.082 min
Delta R.T.: -0.002 min
Response: 35354408
Conc: 392.65 ng/ml

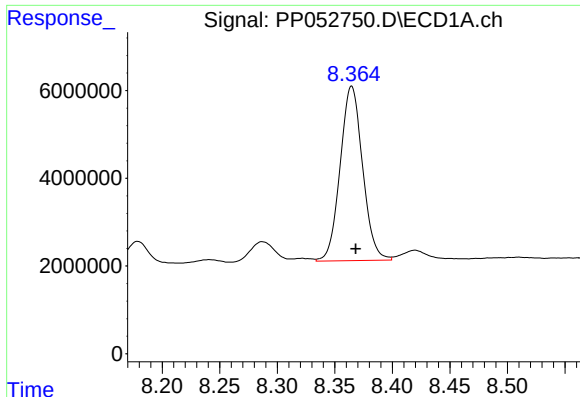

#35 AR-1260-5


R.T.: 8.365 min
Delta R.T.: -0.004 min
Response: 54150163
Conc: 426.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

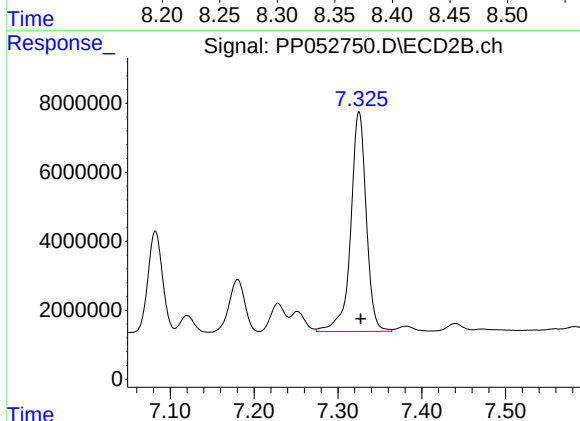


#35 AR-1260-5

R.T.: 7.325 min
Delta R.T.: -0.002 min
Response: 82084049
Conc: 400.71 ng/ml

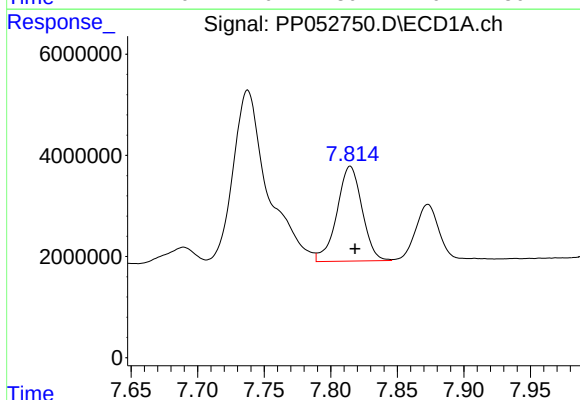


#36 AR-1262-1

R.T.: 7.815 min
Delta R.T.: -0.004 min
Response: 24671855
Conc: 257.39 ng/ml

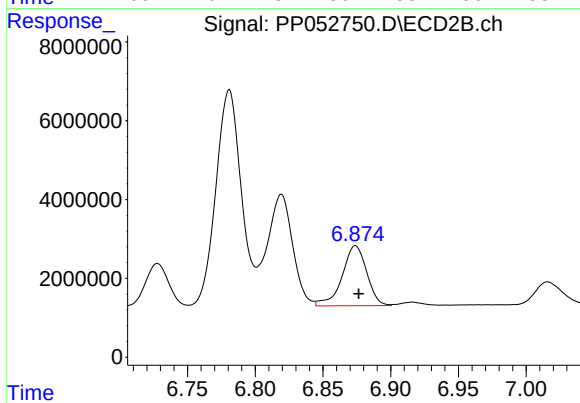

#36 AR-1262-1


R.T.: 6.874 min
Delta R.T.: -0.003 min
Response: 19251202
Conc: 336.13 ng/ml

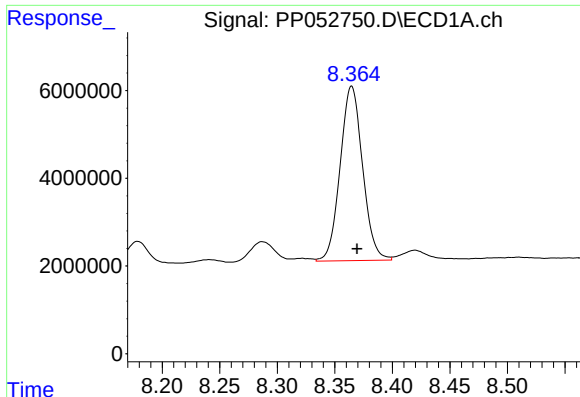

#37 AR-1262-2


R.T.: 8.365 min
Delta R.T.: -0.005 min
Response: 54150163
Conc: 364.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

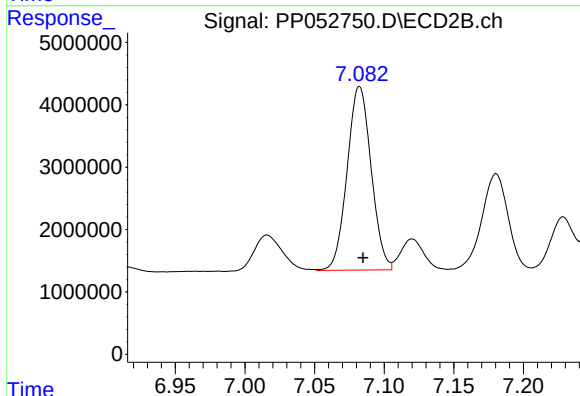


#37 AR-1262-2

R.T.: 7.082 min
Delta R.T.: -0.003 min
Response: 35354408
Conc: 285.50 ng/ml

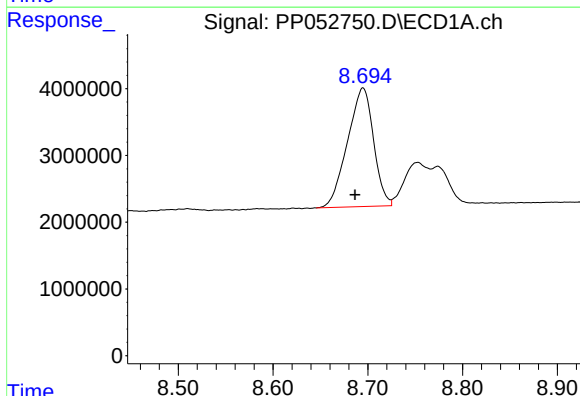


#38 AR-1262-3

R.T.: 8.695 min
Delta R.T.: 0.008 min
Response: 33896625
Conc: 341.61 ng/ml

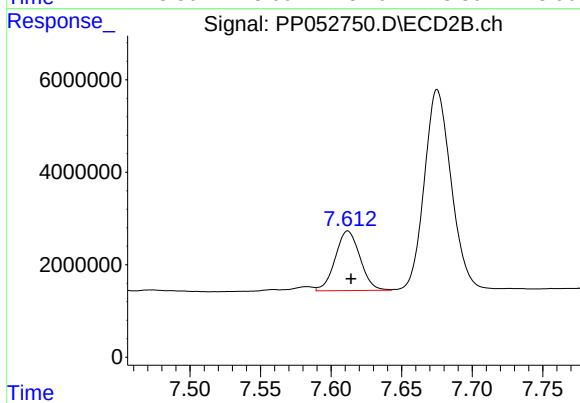

#38 AR-1262-3


R.T.: 7.612 min
Delta R.T.: -0.002 min
Response: 15723090
Conc: 155.80 ng/ml

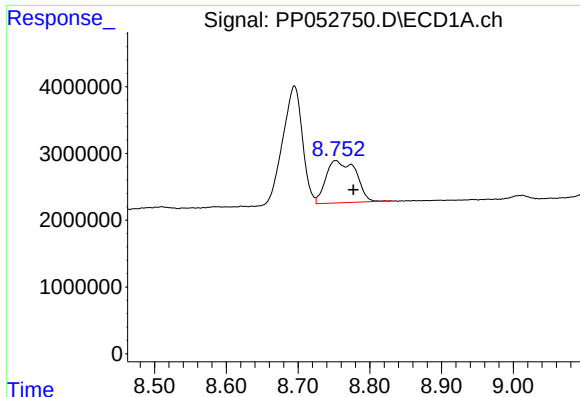

#39 AR-1262-4


R.T.: 8.752 min
Delta R.T.: -0.025 min
Response: 18302323
Conc: 392.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

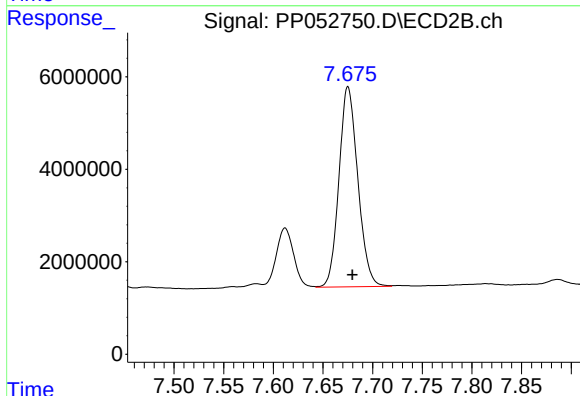


#39 AR-1262-4

R.T.: 7.675 min
Delta R.T.: -0.004 min
Response: 57263135
Conc: 320.04 ng/ml

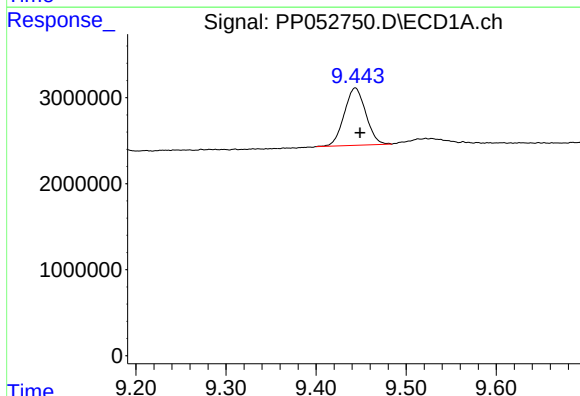


#40 AR-1262-5

R.T.: 9.444 min
Delta R.T.: -0.005 min
Response: 11049604
Conc: 241.46 ng/ml

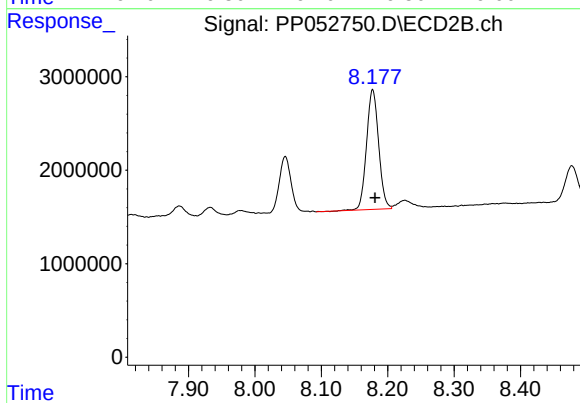

#40 AR-1262-5


R.T.: 8.177 min
Delta R.T.: -0.004 min
Response: 16243571
Conc: 216.90 ng/ml

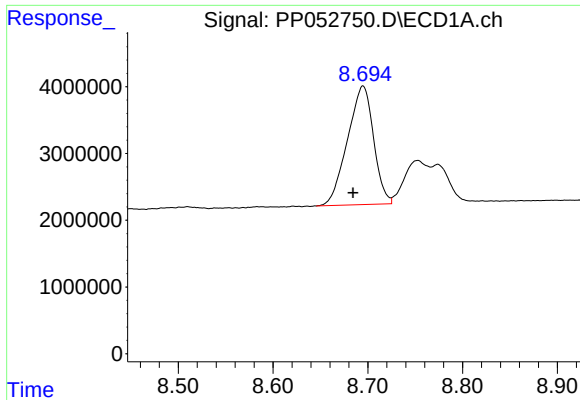

#41 AR-1268-1


R.T.: 8.695 min
Delta R.T.: 0.011 min
Response: 33896625
Conc: 180.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

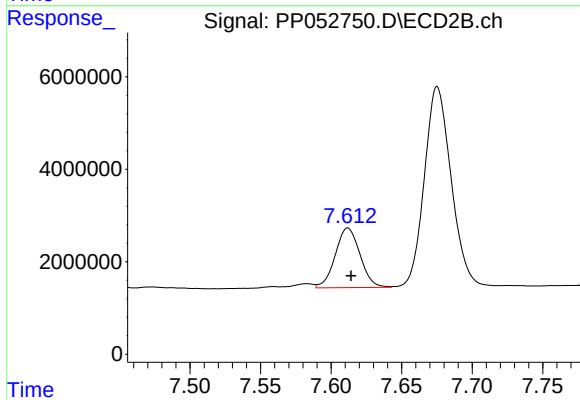


#41 AR-1268-1

R.T.: 7.612 min
Delta R.T.: -0.002 min
Response: 15723090
Conc: 51.29 ng/ml

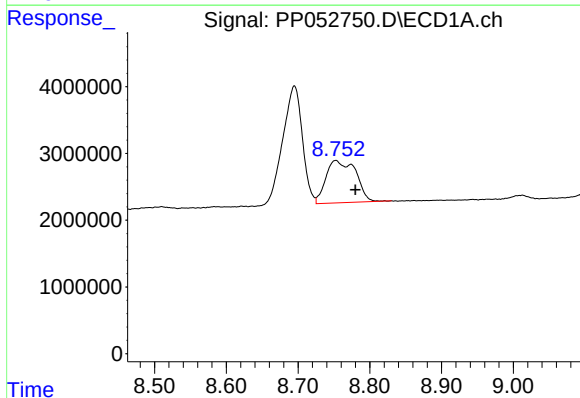


#42 AR-1268-2

R.T.: 8.752 min
Delta R.T.: -0.028 min
Response: 18302323
Conc: 111.83 ng/ml

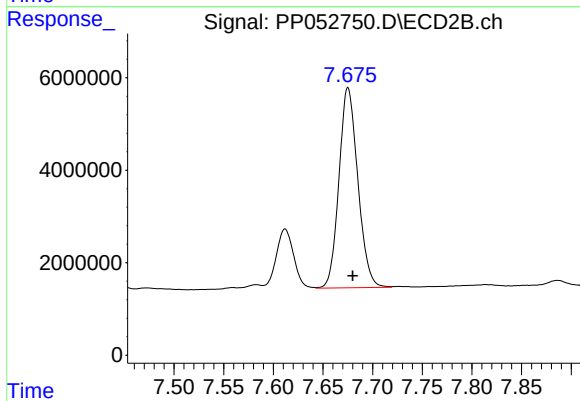

#42 AR-1268-2


R.T.: 7.675 min
Delta R.T.: -0.005 min
Response: 57263135
Conc: 211.13 ng/ml

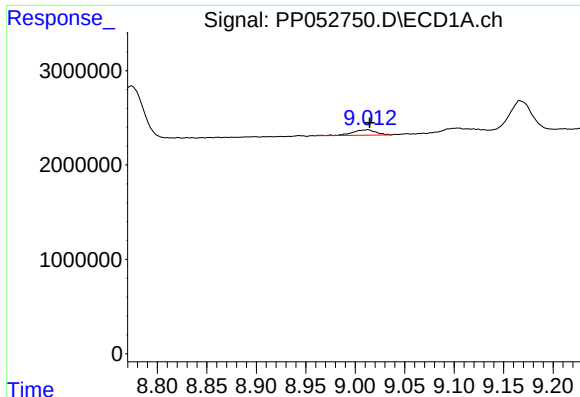

#43 AR-1268-3


R.T.: 9.012 min
Delta R.T.: -0.003 min
Response: 945516
Conc: 6.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

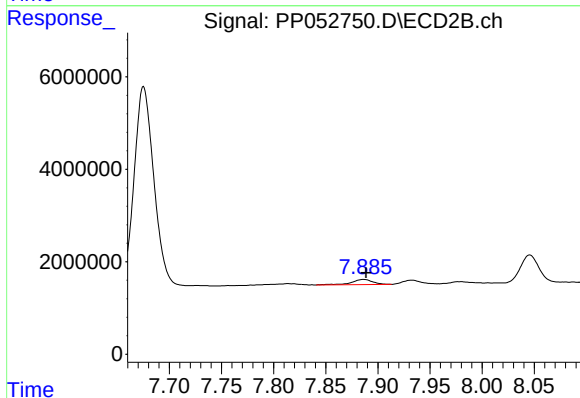


#43 AR-1268-3

R.T.: 7.886 min
Delta R.T.: -0.002 min
Response: 1596725
Conc: 6.81 ng/ml

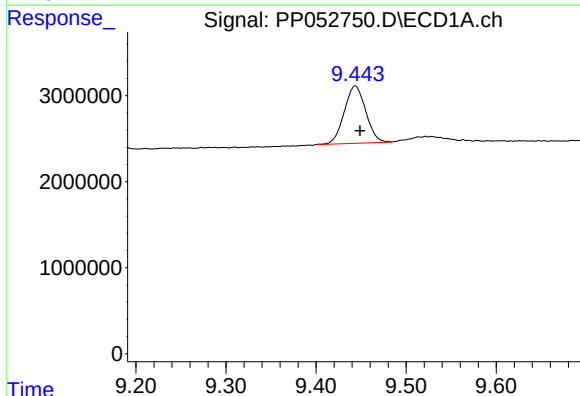


#44 AR-1268-4

R.T.: 9.444 min
Delta R.T.: -0.005 min
Response: 11049604
Conc: 217.27 ng/ml

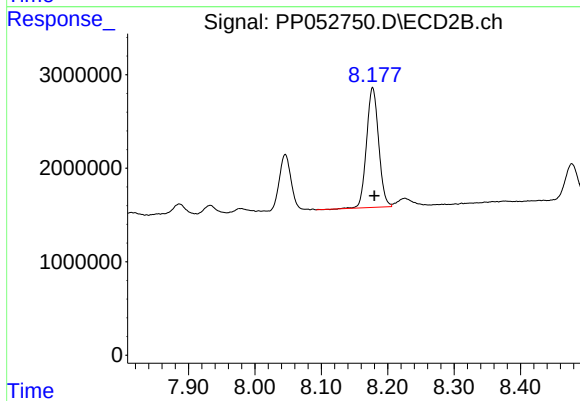

#44 AR-1268-4


R.T.: 8.177 min
Delta R.T.: -0.003 min
Response: 16243571
Conc: 191.23 ng/ml

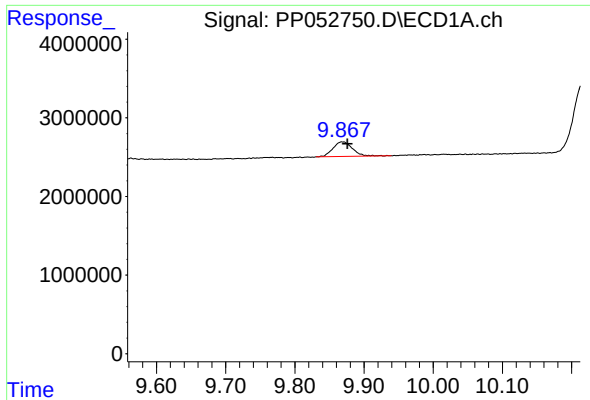

#45 AR-1268-5

R.T.: 9.869 min
Delta R.T.: -0.007 min
Response: 3667910
Conc: 8.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1MSD

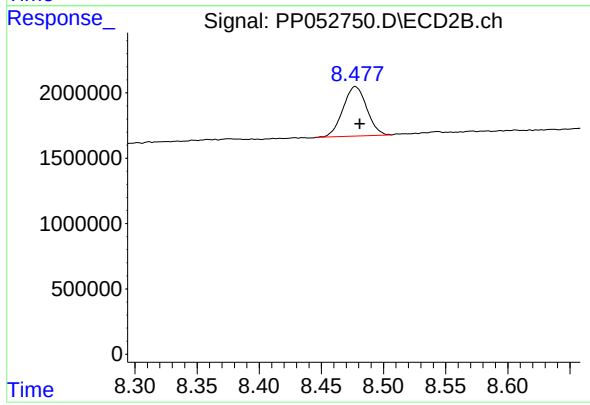

#45 AR-1268-5

R.T.: 8.477 min
Delta R.T.: -0.003 min
Response: 5038487
Conc: 7.68 ng/ml