

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2022 15:52
 Operator : YP\AJ
 Sample : N5257-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HOLLAND-RD-COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:18:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.408	3.652	38229748	35978960	17.301	19.146
2)	SA Decachlor...	10.218	8.741	18589448	21519268	14.645	12.831
Target Compounds							
3)	L1 AR-1016-1	5.582	4.758	1184430	186892	17.666	2.839 #
4)	L1 AR-1016-2	5.607	4.778	1029374	41952	10.306	0.457 #
5)	L1 AR-1016-3	5.656	0.000	2164378	0	35.563	N.D. #
6)	L1 AR-1016-4	0.000	4.995	0	352933	N.D.	9.059 #
7)	L1 AR-1016-5	6.065	5.202	114696	372592	2.381	7.415 #
8)	L2 AR-1221-1	4.616	0.000	1893119	0	73.830	N.D. #
9)	L2 AR-1221-2	4.716	3.954	449021	613679	23.604	35.056 #
10)	L2 AR-1221-3	4.802f	4.033	284320	175354	4.988	3.231 #
11)	L3 AR-1232-1	4.802f	4.033	284320	175354	6.552	4.206 #
12)	L3 AR-1232-2	5.335f	4.778	499329	41952	20.125	1.012 #
13)	L3 AR-1232-3	5.607	0.000	1029374	0	23.515	N.D. #
14)	L3 AR-1232-4	0.000	5.039	0	129506	N.D.	6.301 #
15)	L3 AR-1232-5	5.860	5.202	221293	372592	12.856	16.049
16)	L4 AR-1242-1	5.582	4.758	1184430	186892	21.045	3.349 #
17)	L4 AR-1242-2	5.607	4.778	1029374	41952	12.461	0.544 #
18)	L4 AR-1242-3	5.656f	0.000	2164378	0	42.558	N.D. #
19)	L4 AR-1242-4	0.000	5.039	0	129506	N.D.	3.053 #
20)	L4 AR-1242-5	6.510	5.569	203903	1096862	5.114	21.699 #
21)	L5 AR-1248-1	5.582	4.758	1184430	186892	29.161	4.669 #
22)	L5 AR-1248-2	5.860	4.995	221293	352933	3.718	6.233 #
23)	L5 AR-1248-3	6.065	5.039	114696	129506	1.767	2.206
24)	L5 AR-1248-4	6.477	5.202	904498	372592	14.044	5.351 #
25)	L5 AR-1248-5	6.510	0.000	203903	0	3.219	N.D. #
26)	L6 AR-1254-1	6.438	5.569	1476586	1096862	19.453	10.214 #
27)	L6 AR-1254-2	6.665	5.718	1017386	1000826	9.103	10.471
28)	L6 AR-1254-3	7.032	6.127	1769140	1838959	15.894	12.036
29)	L6 AR-1254-4	7.318	6.358	507856	401525	7.212	4.422 #
30)	L6 AR-1254-5	7.758f	6.780	2090984	2042791	26.558	14.683 #
31)	L7 AR-1260-1	7.196	6.259	570235	985403	6.675	9.688 #
32)	L7 AR-1260-2	7.452	6.450	1756256	1455220	18.807	11.966 #
33)	L7 AR-1260-3	7.819	6.604	533844	714350	8.449	6.124 #
34)	L7 AR-1260-4	8.029f	7.082	536320	515840	7.490	5.729
35)	L7 AR-1260-5	8.366	7.324	474371	528238	3.732	2.579 #
36)	L8 AR-1262-1	7.819	6.882	533844	207917	5.569	3.630 #
37)	L8 AR-1262-2	8.366	7.082	474371	515840	3.189	4.166 #
38)	L8 AR-1262-3	8.703f	7.614	307249	296567	3.096	2.939
39)	L8 AR-1262-4	8.778	7.677	571035	329496	12.257	1.842 #
40)	L8 AR-1262-5	0.000	8.181	0	58146	N.D.	0.776 #
41)	L9 AR-1268-1	8.703f	7.614	307249	296567	1.634	0.967 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2022 15:52
Operator : YP\AJ
Sample : N5257-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:18:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.778	7.677	571035	329496	3.489	1.215 #
43) L9	AR-1268-3	0.000	7.891	0	600016	N.D.	2.560 #
44) L9	AR-1268-4	0.000	8.181	0	58146	N.D.	0.685 #
45) L9	AR-1268-5	9.867	8.483	324040	114029	0.754	0.174 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2022 15:52
Operator : YP\AJ
Sample : N5257-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:18:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

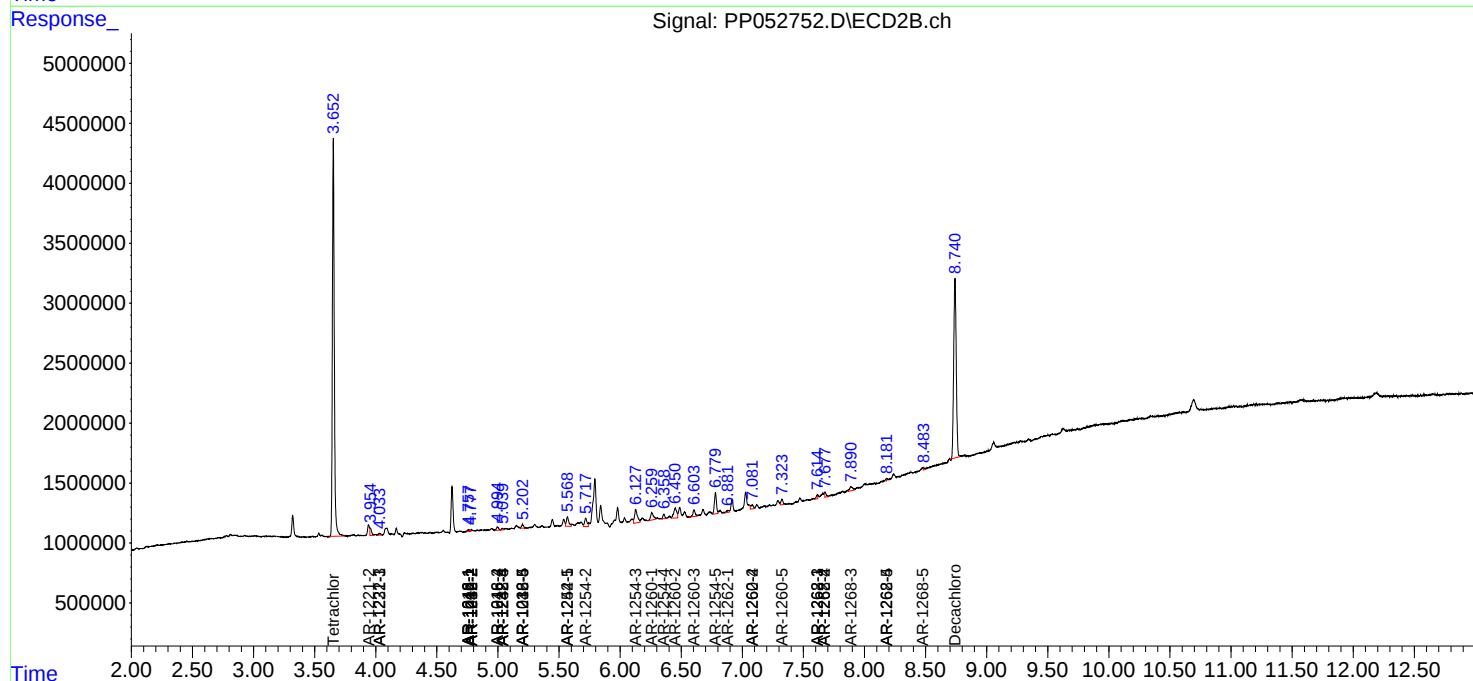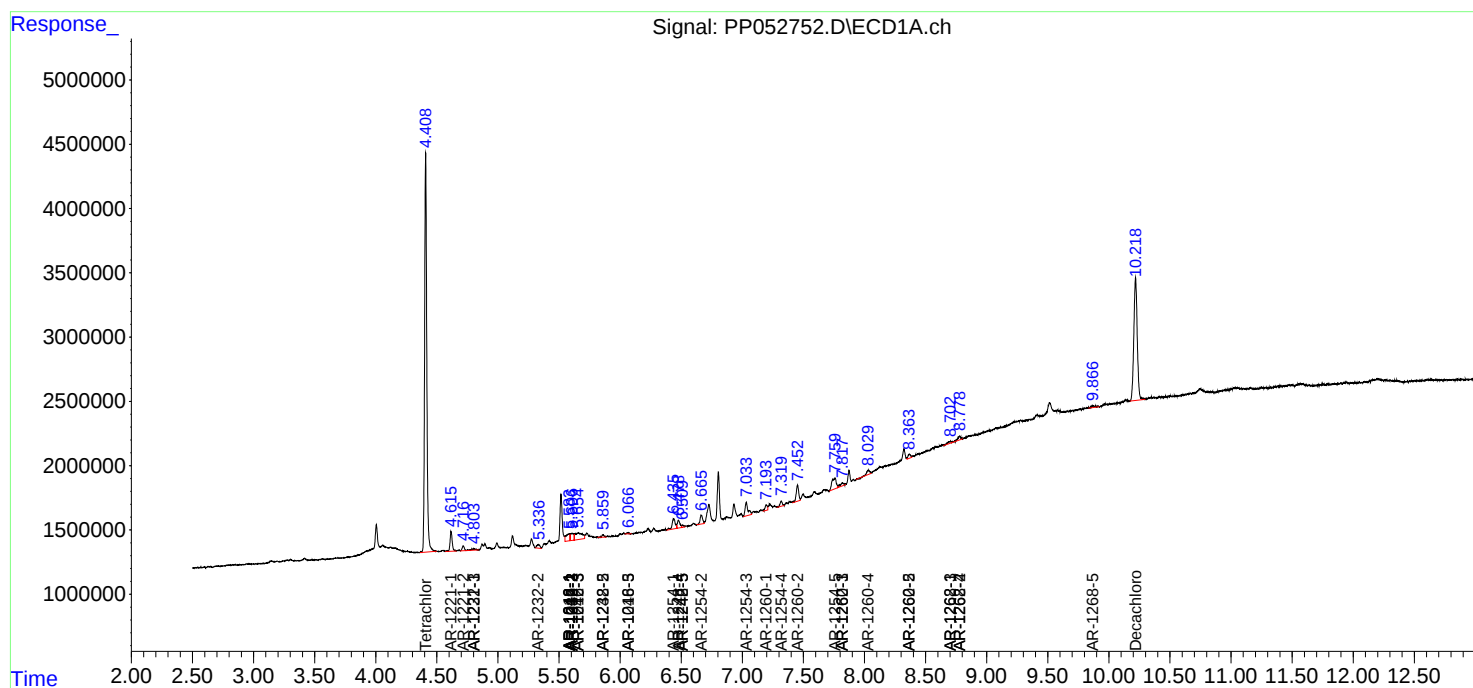


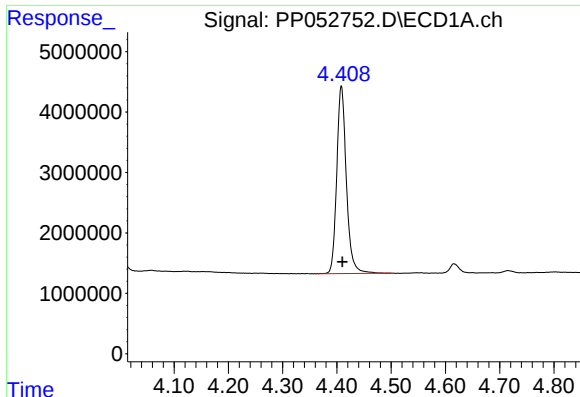

#1 Tetrachloro-m-xylene


R.T.: 4.408 min
Delta R.T.: -0.002 min
Response: 38229748
Conc: 17.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

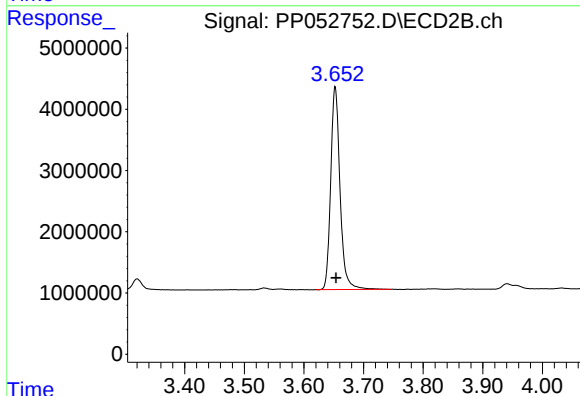


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.001 min
Response: 35978960
Conc: 19.15 ng/ml

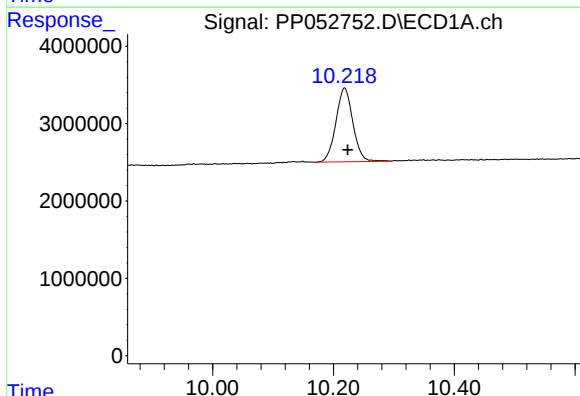


#2 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.005 min
Response: 18589448
Conc: 14.65 ng/ml

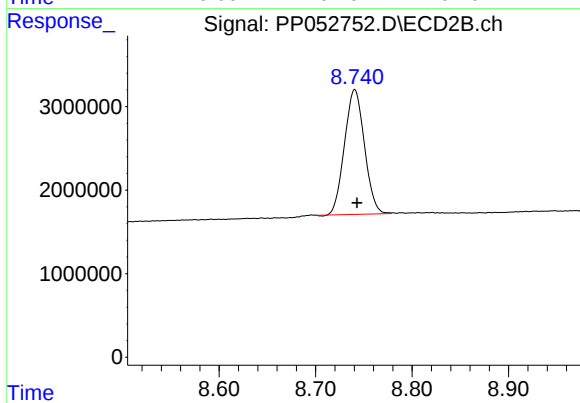

#2 Decachlorobiphenyl


R.T.: 8.741 min
Delta R.T.: -0.002 min
Response: 21519268
Conc: 12.83 ng/ml

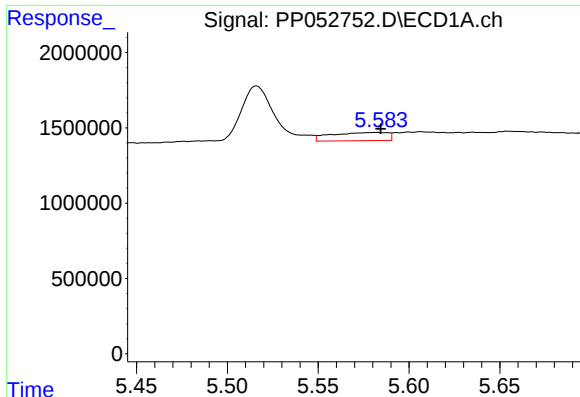

#3 AR-1016-1


R.T.: 5.582 min
Delta R.T.: -0.002 min
Response: 1184430
Conc: 17.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

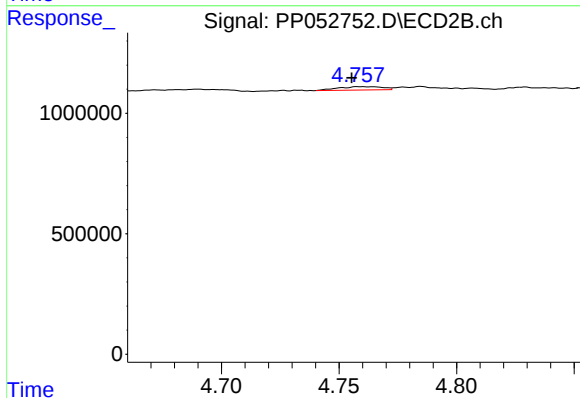


#3 AR-1016-1

R.T.: 4.758 min
Delta R.T.: 0.002 min
Response: 186892
Conc: 2.84 ng/ml

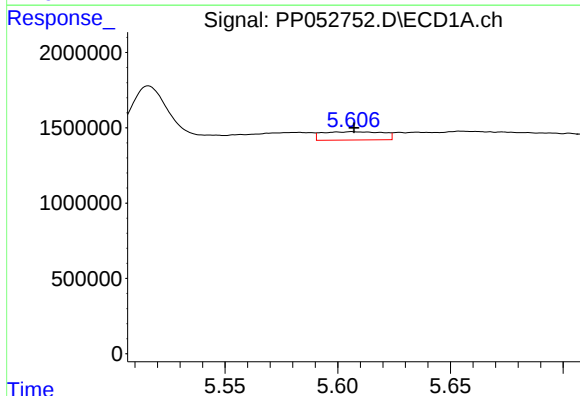


#4 AR-1016-2

R.T.: 5.607 min
Delta R.T.: 0.000 min
Response: 1029374
Conc: 10.31 ng/ml

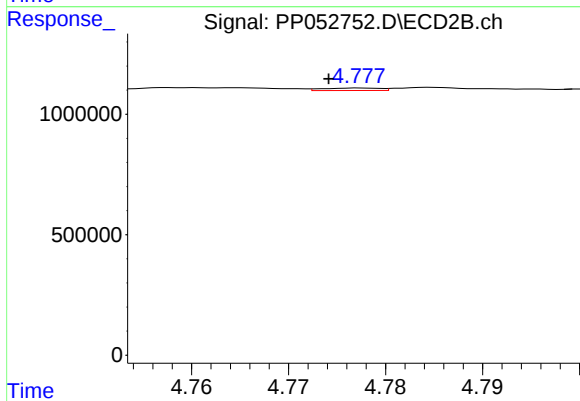

#4 AR-1016-2


R.T.: 4.778 min
Delta R.T.: 0.003 min
Response: 41952
Conc: 0.46 ng/ml

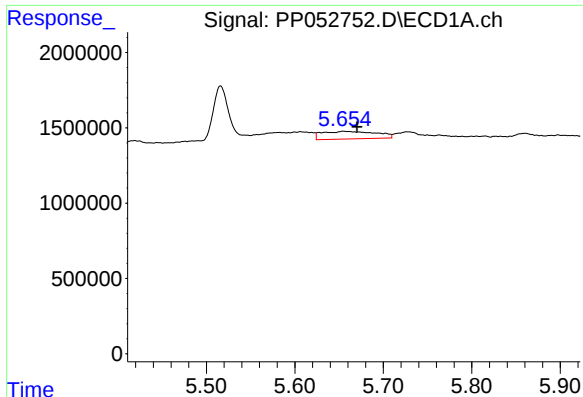

#5 AR-1016-3


R.T.: 5.656 min
Delta R.T.: -0.014 min
Response: 2164378
Conc: 35.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

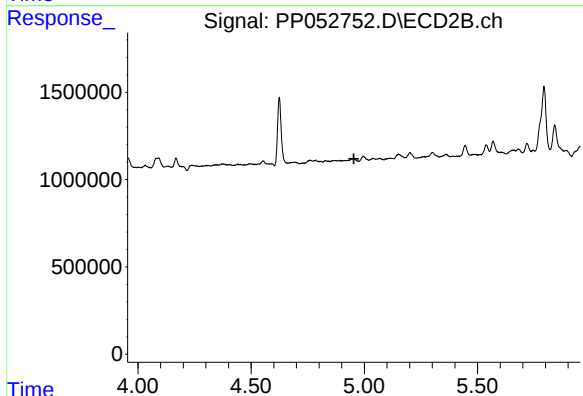


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

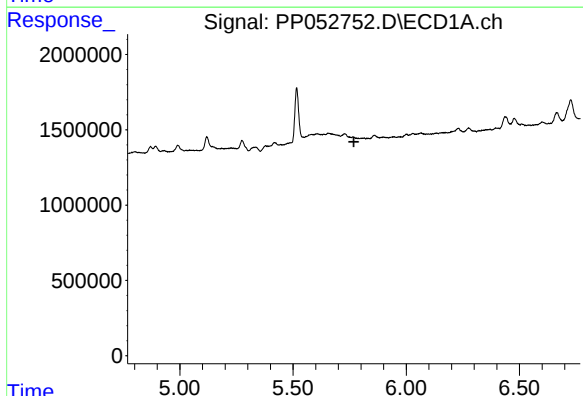


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.769 min
Response: 0
Conc: N.D.

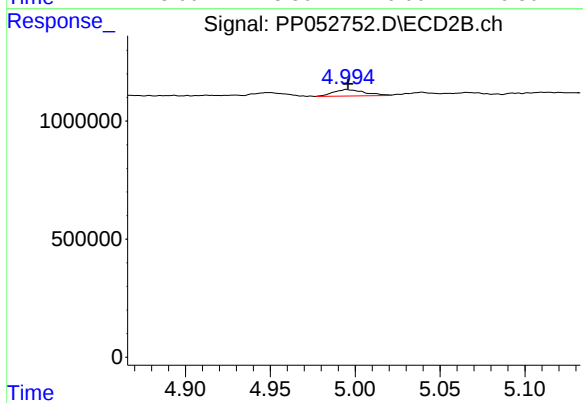

#6 AR-1016-4


R.T.: 4.995 min
Delta R.T.: -0.001 min
Response: 352933
Conc: 9.06 ng/ml

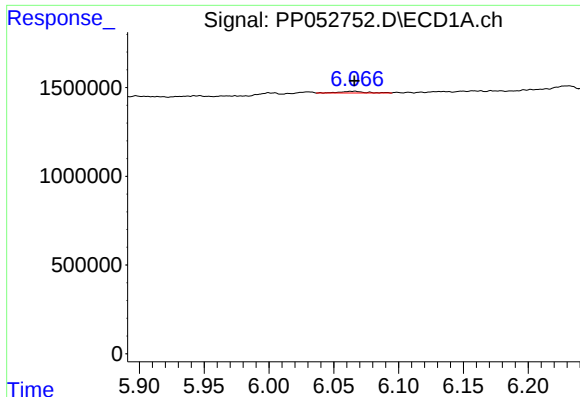

#7 AR-1016-5


R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 114696
Conc: 2.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

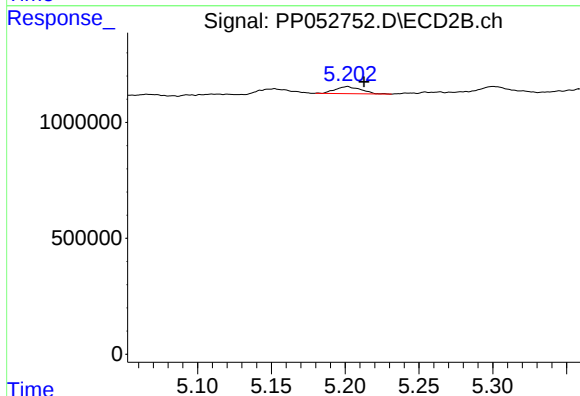


#7 AR-1016-5

R.T.: 5.202 min
Delta R.T.: -0.011 min
Response: 372592
Conc: 7.42 ng/ml

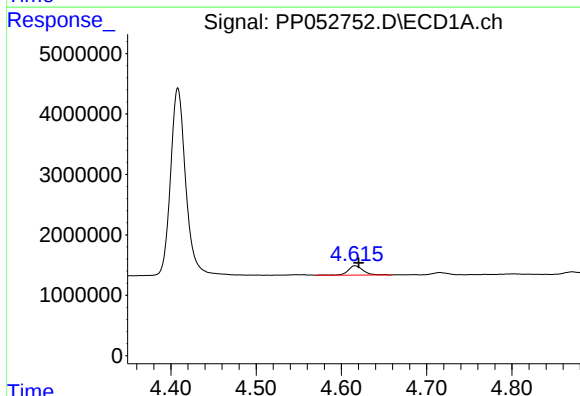


#8 AR-1221-1

R.T.: 4.616 min
Delta R.T.: -0.004 min
Response: 1893119
Conc: 73.83 ng/ml

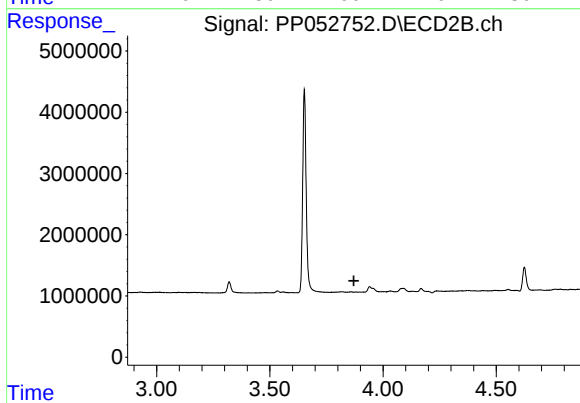

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 3.872 min
Response: 0
Conc: N.D.

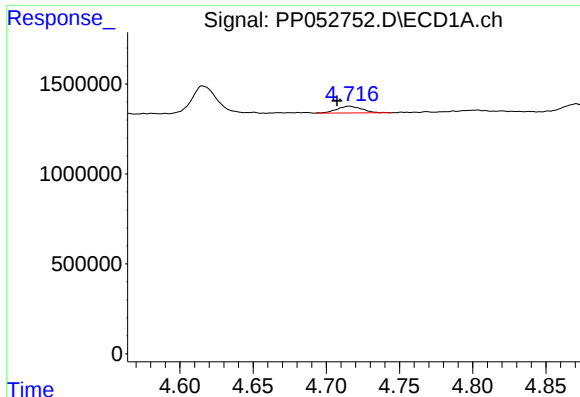

#9 AR-1221-2


R.T.: 4.716 min
Delta R.T.: 0.009 min
Response: 449021
Conc: 23.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

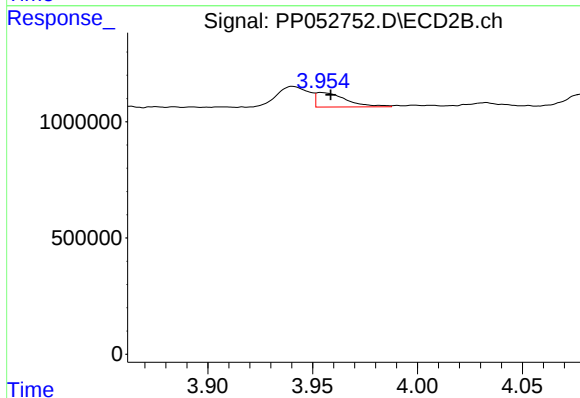


#9 AR-1221-2

R.T.: 3.954 min
Delta R.T.: -0.004 min
Response: 613679
Conc: 35.06 ng/ml

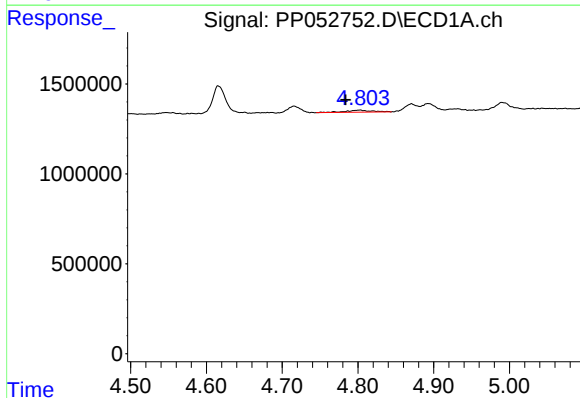


#10 AR-1221-3

R.T.: 4.802 min
Delta R.T.: 0.018 min
Response: 284320
Conc: 4.99 ng/ml

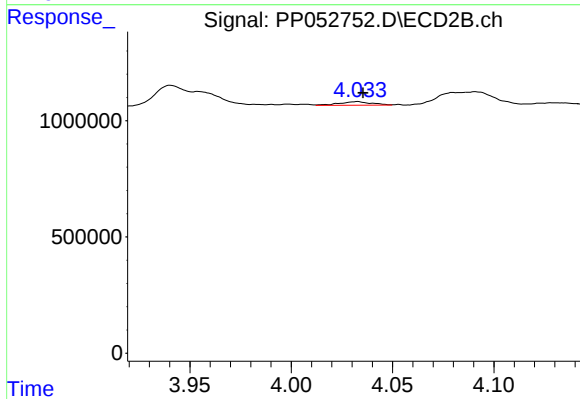

#10 AR-1221-3


R.T.: 4.033 min
Delta R.T.: -0.003 min
Response: 175354
Conc: 3.23 ng/ml

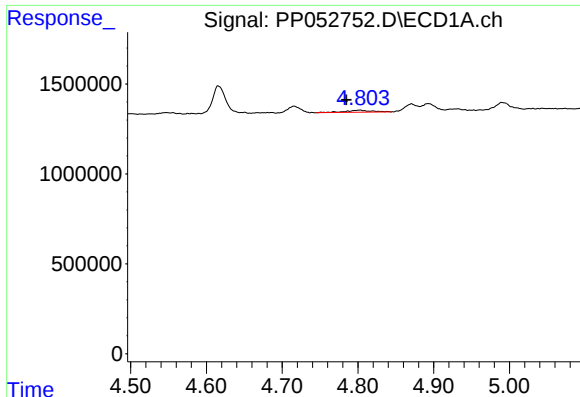

#11 AR-1232-1


R.T.: 4.802 min
Delta R.T.: 0.017 min
Response: 284320
Conc: 6.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

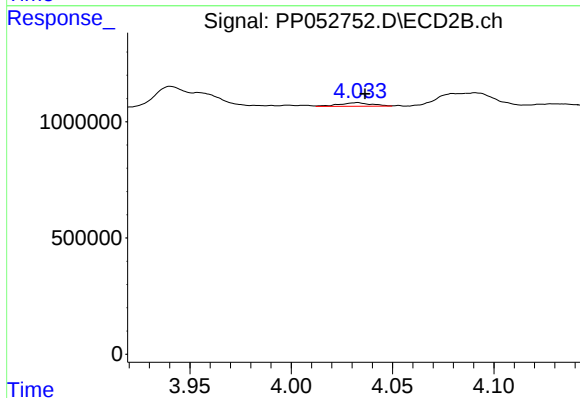


#11 AR-1232-1

R.T.: 4.033 min
Delta R.T.: -0.003 min
Response: 175354
Conc: 4.21 ng/ml

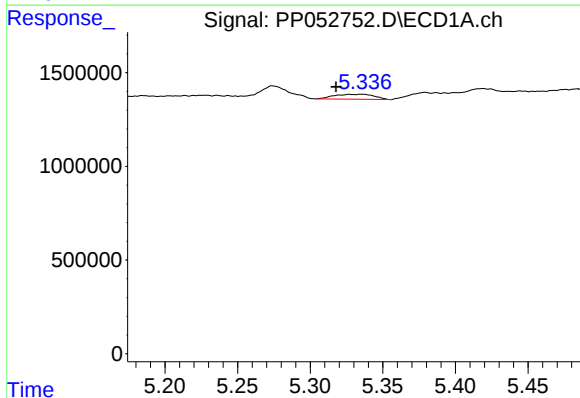


#12 AR-1232-2

R.T.: 5.335 min
Delta R.T.: 0.017 min
Response: 499329
Conc: 20.13 ng/ml

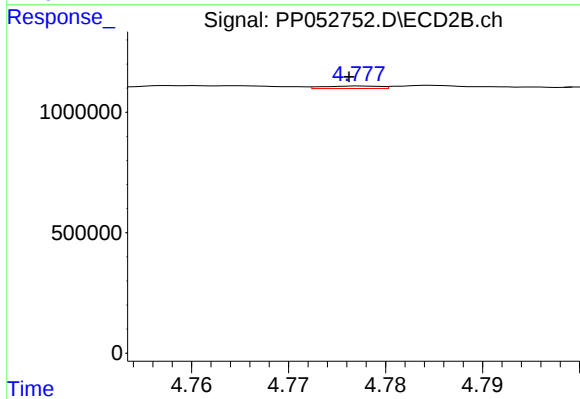

#12 AR-1232-2


R.T.: 4.778 min
Delta R.T.: 0.001 min
Response: 41952
Conc: 1.01 ng/ml

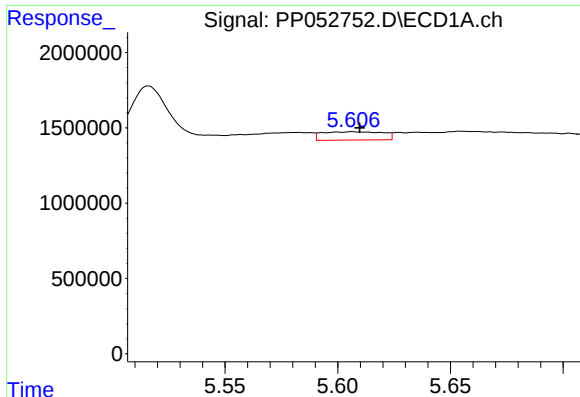

#13 AR-1232-3


R.T.: 5.607 min
Delta R.T.: -0.003 min
Response: 1029374
Conc: 23.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

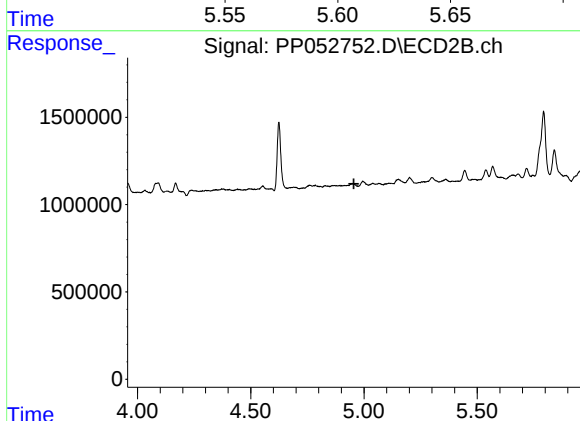


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.955 min
Response: 0
Conc: N.D.

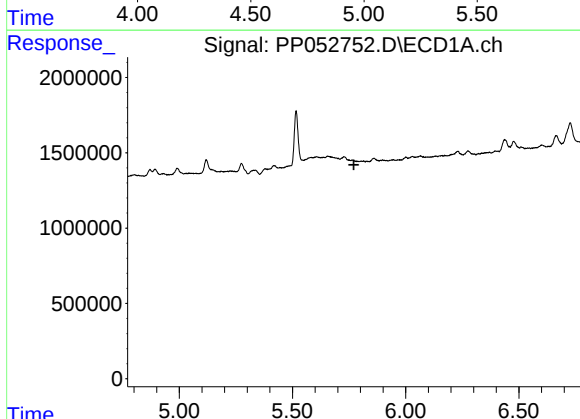


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.771 min
Response: 0
Conc: N.D.

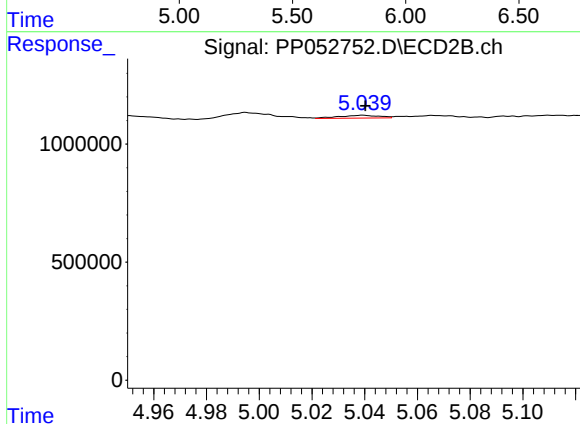

#14 AR-1232-4


R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 129506
Conc: 6.30 ng/ml

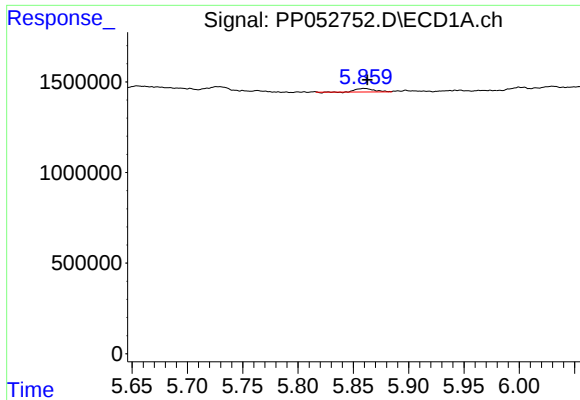

#15 AR-1232-5


R.T.: 5.860 min
Delta R.T.: -0.003 min
Response: 221293
Conc: 12.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

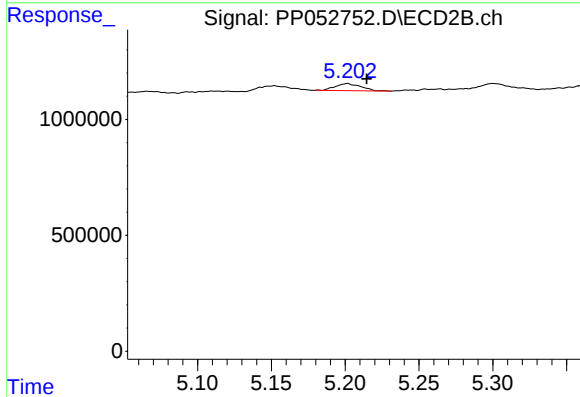


#15 AR-1232-5

R.T.: 5.202 min
Delta R.T.: -0.013 min
Response: 372592
Conc: 16.05 ng/ml

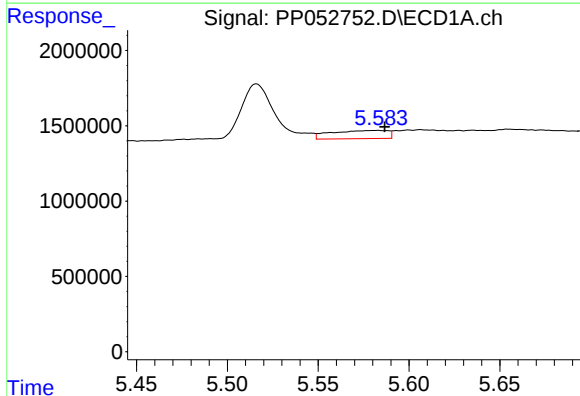


#16 AR-1242-1

R.T.: 5.582 min
Delta R.T.: -0.005 min
Response: 1184430
Conc: 21.05 ng/ml

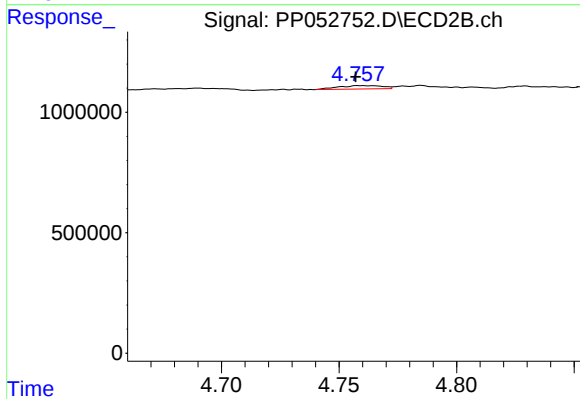

#16 AR-1242-1


R.T.: 4.758 min
Delta R.T.: 0.000 min
Response: 186892
Conc: 3.35 ng/ml

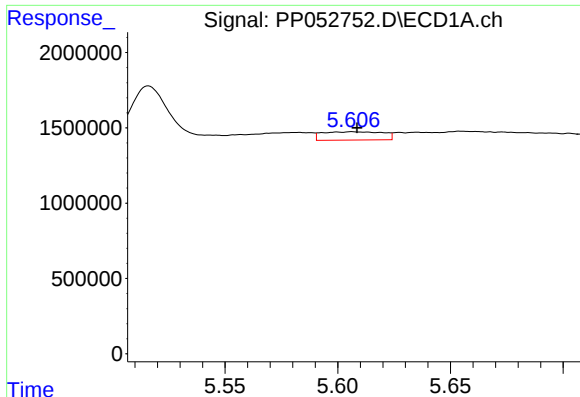

#17 AR-1242-2


R.T.: 5.607 min
Delta R.T.: -0.002 min
Response: 1029374
Conc: 12.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

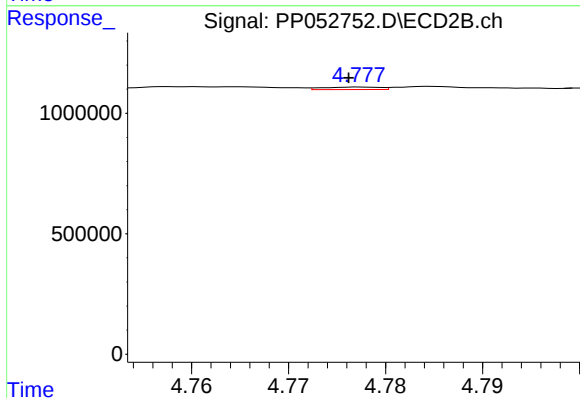


#17 AR-1242-2

R.T.: 4.778 min
Delta R.T.: 0.001 min
Response: 41952
Conc: 0.54 ng/ml

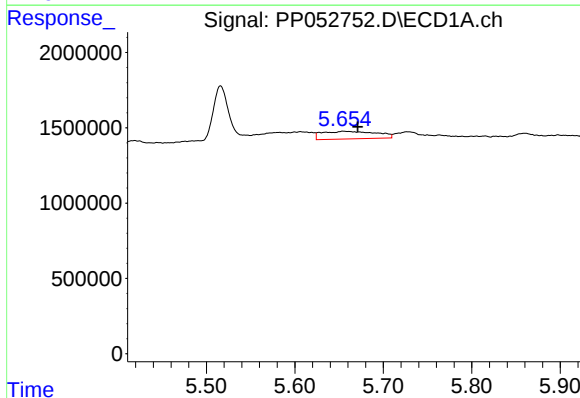


#18 AR-1242-3

R.T.: 5.656 min
Delta R.T.: -0.015 min
Response: 2164378
Conc: 42.56 ng/ml

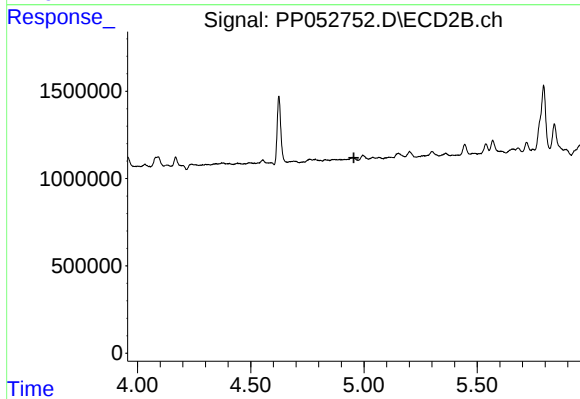

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

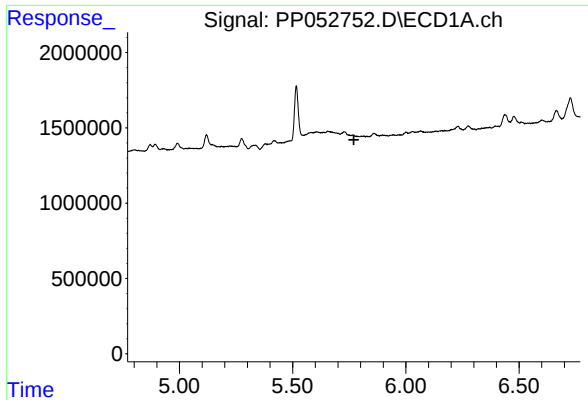

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

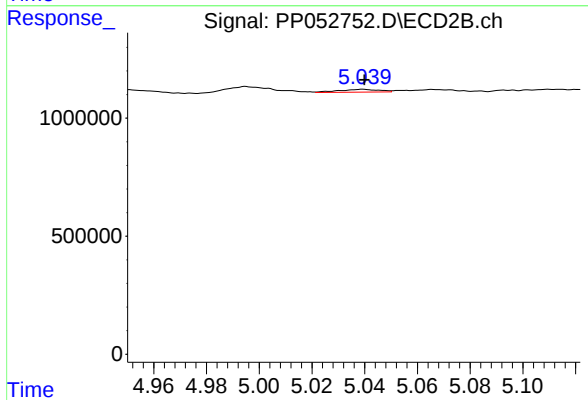


#19 AR-1242-4

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 129506
Conc: 3.05 ng/ml

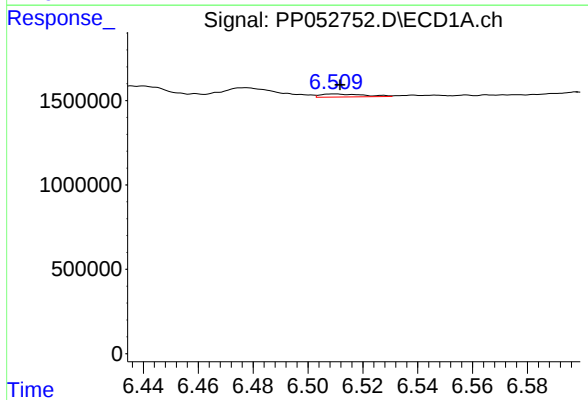


#20 AR-1242-5

R.T.: 6.510 min
Delta R.T.: -0.001 min
Response: 203903
Conc: 5.11 ng/ml

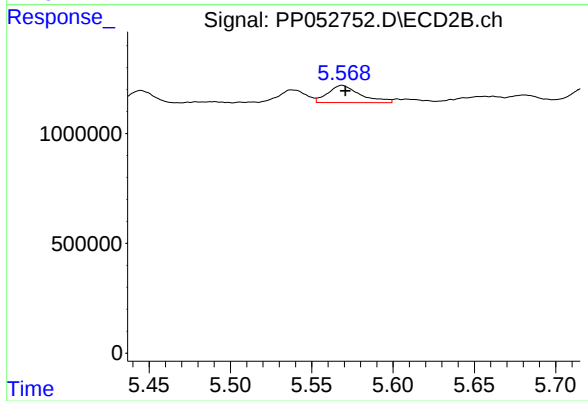

#20 AR-1242-5


R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 1096862
Conc: 21.70 ng/ml

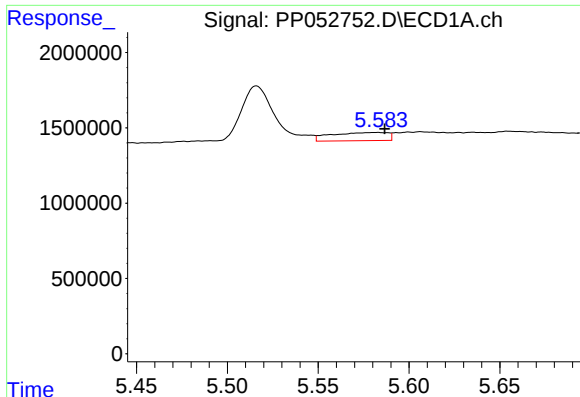

#21 AR-1248-1


R.T.: 5.582 min
Delta R.T.: -0.005 min
Response: 1184430
Conc: 29.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

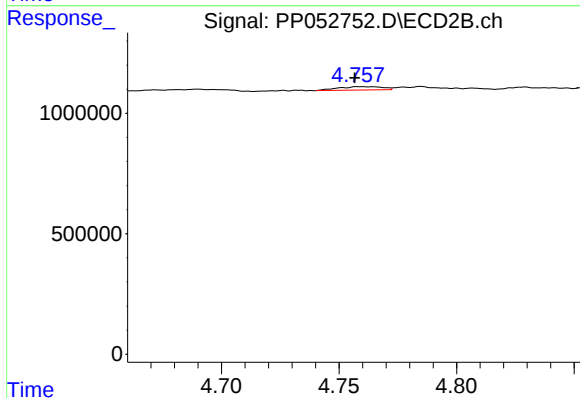


#21 AR-1248-1

R.T.: 4.758 min
Delta R.T.: 0.001 min
Response: 186892
Conc: 4.67 ng/ml

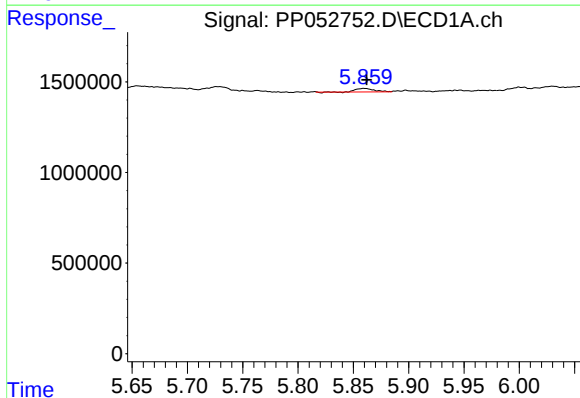


#22 AR-1248-2

R.T.: 5.860 min
Delta R.T.: -0.003 min
Response: 221293
Conc: 3.72 ng/ml

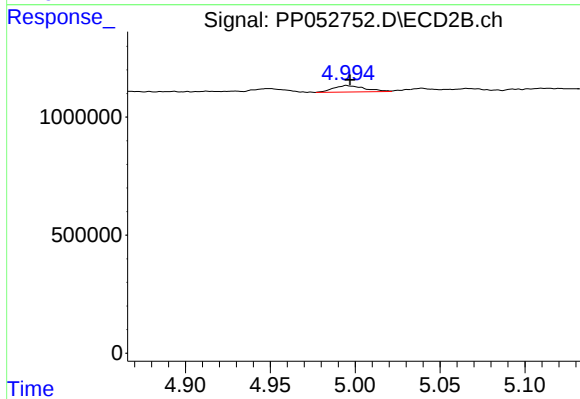

#22 AR-1248-2


R.T.: 4.995 min
Delta R.T.: -0.002 min
Response: 352933
Conc: 6.23 ng/ml

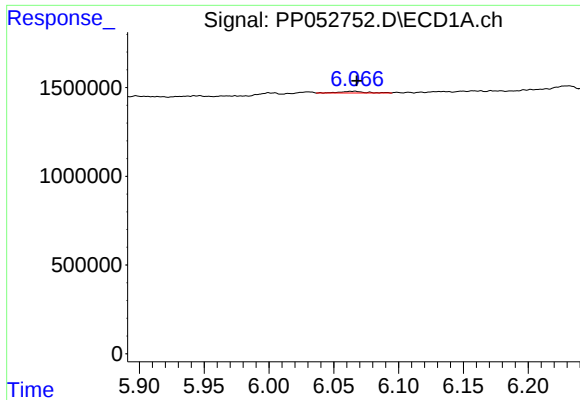

#23 AR-1248-3


R.T.: 6.065 min
Delta R.T.: -0.003 min
Response: 114696
Conc: 1.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

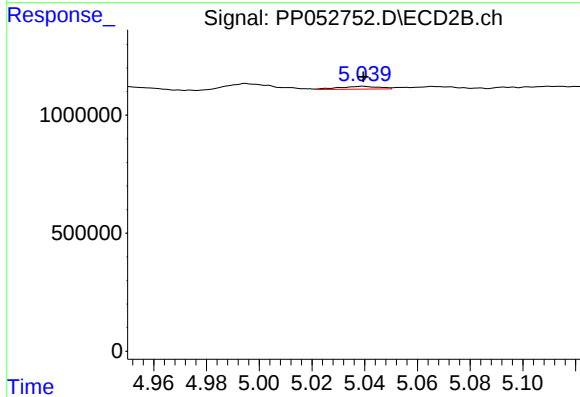


#23 AR-1248-3

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 129506
Conc: 2.21 ng/ml

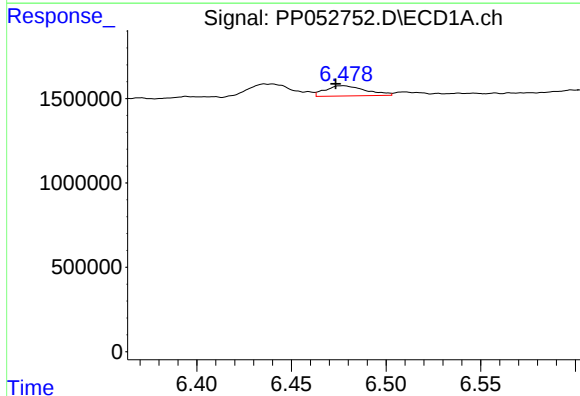


#24 AR-1248-4

R.T.: 6.477 min
Delta R.T.: 0.004 min
Response: 904498
Conc: 14.04 ng/ml

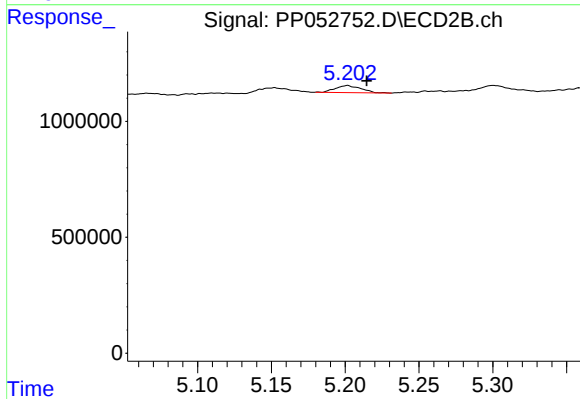

#24 AR-1248-4


R.T.: 5.202 min
Delta R.T.: -0.013 min
Response: 372592
Conc: 5.35 ng/ml

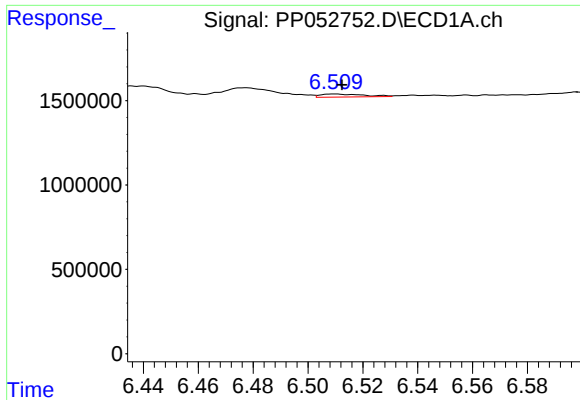

#25 AR-1248-5


R.T.: 6.510 min
Delta R.T.: -0.002 min
Response: 203903
Conc: 3.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

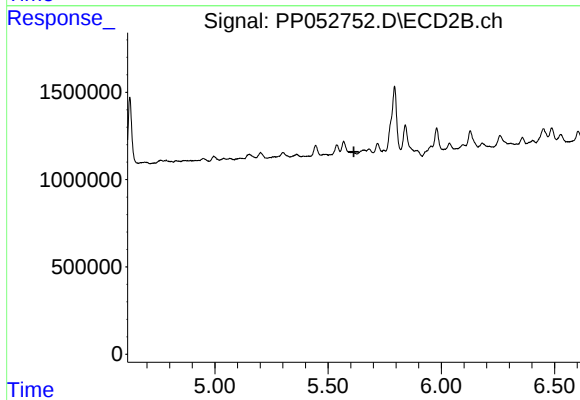


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.613 min
Response: 0
Conc: N.D.

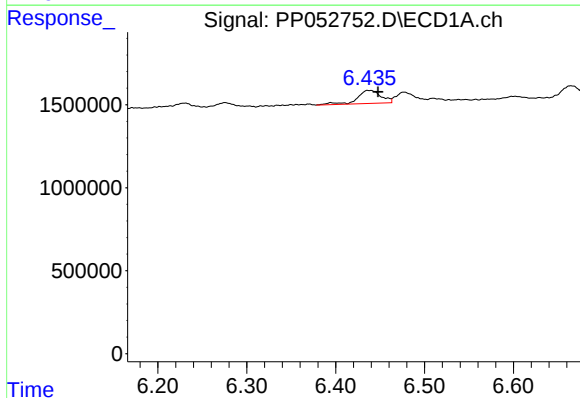


#26 AR-1254-1

R.T.: 6.438 min
Delta R.T.: -0.010 min
Response: 1476586
Conc: 19.45 ng/ml

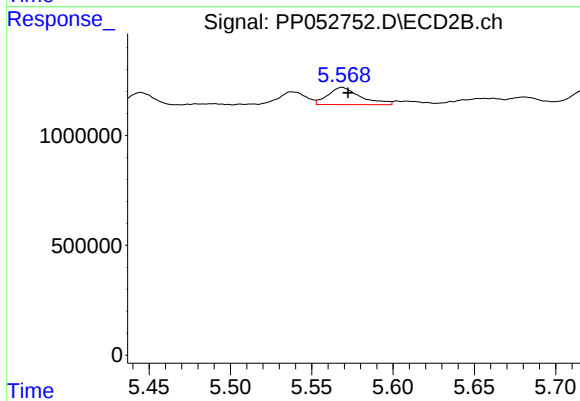

#26 AR-1254-1


R.T.: 5.569 min
Delta R.T.: -0.004 min
Response: 1096862
Conc: 10.21 ng/ml

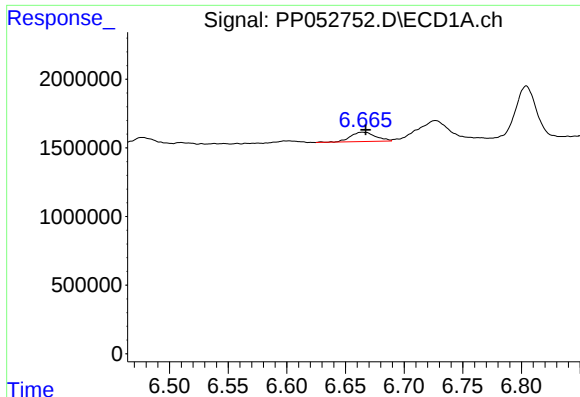

#27 AR-1254-2


R.T.: 6.665 min
Delta R.T.: -0.002 min
Response: 1017386
Conc: 9.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

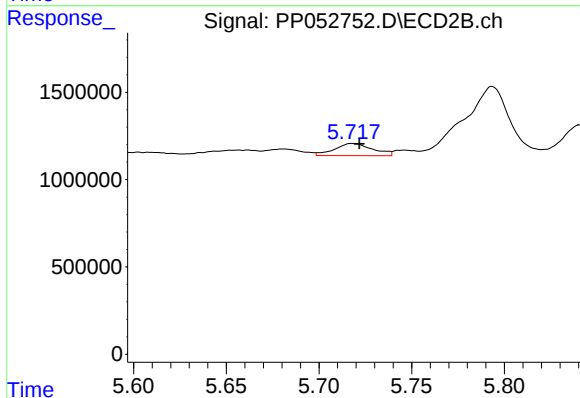


#27 AR-1254-2

R.T.: 5.718 min
Delta R.T.: -0.004 min
Response: 1000826
Conc: 10.47 ng/ml

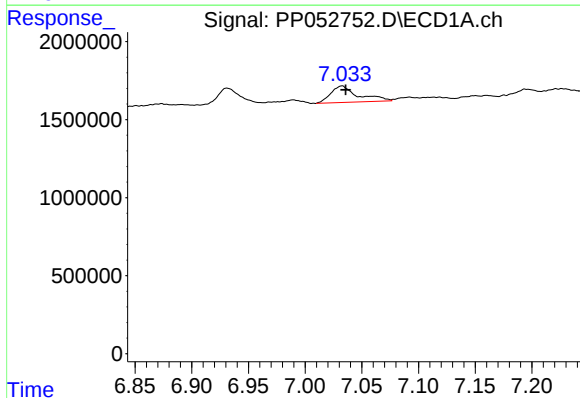


#28 AR-1254-3

R.T.: 7.032 min
Delta R.T.: -0.004 min
Response: 1769140
Conc: 15.89 ng/ml

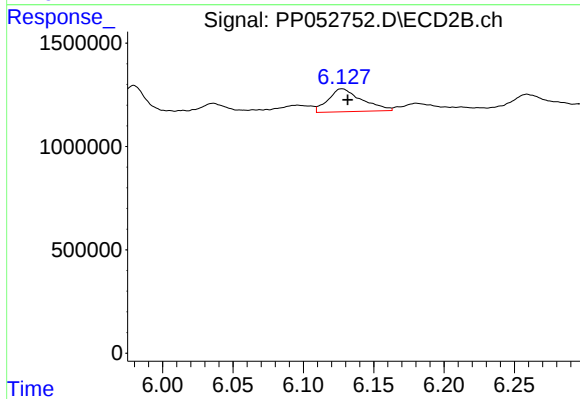

#28 AR-1254-3


R.T.: 6.127 min
Delta R.T.: -0.004 min
Response: 1838959
Conc: 12.04 ng/ml

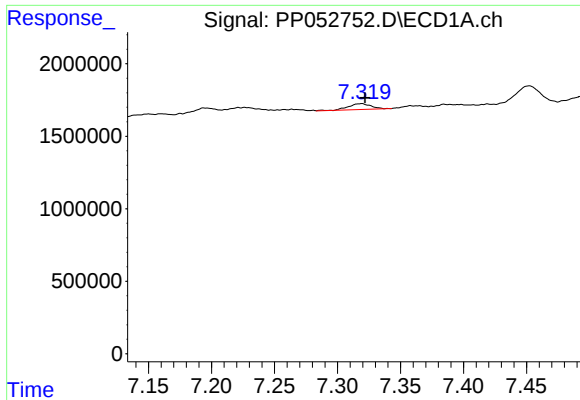

#29 AR-1254-4


R.T.: 7.318 min
Delta R.T.: -0.003 min
Response: 507856
Conc: 7.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

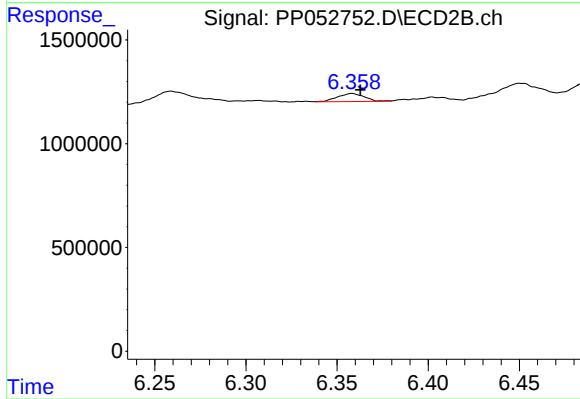


#29 AR-1254-4

R.T.: 6.358 min
Delta R.T.: -0.005 min
Response: 401525
Conc: 4.42 ng/ml

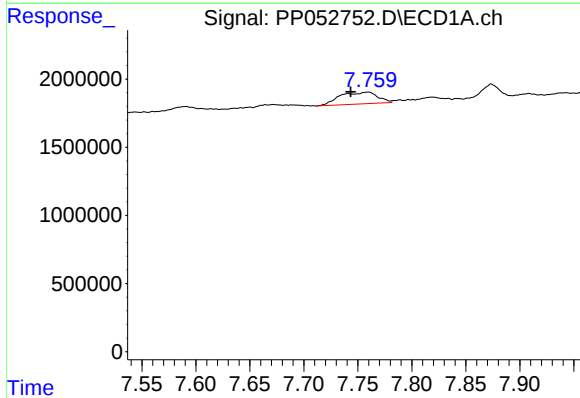


#30 AR-1254-5

R.T.: 7.758 min
Delta R.T.: 0.015 min
Response: 2090984
Conc: 26.56 ng/ml

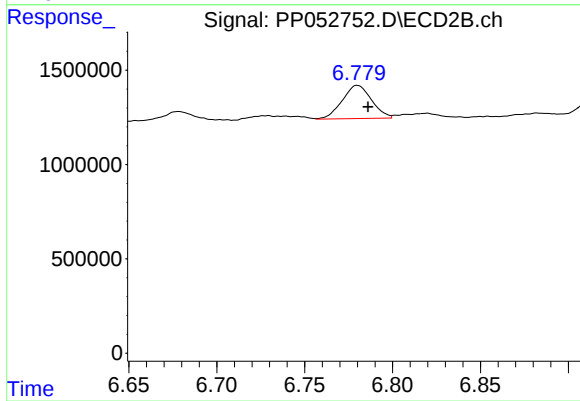

#30 AR-1254-5


R.T.: 6.780 min
Delta R.T.: -0.006 min
Response: 2042791
Conc: 14.68 ng/ml

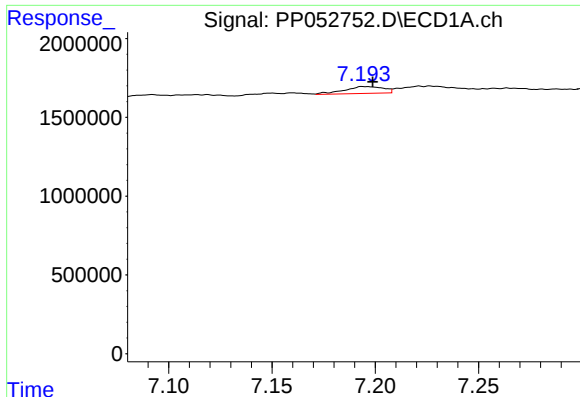

#31 AR-1260-1


R.T.: 7.196 min
Delta R.T.: -0.003 min
Response: 570235
Conc: 6.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

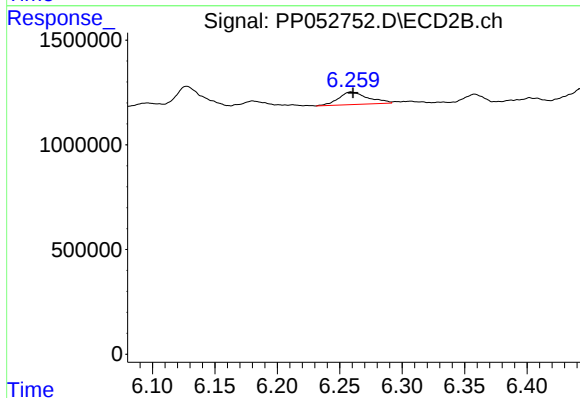


#31 AR-1260-1

R.T.: 6.259 min
Delta R.T.: -0.002 min
Response: 985403
Conc: 9.69 ng/ml

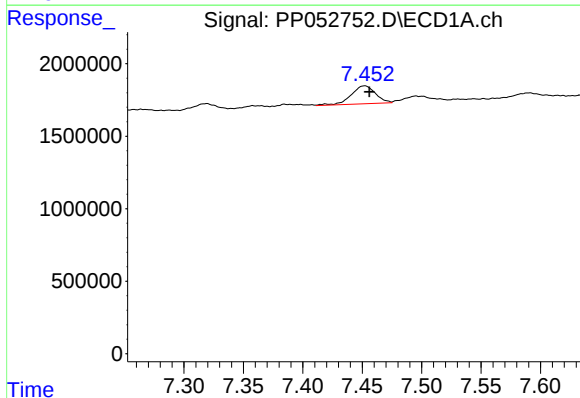


#32 AR-1260-2

R.T.: 7.452 min
Delta R.T.: -0.004 min
Response: 1756256
Conc: 18.81 ng/ml

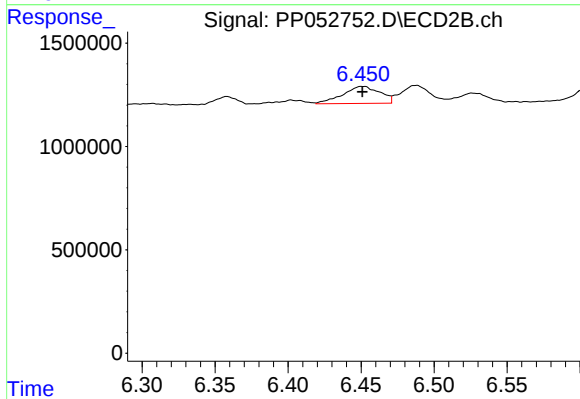

#32 AR-1260-2


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 1455220
Conc: 11.97 ng/ml

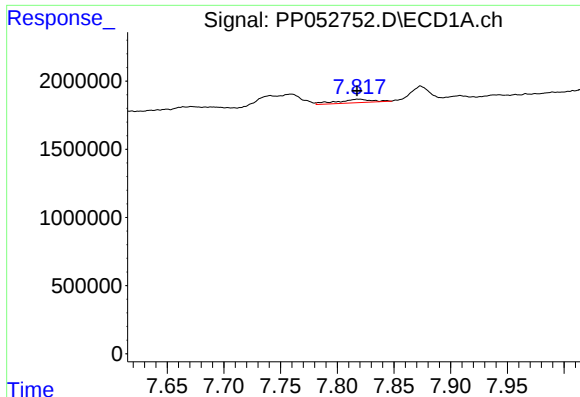

#33 AR-1260-3


R.T.: 7.819 min
Delta R.T.: 0.001 min
Response: 533844
Conc: 8.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

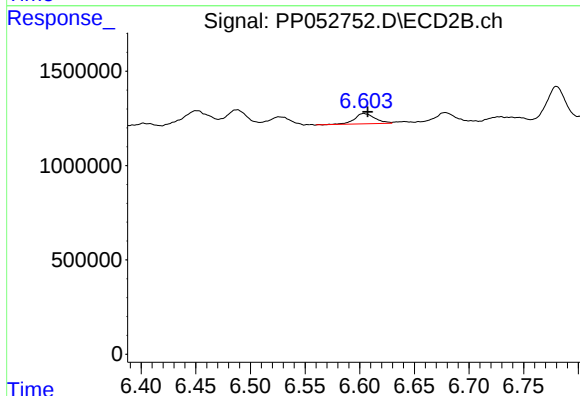


#33 AR-1260-3

R.T.: 6.604 min
Delta R.T.: -0.004 min
Response: 714350
Conc: 6.12 ng/ml

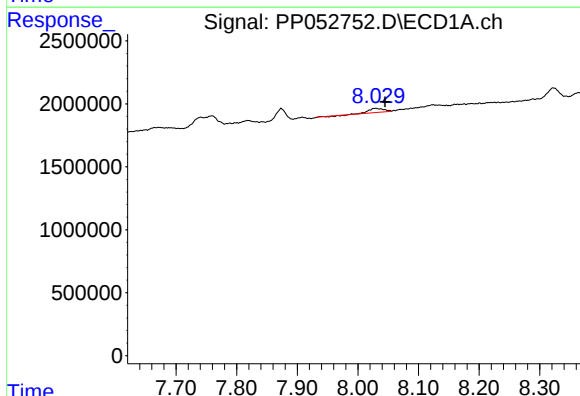


#34 AR-1260-4

R.T.: 8.029 min
Delta R.T.: -0.016 min
Response: 536320
Conc: 7.49 ng/ml

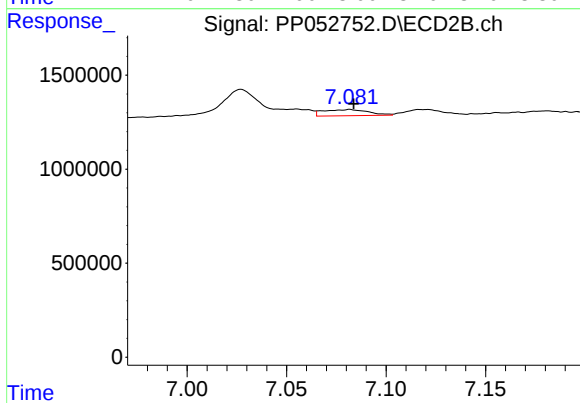

#34 AR-1260-4


R.T.: 7.082 min
Delta R.T.: -0.002 min
Response: 515840
Conc: 5.73 ng/ml

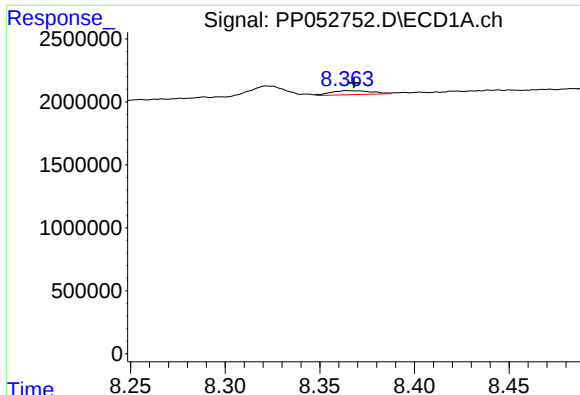

#35 AR-1260-5


R.T.: 8.366 min
Delta R.T.: -0.002 min
Response: 474371
Conc: 3.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

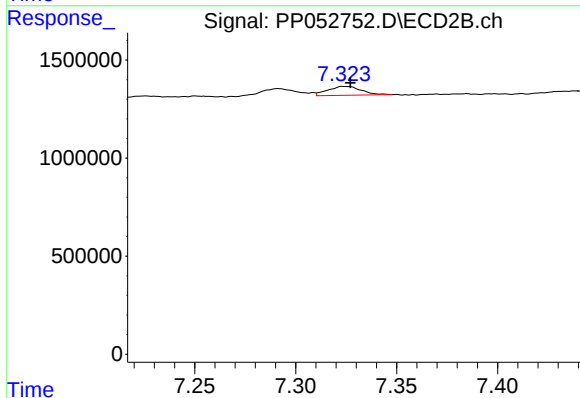


#35 AR-1260-5

R.T.: 7.324 min
Delta R.T.: -0.004 min
Response: 528238
Conc: 2.58 ng/ml

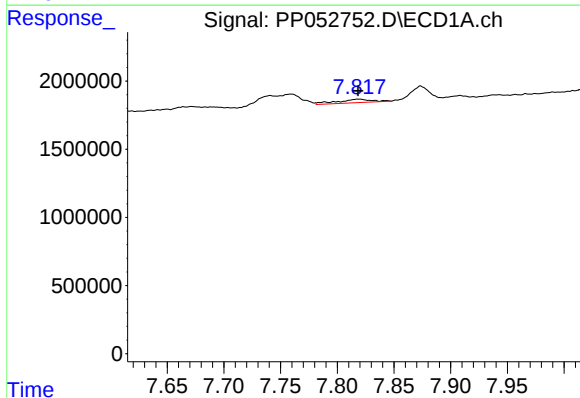


#36 AR-1262-1

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 533844
Conc: 5.57 ng/ml

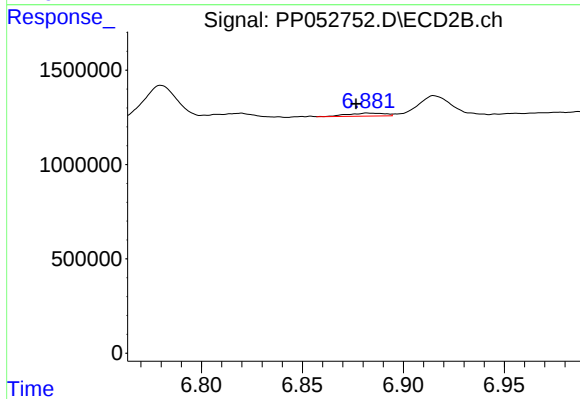

#36 AR-1262-1


R.T.: 6.882 min
Delta R.T.: 0.005 min
Response: 207917
Conc: 3.63 ng/ml

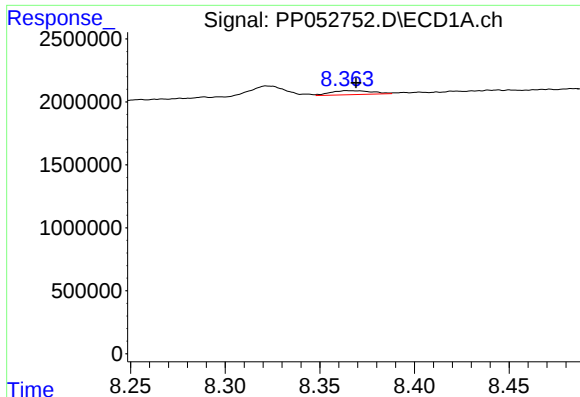

#37 AR-1262-2


R.T.: 8.366 min
Delta R.T.: -0.003 min
Response: 474371
Conc: 3.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

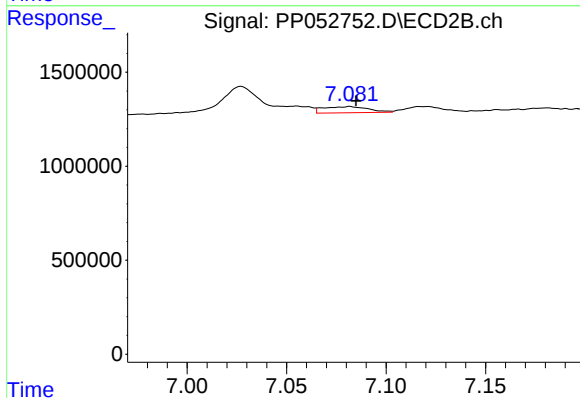


#37 AR-1262-2

R.T.: 7.082 min
Delta R.T.: -0.003 min
Response: 515840
Conc: 4.17 ng/ml

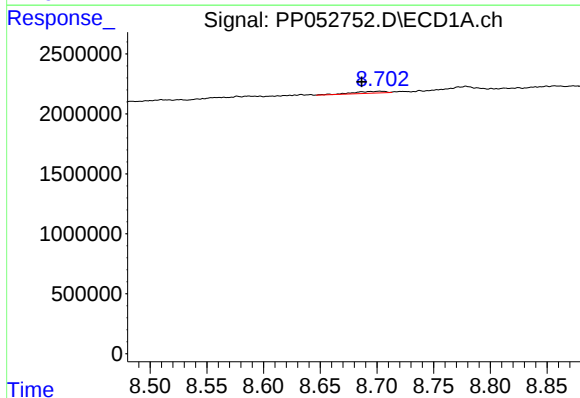


#38 AR-1262-3

R.T.: 8.703 min
Delta R.T.: 0.016 min
Response: 307249
Conc: 3.10 ng/ml

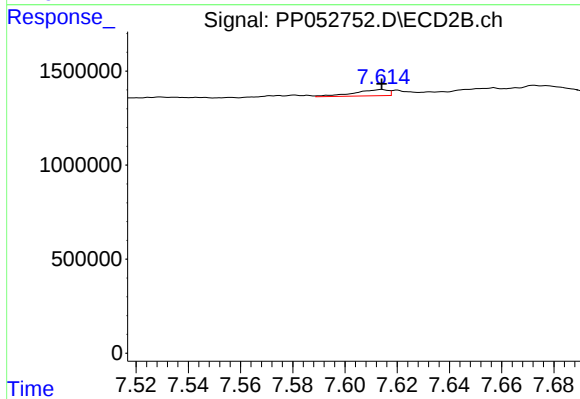

#38 AR-1262-3


R.T.: 7.614 min
Delta R.T.: 0.000 min
Response: 296567
Conc: 2.94 ng/ml

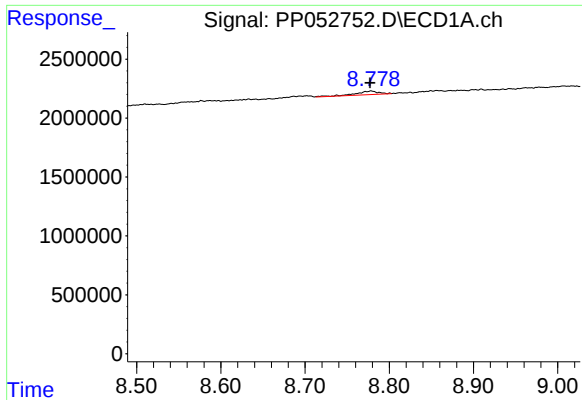

#39 AR-1262-4


R.T.: 8.778 min
Delta R.T.: 0.000 min
Response: 571035
Conc: 12.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

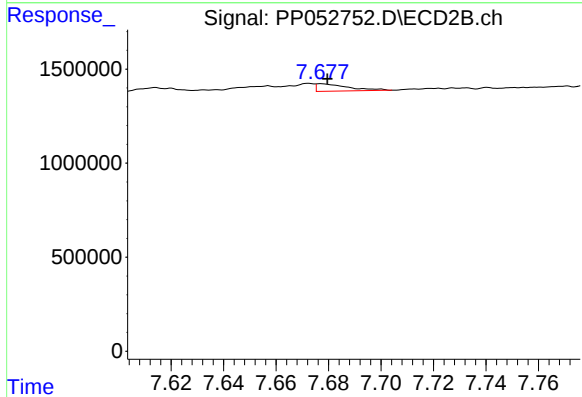


#39 AR-1262-4

R.T.: 7.677 min
Delta R.T.: -0.003 min
Response: 329496
Conc: 1.84 ng/ml

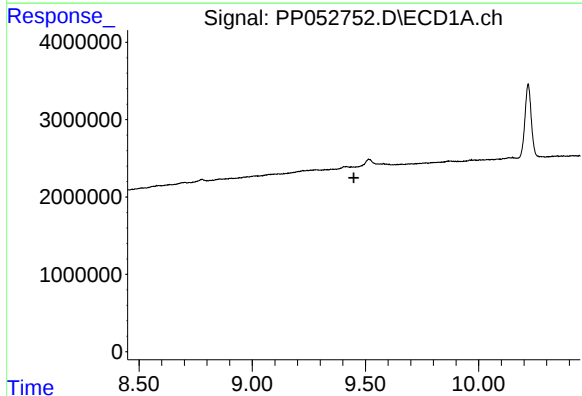


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.449 min
Response: 0
Conc: N.D.

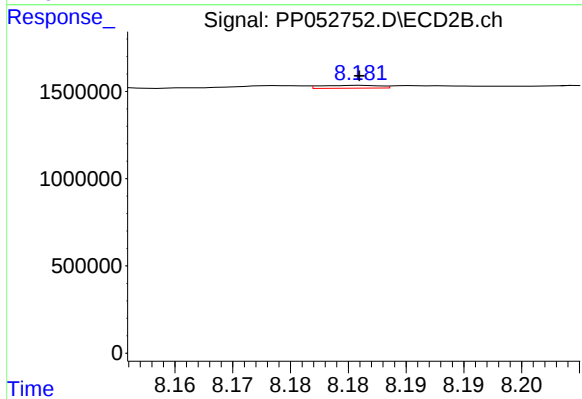

#40 AR-1262-5


R.T.: 8.181 min
Delta R.T.: 0.000 min
Response: 58146
Conc: 0.78 ng/ml

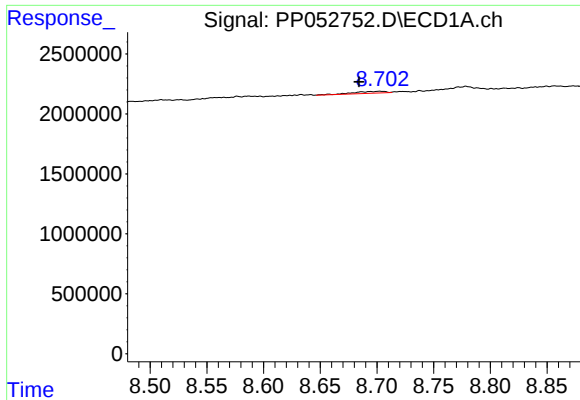

#41 AR-1268-1


R.T.: 8.703 min
Delta R.T.: 0.018 min
Response: 307249
Conc: 1.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

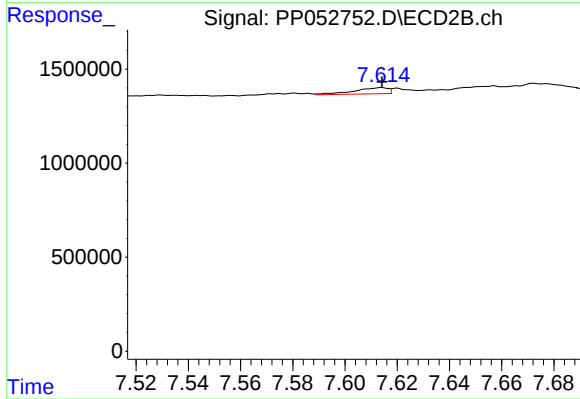


#41 AR-1268-1

R.T.: 7.614 min
Delta R.T.: 0.000 min
Response: 296567
Conc: 0.97 ng/ml

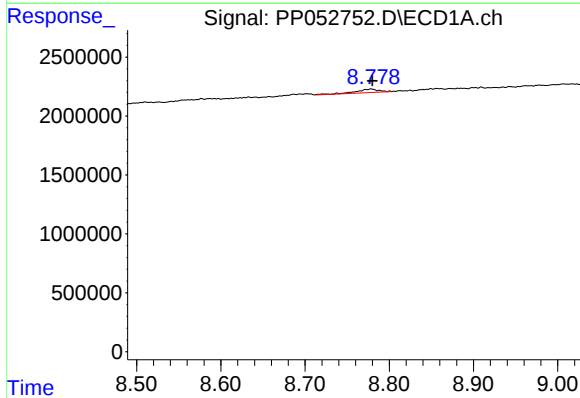


#42 AR-1268-2

R.T.: 8.778 min
Delta R.T.: -0.002 min
Response: 571035
Conc: 3.49 ng/ml

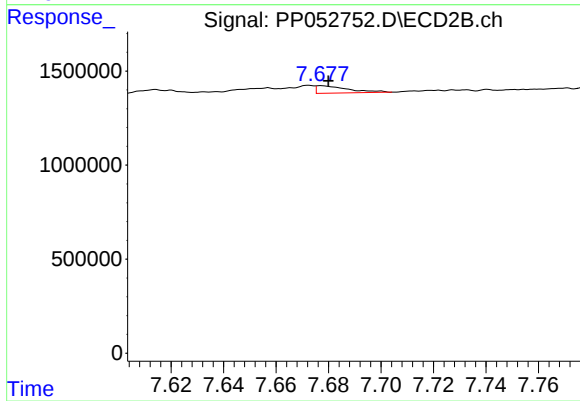

#42 AR-1268-2


R.T.: 7.677 min
Delta R.T.: -0.003 min
Response: 329496
Conc: 1.21 ng/ml

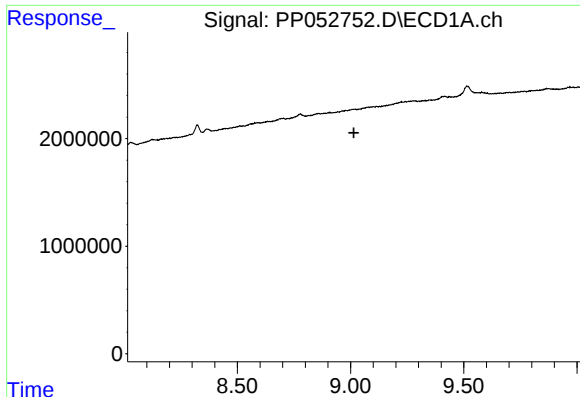

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

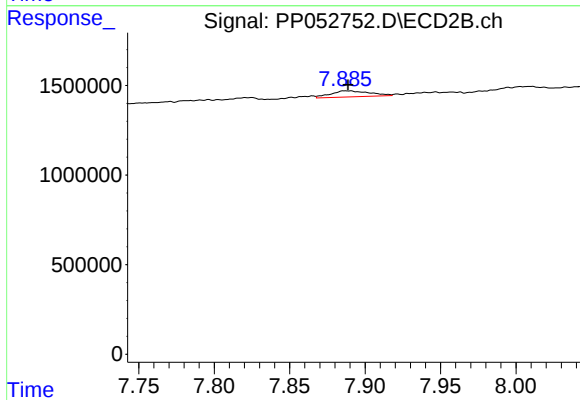


#43 AR-1268-3

R.T.: 7.891 min
Delta R.T.: 0.002 min
Response: 600016
Conc: 2.56 ng/ml

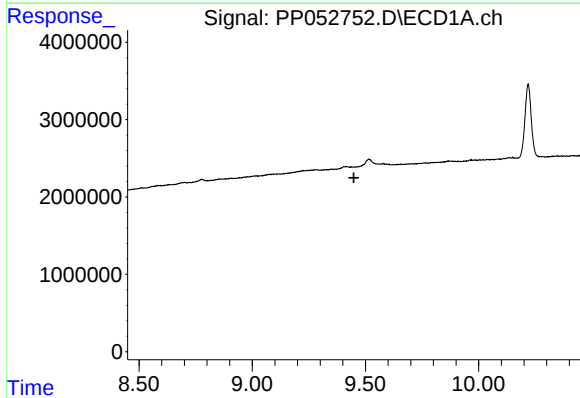


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.449 min
Response: 0
Conc: N.D.

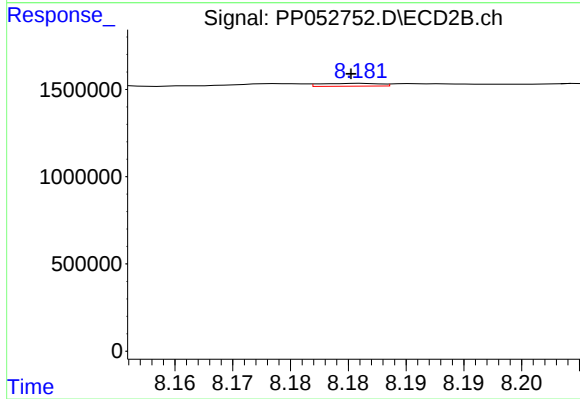

#44 AR-1268-4


R.T.: 8.181 min
Delta R.T.: 0.000 min
Response: 58146
Conc: 0.68 ng/ml

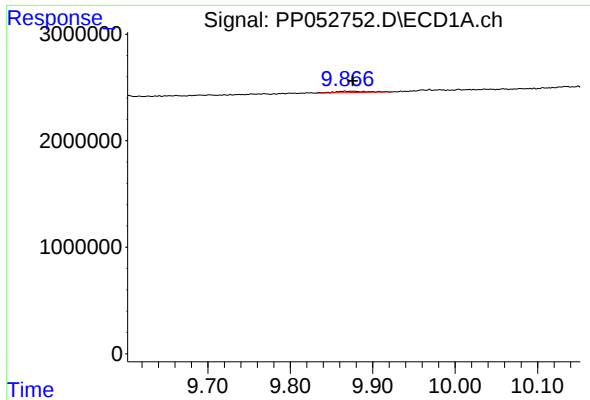

#45 AR-1268-5

R.T.: 9.867 min
Delta R.T.: -0.009 min
Response: 324040
Conc: 0.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-3

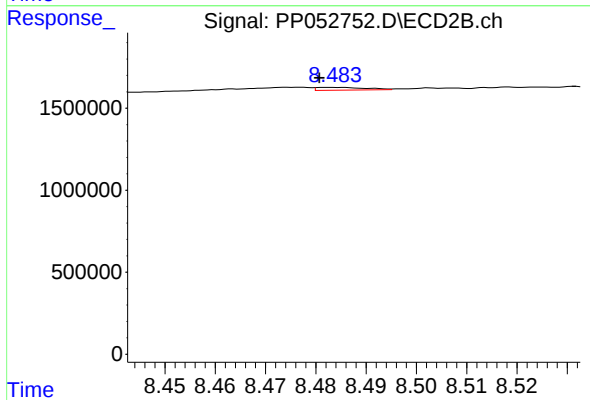

#45 AR-1268-5

R.T.: 8.483 min
Delta R.T.: 0.002 min
Response: 114029
Conc: 0.17 ng/ml