

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2022 20:00
 Operator : YP\AJ
 Sample : N5273-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LIDEN-GAS-PIPELINE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:27:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.408	3.652	46986254	43898316	21.264	23.360
2)	SA Decachlor...	10.215	8.739	33639680	42446635	26.502	25.309
Target Compounds							
3)	L1 AR-1016-1	5.583	4.754	143279	50107	2.137	0.761 #
4)	L1 AR-1016-2	5.605	4.763	317811	25573	3.182	0.279 #
5)	L1 AR-1016-3	5.658	0.000	262211	0	4.308	N.D. #
6)	L1 AR-1016-4	5.782	0.000	11667	0	0.241	N.D. #
7)	L1 AR-1016-5	6.060	0.000	99132	0	2.058	N.D. #
8)	L2 AR-1221-1	4.616	0.000	1125919	0	43.910	N.D. #
9)	L2 AR-1221-2	4.715	3.955	623949	722758	32.800	41.287 #
10)	L2 AR-1221-3	4.792	0.000	35322	0	0.620	N.D. #
11)	L3 AR-1232-1	4.792	0.000	35322	0	0.814	N.D. #
12)	L3 AR-1232-2	5.324	4.763	676504	25573	27.266	0.617 #
13)	L3 AR-1232-3	5.605	0.000	317811	0	7.260	N.D. #
14)	L3 AR-1232-4	5.782	0.000	11667	0	0.547	N.D. #
15)	L3 AR-1232-5	5.853	0.000	108763	0	6.319	N.D. #
16)	L4 AR-1242-1	5.583	4.754	143279	50107	2.546	0.898 #
17)	L4 AR-1242-2	5.605	4.763	317811	25573	3.847	0.332 #
18)	L4 AR-1242-3	5.658	0.000	262211	0	5.156	N.D. #
19)	L4 AR-1242-4	5.782	0.000	11667	0	0.288	N.D. #
20)	L4 AR-1242-5	6.511	5.567	668530	377919	16.769	7.476 #
21)	L5 AR-1248-1	5.583	4.754	143279	50107	3.528	1.252 #
22)	L5 AR-1248-2	5.853	0.000	108763	0	1.827	N.D. #
23)	L5 AR-1248-3	6.060	0.000	99132	0	1.527	N.D. #
24)	L5 AR-1248-4	6.464	0.000	460238	0	7.146	N.D. #
25)	L5 AR-1248-5	6.511	0.000	668530	0	10.553	N.D. #
26)	L6 AR-1254-1	6.443	5.567	574781	377919	7.572	3.519 #
27)	L6 AR-1254-2	6.661	5.718	2043939	437474	18.288	4.577 #
28)	L6 AR-1254-3	7.040	6.144	4467239	6292357	40.133	41.184
29)	L6 AR-1254-4	7.326	6.357	85200	1867735	1.210	20.571 #
30)	L6 AR-1254-5	7.757	6.779	2428267	3652875	30.842	26.255
31)	L7 AR-1260-1	7.194	6.258	731525	1278603	8.563	12.571 #
32)	L7 AR-1260-2	7.442	6.450	7823230	1310383	83.777	10.775 #
33)	L7 AR-1260-3	7.817	6.606	133687	457513	2.116	3.922 #
34)	L7 AR-1260-4	8.024f	7.082	749322	172297	10.465	1.914 #
35)	L7 AR-1260-5	8.364	7.325	379929	469100	2.989	2.290
36)	L8 AR-1262-1	7.817	6.878	133687	68306	1.395	1.193
37)	L8 AR-1262-2	8.364	7.082	379929	172297	2.554	1.391 #
38)	L8 AR-1262-3	8.687	7.614	179978	869218	1.814	8.613 #
39)	L8 AR-1262-4	8.775	7.676	561490	708446	12.052	3.959 #
40)	L8 AR-1262-5	9.449	8.199f	173177	279461	3.784	3.732
41)	L9 AR-1268-1	8.687	7.614	179978	869218	0.957	2.836 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2022 20:00
 Operator : YP\AJ
 Sample : N5273-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LIDEN-GAS-PIPELINE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:27:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.775	7.676	561490	708446	3.431	2.612
43) L9	AR-1268-3	9.017	7.892	140311	162051	0.926	0.691 #
44) L9	AR-1268-4	9.449	8.199f	173177	279461	3.405	3.290
45) L9	AR-1268-5	9.873	8.479	328154	231829	0.764	0.354 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052765.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2022 20:00
Operator : YP\AJ
Sample : N5273-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:27:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

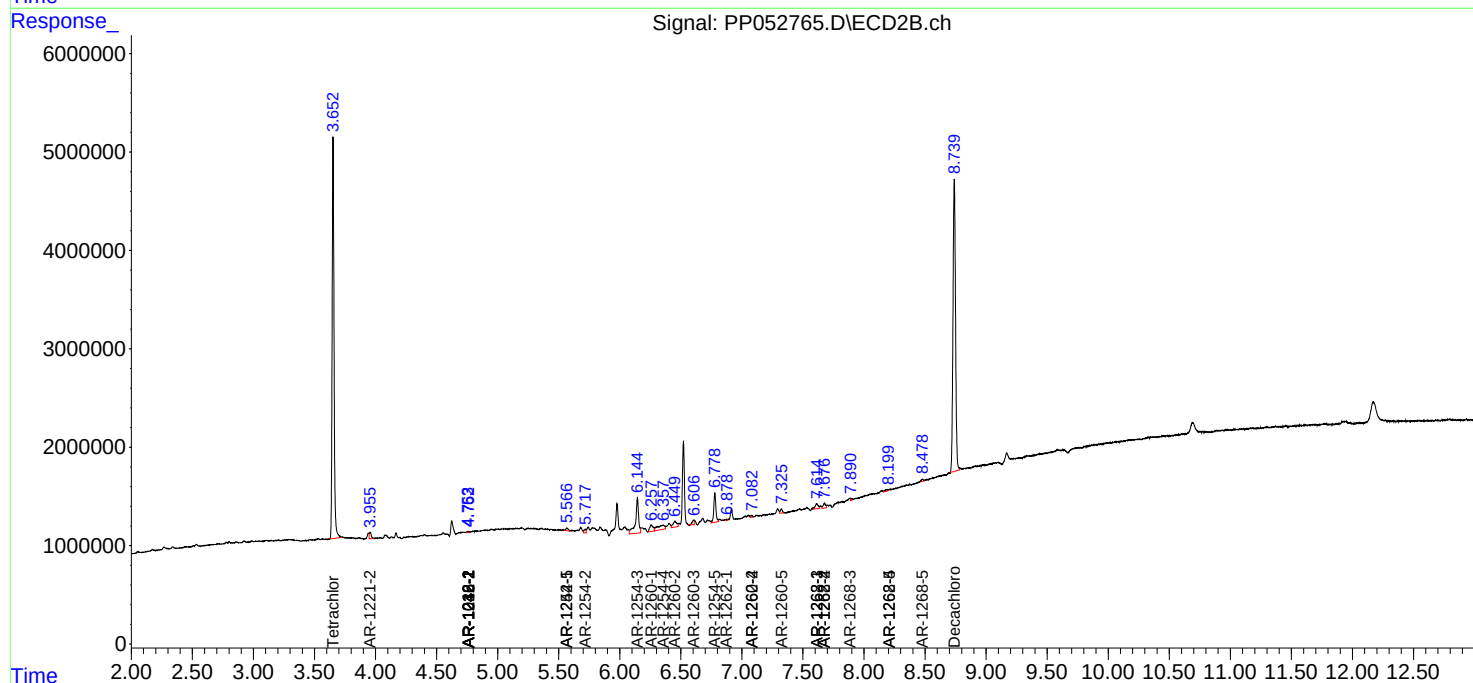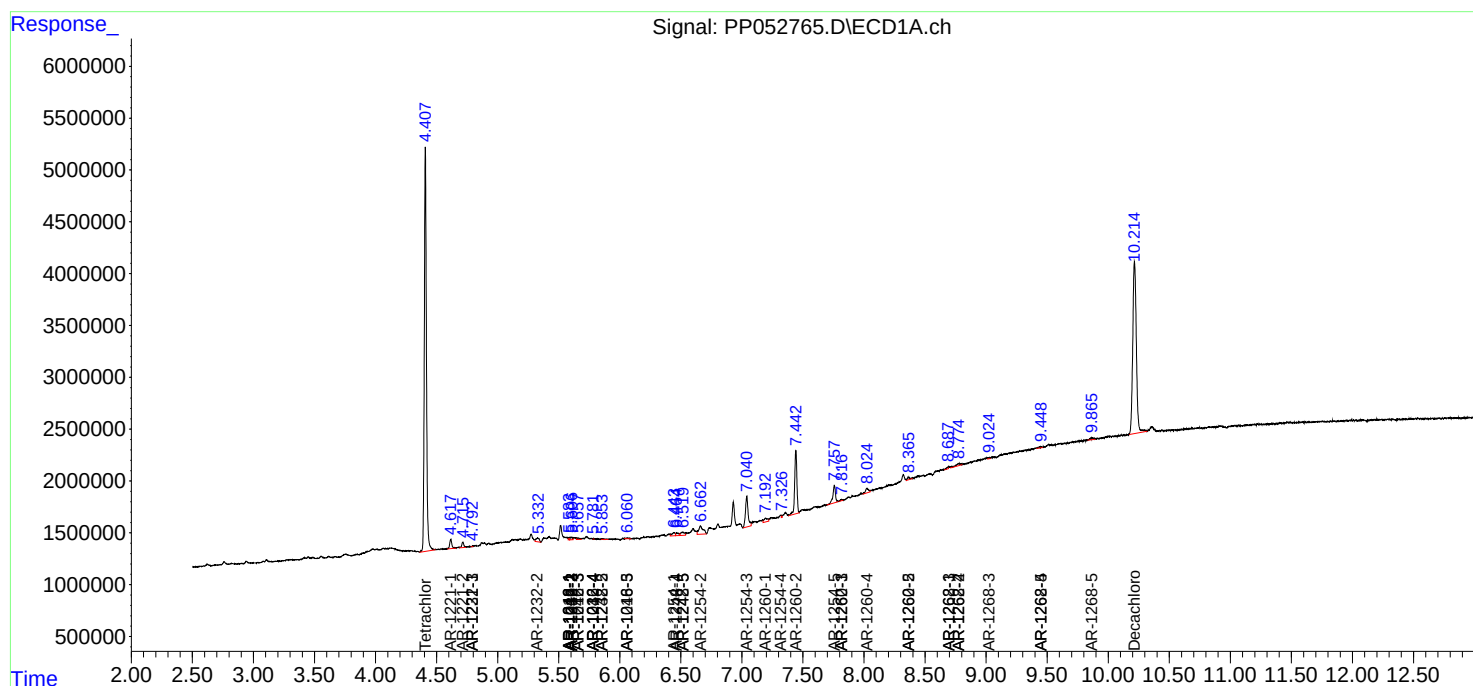


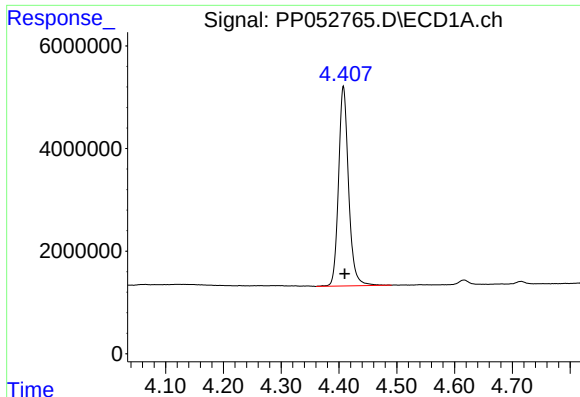

#1 Tetrachloro-m-xylene


R.T.: 4.408 min
Delta R.T.: -0.002 min
Response: 46986254
Conc: 21.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

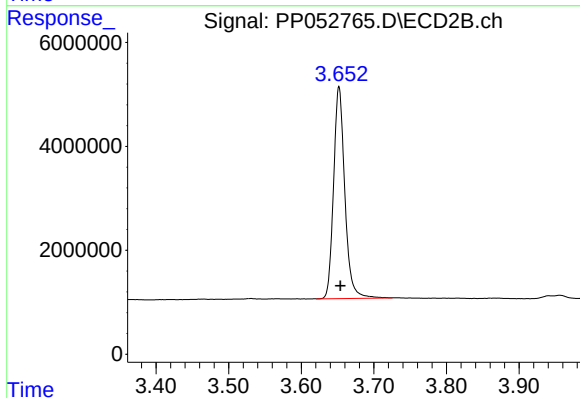


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.002 min
Response: 43898316
Conc: 23.36 ng/ml

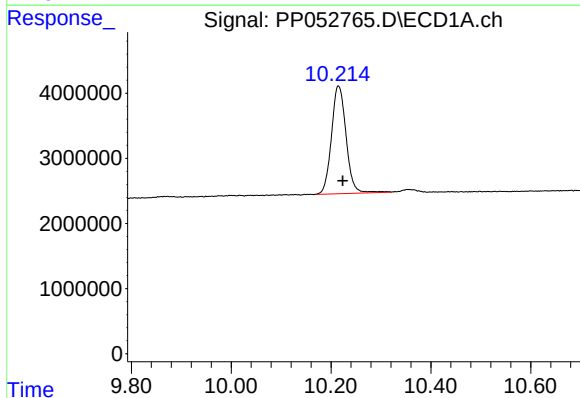


#2 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: -0.009 min
Response: 33639680
Conc: 26.50 ng/ml

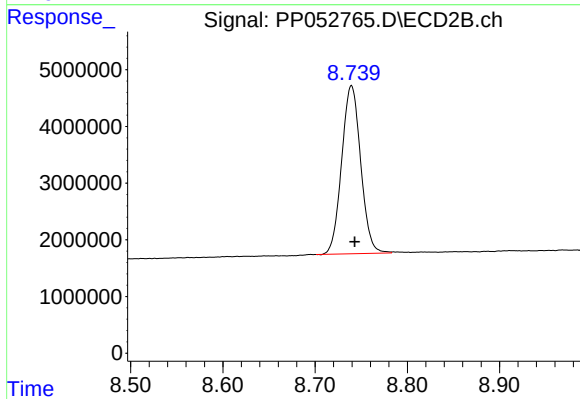

#2 Decachlorobiphenyl


R.T.: 8.739 min
Delta R.T.: -0.003 min
Response: 42446635
Conc: 25.31 ng/ml

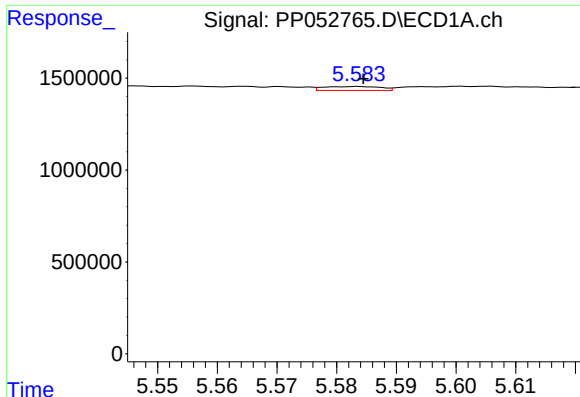

#3 AR-1016-1


R.T.: 5.583 min
Delta R.T.: -0.001 min
Response: 143279
Conc: 2.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

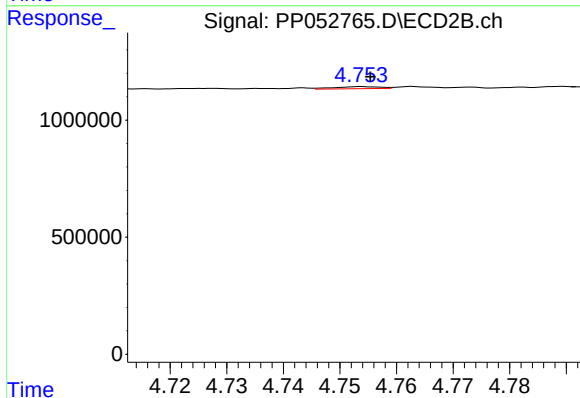


#3 AR-1016-1

R.T.: 4.754 min
Delta R.T.: -0.002 min
Response: 50107
Conc: 0.76 ng/ml

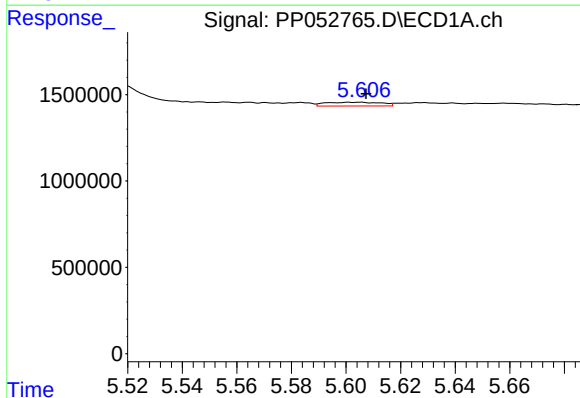


#4 AR-1016-2

R.T.: 5.605 min
Delta R.T.: -0.002 min
Response: 317811
Conc: 3.18 ng/ml

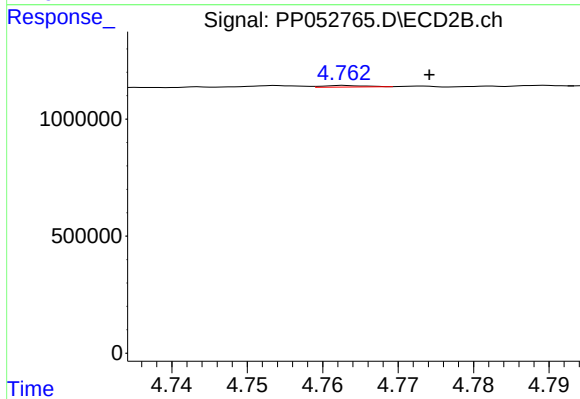

#4 AR-1016-2


R.T.: 4.763 min
Delta R.T.: -0.011 min
Response: 25573
Conc: 0.28 ng/ml

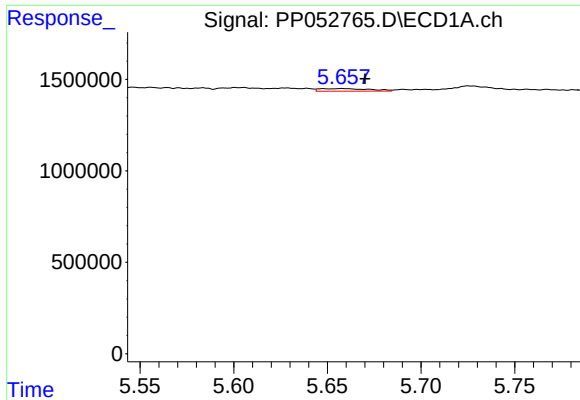

#5 AR-1016-3


R.T.: 5.658 min
Delta R.T.: -0.012 min
Response: 262211
Conc: 4.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

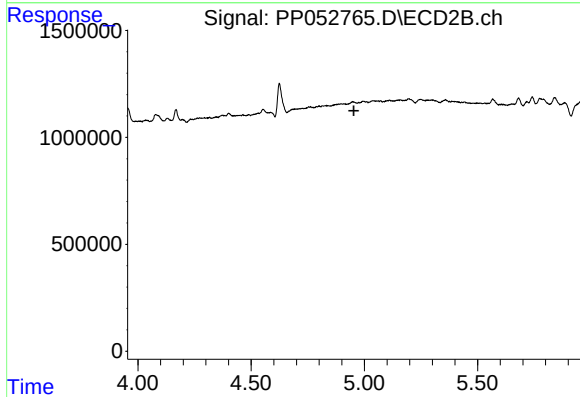


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

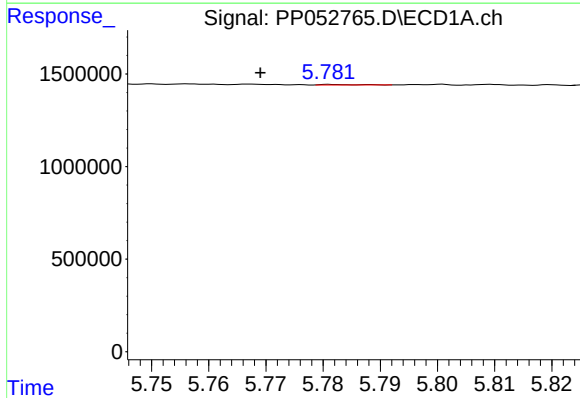


#6 AR-1016-4

R.T.: 5.782 min
Delta R.T.: 0.013 min
Response: 11667
Conc: 0.24 ng/ml

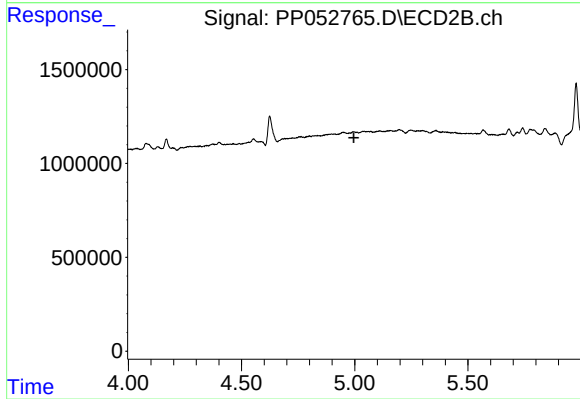

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.996 min
Response: 0
Conc: N.D.

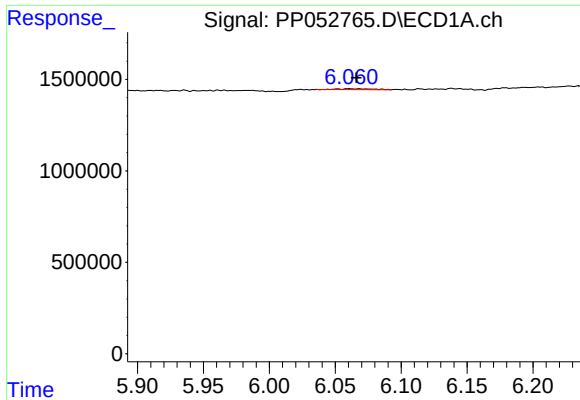

#7 AR-1016-5


R.T.: 6.060 min
Delta R.T.: -0.006 min
Response: 99132
Conc: 2.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

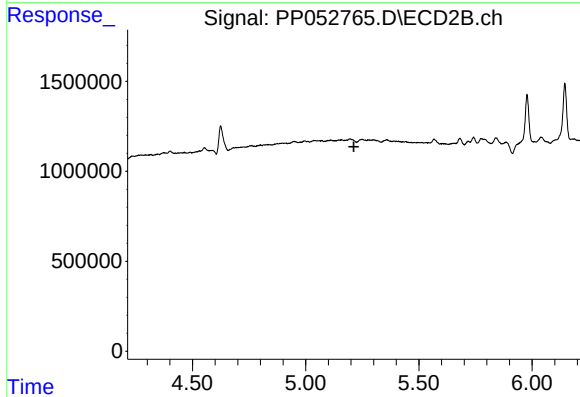


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

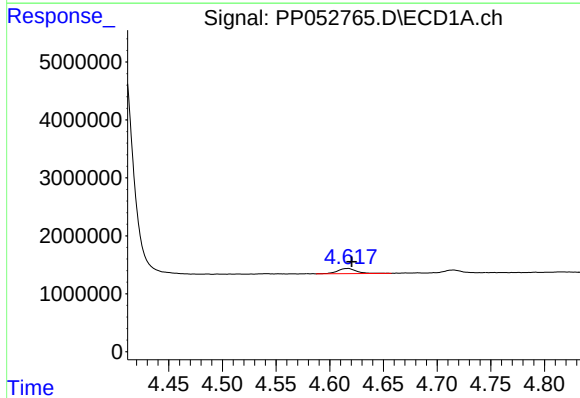


#8 AR-1221-1

R.T.: 4.616 min
Delta R.T.: -0.004 min
Response: 1125919
Conc: 43.91 ng/ml

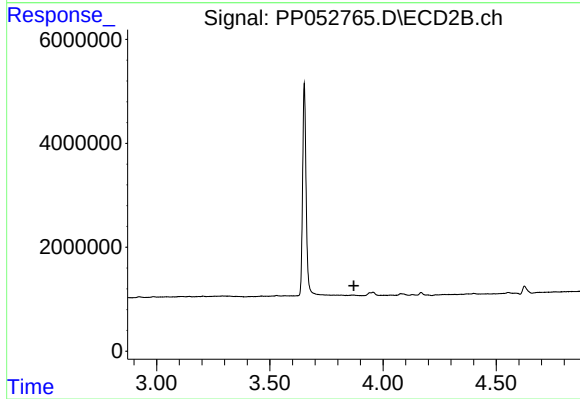

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.872 min
Response: 0
Conc: N.D.

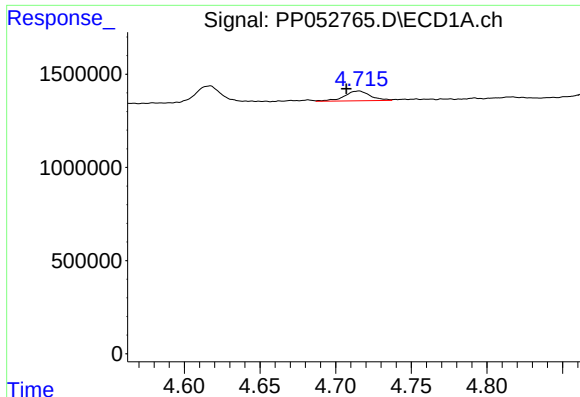

#9 AR-1221-2


R.T.: 4.715 min
Delta R.T.: 0.008 min
Response: 623949
Conc: 32.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

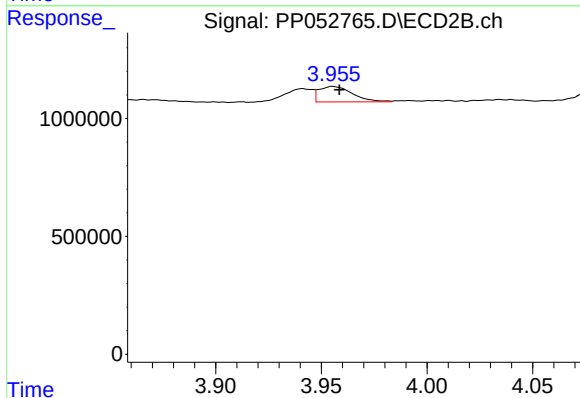


#9 AR-1221-2

R.T.: 3.955 min
Delta R.T.: -0.003 min
Response: 722758
Conc: 41.29 ng/ml

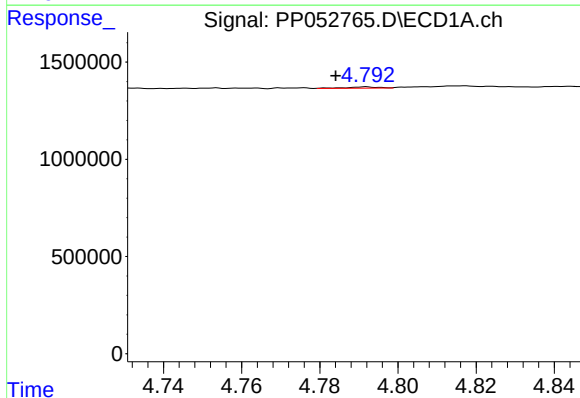


#10 AR-1221-3

R.T.: 4.792 min
Delta R.T.: 0.008 min
Response: 35322
Conc: 0.62 ng/ml

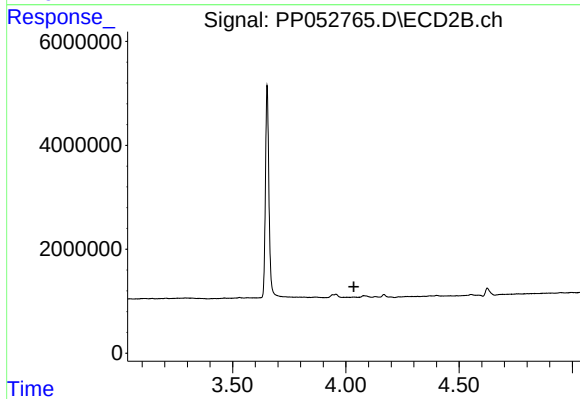

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.036 min
Response: 0
Conc: N.D.

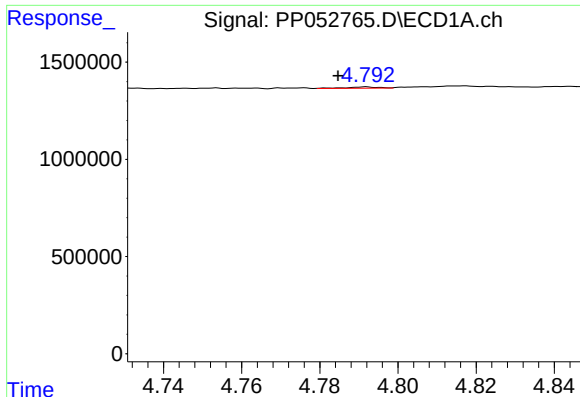

#11 AR-1232-1


R.T.: 4.792 min
Delta R.T.: 0.007 min
Response: 35322
Conc: 0.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

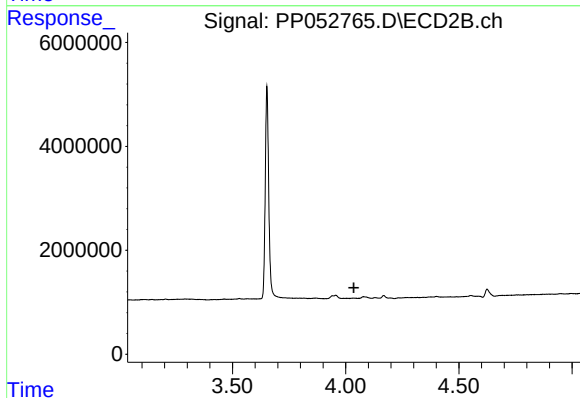


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.036 min
Response: 0
Conc: N.D.

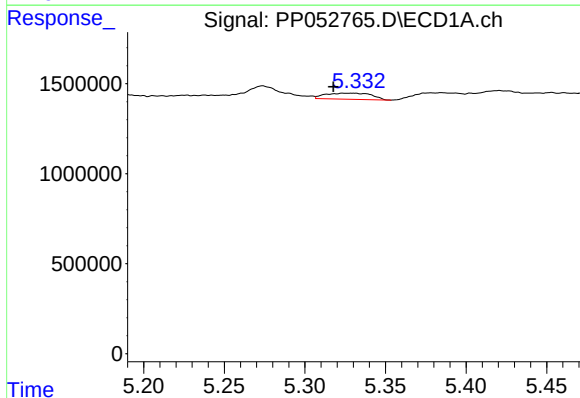


#12 AR-1232-2

R.T.: 5.324 min
Delta R.T.: 0.007 min
Response: 676504
Conc: 27.27 ng/ml

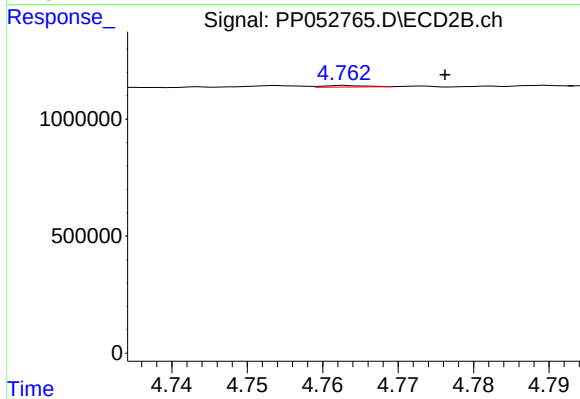

#12 AR-1232-2


R.T.: 4.763 min
Delta R.T.: -0.013 min
Response: 25573
Conc: 0.62 ng/ml

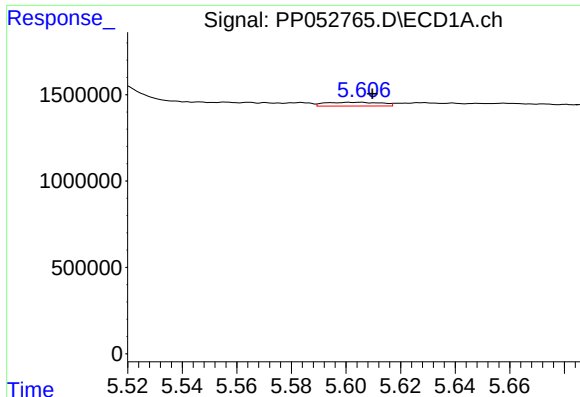

#13 AR-1232-3


R.T.: 5.605 min
Delta R.T.: -0.005 min
Response: 317811
Conc: 7.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

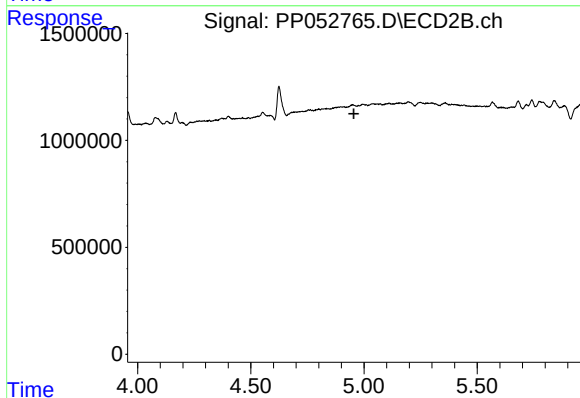


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.955 min
Response: 0
Conc: N.D.

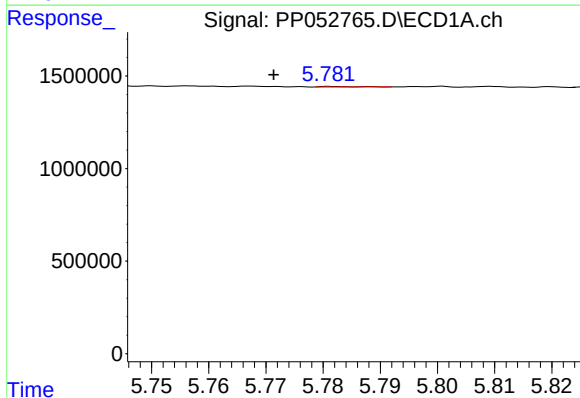


#14 AR-1232-4

R.T.: 5.782 min
Delta R.T.: 0.010 min
Response: 11667
Conc: 0.55 ng/ml

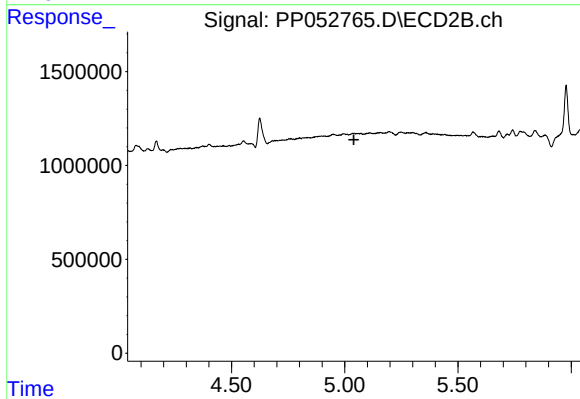

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.040 min
Response: 0
Conc: N.D.

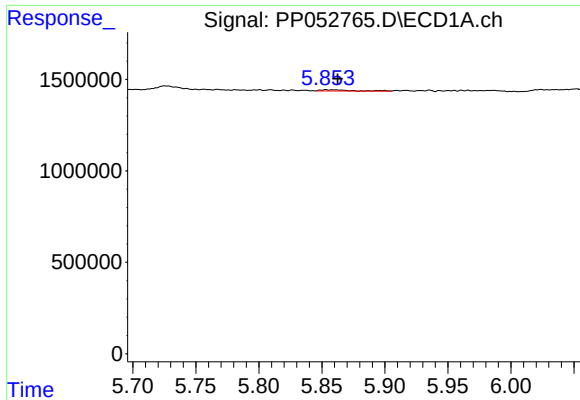

#15 AR-1232-5


R.T.: 5.853 min
Delta R.T.: -0.009 min
Response: 108763
Conc: 6.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

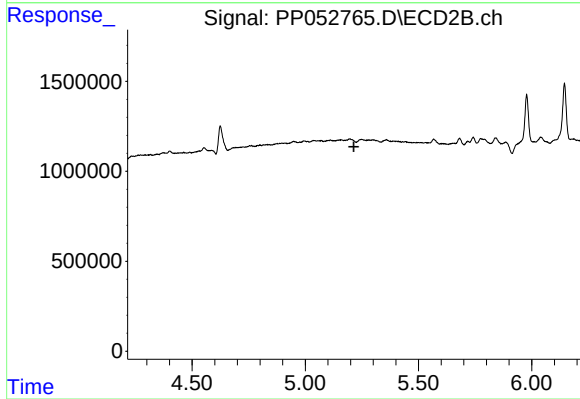


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.215 min
Response: 0
Conc: N.D.

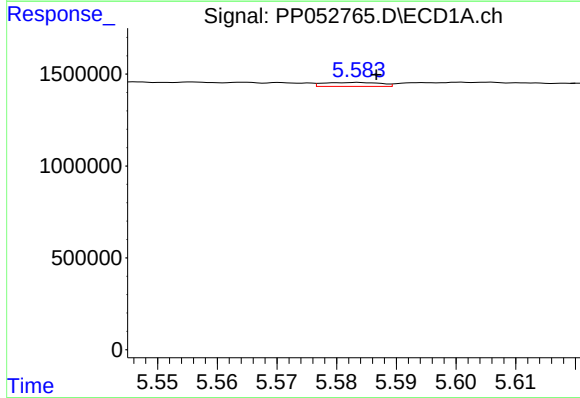


#16 AR-1242-1

R.T.: 5.583 min
Delta R.T.: -0.003 min
Response: 143279
Conc: 2.55 ng/ml

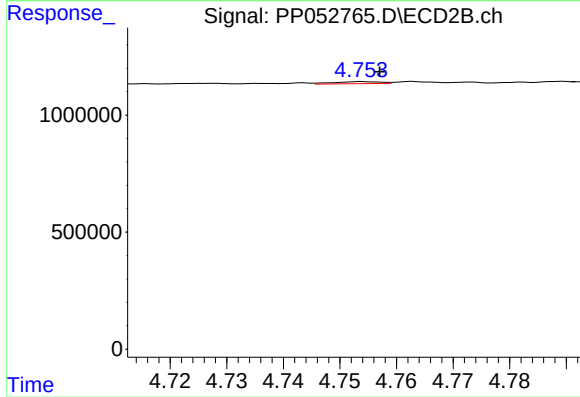

#16 AR-1242-1


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 50107
Conc: 0.90 ng/ml

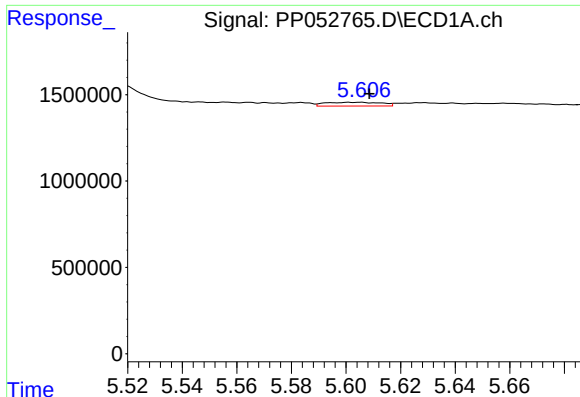

#17 AR-1242-2


R.T.: 5.605 min
Delta R.T.: -0.004 min
Response: 317811
Conc: 3.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

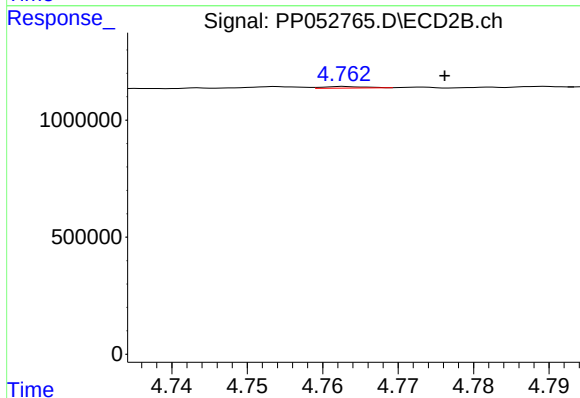


#17 AR-1242-2

R.T.: 4.763 min
Delta R.T.: -0.013 min
Response: 25573
Conc: 0.33 ng/ml

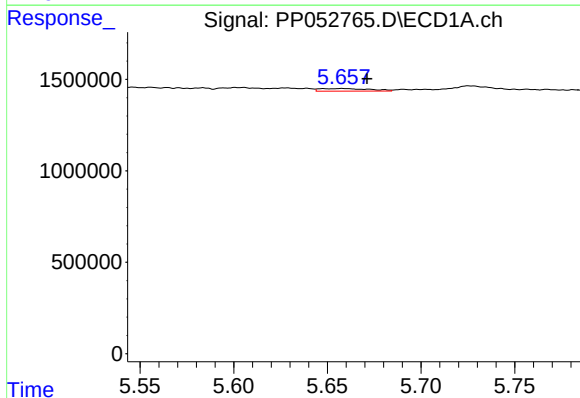


#18 AR-1242-3

R.T.: 5.658 min
Delta R.T.: -0.013 min
Response: 262211
Conc: 5.16 ng/ml

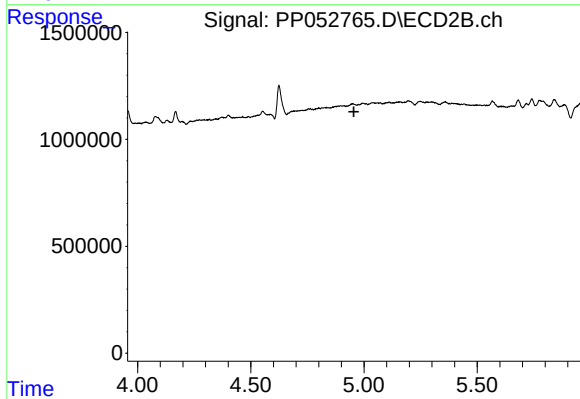

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

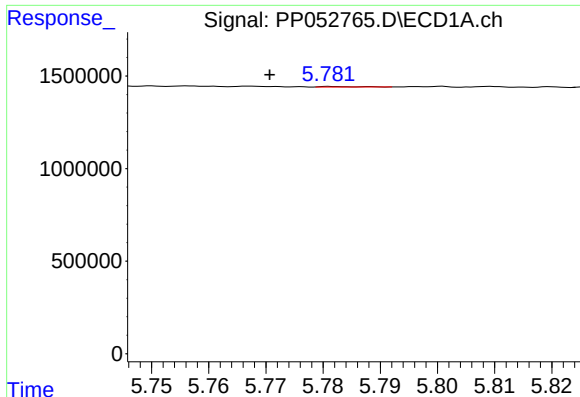

#19 AR-1242-4


R.T.: 5.782 min
Delta R.T.: 0.011 min
Response: 11667
Conc: 0.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

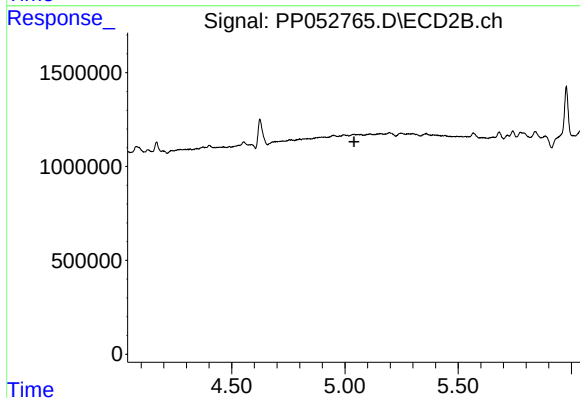


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.040 min
Response: 0
Conc: N.D.

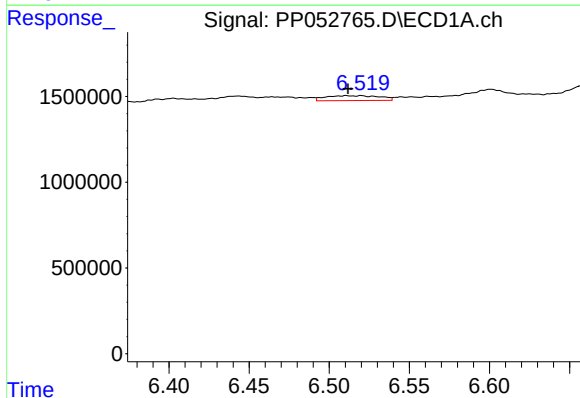


#20 AR-1242-5

R.T.: 6.511 min
Delta R.T.: 0.000 min
Response: 668530
Conc: 16.77 ng/ml

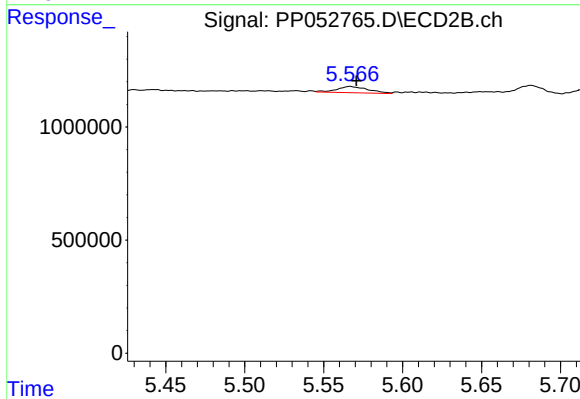

#20 AR-1242-5


R.T.: 5.567 min
Delta R.T.: -0.004 min
Response: 377919
Conc: 7.48 ng/ml

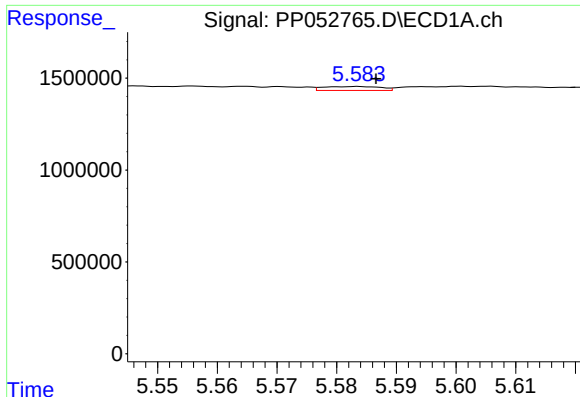

#21 AR-1248-1


R.T.: 5.583 min
Delta R.T.: -0.003 min
Response: 143279
Conc: 3.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

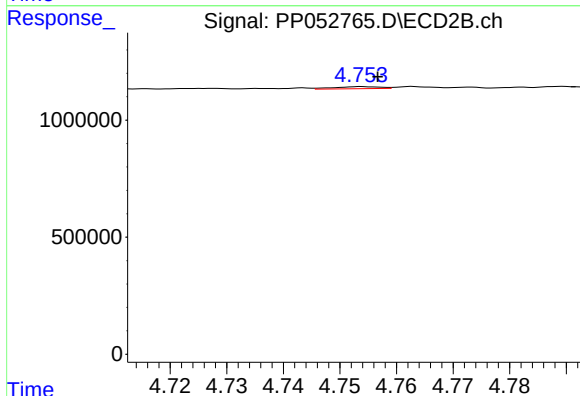


#21 AR-1248-1

R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 50107
Conc: 1.25 ng/ml

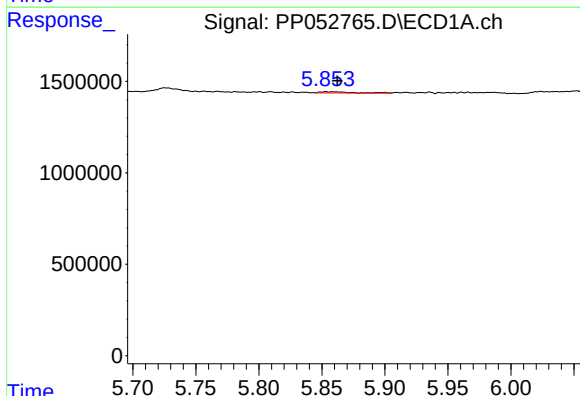


#22 AR-1248-2

R.T.: 5.853 min
Delta R.T.: -0.009 min
Response: 108763
Conc: 1.83 ng/ml

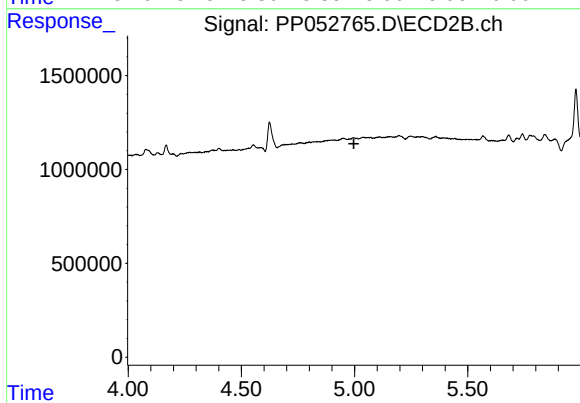

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 4.997 min
Response: 0
Conc: N.D.

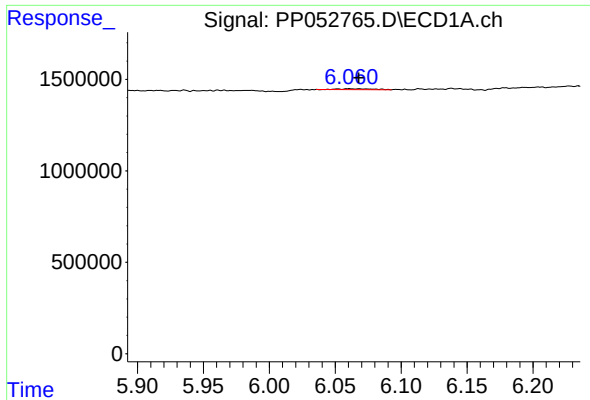

#23 AR-1248-3


R.T.: 6.060 min
Delta R.T.: -0.008 min
Response: 99132
Conc: 1.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

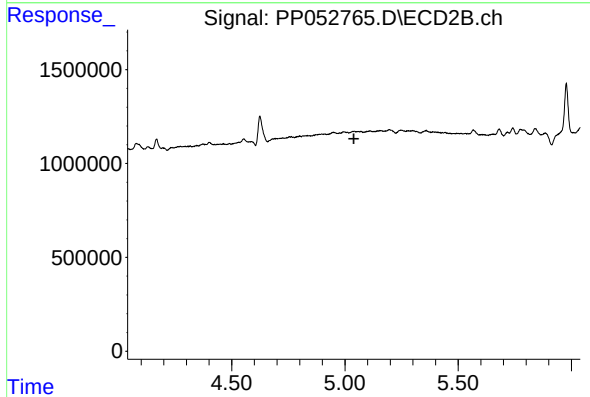


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.039 min
Response: 0
Conc: N.D.

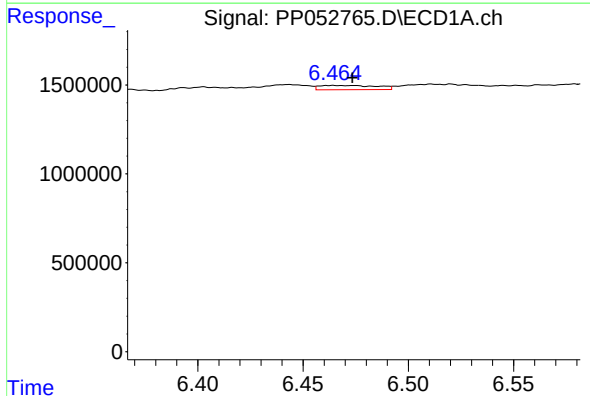


#24 AR-1248-4

R.T.: 6.464 min
Delta R.T.: -0.010 min
Response: 460238
Conc: 7.15 ng/ml

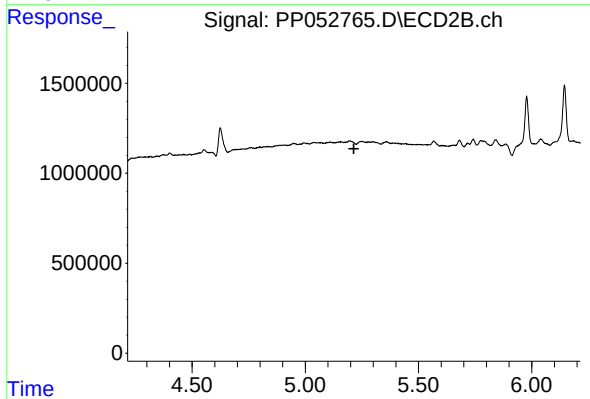

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.215 min
Response: 0
Conc: N.D.

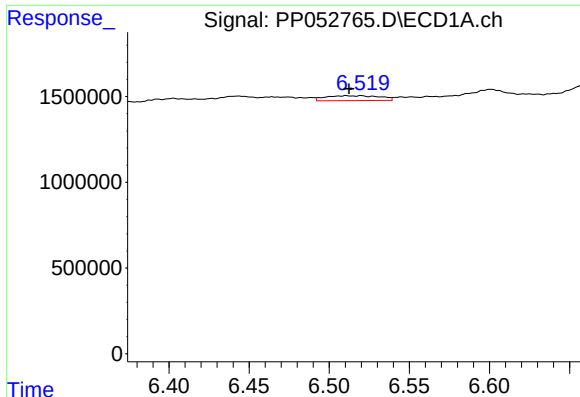

#25 AR-1248-5


R.T.: 6.511 min
Delta R.T.: -0.002 min
Response: 668530
Conc: 10.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

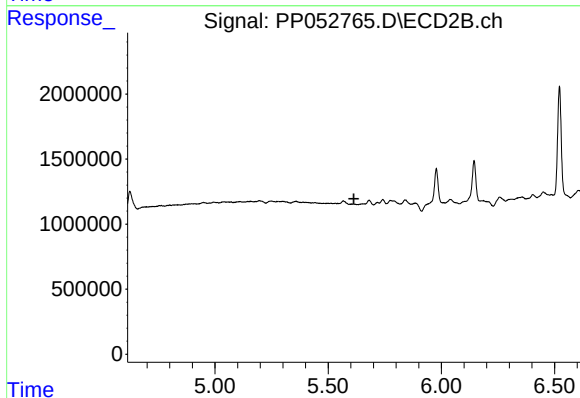


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.613 min
Response: 0
Conc: N.D.

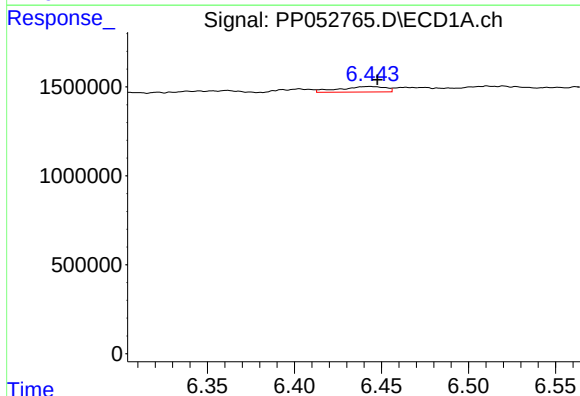


#26 AR-1254-1

R.T.: 6.443 min
Delta R.T.: -0.004 min
Response: 574781
Conc: 7.57 ng/ml

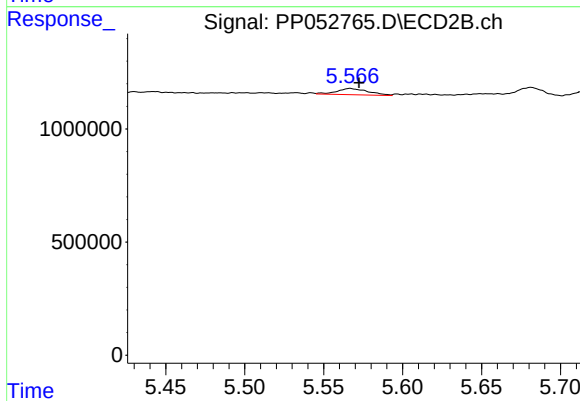

#26 AR-1254-1


R.T.: 5.567 min
Delta R.T.: -0.006 min
Response: 377919
Conc: 3.52 ng/ml

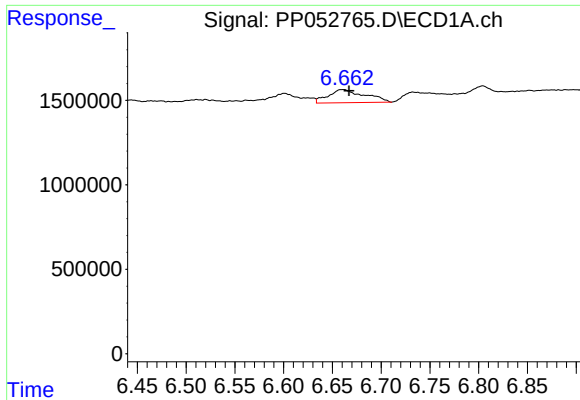

#27 AR-1254-2


R.T.: 6.661 min
Delta R.T.: -0.006 min
Response: 2043939
Conc: 18.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

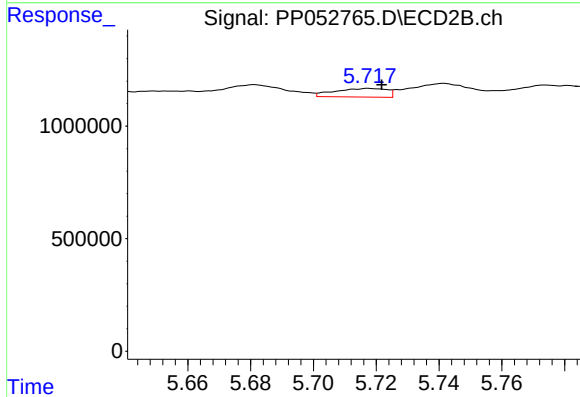


#27 AR-1254-2

R.T.: 5.718 min
Delta R.T.: -0.004 min
Response: 437474
Conc: 4.58 ng/ml

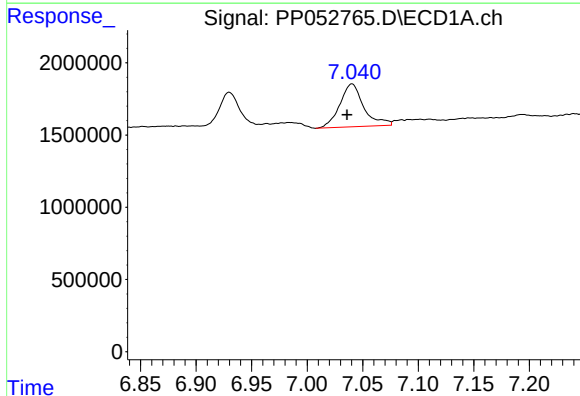


#28 AR-1254-3

R.T.: 7.040 min
Delta R.T.: 0.004 min
Response: 4467239
Conc: 40.13 ng/ml

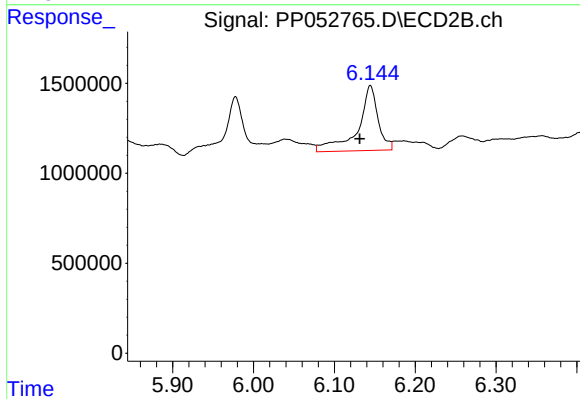

#28 AR-1254-3


R.T.: 6.144 min
Delta R.T.: 0.013 min
Response: 6292357
Conc: 41.18 ng/ml

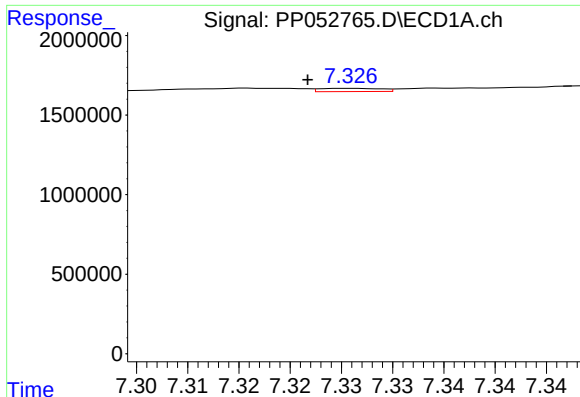

#29 AR-1254-4


R.T.: 7.326 min
Delta R.T.: 0.004 min
Response: 85200
Conc: 1.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

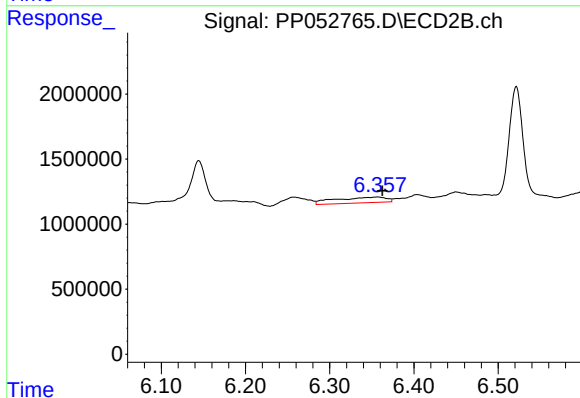


#29 AR-1254-4

R.T.: 6.357 min
Delta R.T.: -0.006 min
Response: 1867735
Conc: 20.57 ng/ml

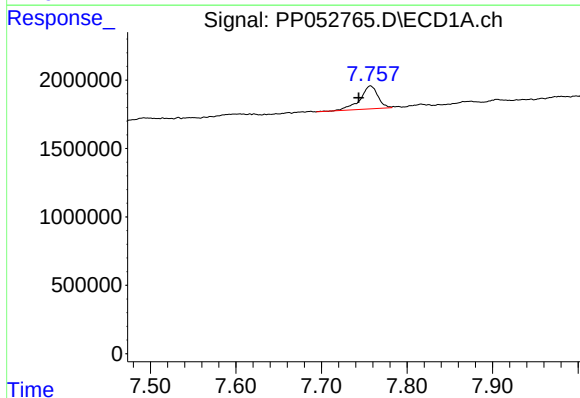


#30 AR-1254-5

R.T.: 7.757 min
Delta R.T.: 0.014 min
Response: 2428267
Conc: 30.84 ng/ml

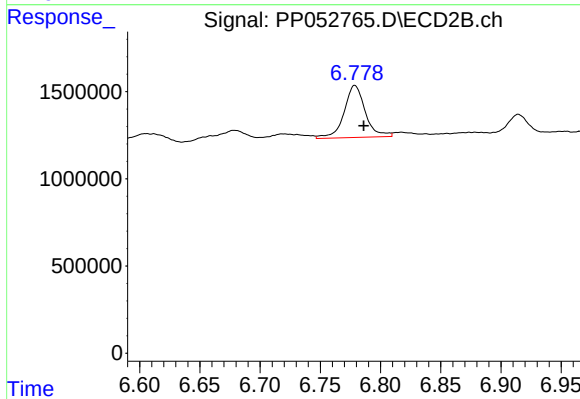

#30 AR-1254-5


R.T.: 6.779 min
Delta R.T.: -0.007 min
Response: 3652875
Conc: 26.26 ng/ml

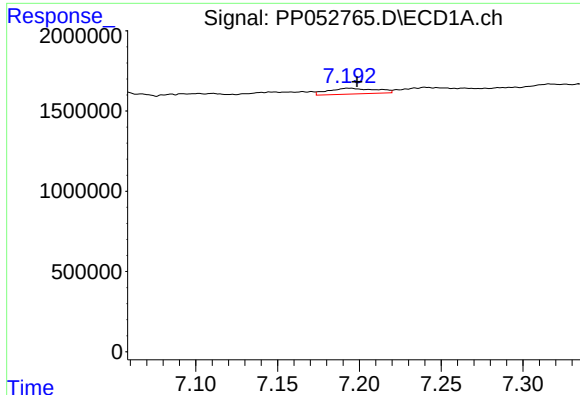

#31 AR-1260-1


R.T.: 7.194 min
Delta R.T.: -0.005 min
Response: 731525
Conc: 8.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

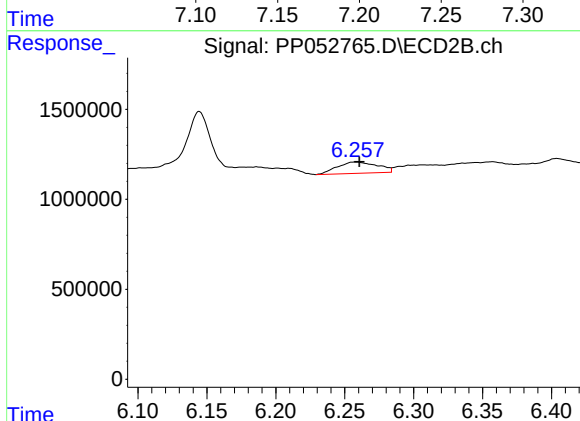


#31 AR-1260-1

R.T.: 6.258 min
Delta R.T.: -0.003 min
Response: 1278603
Conc: 12.57 ng/ml

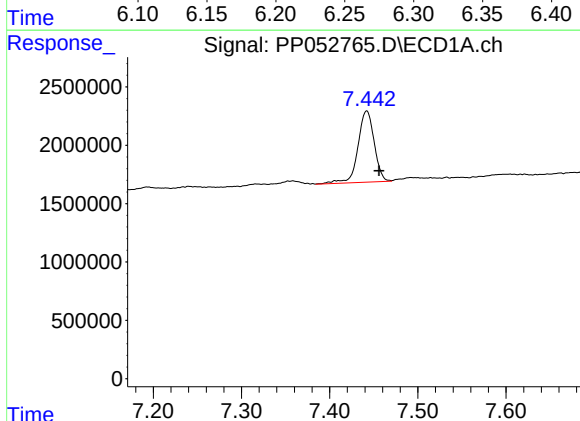


#32 AR-1260-2

R.T.: 7.442 min
Delta R.T.: -0.014 min
Response: 7823230
Conc: 83.78 ng/ml

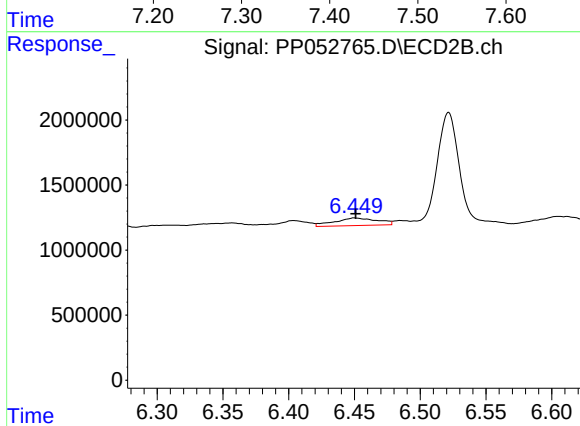

#32 AR-1260-2


R.T.: 6.450 min
Delta R.T.: -0.001 min
Response: 1310383
Conc: 10.77 ng/ml

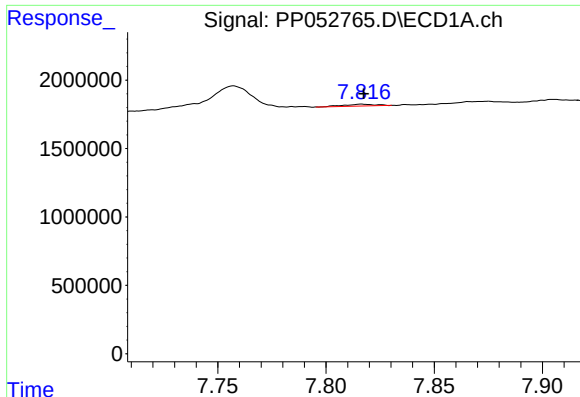

#33 AR-1260-3


R.T.: 7.817 min
Delta R.T.: 0.000 min
Response: 133687
Conc: 2.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

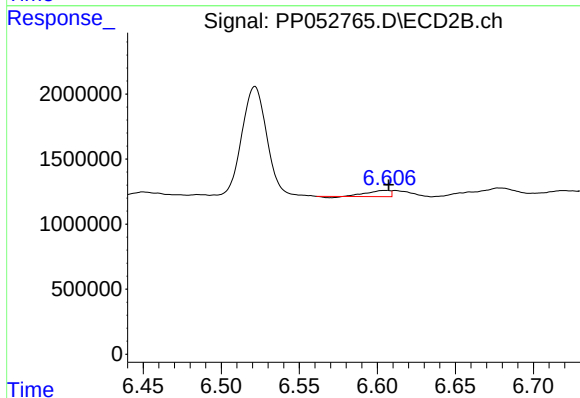


#33 AR-1260-3

R.T.: 6.606 min
Delta R.T.: -0.001 min
Response: 457513
Conc: 3.92 ng/ml

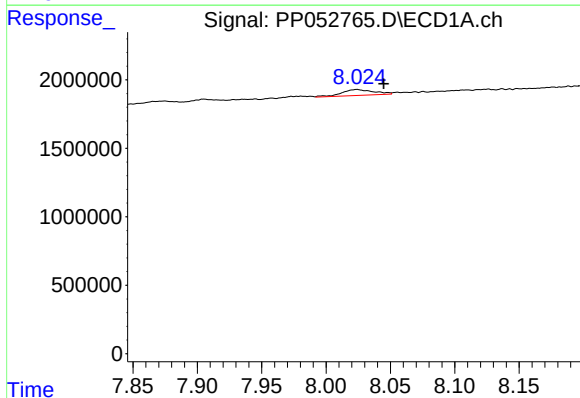


#34 AR-1260-4

R.T.: 8.024 min
Delta R.T.: -0.021 min
Response: 749322
Conc: 10.47 ng/ml

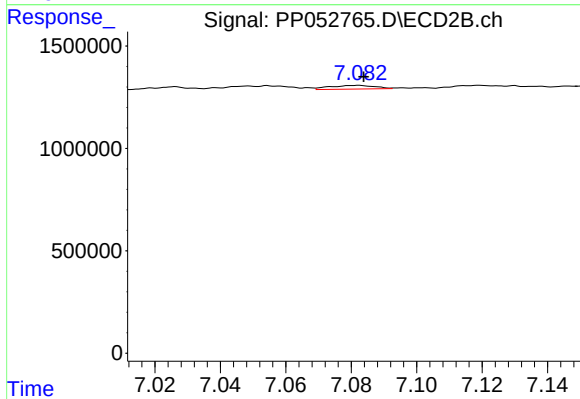

#34 AR-1260-4


R.T.: 7.082 min
Delta R.T.: -0.002 min
Response: 172297
Conc: 1.91 ng/ml

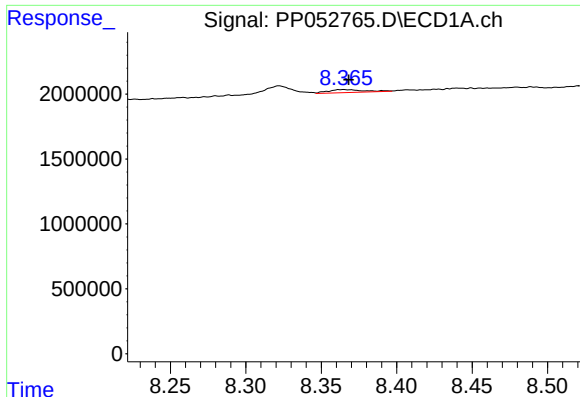

#35 AR-1260-5


R.T.: 8.364 min
Delta R.T.: -0.004 min
Response: 379929
Conc: 2.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

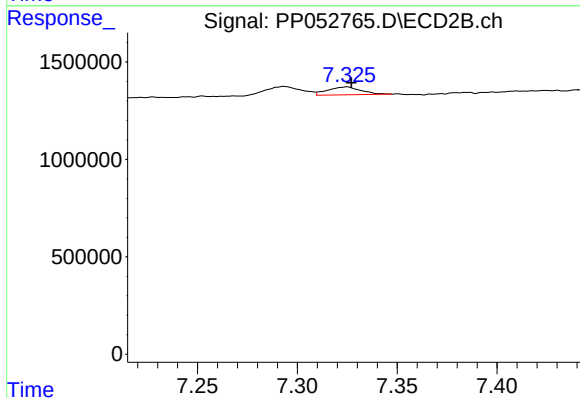


#35 AR-1260-5

R.T.: 7.325 min
Delta R.T.: -0.002 min
Response: 469100
Conc: 2.29 ng/ml

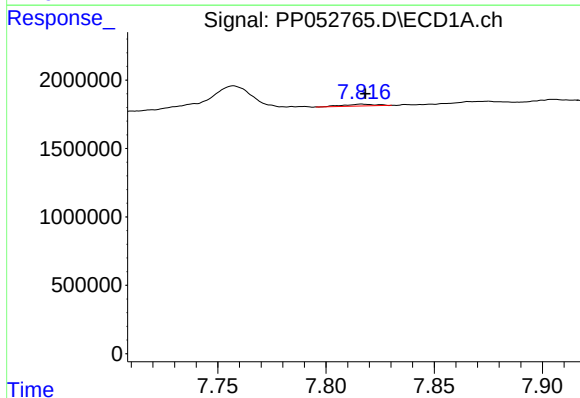


#36 AR-1262-1

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 133687
Conc: 1.39 ng/ml

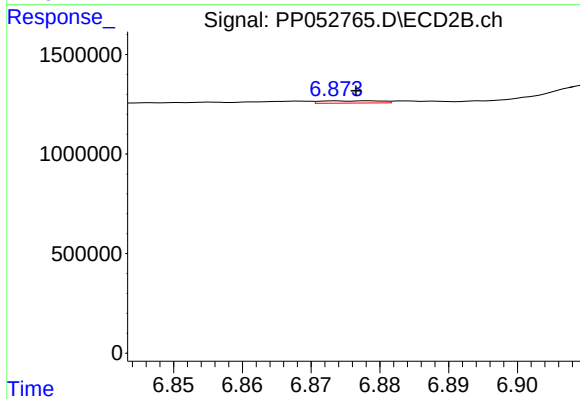

#36 AR-1262-1


R.T.: 6.878 min
Delta R.T.: 0.002 min
Response: 68306
Conc: 1.19 ng/ml

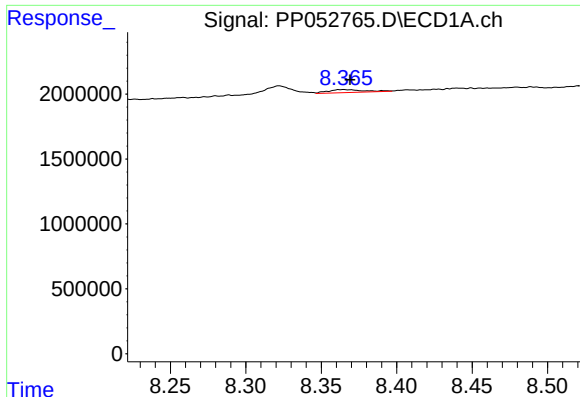

#37 AR-1262-2


R.T.: 8.364 min
Delta R.T.: -0.005 min
Response: 379929
Conc: 2.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

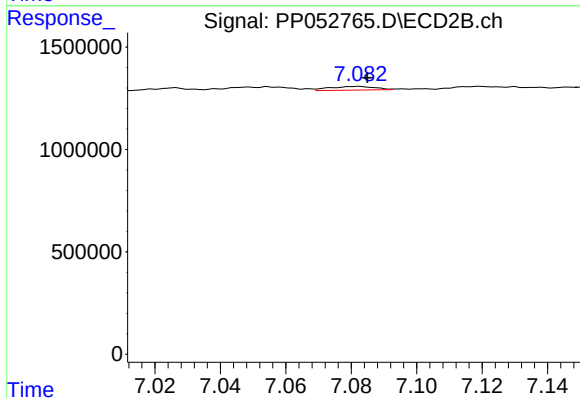


#37 AR-1262-2

R.T.: 7.082 min
Delta R.T.: -0.003 min
Response: 172297
Conc: 1.39 ng/ml

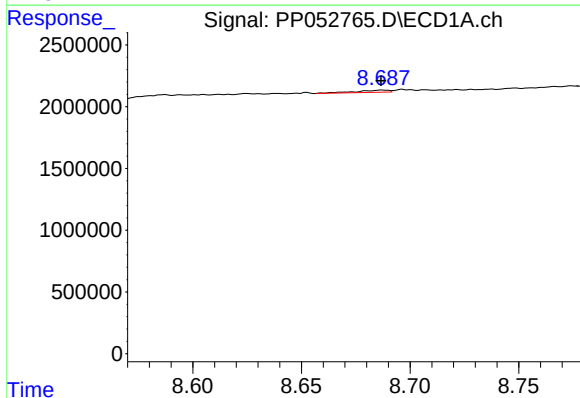


#38 AR-1262-3

R.T.: 8.687 min
Delta R.T.: 0.000 min
Response: 179978
Conc: 1.81 ng/ml

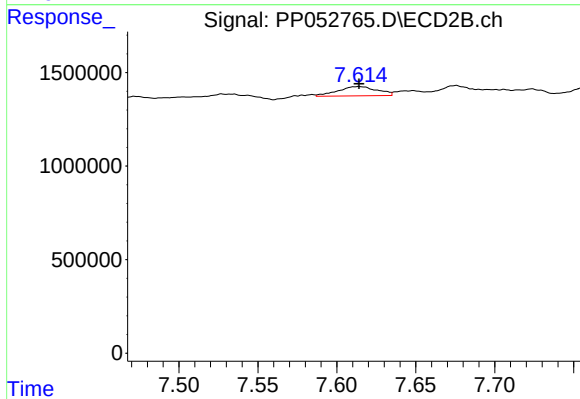

#38 AR-1262-3


R.T.: 7.614 min
Delta R.T.: 0.000 min
Response: 869218
Conc: 8.61 ng/ml

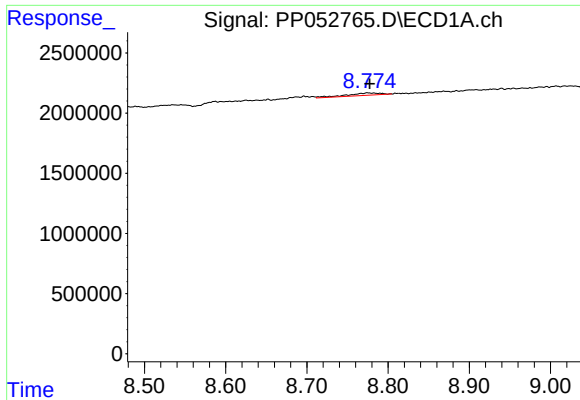

#39 AR-1262-4


R.T.: 8.775 min
Delta R.T.: -0.002 min
Response: 561490
Conc: 12.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

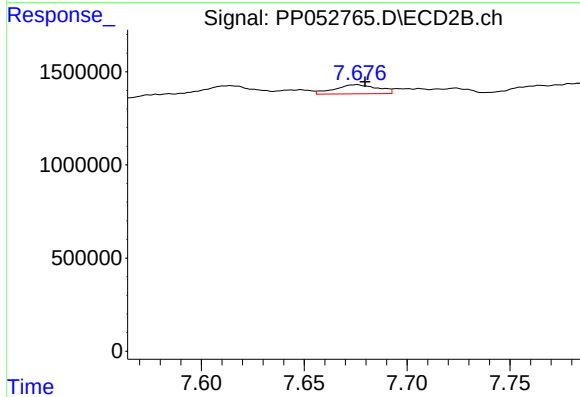


#39 AR-1262-4

R.T.: 7.676 min
Delta R.T.: -0.004 min
Response: 708446
Conc: 3.96 ng/ml

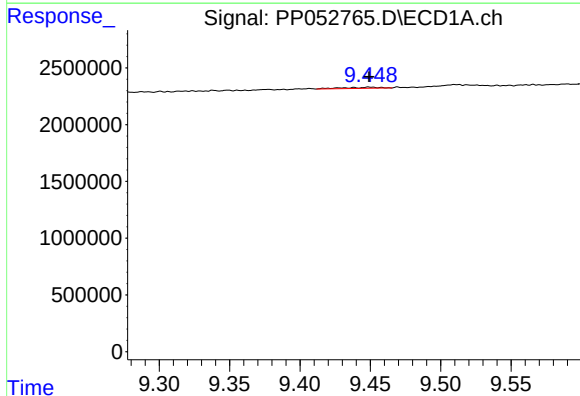


#40 AR-1262-5

R.T.: 9.449 min
Delta R.T.: 0.000 min
Response: 173177
Conc: 3.78 ng/ml

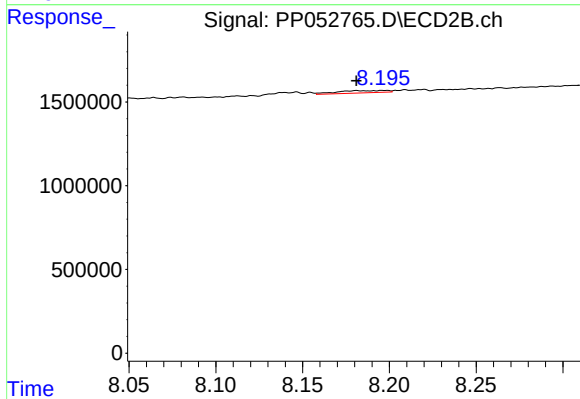

#40 AR-1262-5


R.T.: 8.199 min
Delta R.T.: 0.018 min
Response: 279461
Conc: 3.73 ng/ml

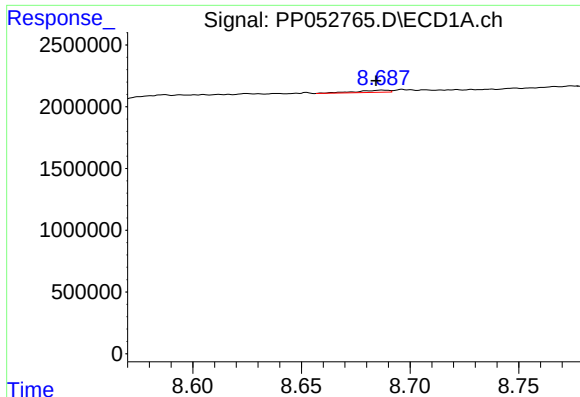

#41 AR-1268-1


R.T.: 8.687 min
Delta R.T.: 0.003 min
Response: 179978
Conc: 0.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

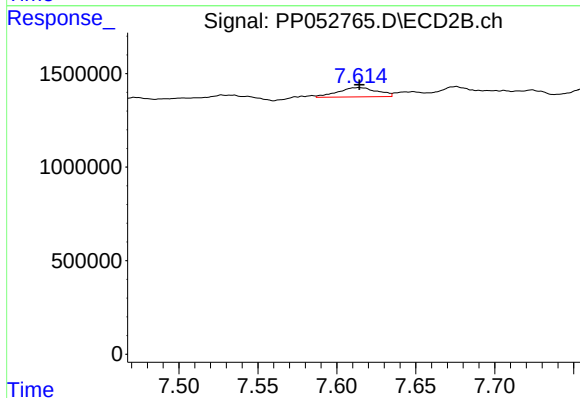


#41 AR-1268-1

R.T.: 7.614 min
Delta R.T.: 0.000 min
Response: 869218
Conc: 2.84 ng/ml

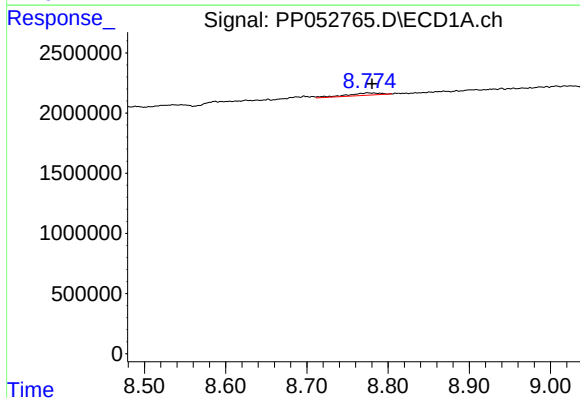


#42 AR-1268-2

R.T.: 8.775 min
Delta R.T.: -0.005 min
Response: 561490
Conc: 3.43 ng/ml

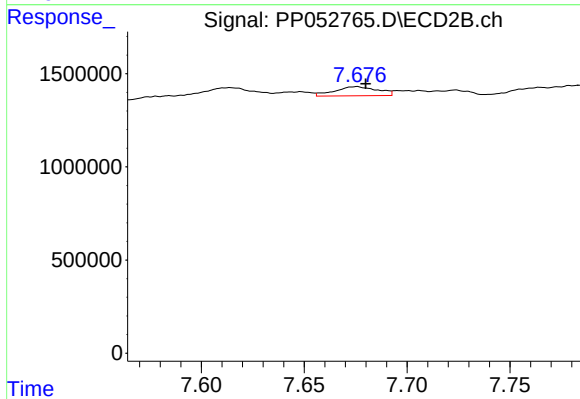

#42 AR-1268-2


R.T.: 7.676 min
Delta R.T.: -0.004 min
Response: 708446
Conc: 2.61 ng/ml

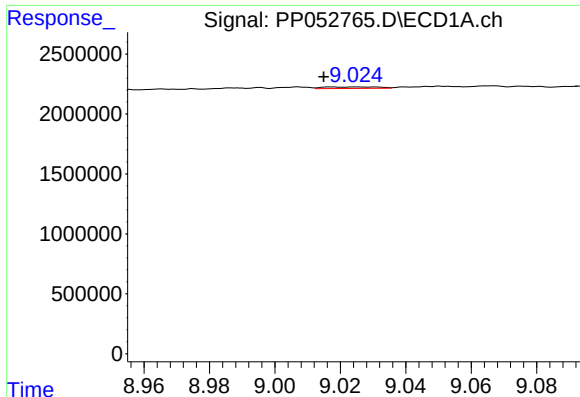

#43 AR-1268-3


R.T.: 9.017 min
Delta R.T.: 0.003 min
Response: 140311
Conc: 0.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

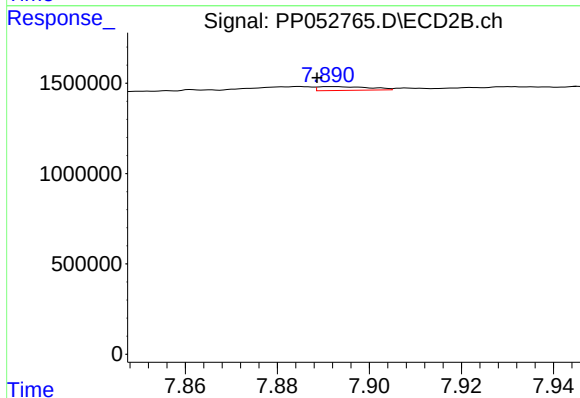


#43 AR-1268-3

R.T.: 7.892 min
Delta R.T.: 0.003 min
Response: 162051
Conc: 0.69 ng/ml

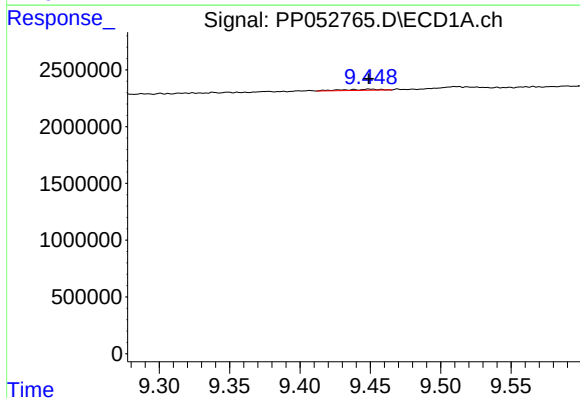


#44 AR-1268-4

R.T.: 9.449 min
Delta R.T.: 0.000 min
Response: 173177
Conc: 3.41 ng/ml

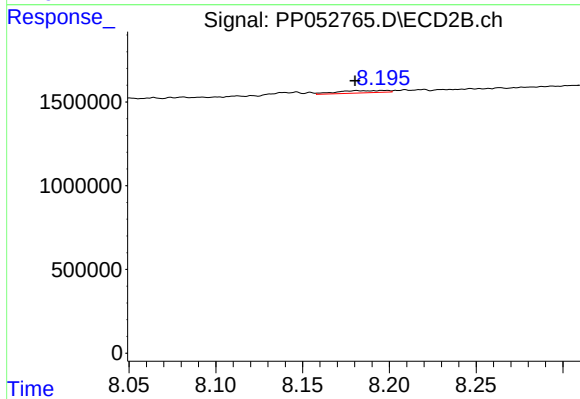

#44 AR-1268-4


R.T.: 8.199 min
Delta R.T.: 0.019 min
Response: 279461
Conc: 3.29 ng/ml

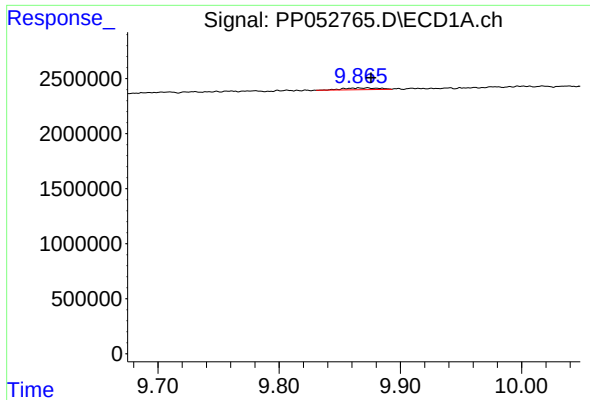

#45 AR-1268-5

R.T.: 9.873 min
Delta R.T.: -0.003 min
Response: 328154
Conc: 0.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIDEN-GAS-PIPELINE

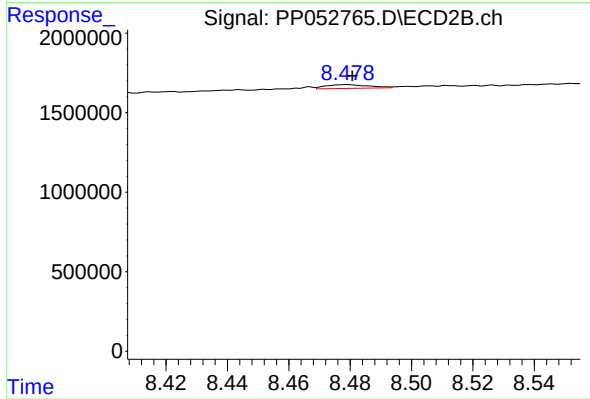

#45 AR-1268-5

R.T.: 8.479 min
Delta R.T.: -0.002 min
Response: 231829
Conc: 0.35 ng/ml