

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052748.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2022 14:46
 Operator : YP\AJ
 Sample : N5257-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HOLLAND-RD-COMP-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/28/2022
 Supervised By :Ankita Jodhani 10/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:14:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.408	3.653	39729297	37512891	17.979	19.962
2) SA Decachlor...	10.217	8.741	18393818	24045872	14.491	14.338
Target Compounds						
26) L6 AR-1254-1	6.443	5.569	2230693	2877268	29.387	26.794
27) L6 AR-1254-2	6.663	5.718	3284521	3476161	29.387	36.368
28) L6 AR-1254-3	7.032	6.127	3772953	5186241	33.896	33.945
29) L6 AR-1254-4	7.318	6.358	1974667	2584419	28.041	28.465
30) L6 AR-1254-5	7.746	6.780	2538827	14404982	32.246m	103.537 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052748.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2022 14:46
Operator : YP\AJ
Sample : N5257-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:14:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

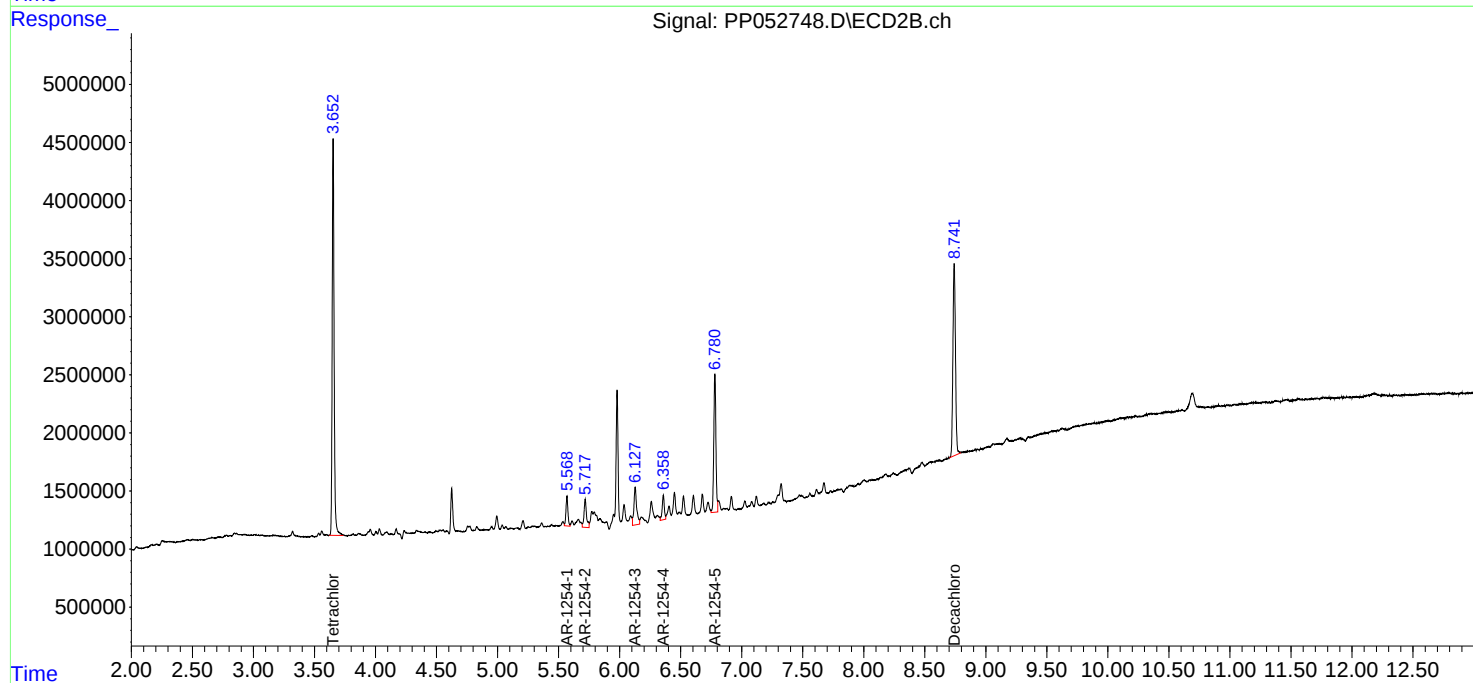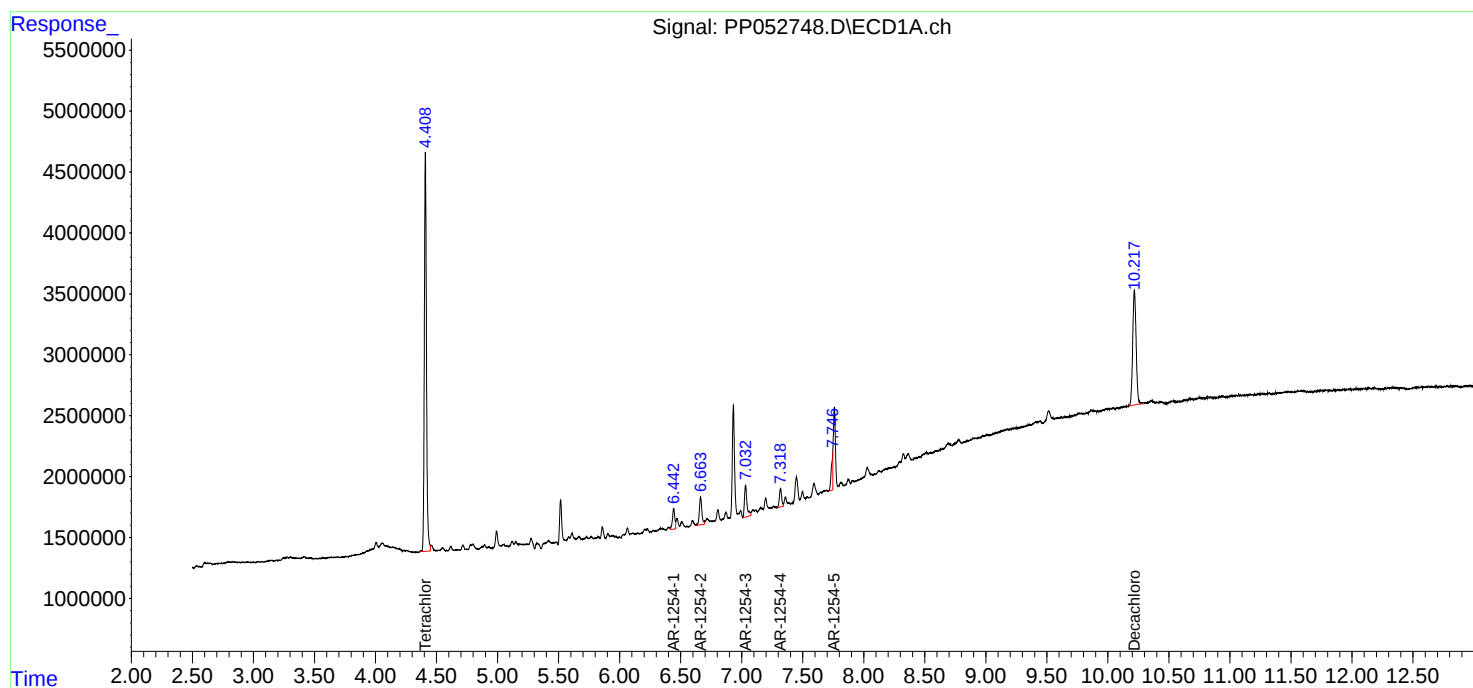

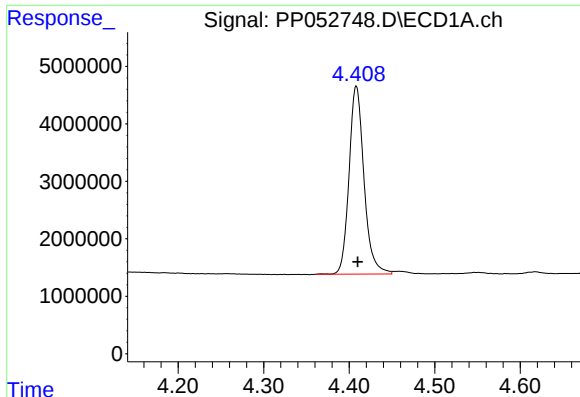


#1 Tetrachloro-m-xylene

R.T.: 4.408 min
Delta R.T.: -0.002 min
Response: 39729297
Conc: 17.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

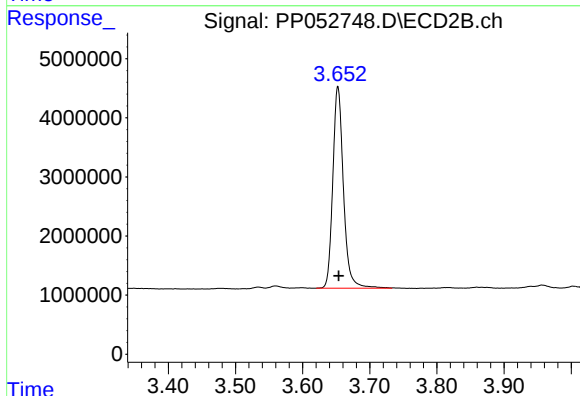


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.001 min
Response: 37512891
Conc: 19.96 ng/ml

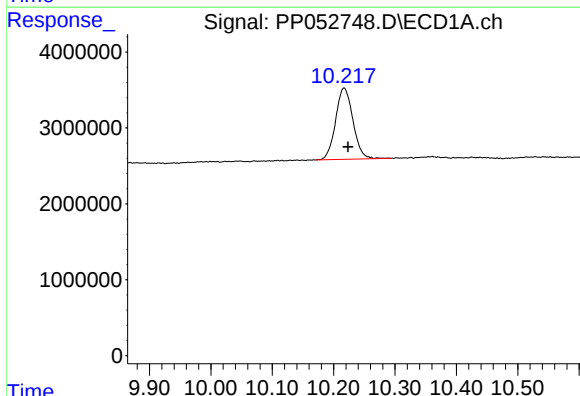


#2 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.007 min
Response: 18393818
Conc: 14.49 ng/ml

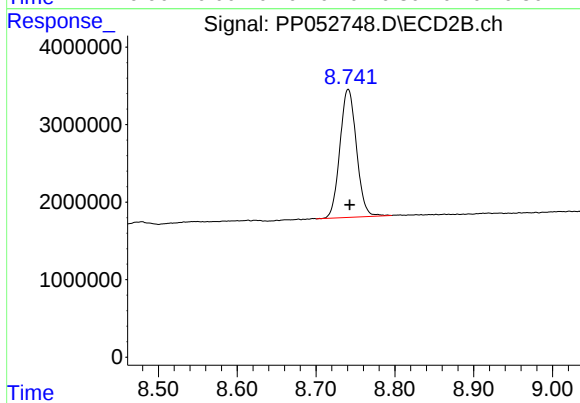

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.002 min
Response: 24045872
Conc: 14.34 ng/ml

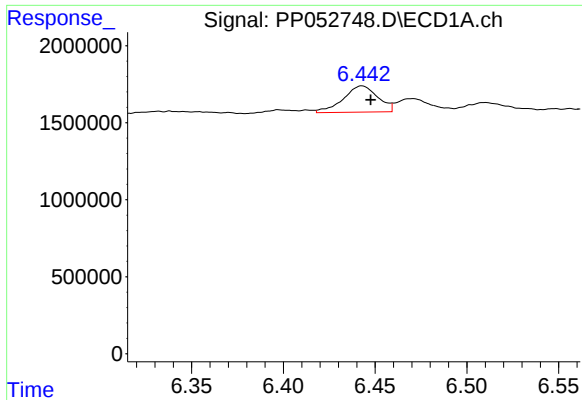


#26 AR-1254-1

R.T.: 6.443 min
Delta R.T.: -0.005 min
Response: 2230693
Conc: 29.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

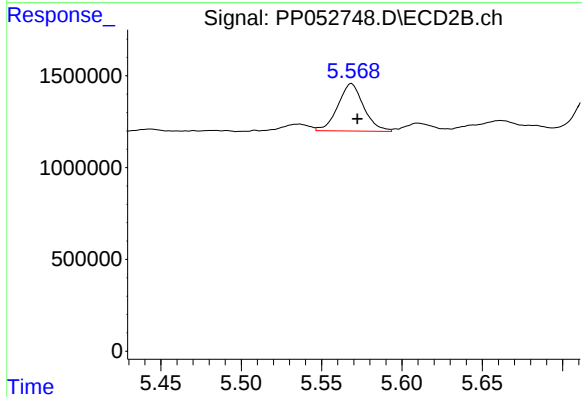


#26 AR-1254-1

R.T.: 5.569 min
Delta R.T.: -0.004 min
Response: 2877268
Conc: 26.79 ng/ml

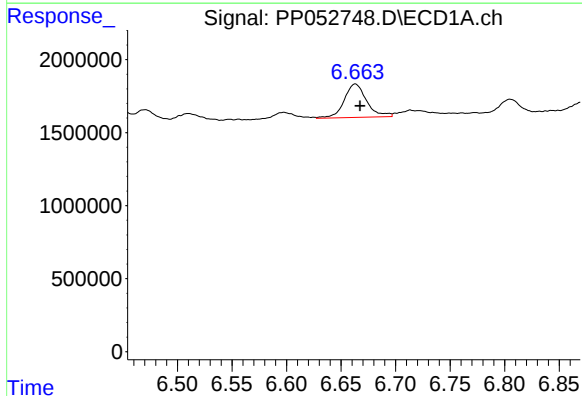


#27 AR-1254-2

R.T.: 6.663 min
Delta R.T.: -0.004 min
Response: 3284521
Conc: 29.39 ng/ml

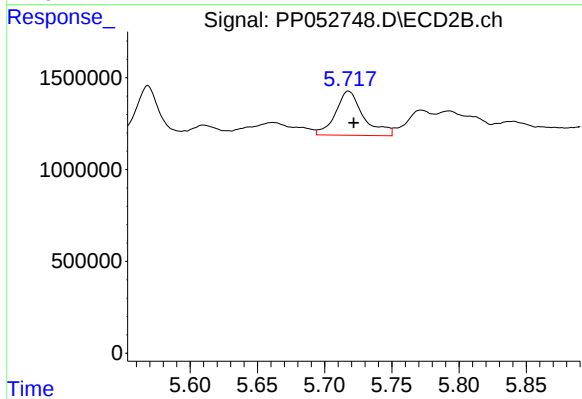

#27 AR-1254-2

R.T.: 5.718 min
Delta R.T.: -0.004 min
Response: 3476161
Conc: 36.37 ng/ml

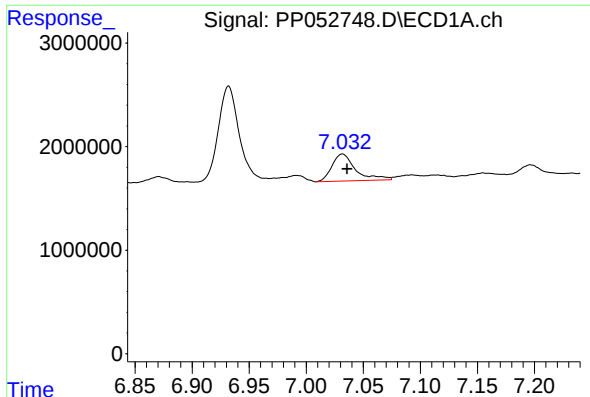


#28 AR-1254-3

R.T.: 7.032 min
Delta R.T.: -0.004 min
Response: 3772953
Conc: 33.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

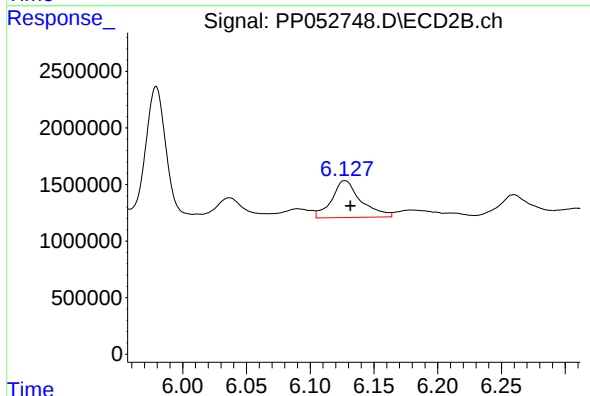


#28 AR-1254-3

R.T.: 6.127 min
Delta R.T.: -0.004 min
Response: 5186241
Conc: 33.94 ng/ml

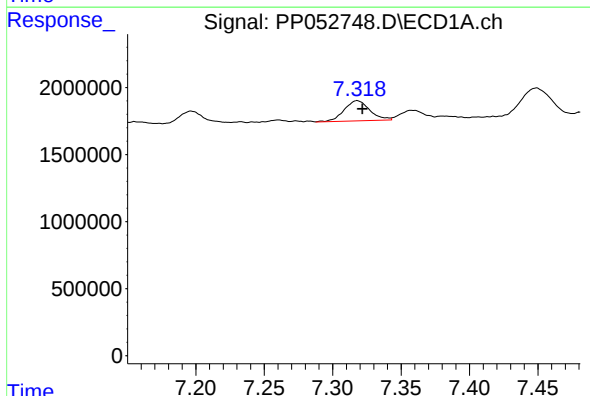


#29 AR-1254-4

R.T.: 7.318 min
Delta R.T.: -0.004 min
Response: 1974667
Conc: 28.04 ng/ml

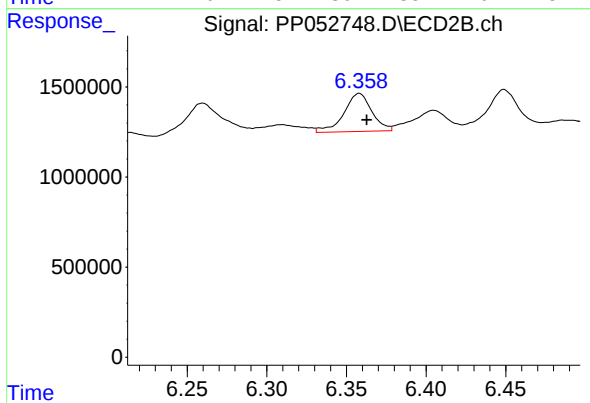

#29 AR-1254-4

R.T.: 6.358 min
Delta R.T.: -0.005 min
Response: 2584419
Conc: 28.46 ng/ml

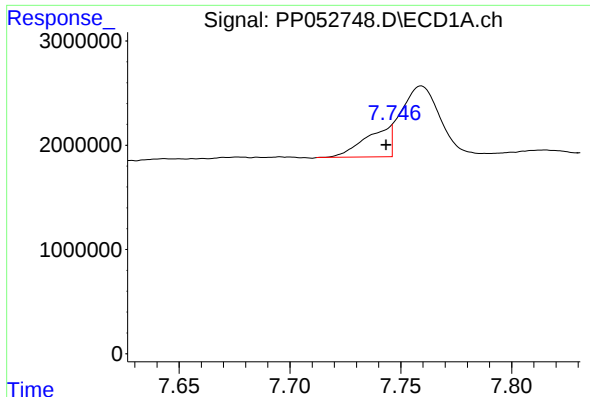


#30 AR-1254-5

R.T.: 7.746 min
Delta R.T.: 0.003 min
Response: 2538827
Conc: 32.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

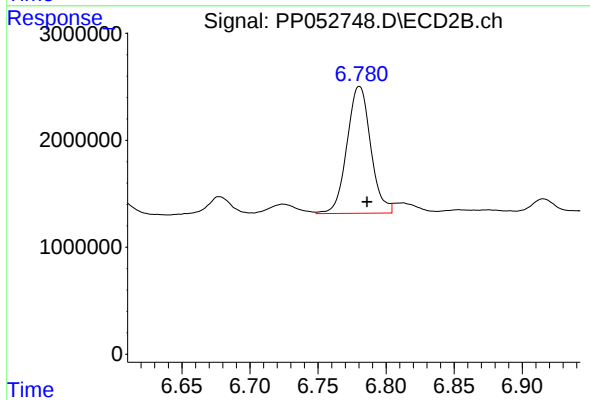

#30 AR-1254-5

R.T.: 6.780 min
Delta R.T.: -0.006 min
Response: 14404982
Conc: 103.54 ng/ml