

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2022 16:09
 Operator : YP\AJ
 Sample : N5257-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HOLLAND-RD-COMP-4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/28/2022
 Supervised By :Ankita Jodhani 10/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:19:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.409	3.653	33411984	31384096	15.121	16.701
2) SA Decachlor...	10.220	8.741	14350935	18197264	11.306	10.850
Target Compounds						
26) L6 AR-1254-1	6.442	5.570	2488344	2465265	32.782	22.958 #
27) L6 AR-1254-2	6.664	5.719	2407687	2629533	21.542	27.510 #
28) L6 AR-1254-3	7.032	6.128	3956045	6466708	35.541	42.325m
29) L6 AR-1254-4	7.318	6.359	1731599	1738907	24.589	19.152m
30) L6 AR-1254-5	7.740	6.781	4802618	12322517	60.999	88.569 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2022 16:09
Operator : YP\AJ
Sample : N5257-07
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:19:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

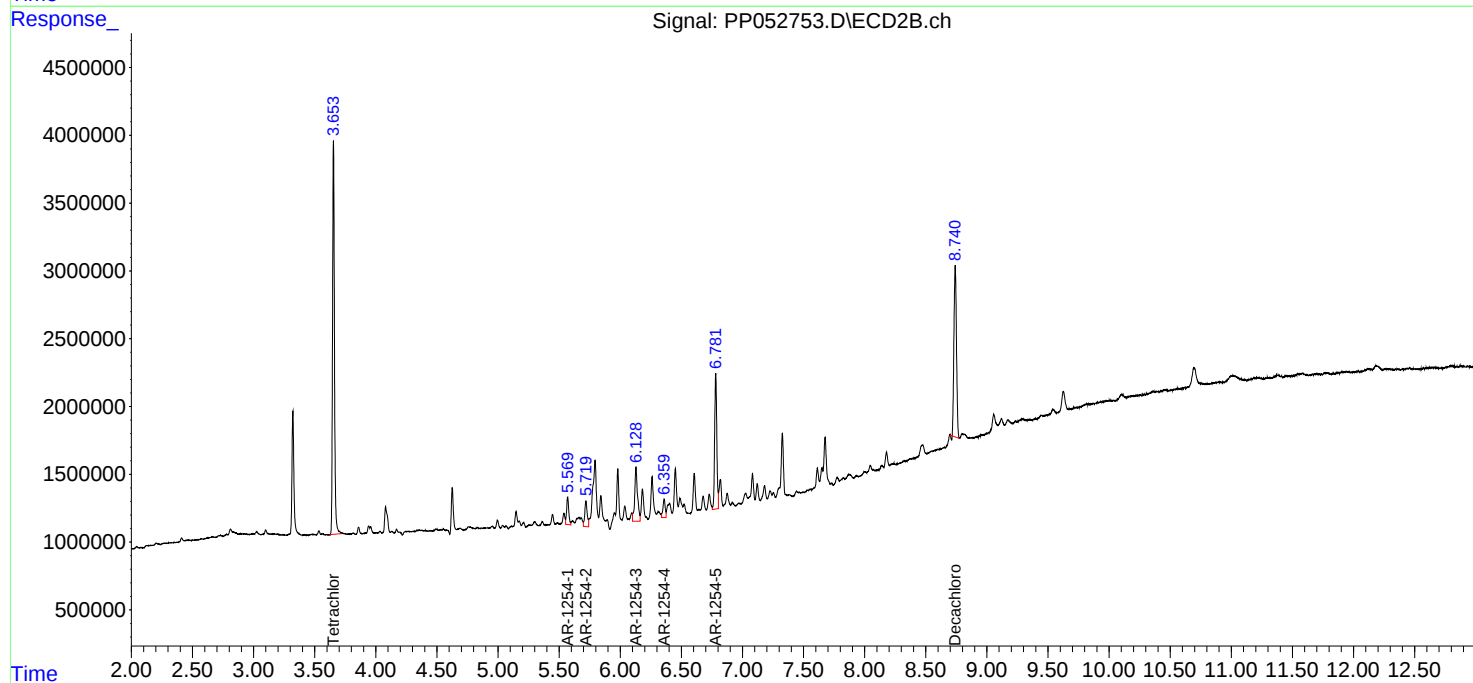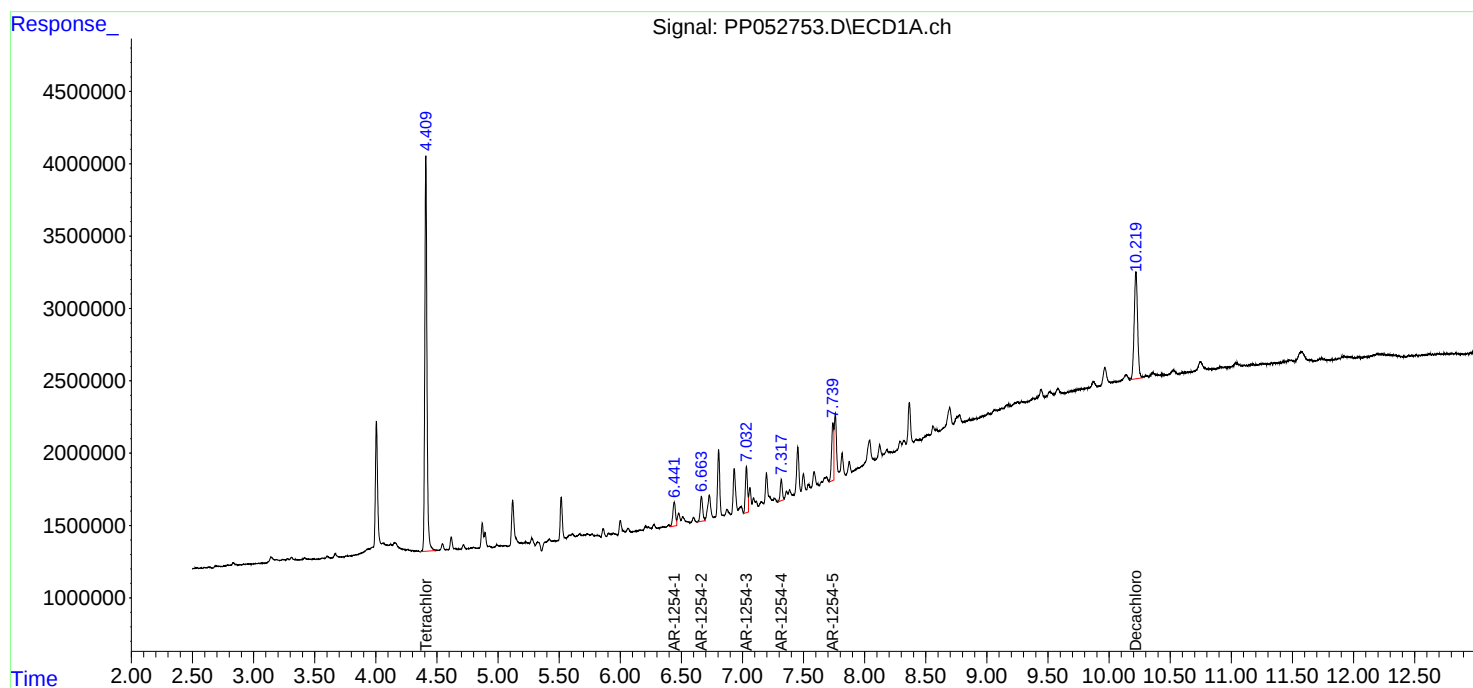

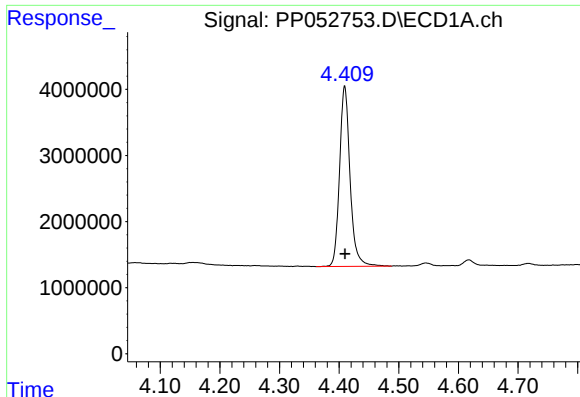


#1 Tetrachloro-m-xylene

R.T.: 4.409 min
Delta R.T.: 0.000 min
Response: 33411984
Conc: 15.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

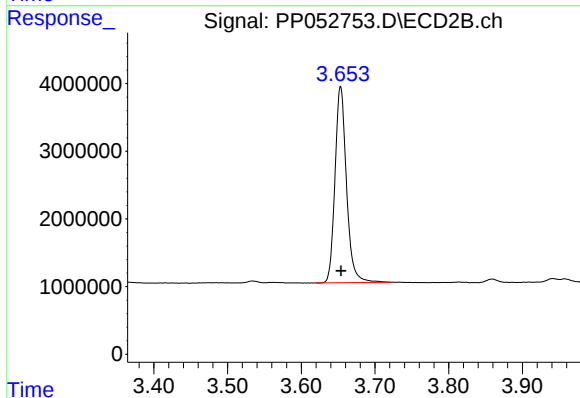


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: 0.000 min
Response: 31384096
Conc: 16.70 ng/ml

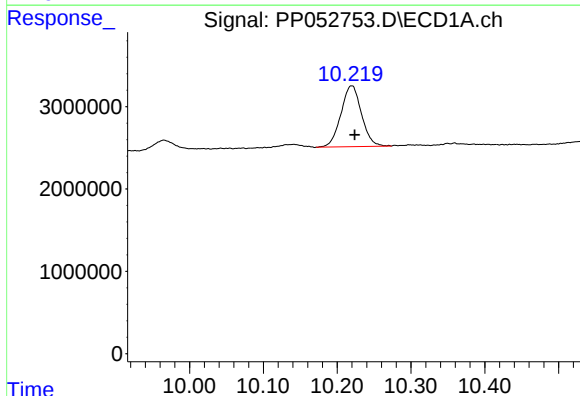


#2 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 14350935
Conc: 11.31 ng/ml

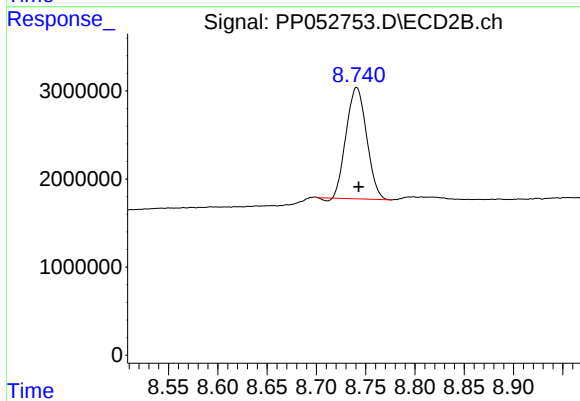

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.002 min
Response: 18197264
Conc: 10.85 ng/ml

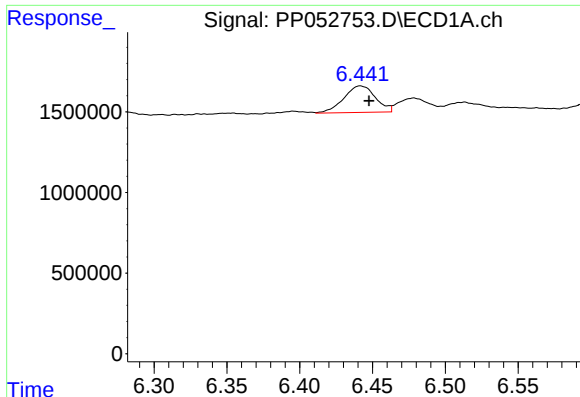


#26 AR-1254-1

R.T.: 6.442 min
Delta R.T.: -0.006 min
Response: 2488344
Conc: 32.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

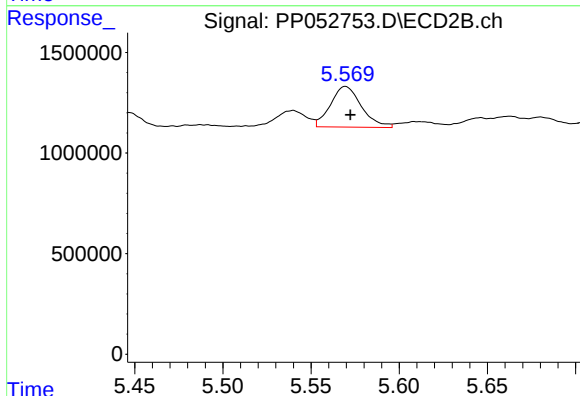


#26 AR-1254-1

R.T.: 5.570 min
Delta R.T.: -0.003 min
Response: 2465265
Conc: 22.96 ng/ml

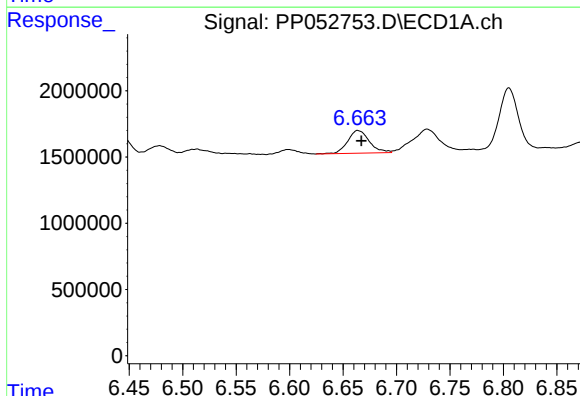


#27 AR-1254-2

R.T.: 6.664 min
Delta R.T.: -0.003 min
Response: 2407687
Conc: 21.54 ng/ml

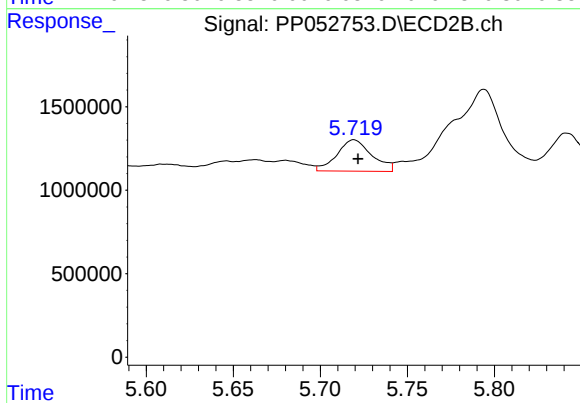

#27 AR-1254-2

R.T.: 5.719 min
Delta R.T.: -0.002 min
Response: 2629533
Conc: 27.51 ng/ml

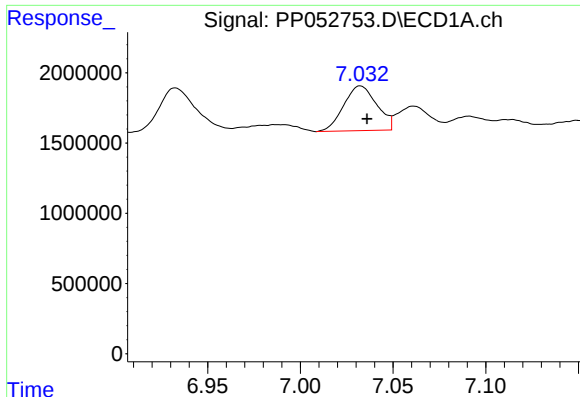


#28 AR-1254-3

R.T.: 7.032 min
Delta R.T.: -0.004 min
Response: 3956045
Conc: 35.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

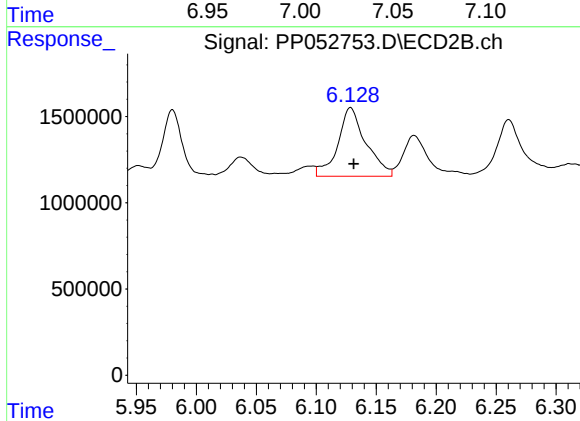


#28 AR-1254-3

R.T.: 6.128 min
Delta R.T.: -0.003 min
Response: 6466708
Conc: 42.33 ng/ml m

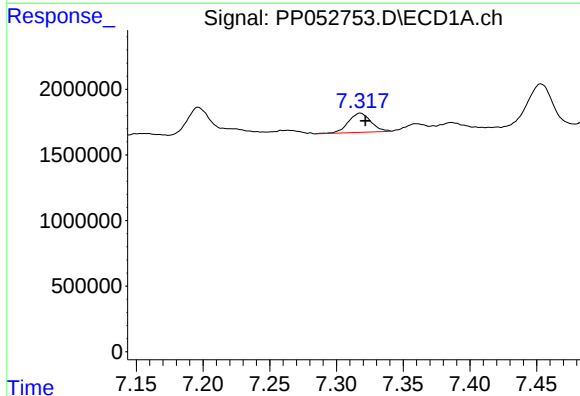


#29 AR-1254-4

R.T.: 7.318 min
Delta R.T.: -0.004 min
Response: 1731599
Conc: 24.59 ng/ml

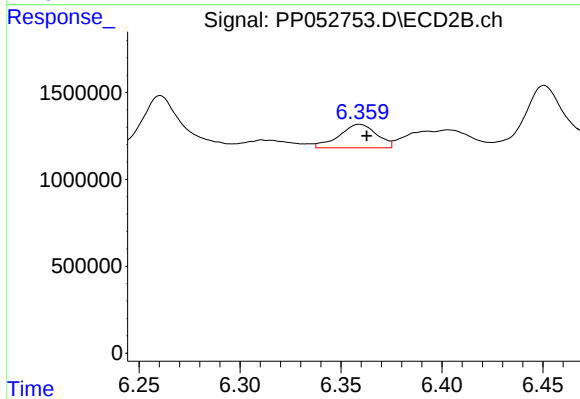

#29 AR-1254-4

R.T.: 6.359 min
Delta R.T.: -0.004 min
Response: 1738907
Conc: 19.15 ng/ml m

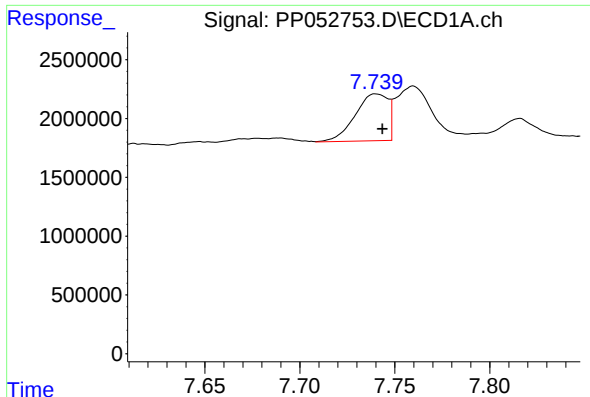


#30 AR-1254-5

R.T.: 7.740 min
Delta R.T.: -0.003 min
Response: 4802618
Conc: 61.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
HOLLAND-RD-COMP-4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2022
Supervised By :Ankita Jodhani 10/28/2022

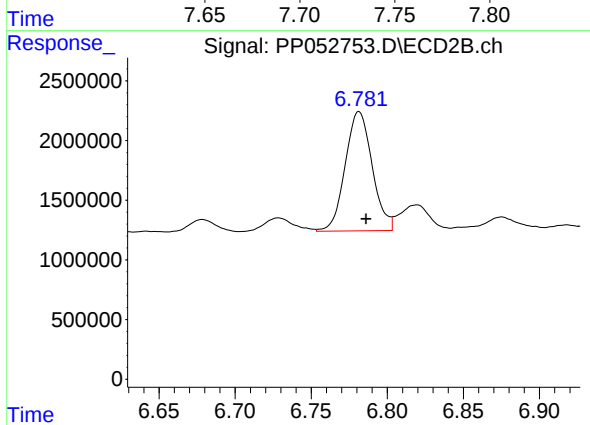

#30 AR-1254-5

R.T.: 6.781 min
Delta R.T.: -0.005 min
Response: 12322517
Conc: 88.57 ng/ml