

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 00:56
 Operator : YP\AJ
 Sample : N5272-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20221104-COMP-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 06:35:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.650	35569836	34605448	16.097	18.415
2) SA Decachlor...	10.211	8.735	17033886	21898853	13.420	13.057

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 00:56
Operator : YP\AJ
Sample : N5272-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20221104-COMP-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:35:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

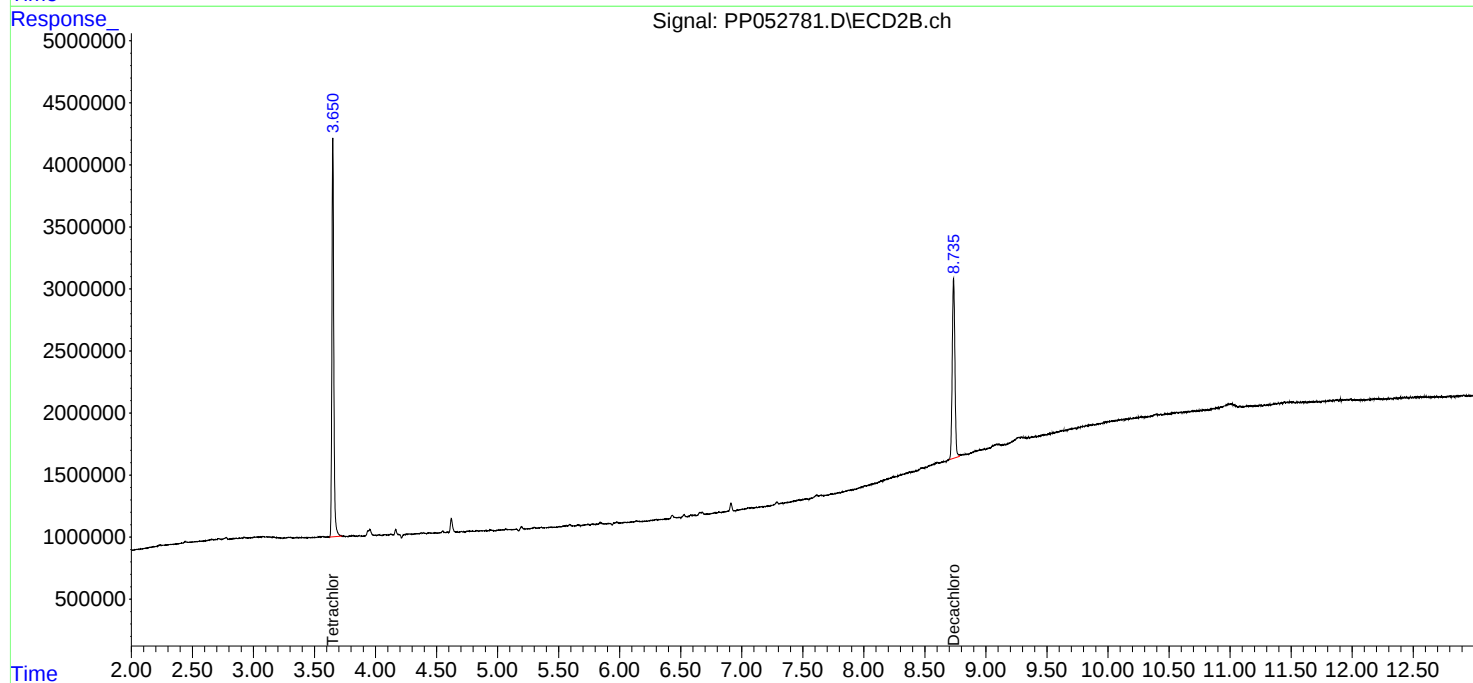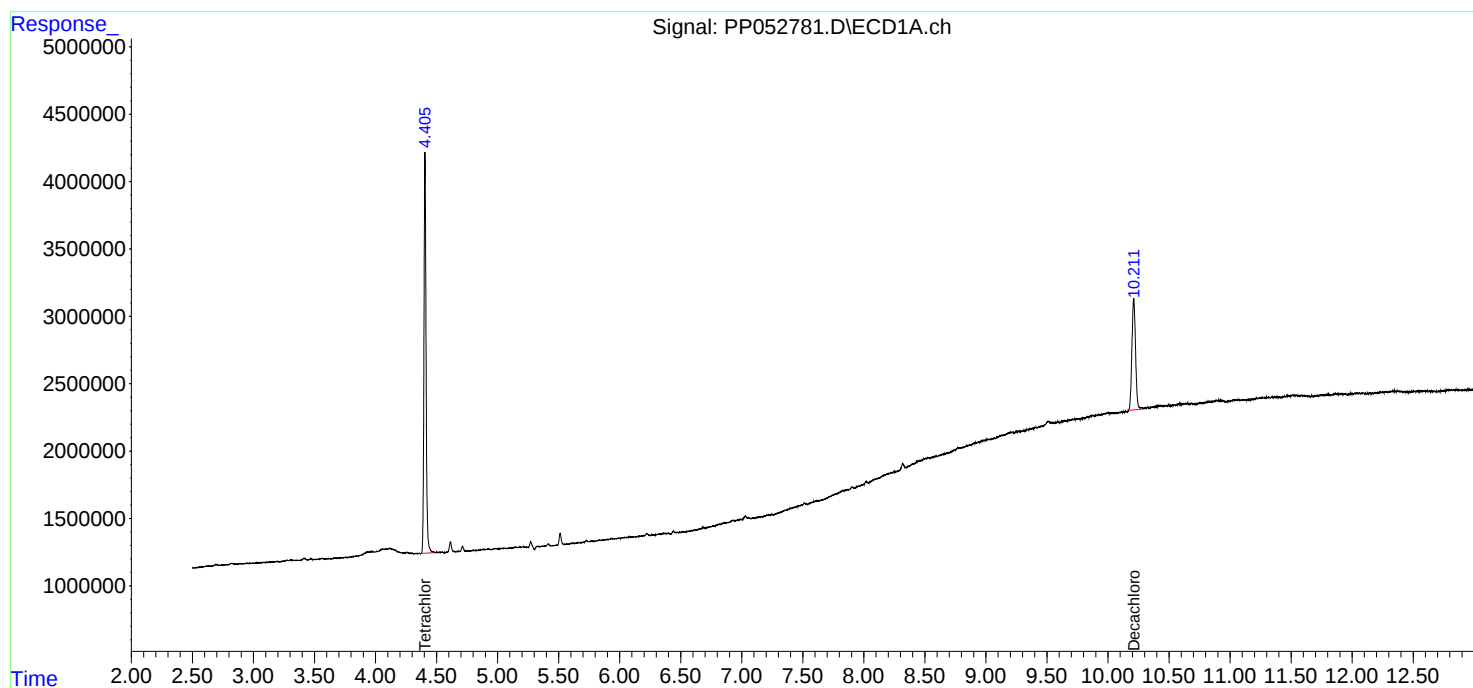


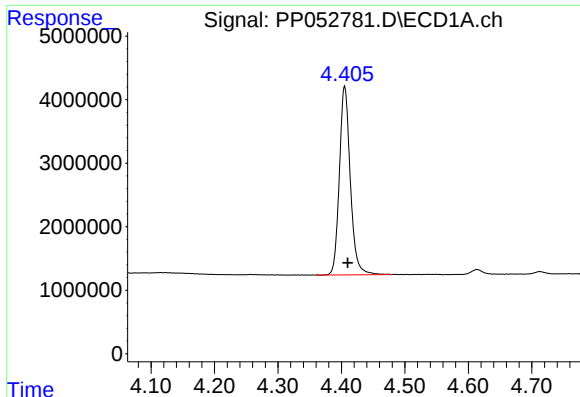

#1 Tetrachloro-m-xylene


R.T.: 4.405 min
Delta R.T.: -0.005 min
Response: 35569836
Conc: 16.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
20221104-COMP-03

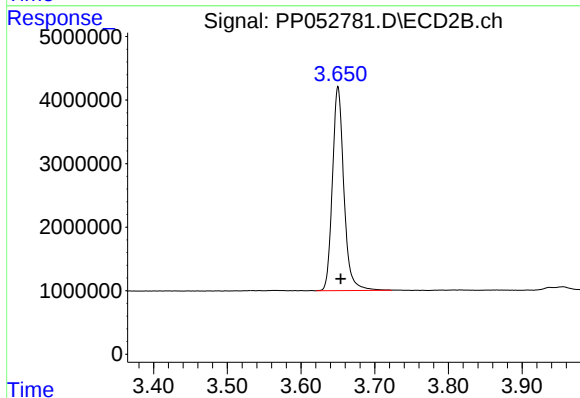


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.003 min
Response: 34605448
Conc: 18.41 ng/ml

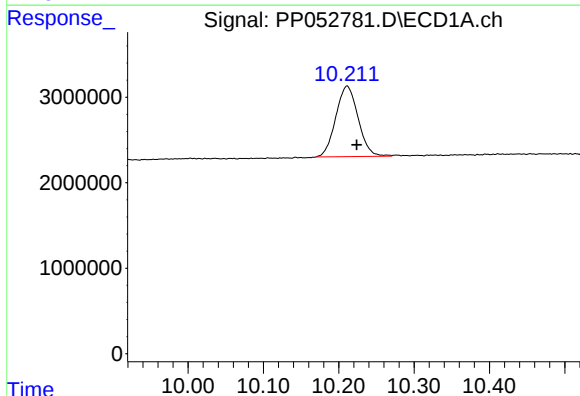

#2 Decachlorobiphenyl

R.T.: 10.211 min
Delta R.T.: -0.013 min
Response: 17033886
Conc: 13.42 ng/ml

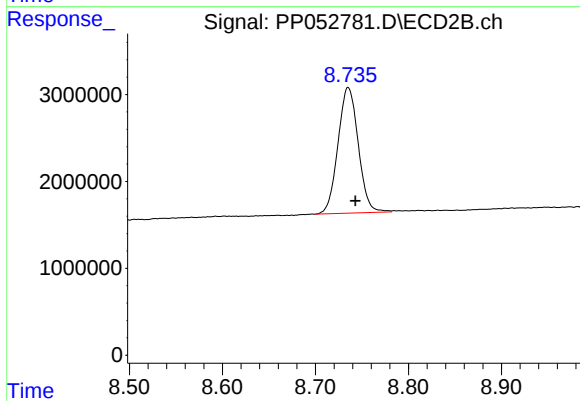

#2 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.008 min
Response: 21898853
Conc: 13.06 ng/ml