

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
 Data File : PP052785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 02:02
 Operator : YP\AJ
 Sample : N5272-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20221117-AMENDED-COMP-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 06:37:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.650	32371959	30399997	14.650	16.177
2) SA Decachlor...	10.212	8.735	7140231	9833044	5.625	5.863

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102722\
Data File : PP052785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 02:02
Operator : YP\AJ
Sample : N5272-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20221117-AMENDED-COMP-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:37:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

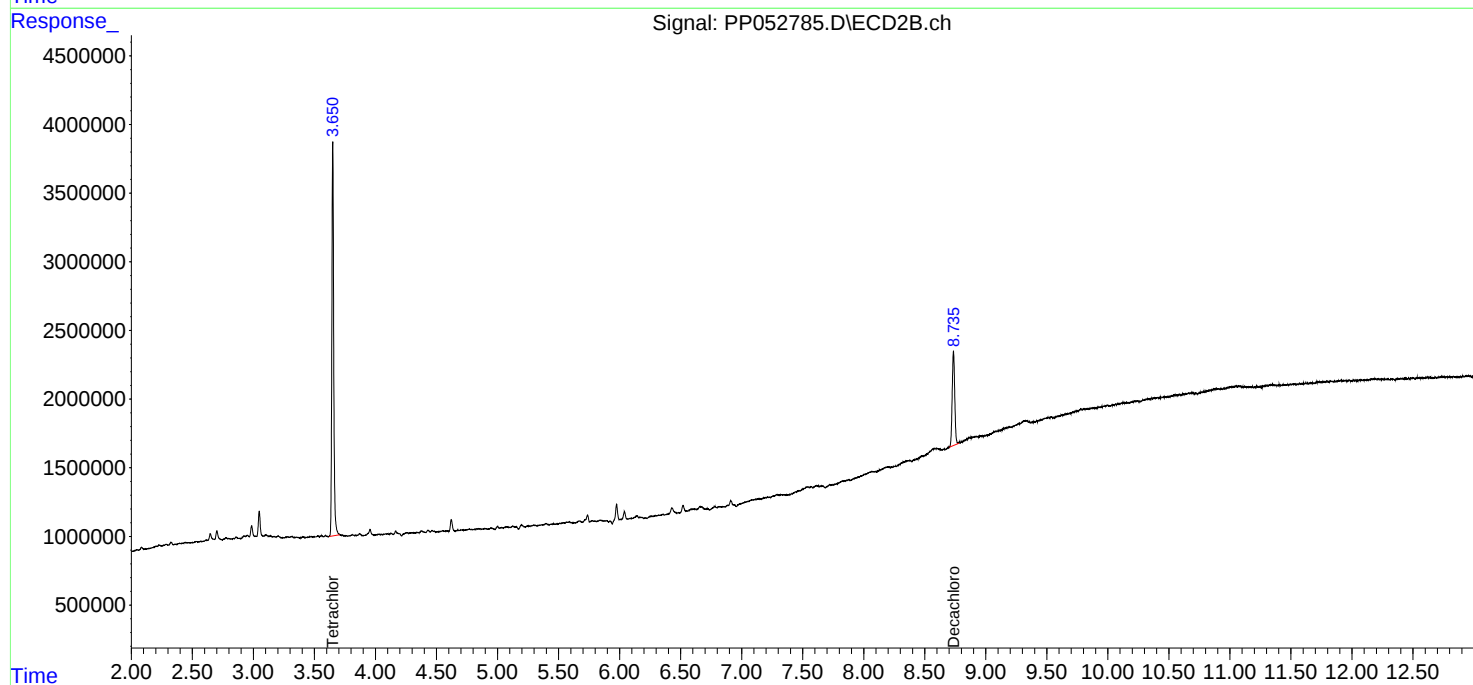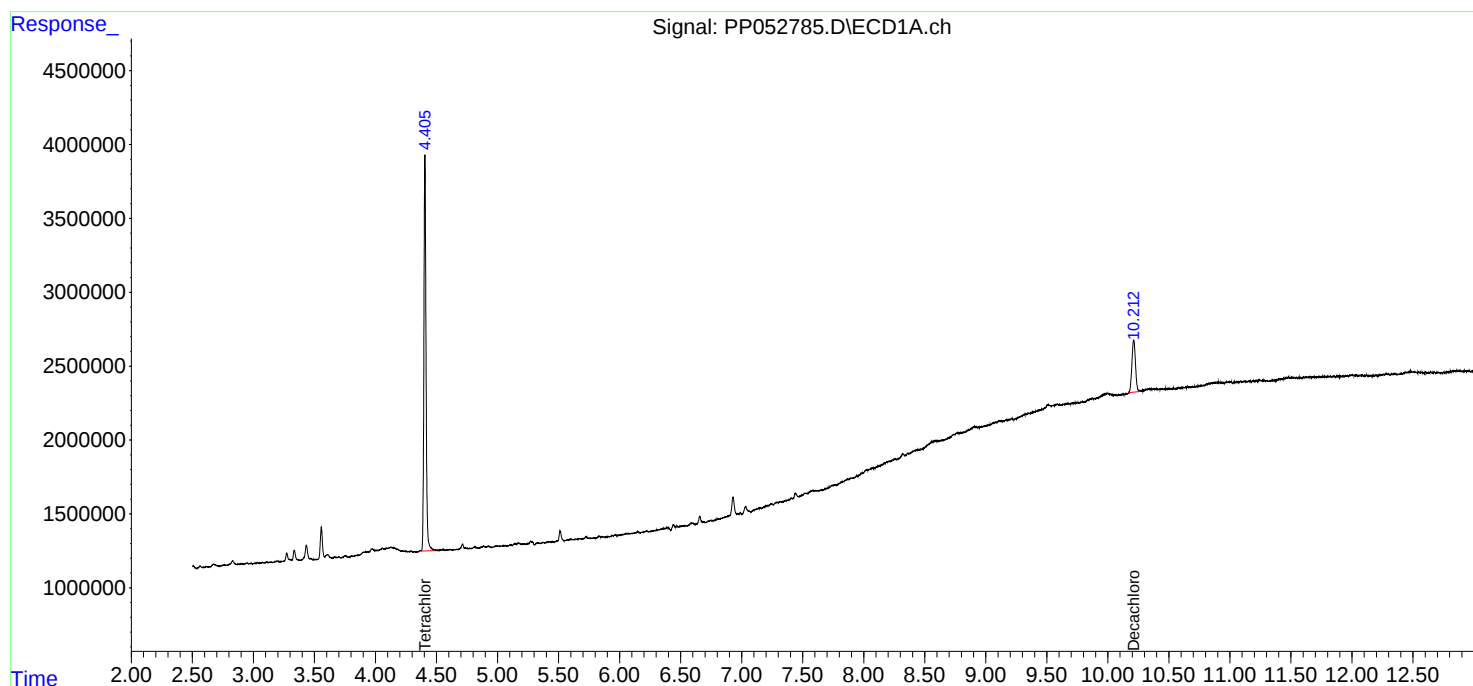


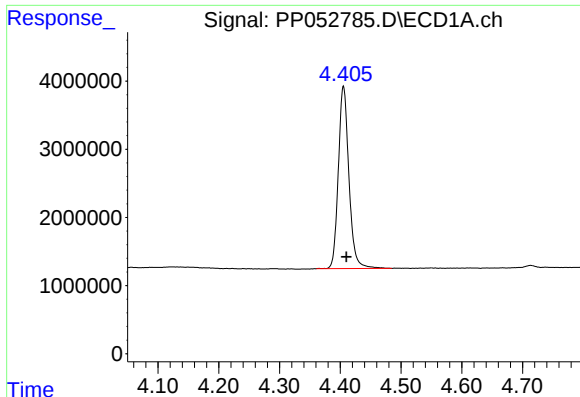

#1 Tetrachloro-m-xylene


R.T.: 4.405 min
Delta R.T.: -0.005 min
Response: 32371959
Conc: 14.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
20221117-AMENDED-COMP-02

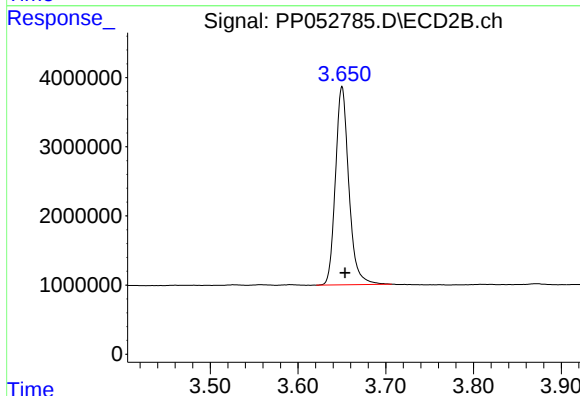


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.003 min
Response: 30399997
Conc: 16.18 ng/ml

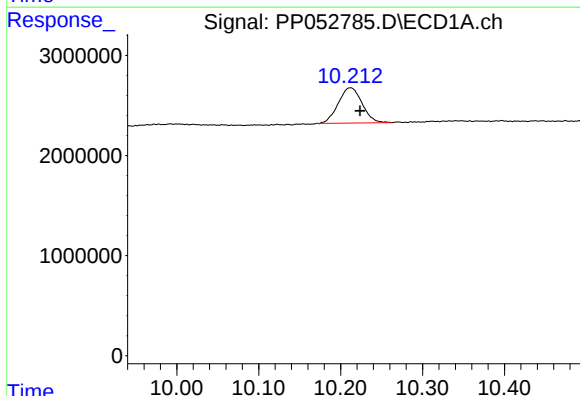

#2 Decachlorobiphenyl

R.T.: 10.212 min
Delta R.T.: -0.012 min
Response: 7140231
Conc: 5.63 ng/ml

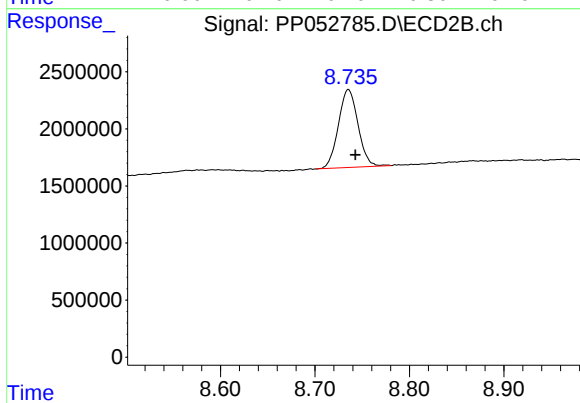

#2 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.007 min
Response: 9833044
Conc: 5.86 ng/ml