

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102725\
 Data File : PP076100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2025 21:26
 Operator : YP\AJ
 Sample : Q3459-05 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC259240LOK-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/28/2025
 Supervised By :mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:08:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.636	3.777	2713080	10555099	1.898	1.595
2) SA Decachlor...	10.400	8.791	2561066	6036388	2.379m	0.734 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102725\
Data File : PP076100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2025 21:26
Operator : YP\AJ
Sample : Q3459-05 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC259240LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:08:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

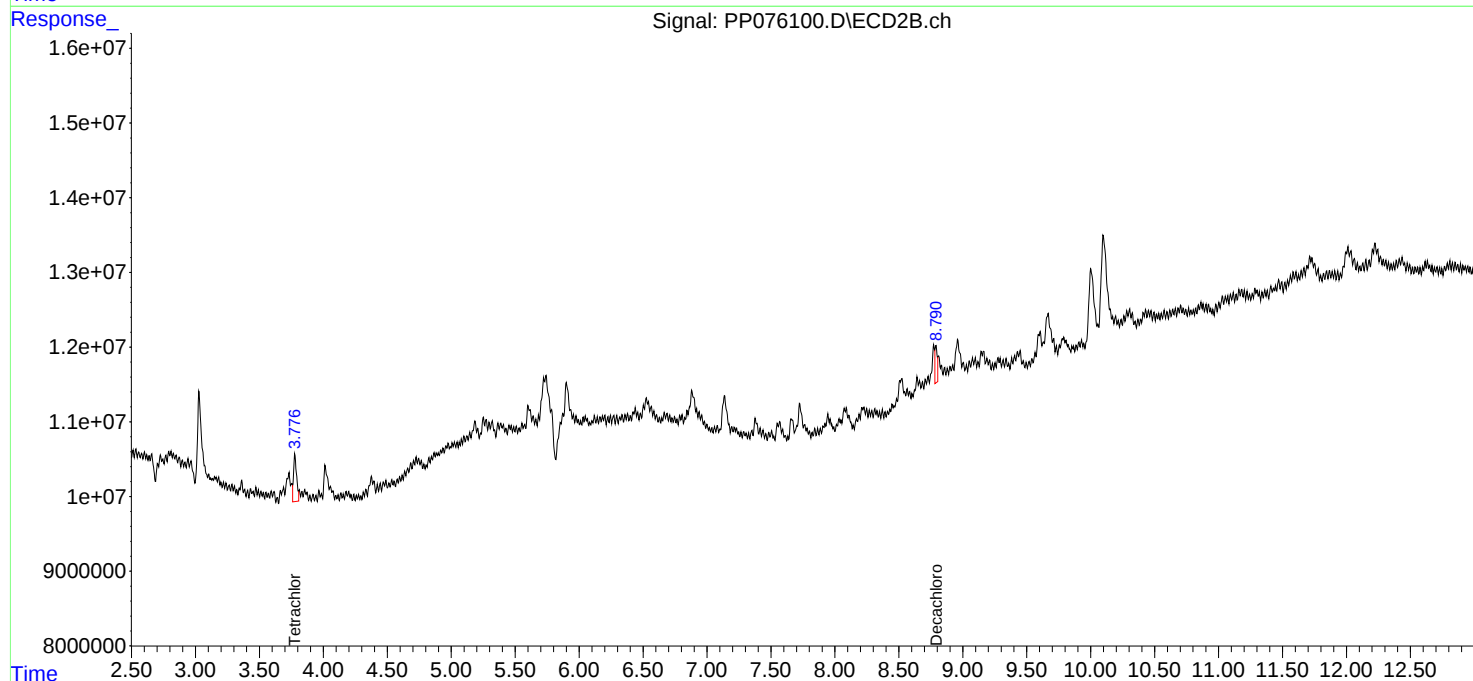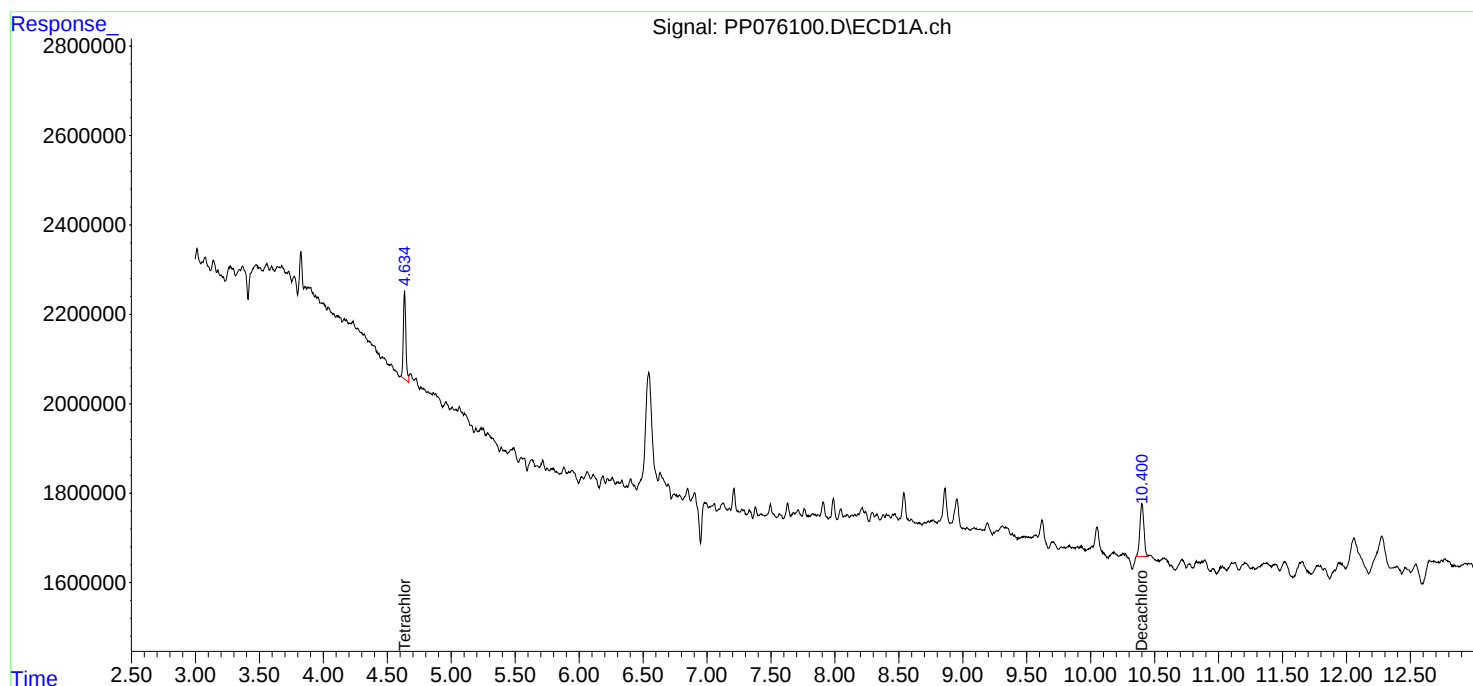

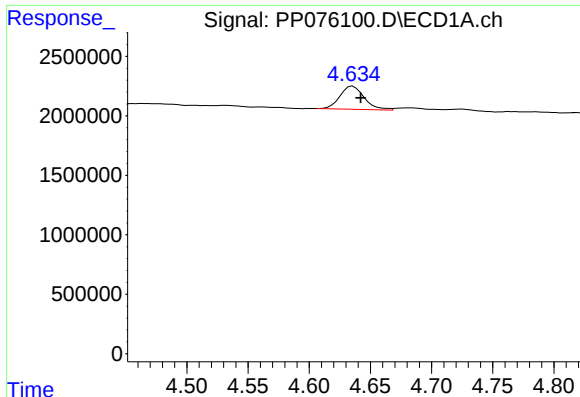


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.006 min
Response: 2713080
Conc: 1.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC259240LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

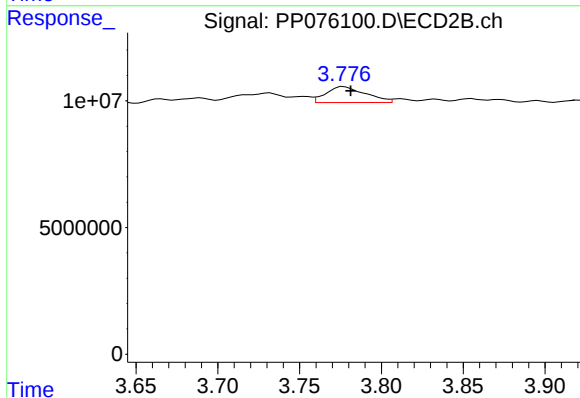


#1 Tetrachloro-m-xylene

R.T.: 3.777 min
Delta R.T.: -0.004 min
Response: 10555099
Conc: 1.59 ng/ml

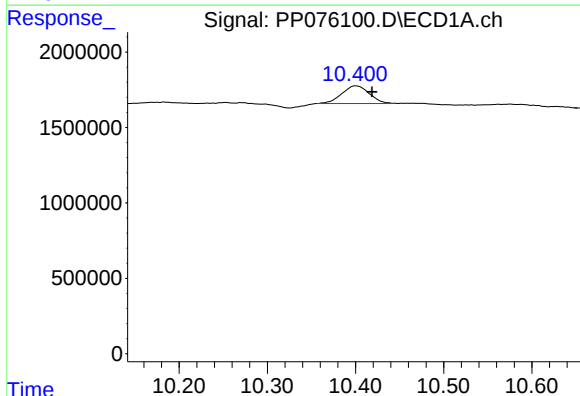

#2 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.019 min
Response: 2561066
Conc: 2.38 ng/ml m

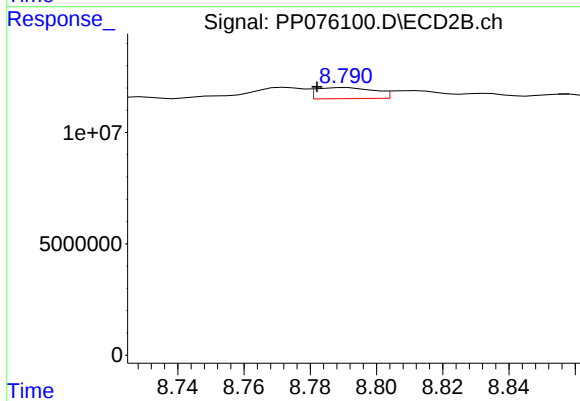

#2 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: 0.009 min
Response: 6036388
Conc: 0.73 ng/ml