

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102725\
 Data File : PP076101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2025 21:42
 Operator : YP\AJ
 Sample : Q3459-06 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC259240LOK-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/28/2025
 Supervised By :mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:08:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.640	3.780	2264891	6267156	1.585	0.947 #
2) SA Decachlor...	10.406	8.783	2271411	7164887	2.110m	0.871m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102725\
Data File : PP076101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2025 21:42
Operator : YP\AJ
Sample : Q3459-06 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC259240LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:08:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

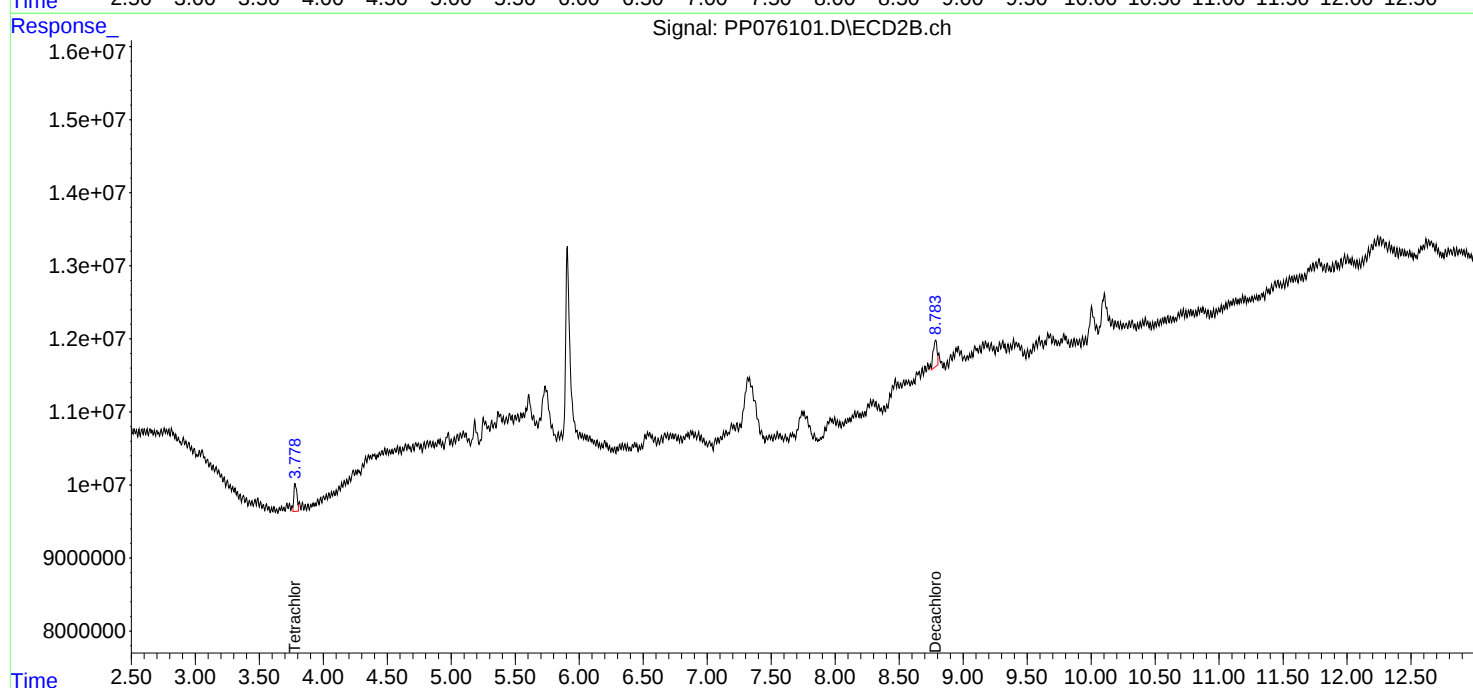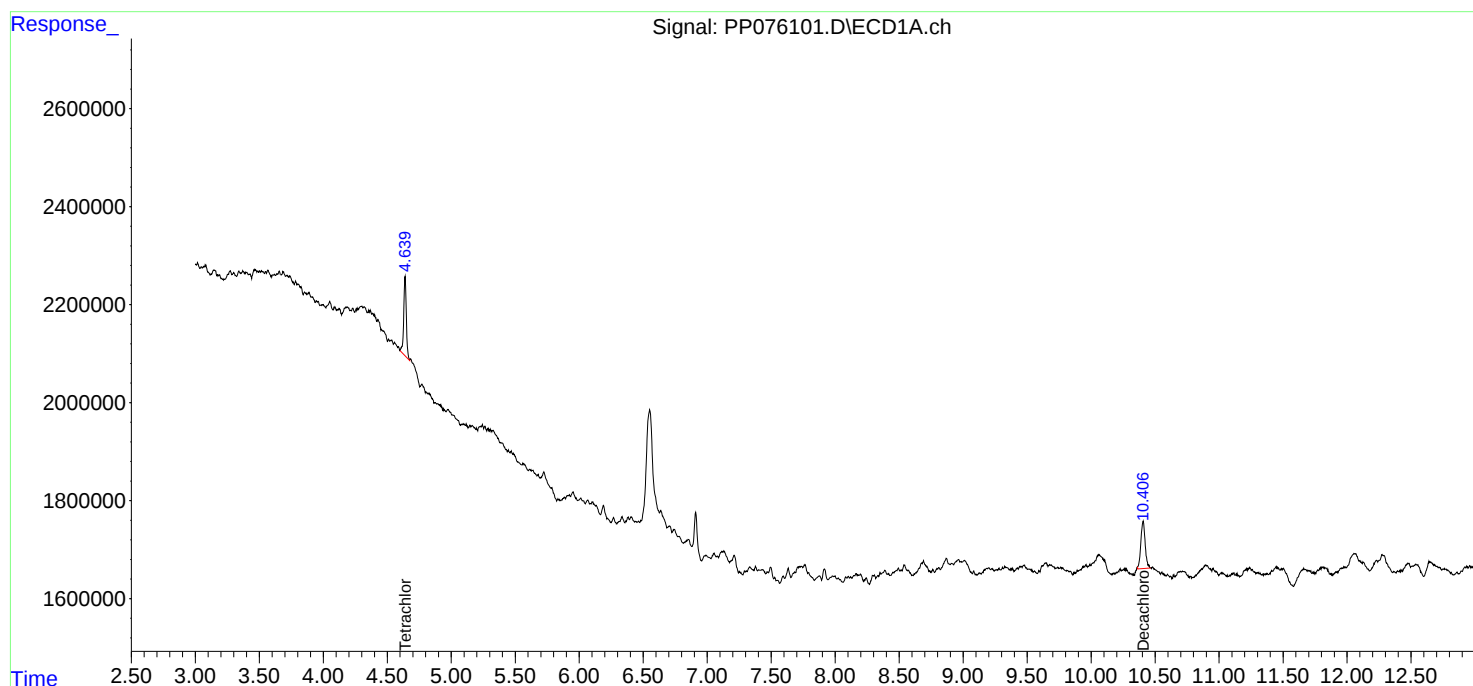

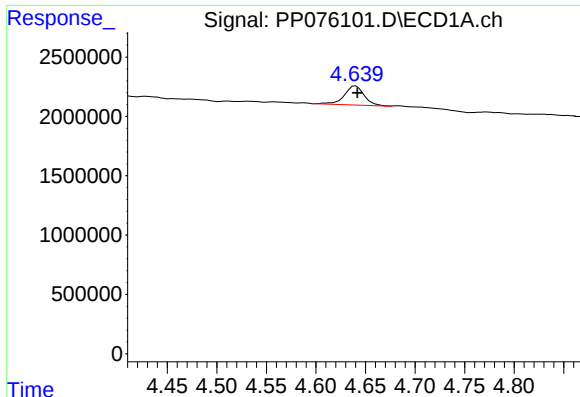


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.002 min
Response: 2264891
Conc: 1.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC259240LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

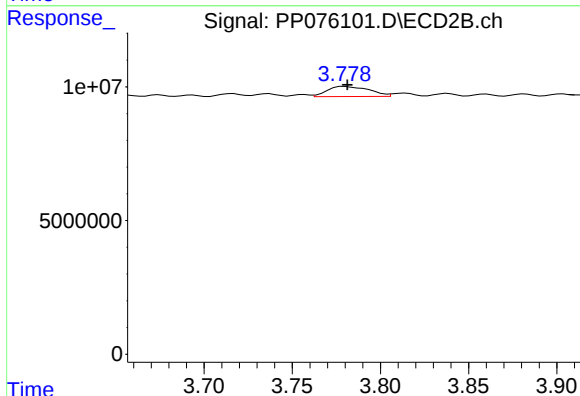


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 6267156
Conc: 0.95 ng/ml

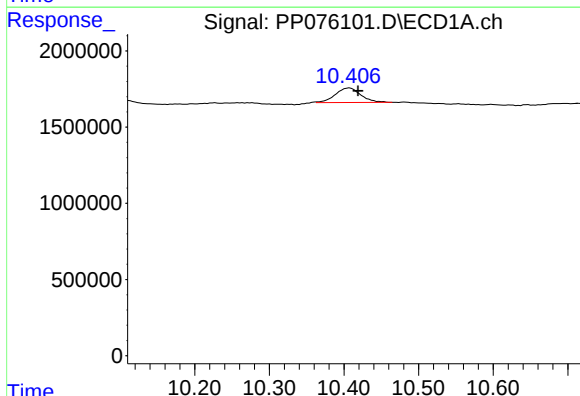

#2 Decachlorobiphenyl

R.T.: 10.406 min
Delta R.T.: -0.013 min
Response: 2271411
Conc: 2.11 ng/ml m

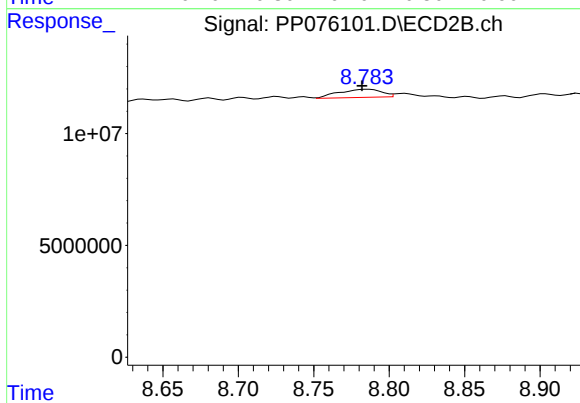

#2 Decachlorobiphenyl

R.T.: 8.783 min
Delta R.T.: 0.001 min
Response: 7164887
Conc: 0.87 ng/ml m