

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102820\
 Data File : PP030905.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2020 11:34
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 11:58:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1232PP102520.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 26 04:46:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.803	4.080	1418264	1267945	21.157	20.392
2)	SA Decachlor...	10.689	9.415	843770	901516	22.974	22.786

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102820\
Data File : PP030905.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2020 11:34
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 11:58:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1232PP102520.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 26 04:46:19 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

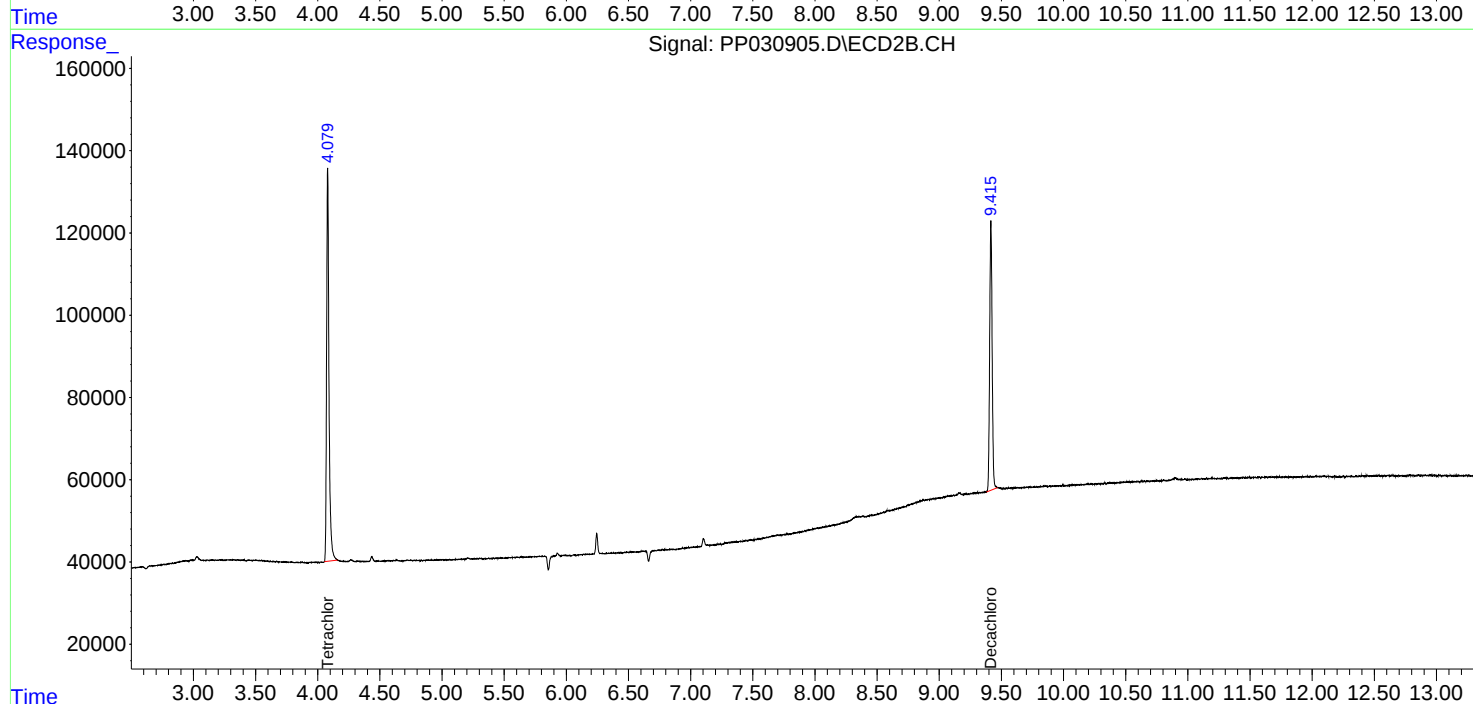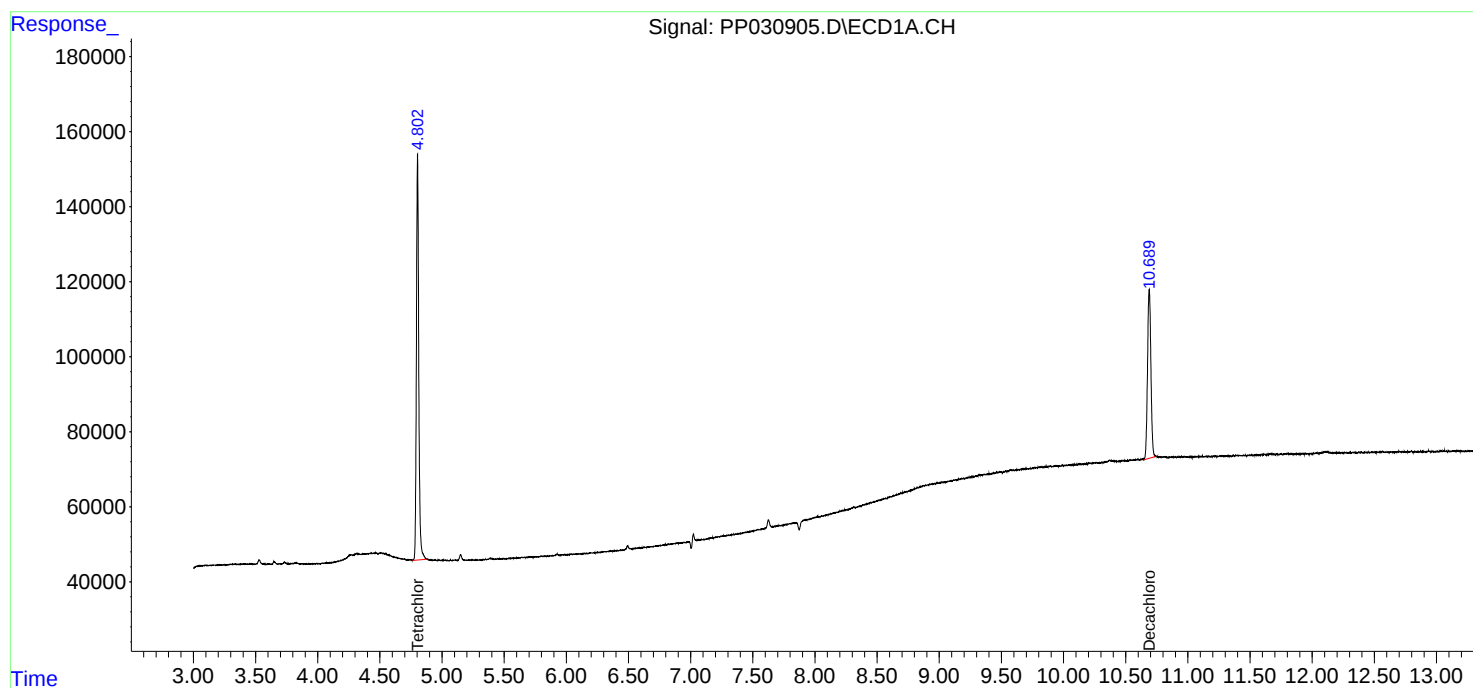


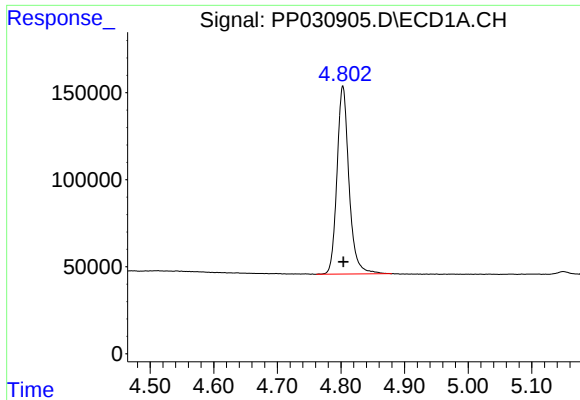

#1 Tetrachloro-m-xylene


R.T.: 4.803 min
Delta R.T.: -0.001 min
Response: 1418264
Conc: 21.16 ng/ml

Instrument :
ECD_P
ClientSampleId :

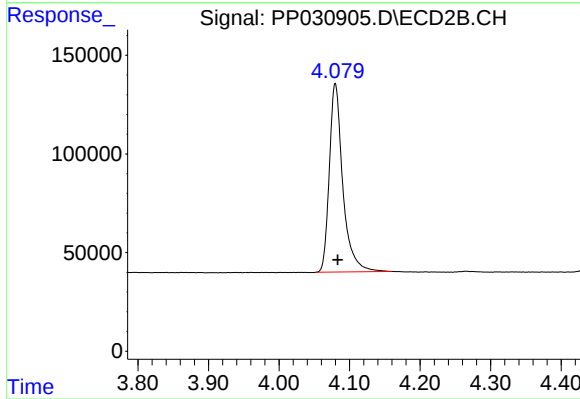


#1 Tetrachloro-m-xylene

R.T.: 4.080 min
Delta R.T.: -0.004 min
Response: 1267945
Conc: 20.39 ng/ml

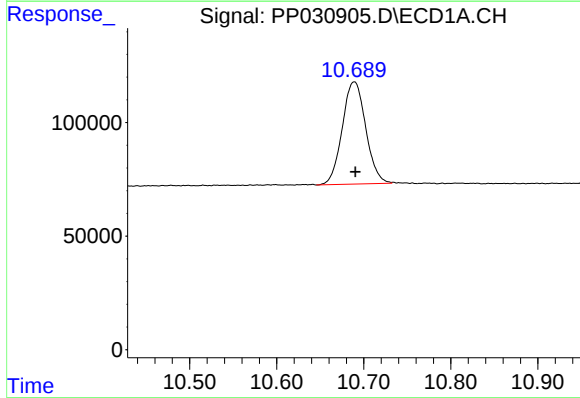

#2 Decachlorobiphenyl

R.T.: 10.689 min
Delta R.T.: -0.001 min
Response: 843770
Conc: 22.97 ng/ml

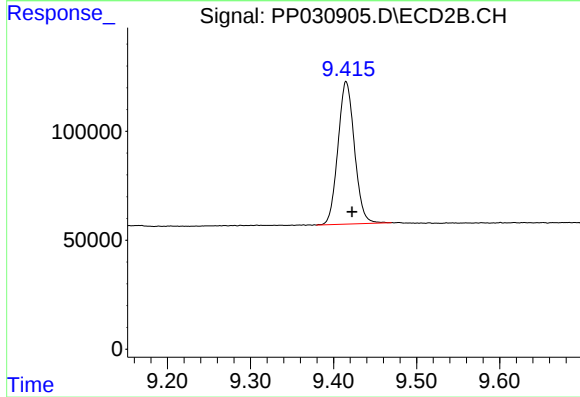

#2 Decachlorobiphenyl

R.T.: 9.415 min
Delta R.T.: -0.007 min
Response: 901516
Conc: 22.79 ng/ml