

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102820\
 Data File : PP030894.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2020 8:30
 Operator : DD\AJ
 Sample : MDL-PCB-BL-S-7
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-S-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 11:30:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1232PP102520.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 26 04:46:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.802	4.080	1112150	988390	16.591	15.896
2)	SA Decachlor...	10.688	9.415	655542	693200	17.849	17.521

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102820\
Data File : PP030894.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2020 8:30
Operator : DD\AJ
Sample : MDL-PCB-BL-S-7
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 11:30:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1232PP102520.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 26 04:46:19 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

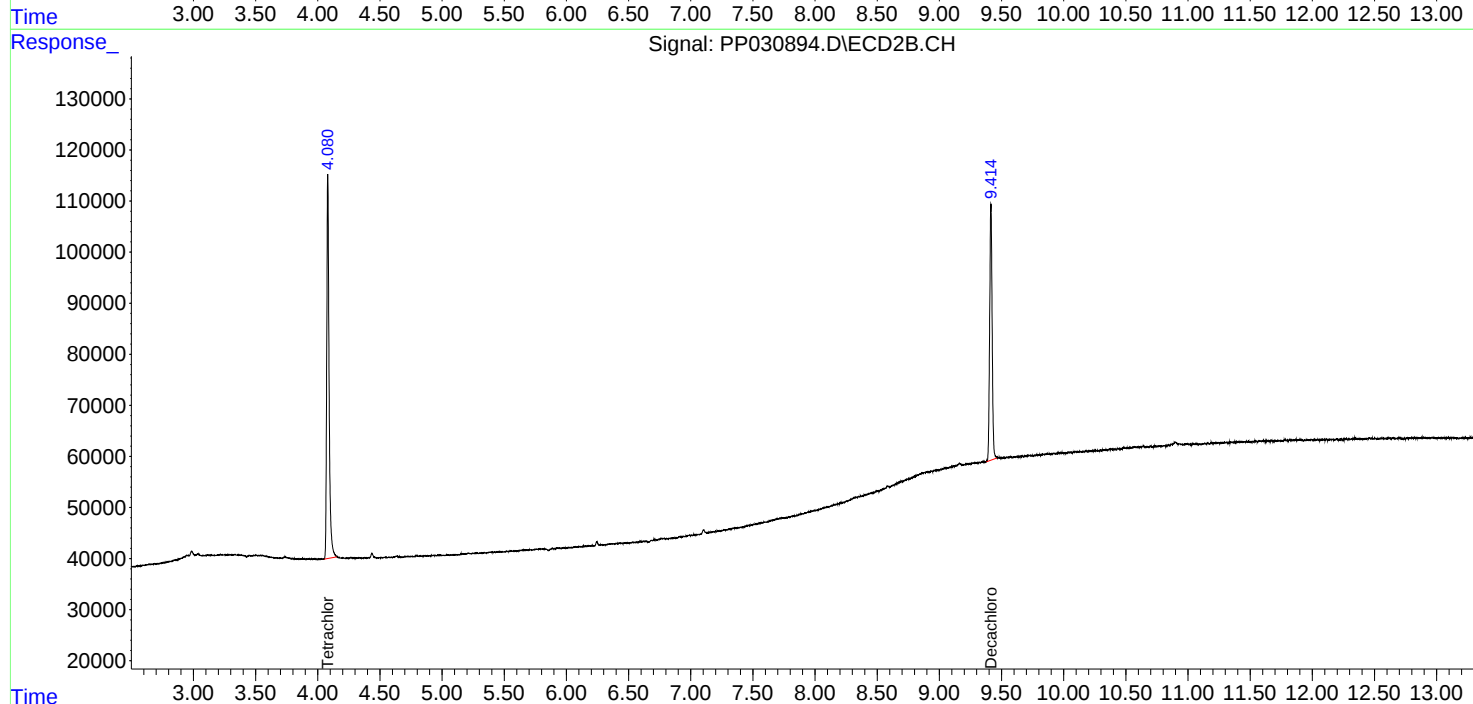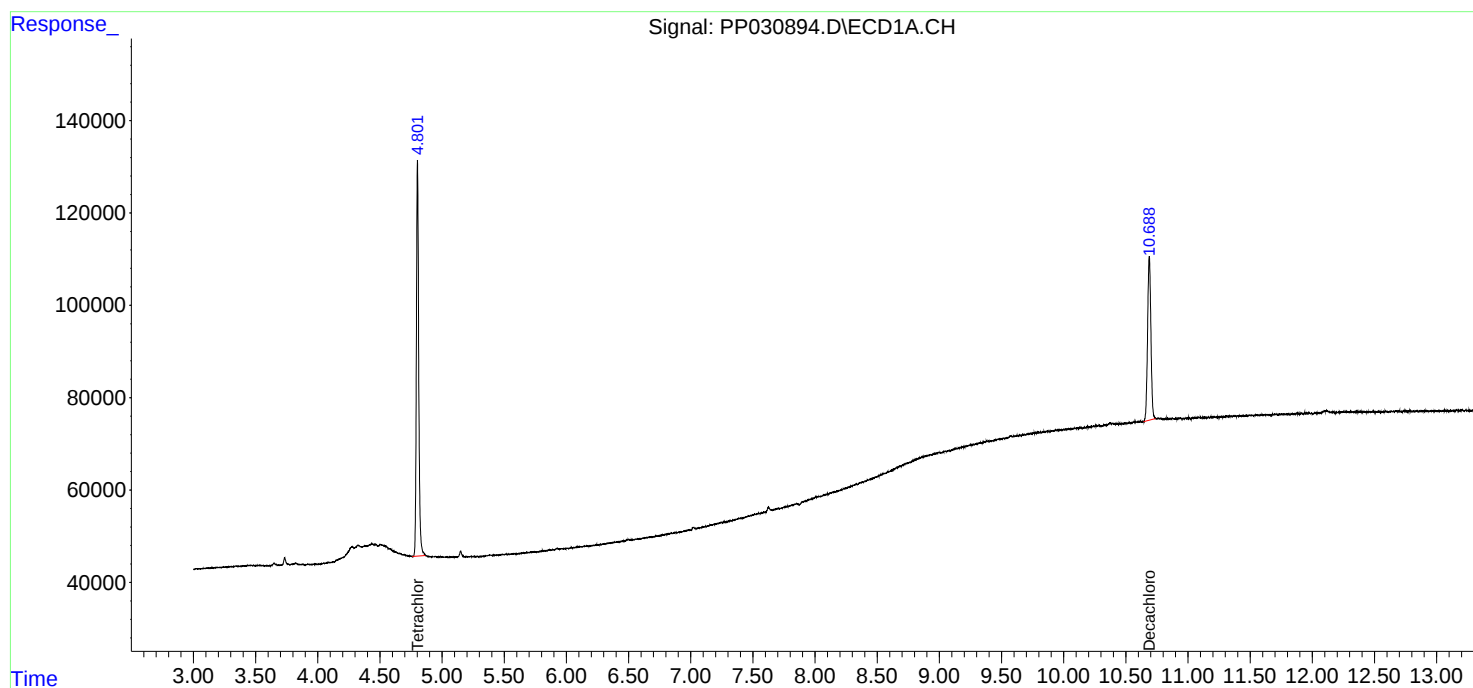


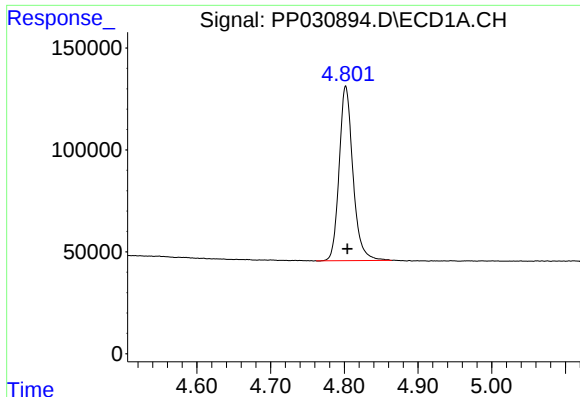

#1 Tetrachloro-m-xylene


R.T.: 4.802 min
Delta R.T.: -0.002 min
Response: 1112150
Conc: 16.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-7

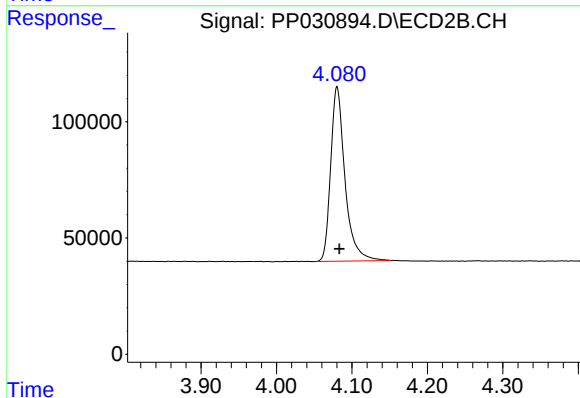


#1 Tetrachloro-m-xylene

R.T.: 4.080 min
Delta R.T.: -0.003 min
Response: 988390
Conc: 15.90 ng/ml

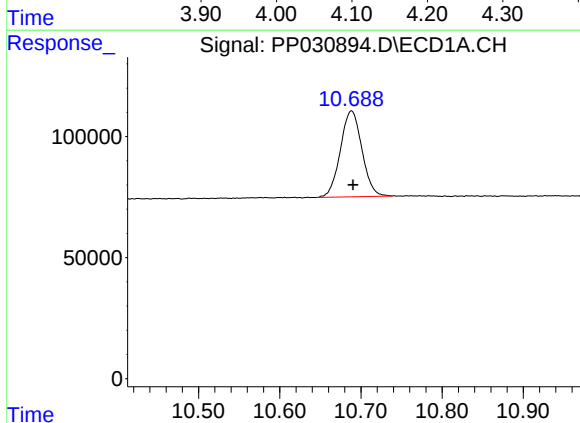

#2 Decachlorobiphenyl

R.T.: 10.688 min
Delta R.T.: -0.002 min
Response: 655542
Conc: 17.85 ng/ml

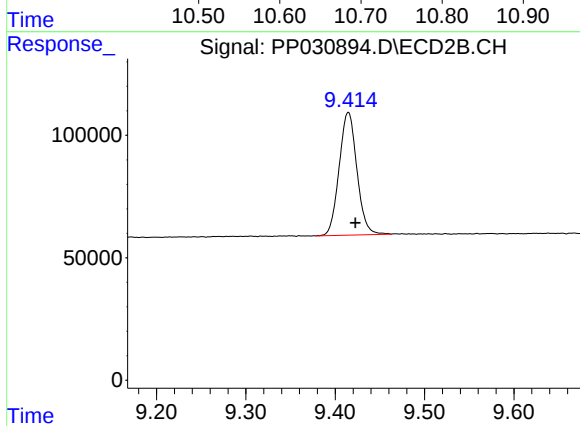

#2 Decachlorobiphenyl

R.T.: 9.415 min
Delta R.T.: -0.008 min
Response: 693200
Conc: 17.52 ng/ml