

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
 Data File : PP040510.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 14:55
 Operator : AJ\MA
 Sample : M4380-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WASTE-CHAR-(SUSPECT)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 15:03:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 28 08:58:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.750	3.772	939351	563073	23.063	20.669
2) SA Decachlor...	10.682	9.056	639133	561710	21.096	20.021

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
Data File : PP040510.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 14:55
Operator : AJ\MA
Sample : M4380-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
WASTE-CHAR-(SUSPECT)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 15:03:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

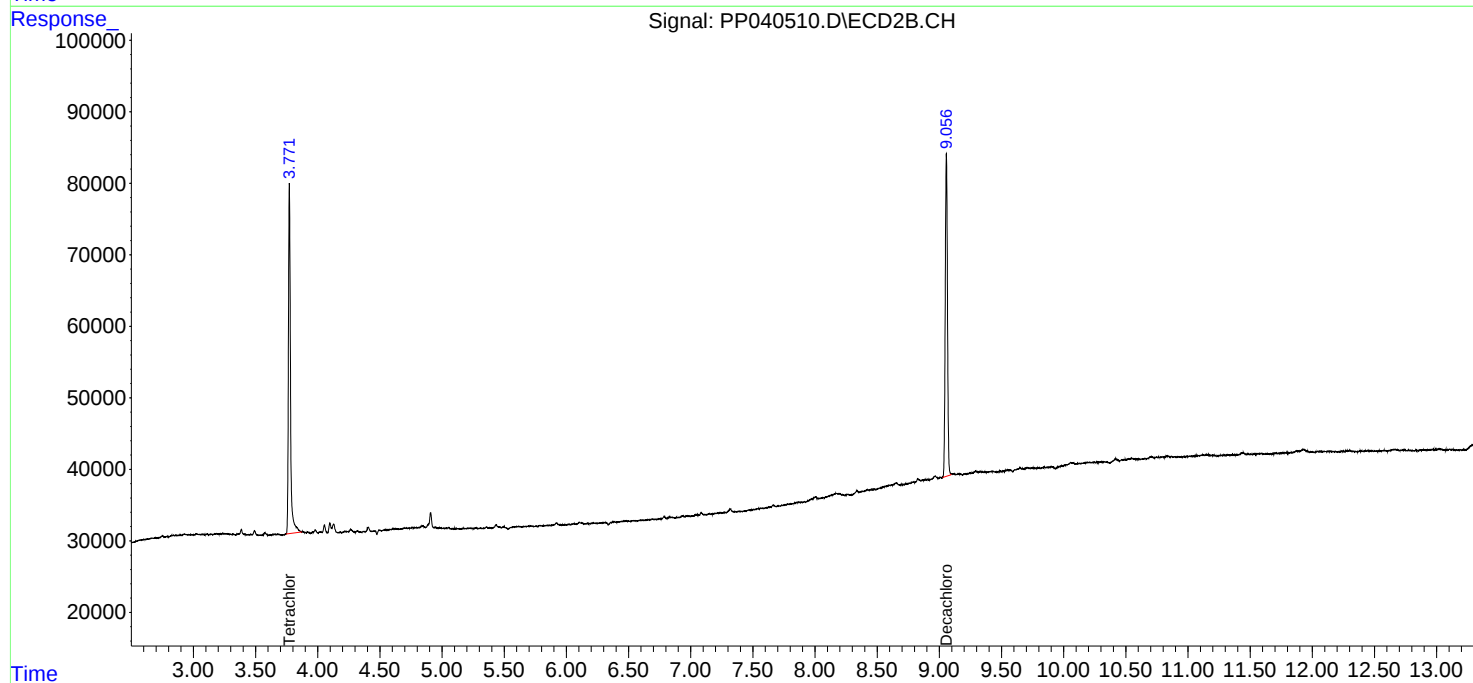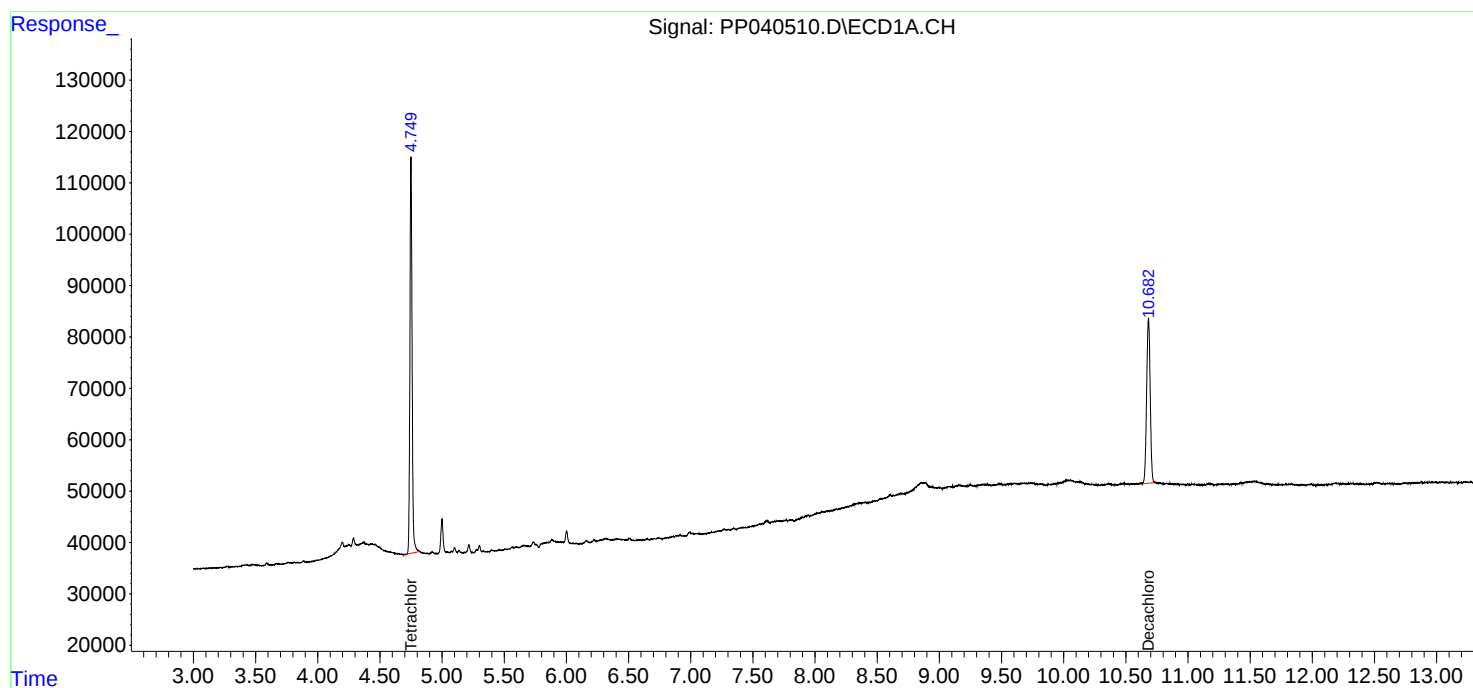


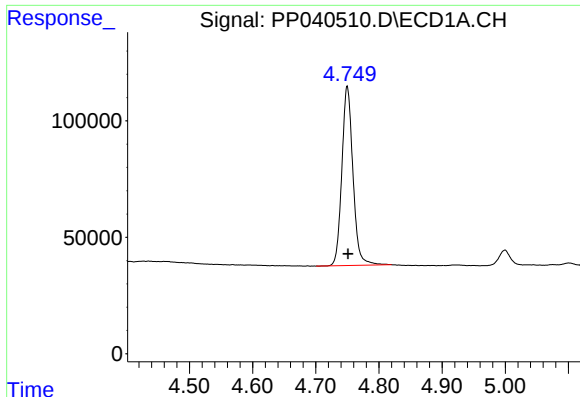

#1 Tetrachloro-m-xylene


R.T.: 4.750 min
Delta R.T.: -0.001 min
Response: 939351
Conc: 23.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
WASTE-CHAR-(SUSPECT)

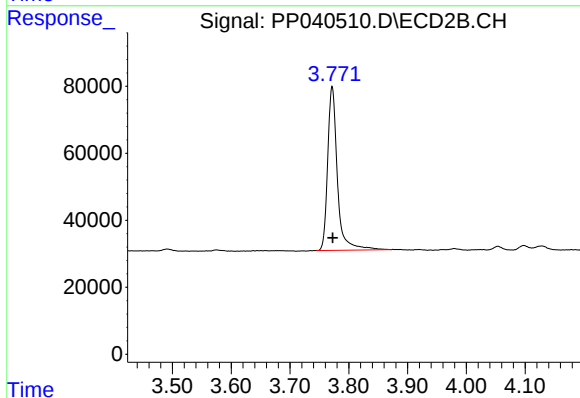


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
Delta R.T.: 0.000 min
Response: 563073
Conc: 20.67 ng/ml

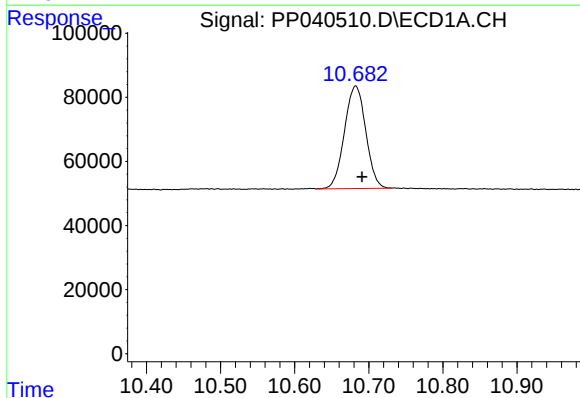

#2 Decachlorobiphenyl

R.T.: 10.682 min
Delta R.T.: -0.009 min
Response: 639133
Conc: 21.10 ng/ml

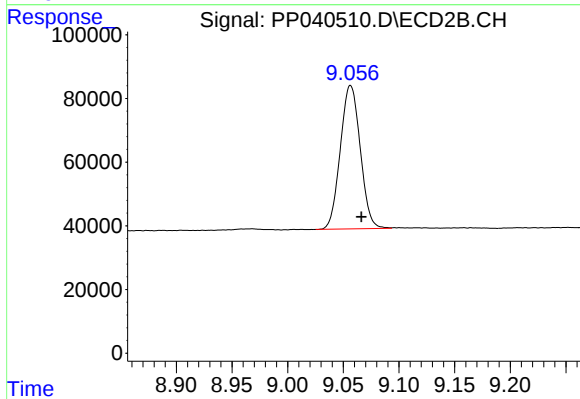

#2 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: -0.010 min
Response: 561710
Conc: 20.02 ng/ml