

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
Data File : PP040514.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 16:02
Operator : AJ\MA
Sample : PB140316BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB140316BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:52:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.751	3.772	854290	500296	20.974	18.364
2) SA Decachlor...	10.680	9.057	619229	551924	20.439	19.672

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
Data File : PP040514.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 16:02
Operator : AJ\MA
Sample : PB140316BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB140316BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:52:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

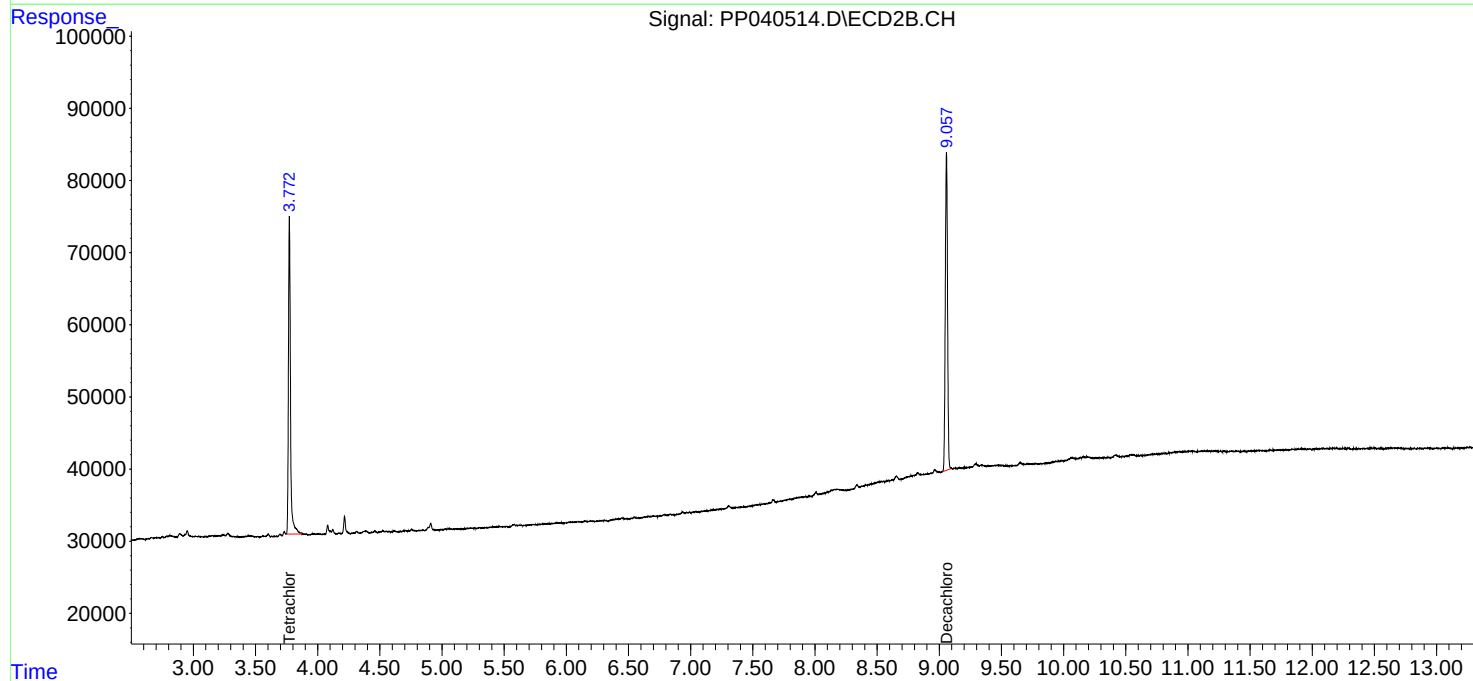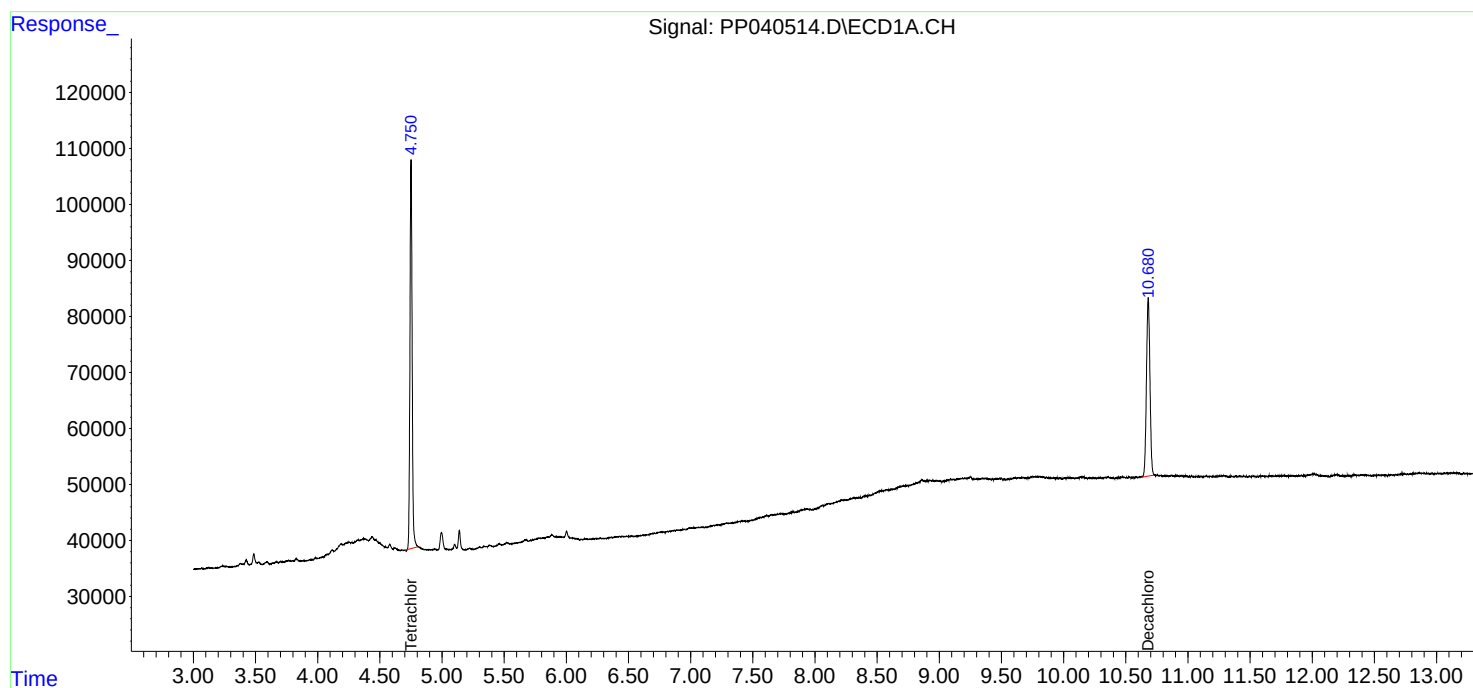


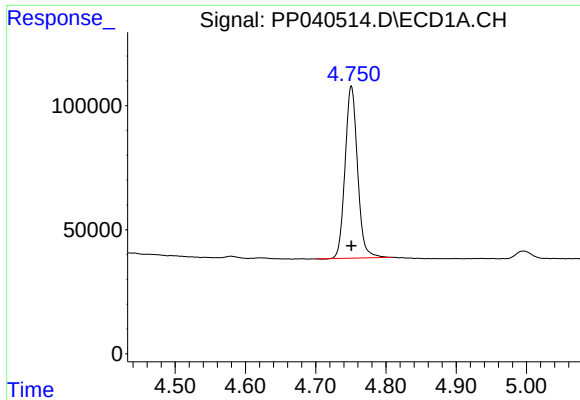

#1 Tetrachloro-m-xylene


R.T.: 4.751 min
Delta R.T.: 0.000 min
Response: 854290
Conc: 20.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB140316BL

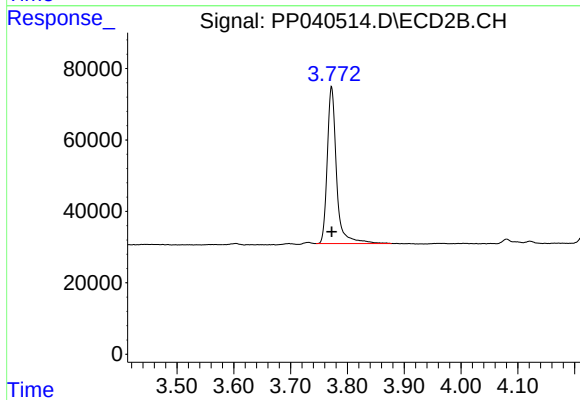


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
Delta R.T.: 0.000 min
Response: 500296
Conc: 18.36 ng/ml

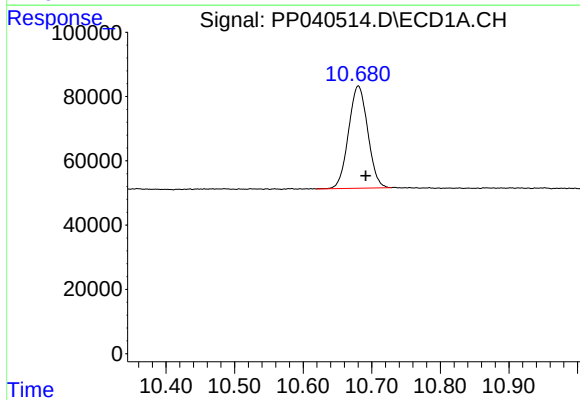

#2 Decachlorobiphenyl

R.T.: 10.680 min
Delta R.T.: -0.011 min
Response: 619229
Conc: 20.44 ng/ml

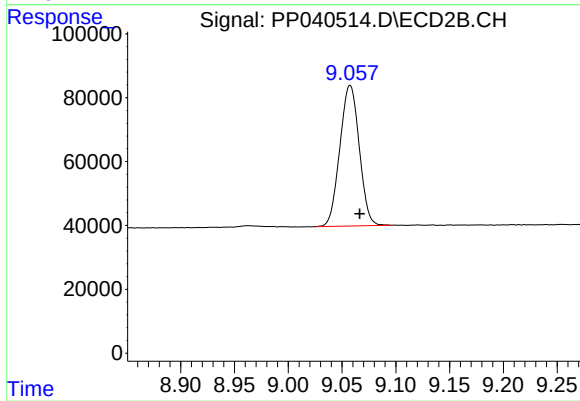

#2 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.009 min
Response: 551924
Conc: 19.67 ng/ml