

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
 Data File : PP040526.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 19:50
 Operator : AJ\MA
 Sample : M4384-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-TOTE

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 10/29/2021
 Supervised By :mohammad ahmed 10/29/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 00:35:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 28 08:58:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.751	3.774	580324	477023	14.248m	17.510
2) SA Decachlor...	10.680	9.056	179952	179826	5.940	6.410
Target Compounds						
16) L4 AR-1242-1	6.069	5.024	95354	27591	98.536	38.008 #
17) L4 AR-1242-2	6.096	5.045	90405	57459	60.171	54.153
18) L4 AR-1242-3	6.162	5.225	78058	83177	82.761	143.023 #
19) L4 AR-1242-4	6.261	5.331	80389	18766	106.588	36.582 #
20) L4 AR-1242-5	7.051	5.896	38087	13116	48.103	19.326 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
Data File : PP040526.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 19:50
Operator : AJ\MA
Sample : M4384-05
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-TOTE


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/29/2021
Supervised By :mohammad ahmed 10/29/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 00:35:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

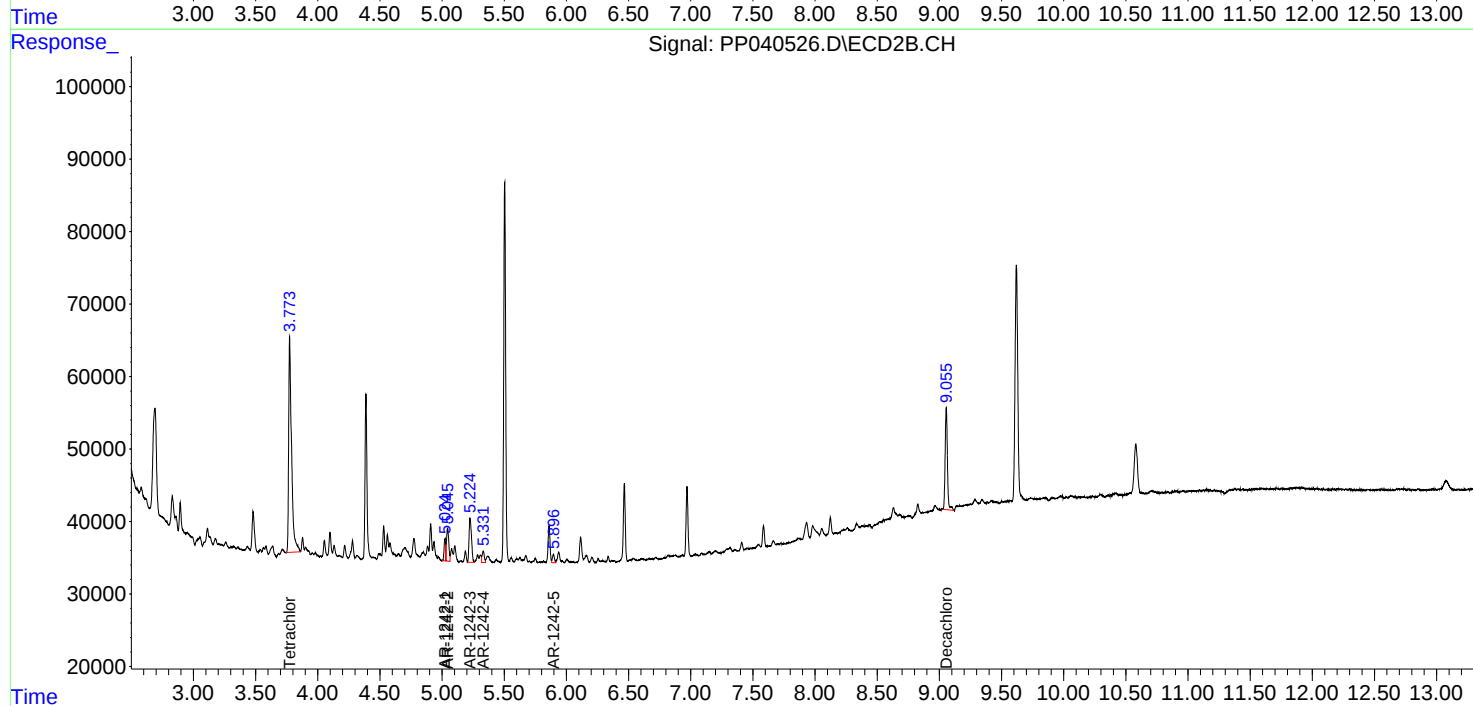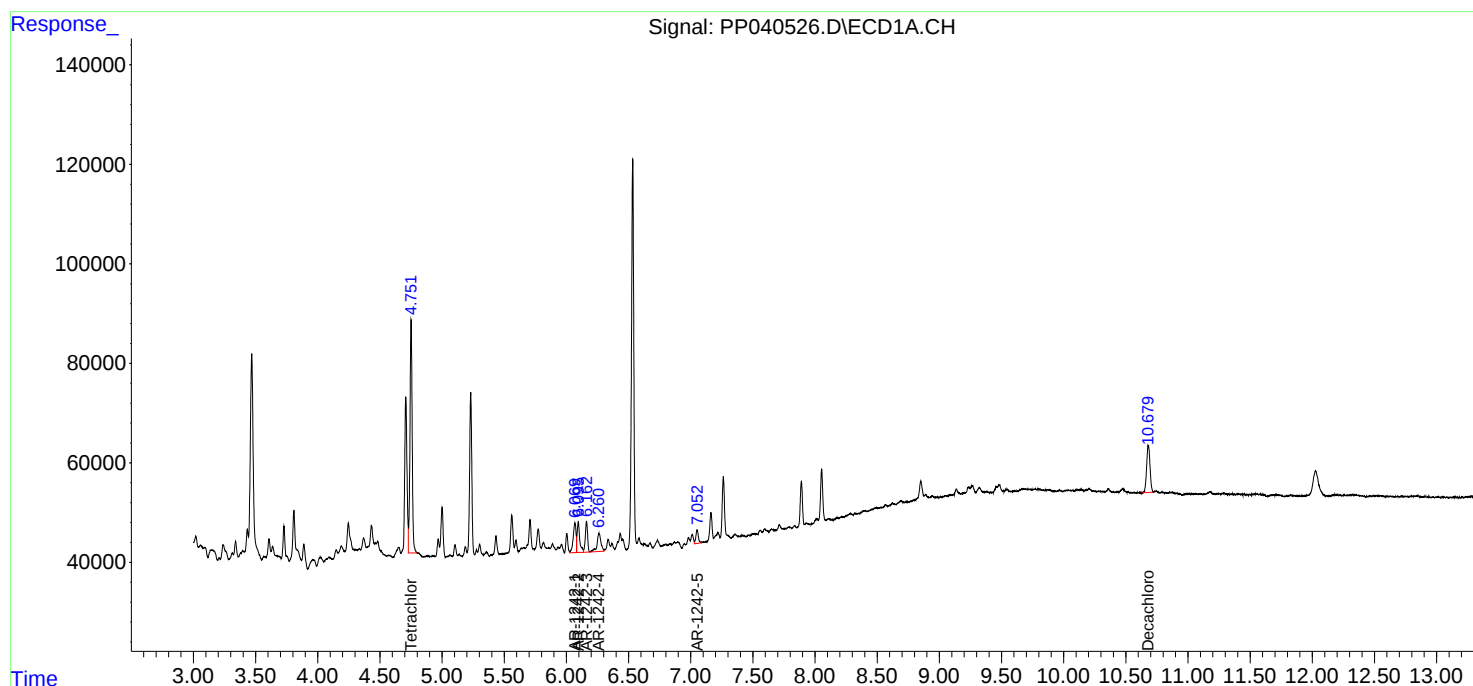

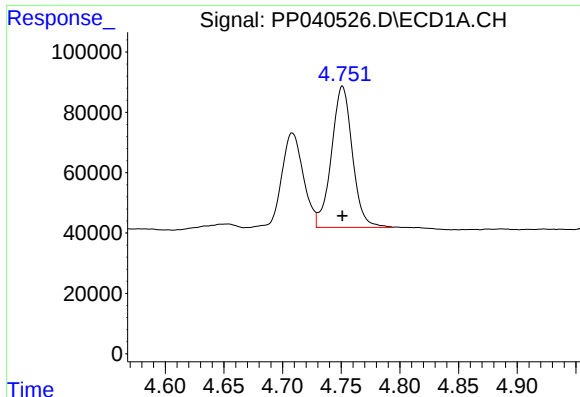


#1 Tetrachloro-m-xylene

R.T.: 4.751 min
Delta R.T.: 0.000 min
Response: 580324
Conc: 14.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-TOTE


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/29/2021
Supervised By :mohammad ahmed 10/29/2021

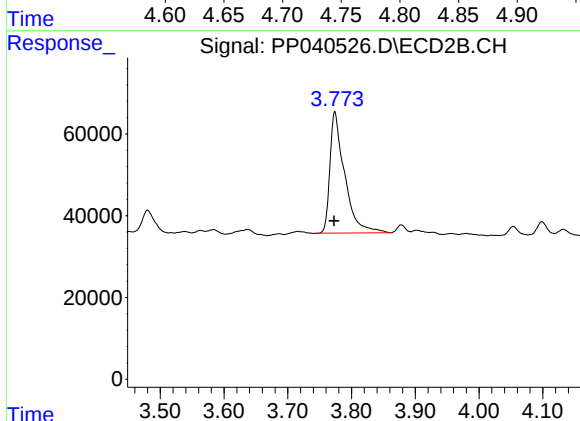


#1 Tetrachloro-m-xylene

R.T.: 3.774 min
Delta R.T.: 0.001 min
Response: 477023
Conc: 17.51 ng/ml

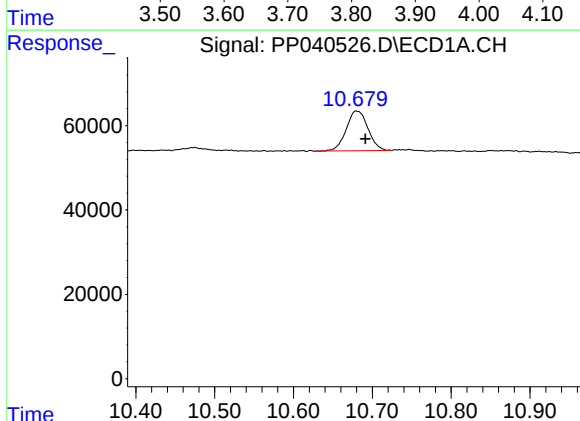


#2 Decachlorobiphenyl

R.T.: 10.680 min
Delta R.T.: -0.012 min
Response: 179952
Conc: 5.94 ng/ml

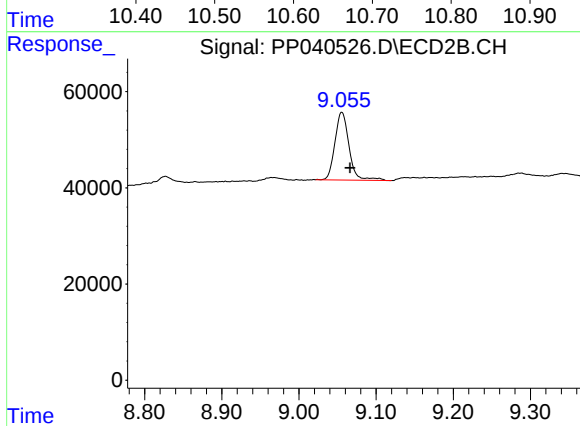

#2 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: -0.011 min
Response: 179826
Conc: 6.41 ng/ml

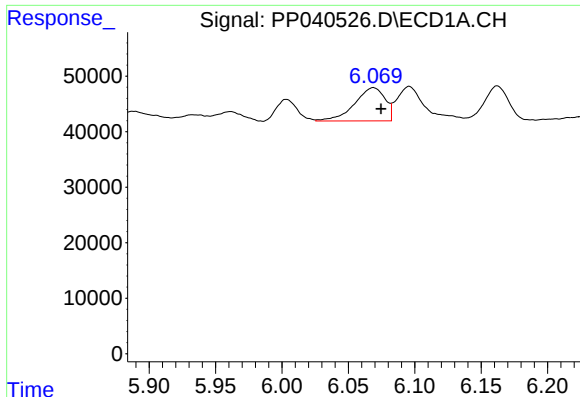


#16 AR-1242-1

R.T.: 6.069 min
Delta R.T.: -0.006 min
Response: 95354
Conc: 98.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-TOTE


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/29/2021
Supervised By :mohammad ahmed 10/29/2021

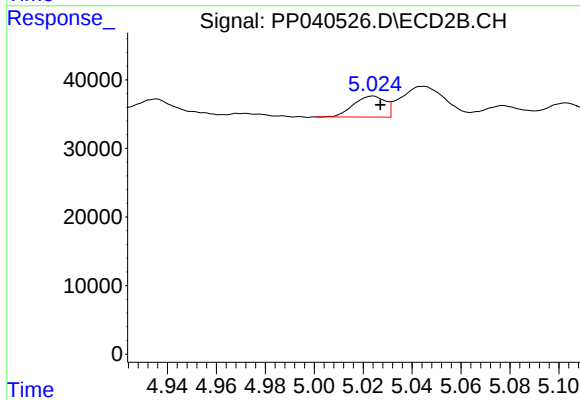


#16 AR-1242-1

R.T.: 5.024 min
Delta R.T.: -0.003 min
Response: 27591
Conc: 38.01 ng/ml

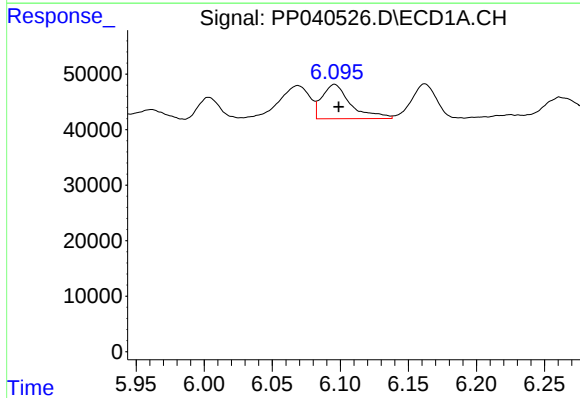


#17 AR-1242-2

R.T.: 6.096 min
Delta R.T.: -0.003 min
Response: 90405
Conc: 60.17 ng/ml

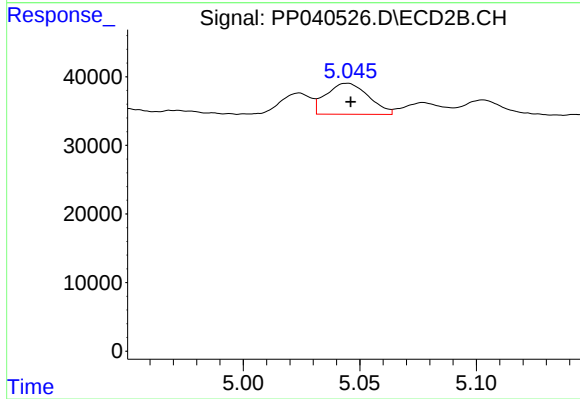

#17 AR-1242-2

R.T.: 5.045 min
Delta R.T.: -0.001 min
Response: 57459
Conc: 54.15 ng/ml

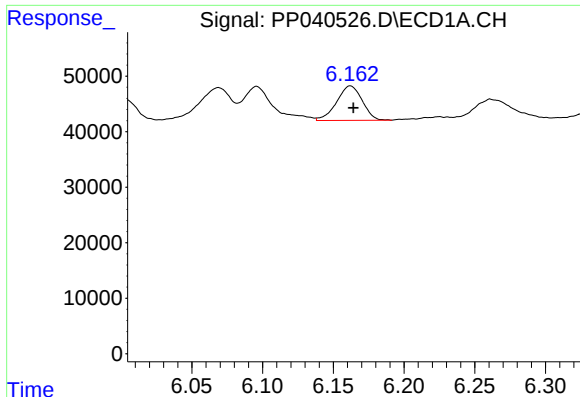


#18 AR-1242-3

R.T.: 6.162 min
Delta R.T.: -0.002 min
Response: 78058
Conc: 82.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-TOTE


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/29/2021
Supervised By :mohammad ahmed 10/29/2021

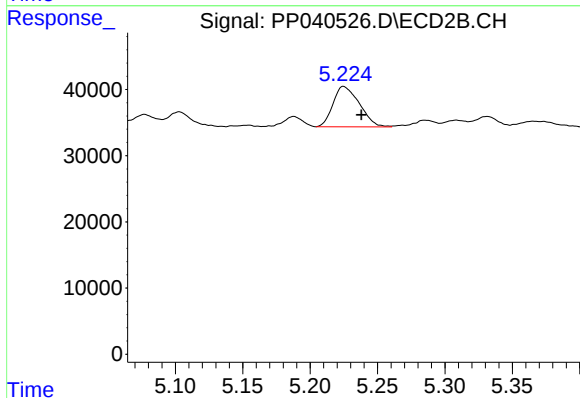


#18 AR-1242-3

R.T.: 5.225 min
Delta R.T.: -0.013 min
Response: 83177
Conc: 143.02 ng/ml

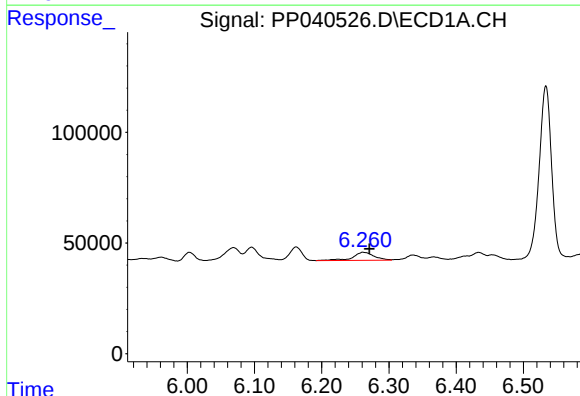


#19 AR-1242-4

R.T.: 6.261 min
Delta R.T.: -0.010 min
Response: 80389
Conc: 106.59 ng/ml

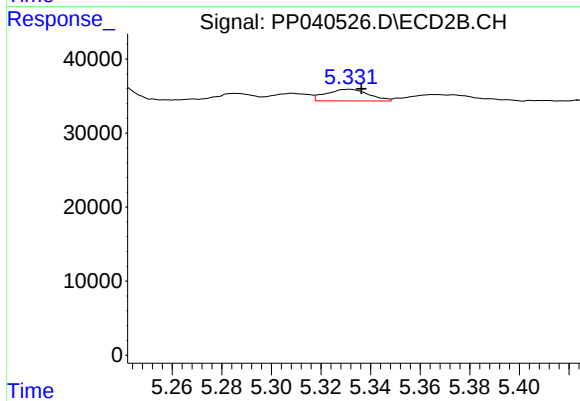

#19 AR-1242-4

R.T.: 5.331 min
Delta R.T.: -0.005 min
Response: 18766
Conc: 36.58 ng/ml

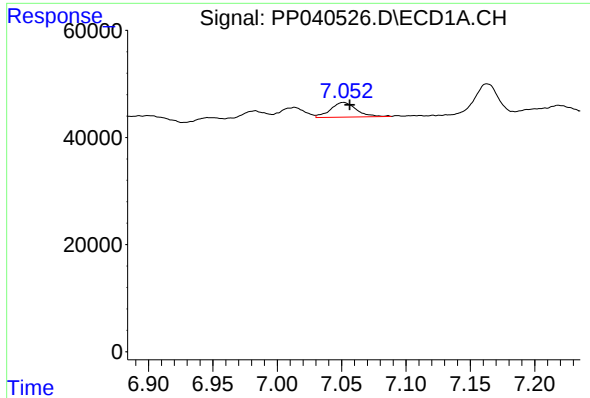


#20 AR-1242-5

R.T.: 7.051 min
Delta R.T.: -0.005 min
Response: 38087
Conc: 48.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-TOTE

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/29/2021
Supervised By :mohammad ahmed 10/29/2021

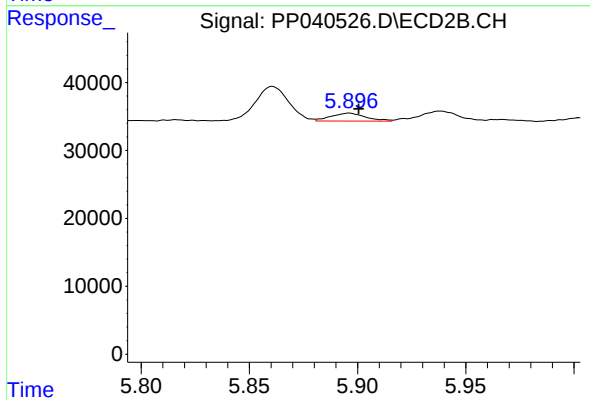

#20 AR-1242-5

R.T.: 5.896 min
Delta R.T.: -0.005 min
Response: 13116
Conc: 19.33 ng/ml