

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
 Data File : PP040539.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 23:55
 Operator : AJ\MA
 Sample : M4384-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-C

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 10/29/2021
 Supervised By :mohammad ahmed 10/29/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 00:43:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 28 08:58:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.752	3.775	599723	341764	14.724	12.545m
2) SA Decachlor...	10.702	9.078	459989	413755	15.183m	14.748

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
Data File : PP040539.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 23:55
Operator : AJ\MA
Sample : M4384-03
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
COMP-C


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/29/2021
Supervised By :mohammad ahmed 10/29/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 00:43:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

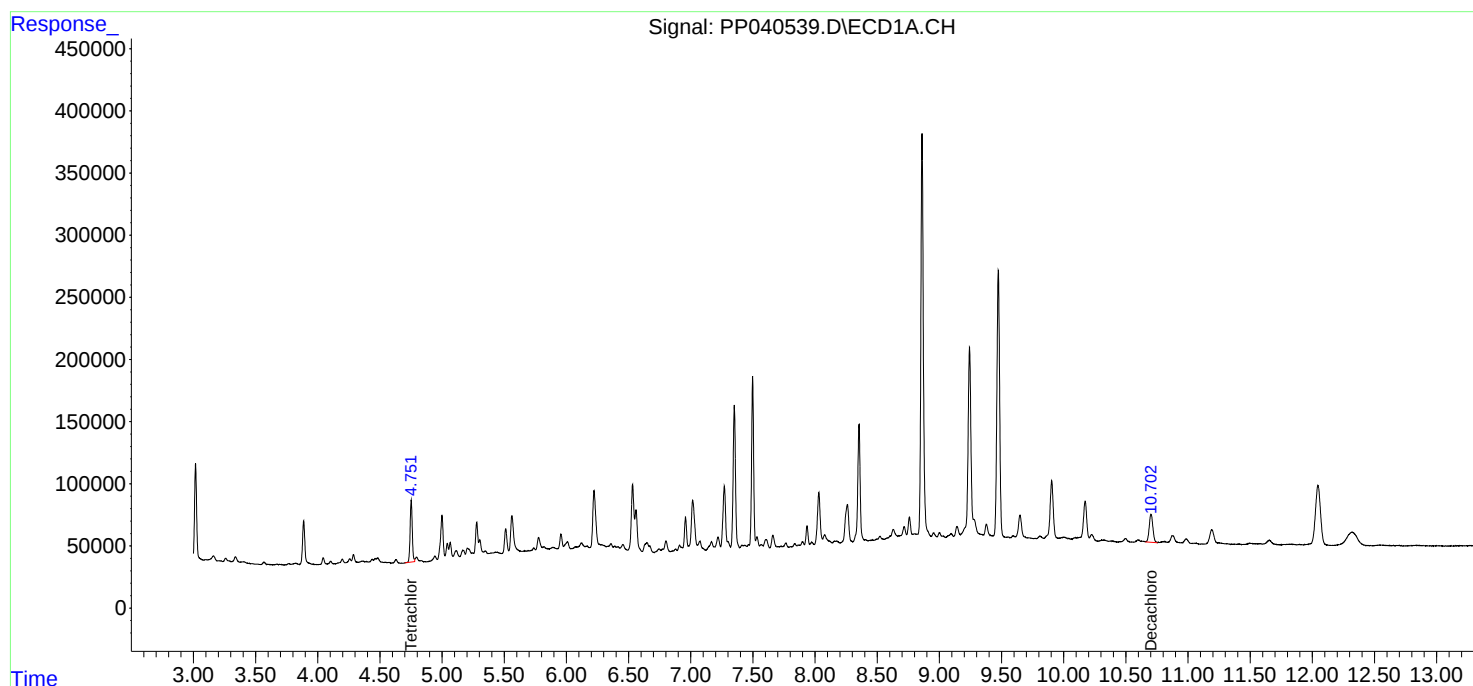

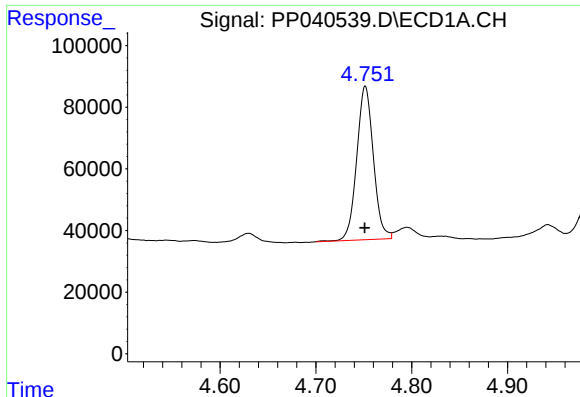


#1 Tetrachloro-m-xylene

R.T.: 4.752 min
Delta R.T.: 0.000 min
Response: 599723
Conc: 14.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-C


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 10/29/2021
Supervised By :mohammad ahmed 10/29/2021

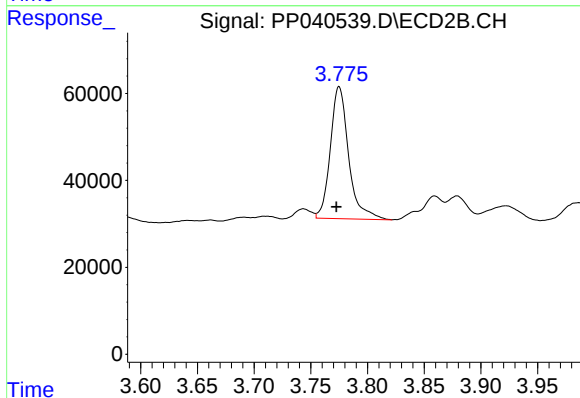


#1 Tetrachloro-m-xylene

R.T.: 3.775 min
Delta R.T.: 0.002 min
Response: 341764
Conc: 12.55 ng/ml m

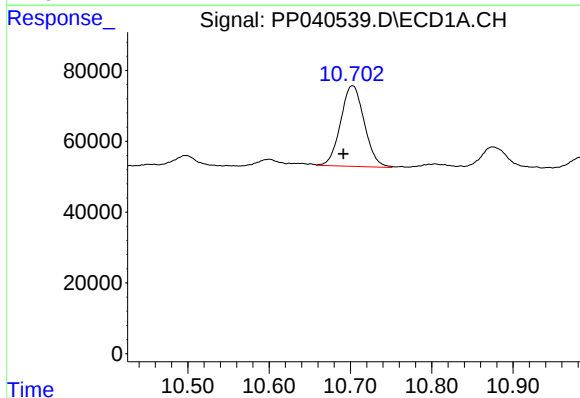

#2 Decachlorobiphenyl

R.T.: 10.702 min
Delta R.T.: 0.011 min
Response: 459989
Conc: 15.18 ng/ml m

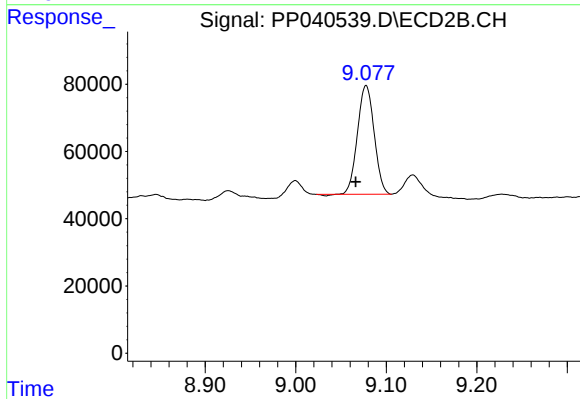

#2 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: 0.011 min
Response: 413755
Conc: 14.75 ng/ml