

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
Data File : PP040548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 3:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 04:38:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.751	3.772	945161	546995	23.205	20.079
2)	SA Decachlor...	10.682	9.055	669436	600435	22.096	21.402

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102821\
Data File : PP040548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 3:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 04:38:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

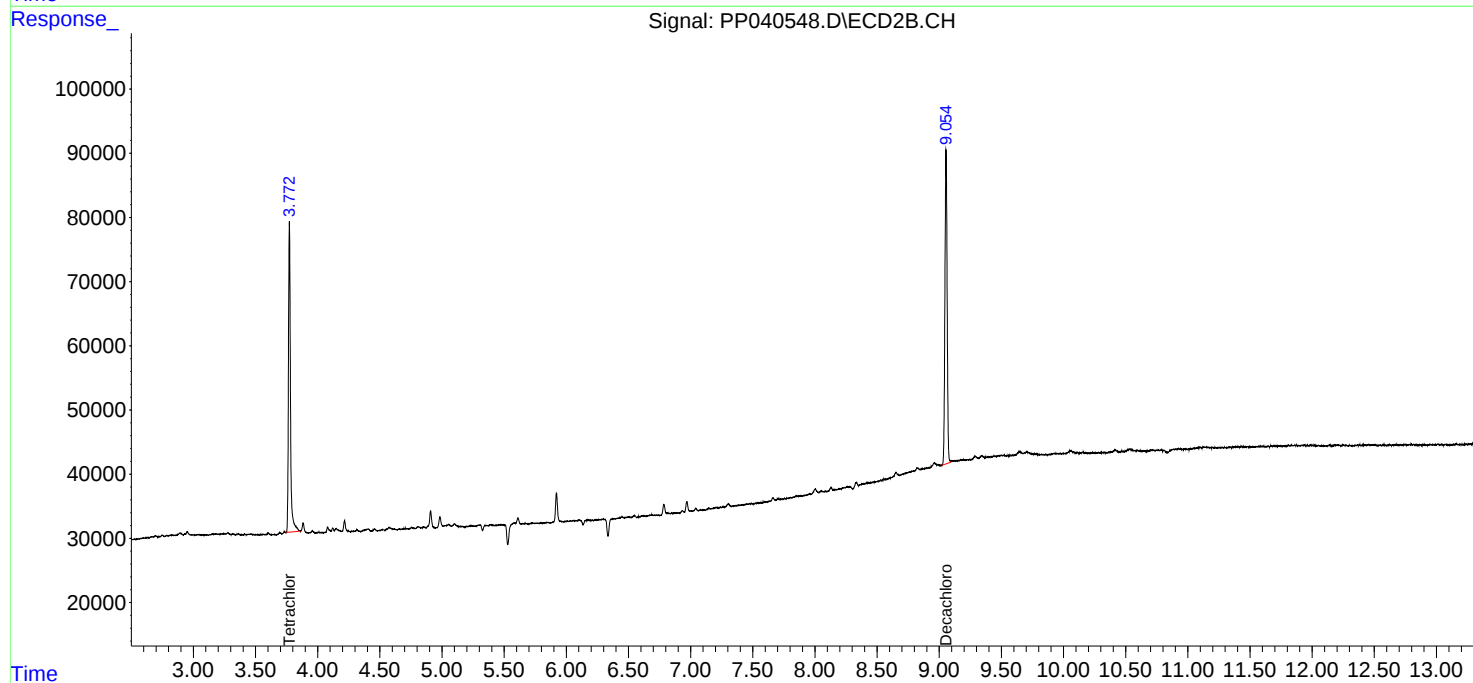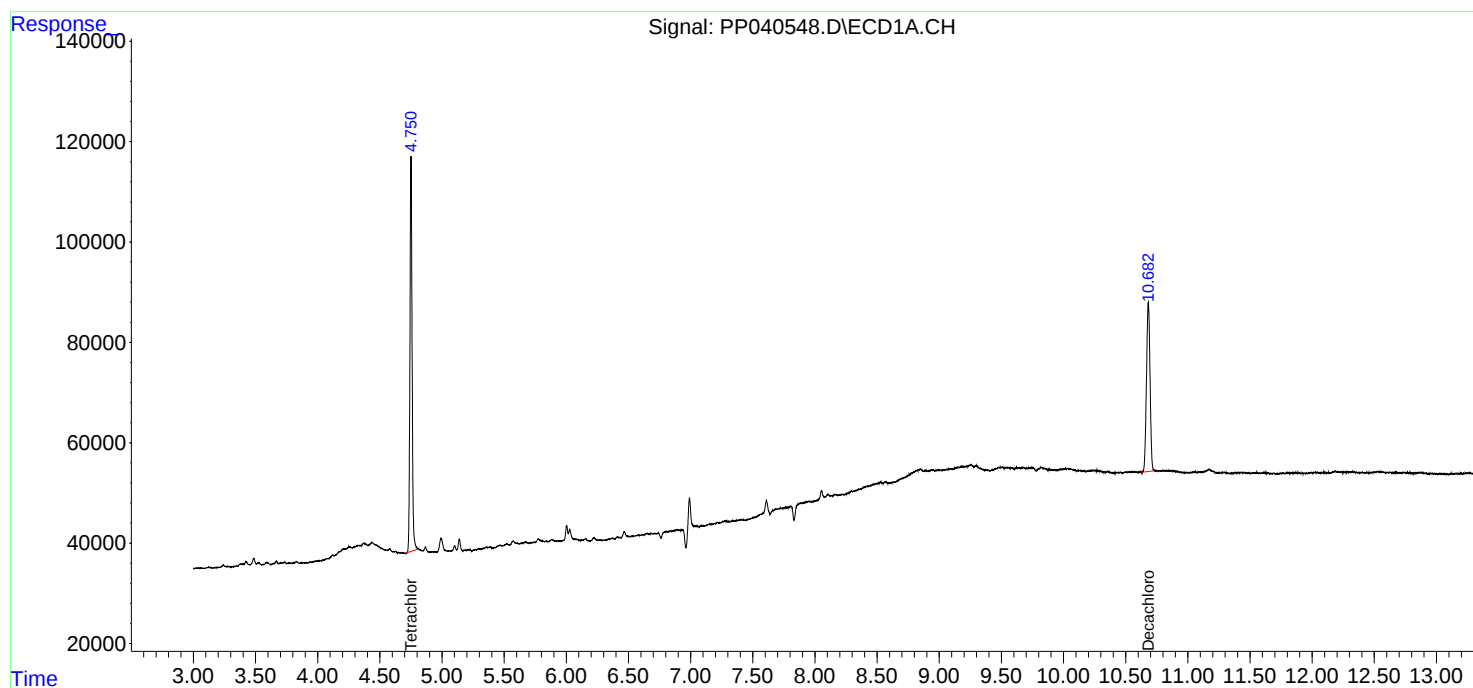


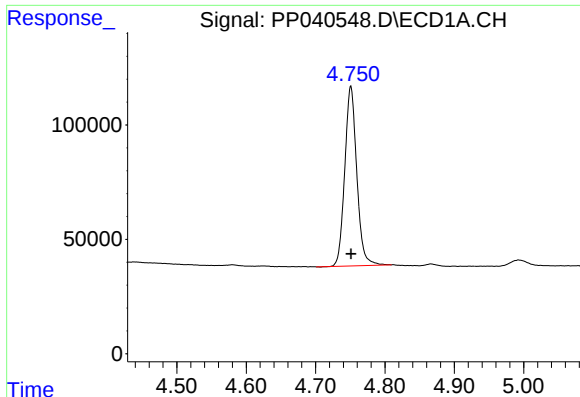

#1 Tetrachloro-m-xylene


R.T.: 4.751 min
Delta R.T.: 0.000 min
Response: 945161
Conc: 23.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

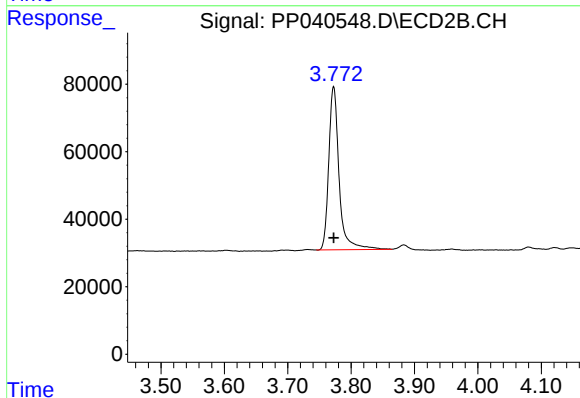


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
Delta R.T.: 0.000 min
Response: 546995
Conc: 20.08 ng/ml

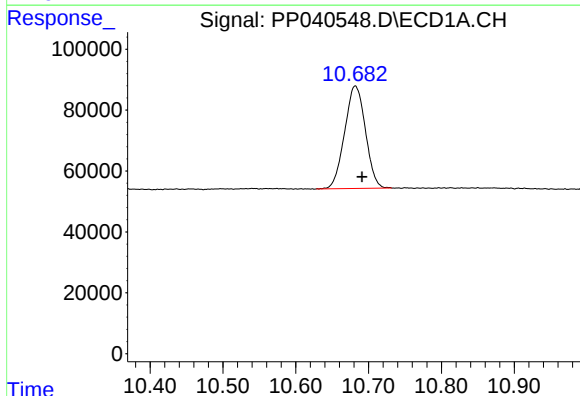

#2 Decachlorobiphenyl

R.T.: 10.682 min
Delta R.T.: -0.009 min
Response: 669436
Conc: 22.10 ng/ml

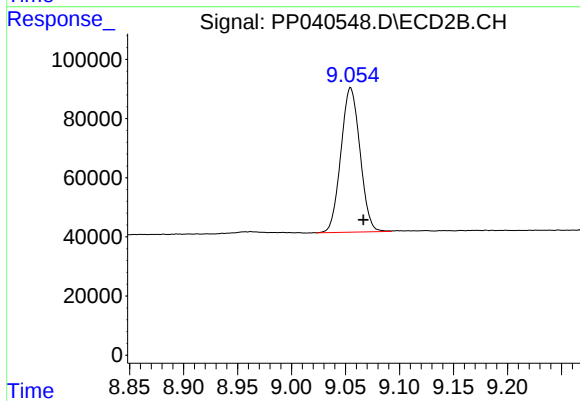

#2 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: -0.012 min
Response: 600435
Conc: 21.40 ng/ml