

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
 Data File : PP052801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 10:44
 Operator : YP\AJ
 Sample : N4955-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:02:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.650	33478437	31668308	15.151	16.852
2) SA Decachlor...	10.209	8.734	22157697	32811086	17.456	19.564
Target Compounds						
21) L5 AR-1248-1	5.579	4.750	724339	799197	17.833	19.968
22) L5 AR-1248-2	5.854	4.991	1043559	1130735	17.533	19.970
23) L5 AR-1248-3	6.060	5.033	1191583	1191055	18.355	20.286
24) L5 AR-1248-4	6.464	5.208	1374433	1479830	21.341	21.252
25) L5 AR-1248-5	6.503	5.606	1416853	1206138	22.366	19.012



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
Data File : PP052801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 10:44
Operator : YP\AJ
Sample : N4955-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:02:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

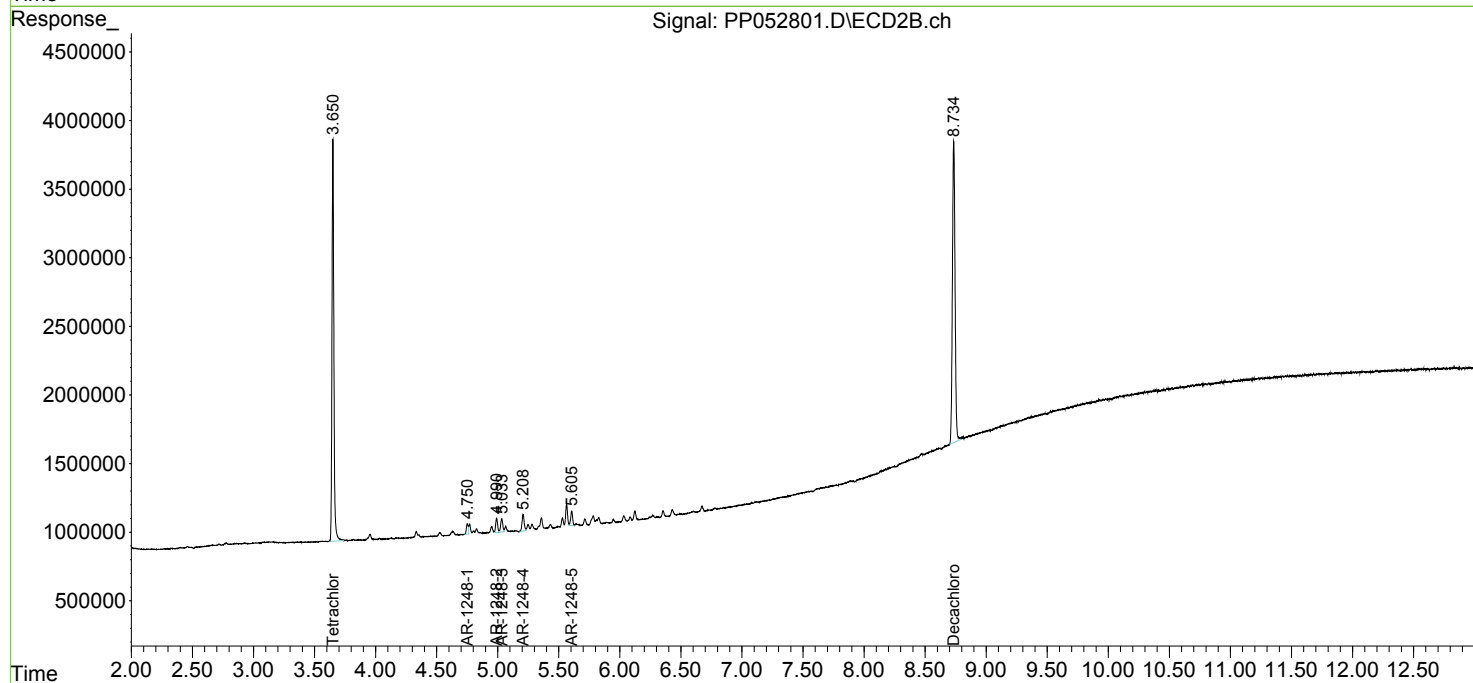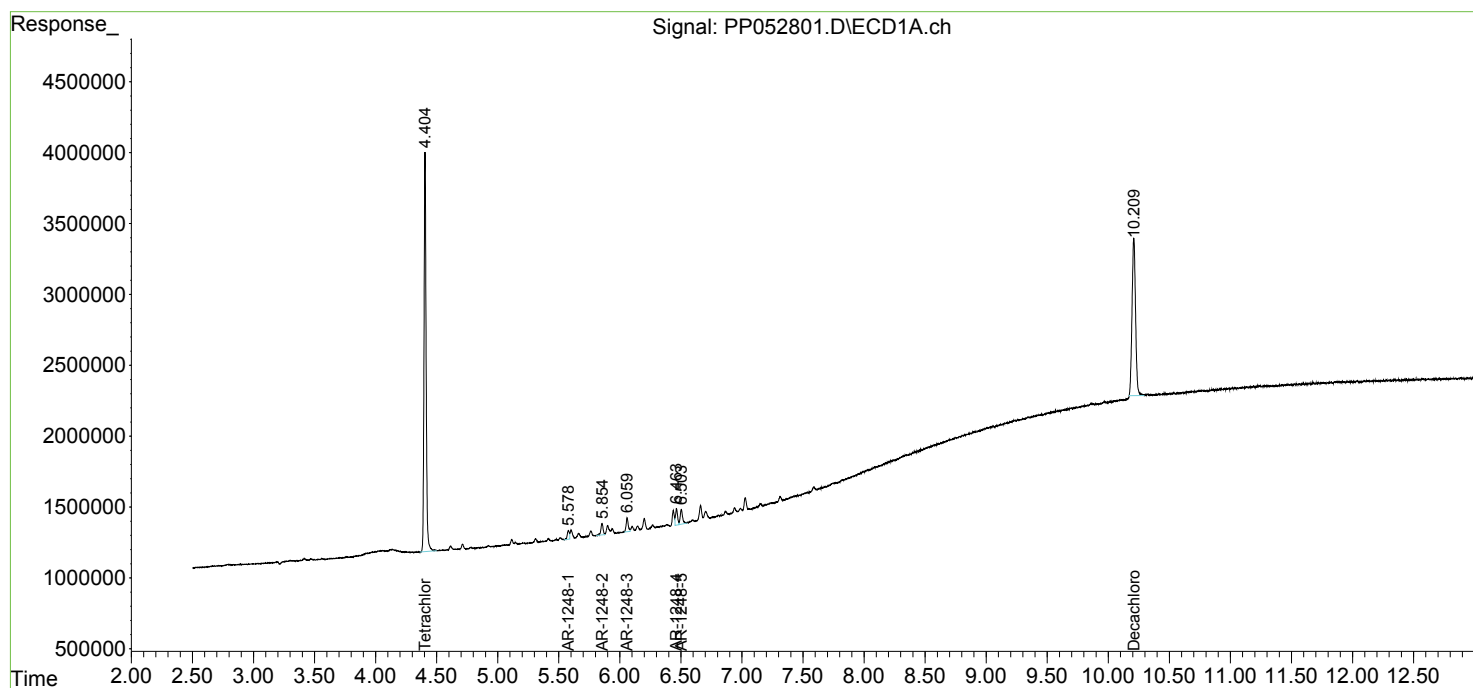


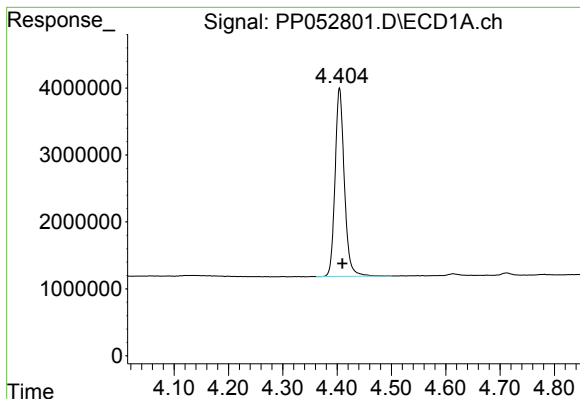

#1 Tetrachloro-m-xylene


R.T.: 4.405 min
Delta R.T.: -0.005 min
Response: 33478437
Conc: 15.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

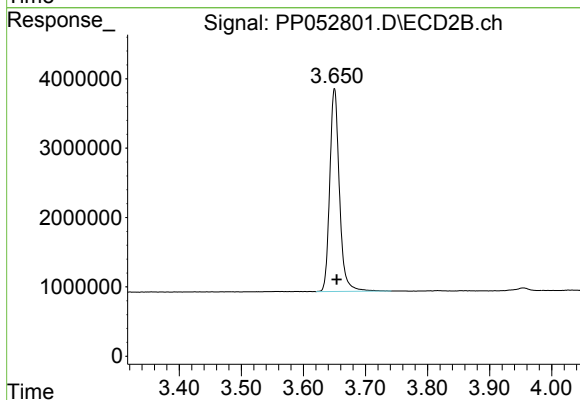


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.004 min
Response: 31668308
Conc: 16.85 ng/ml

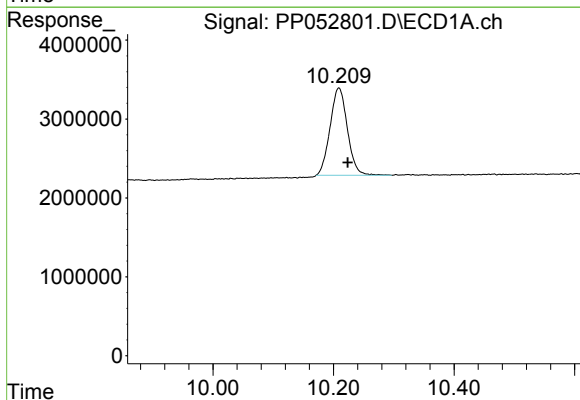


#2 Decachlorobiphenyl

R.T.: 10.209 min
Delta R.T.: -0.015 min
Response: 22157697
Conc: 17.46 ng/ml

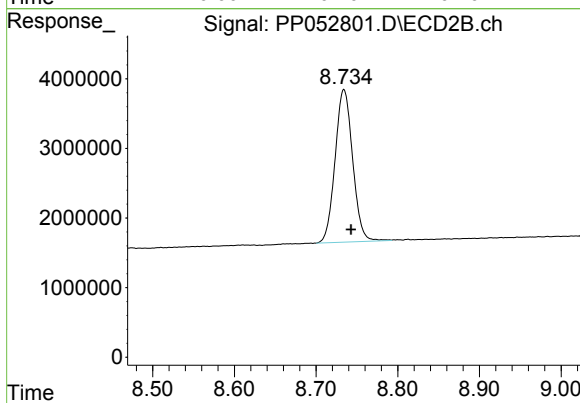

#2 Decachlorobiphenyl


R.T.: 8.734 min
Delta R.T.: -0.009 min
Response: 32811086
Conc: 19.56 ng/ml

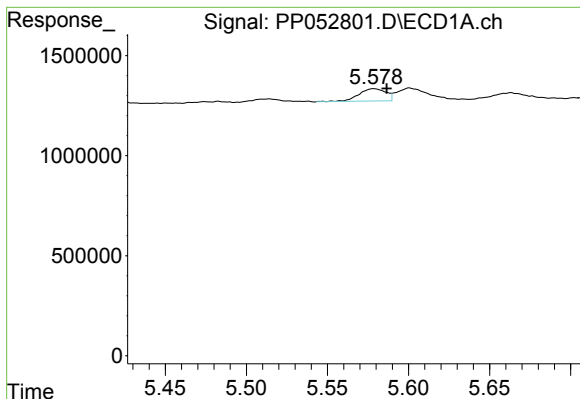

#21 AR-1248-1


R.T.: 5.579 min
Delta R.T.: -0.008 min
Response: 724339
Conc: 17.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

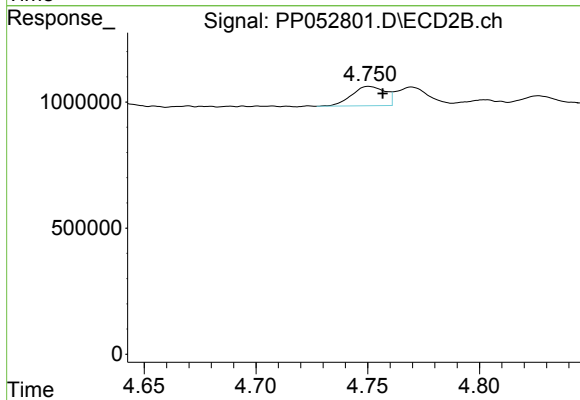


#21 AR-1248-1

R.T.: 4.750 min
Delta R.T.: -0.006 min
Response: 799197
Conc: 19.97 ng/ml

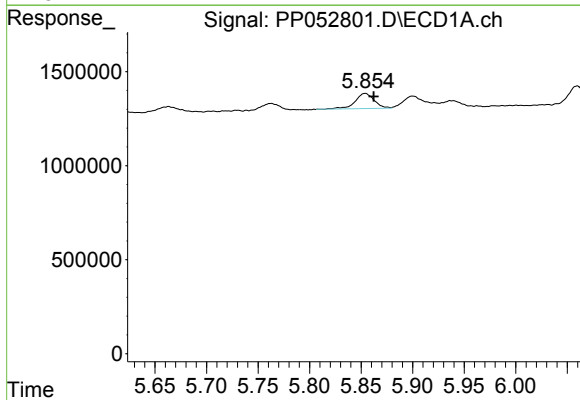


#22 AR-1248-2

R.T.: 5.854 min
Delta R.T.: -0.008 min
Response: 1043559
Conc: 17.53 ng/ml

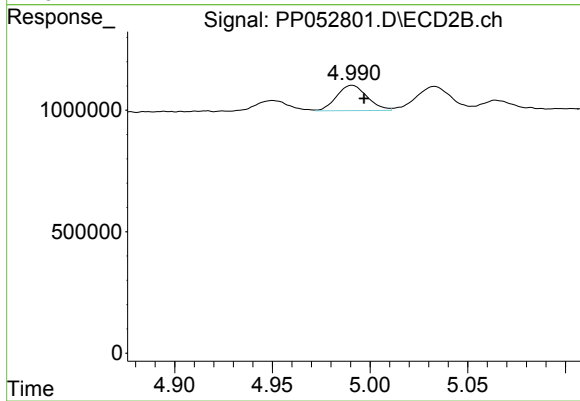

#22 AR-1248-2


R.T.: 4.991 min
Delta R.T.: -0.006 min
Response: 1130735
Conc: 19.97 ng/ml

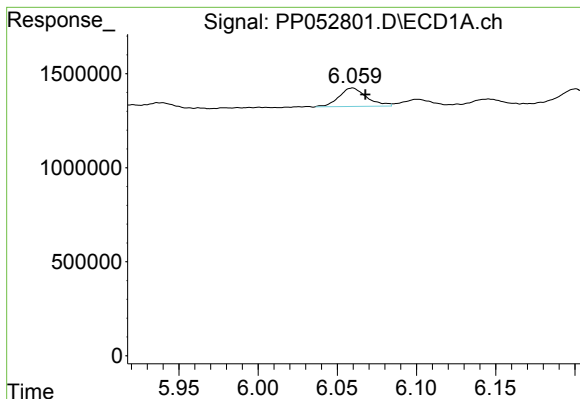

#23 AR-1248-3


R.T.: 6.060 min
Delta R.T.: -0.008 min
Response: 1191583
Conc: 18.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

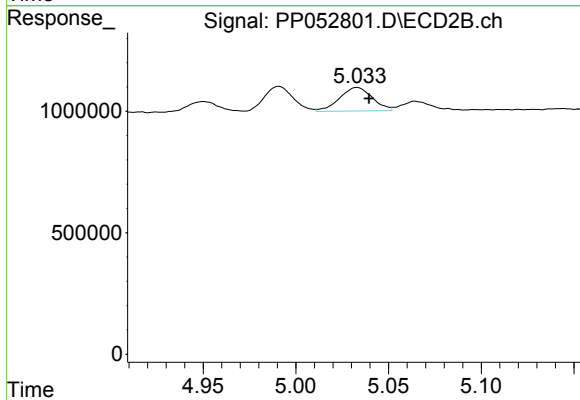


#23 AR-1248-3

R.T.: 5.033 min
Delta R.T.: -0.006 min
Response: 1191055
Conc: 20.29 ng/ml

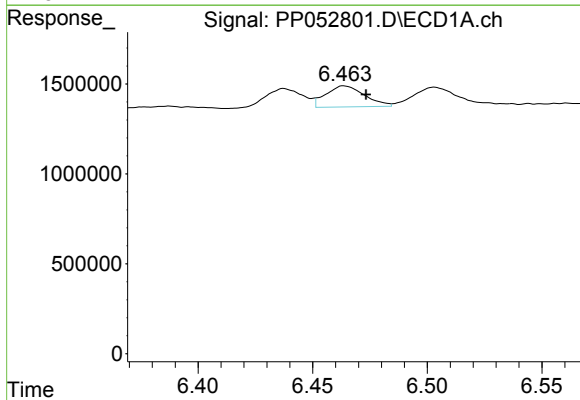


#24 AR-1248-4

R.T.: 6.464 min
Delta R.T.: -0.009 min
Response: 1374433
Conc: 21.34 ng/ml

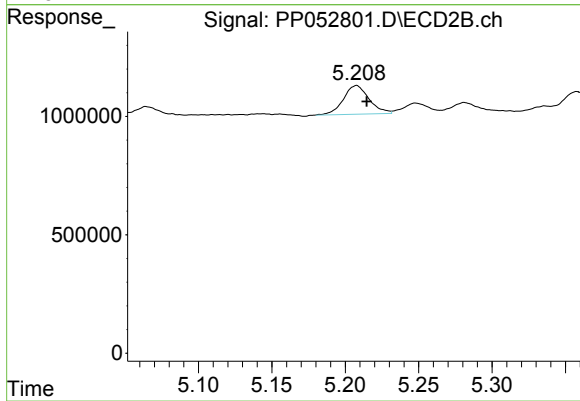

#24 AR-1248-4


R.T.: 5.208 min
Delta R.T.: -0.007 min
Response: 1479830
Conc: 21.25 ng/ml

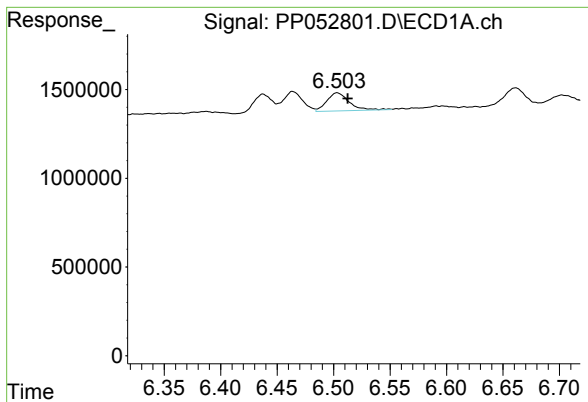

#25 AR-1248-5

R.T.: 6.503 min
Delta R.T.: -0.009 min
Response: 1416853
Conc: 22.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

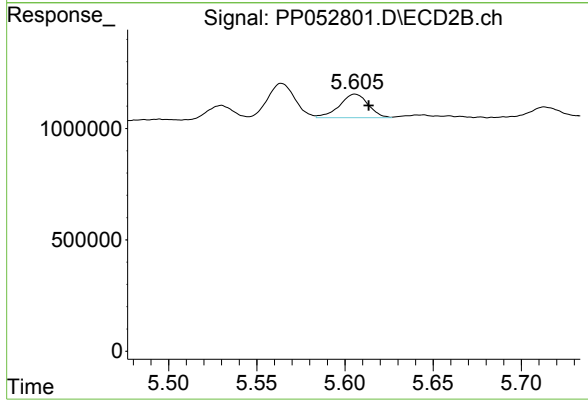

#25 AR-1248-5

R.T.: 5.606 min
Delta R.T.: -0.008 min
Response: 1206138
Conc: 19.01 ng/ml