

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
 Data File : PP052802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 11:01
 Operator : YP\AJ
 Sample : N4955-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:03:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.651	34385036	31971256	15.561	17.013
2) SA Decachlor...	10.210	8.735	22896582	33502937	18.039	19.976
Target Compounds						
26) L6 AR-1254-1	6.440	5.565	1593228	2004108	20.989	18.663
27) L6 AR-1254-2	6.659	5.714	2099016	1725979	18.780	18.057
28) L6 AR-1254-3	7.027	6.124	2460150	2610617	22.102	17.087
29) L6 AR-1254-4	7.314	6.355	1249462	1543255	17.743	16.997
30) L6 AR-1254-5	7.735	6.777	1270651	2182862	16.139	15.689



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
Data File : PP052802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 11:01
Operator : YP\AJ
Sample : N4955-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:03:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

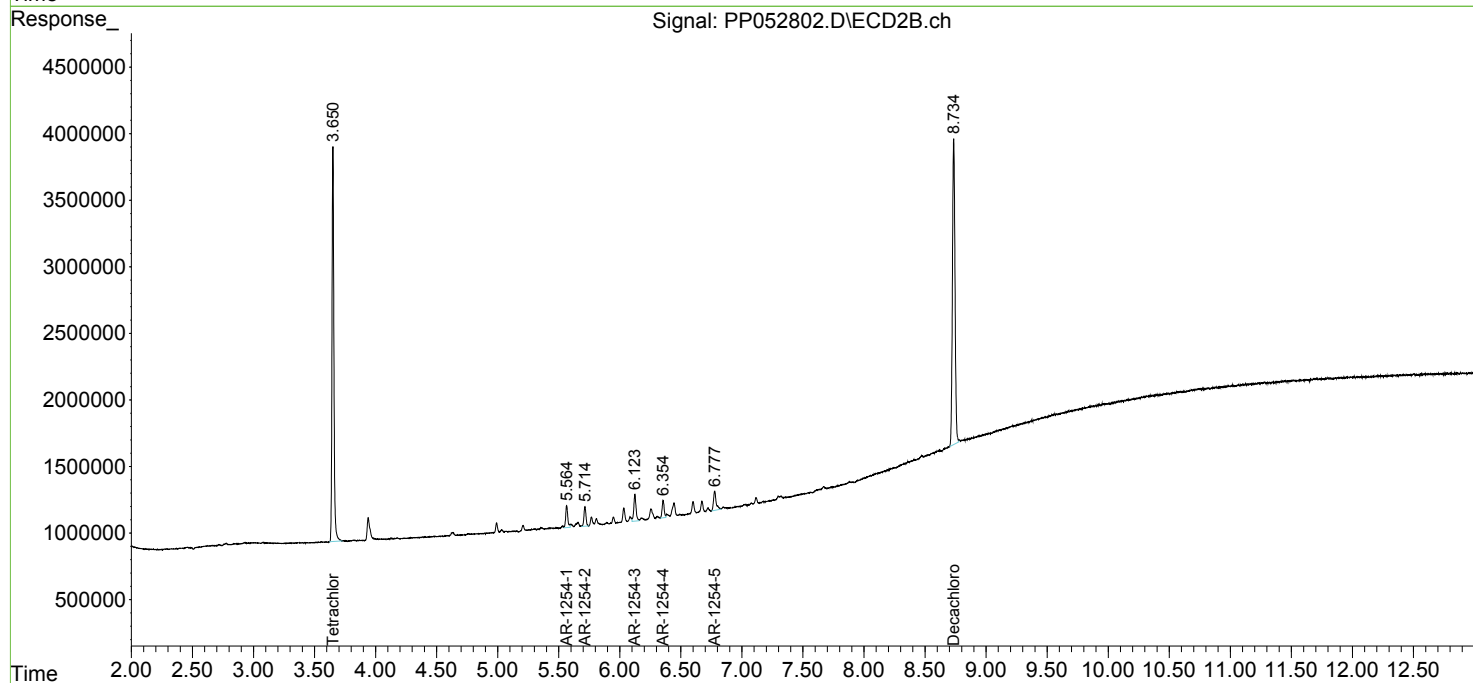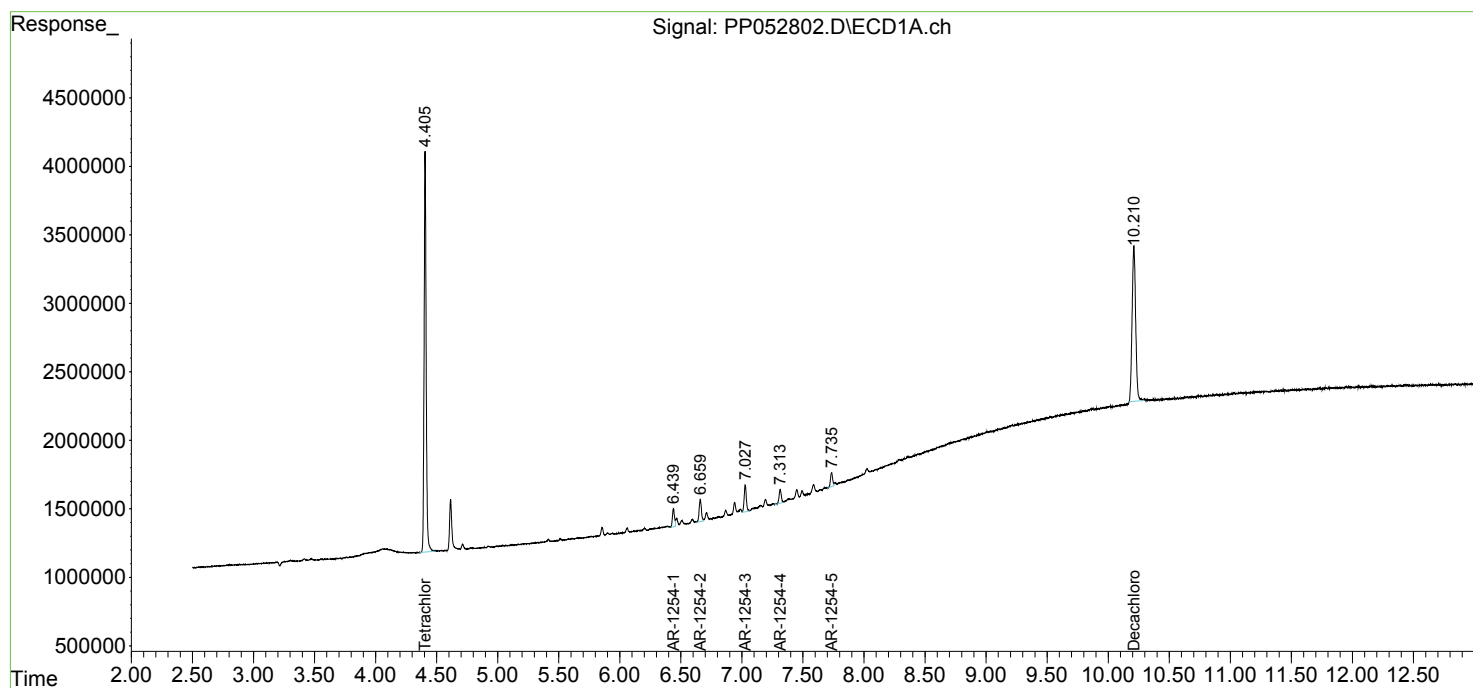


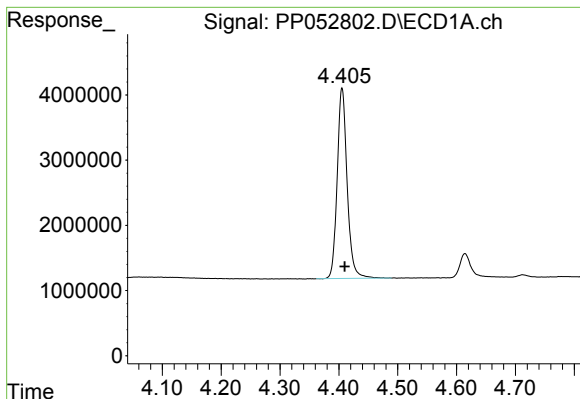

#1 Tetrachloro-m-xylene


R.T.: 4.405 min
Delta R.T.: -0.005 min
Response: 34385036
Conc: 15.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

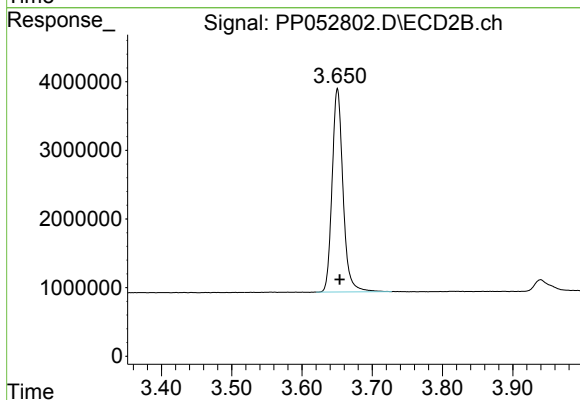


#1 Tetrachloro-m-xylene

R.T.: 3.651 min
Delta R.T.: -0.003 min
Response: 31971256
Conc: 17.01 ng/ml

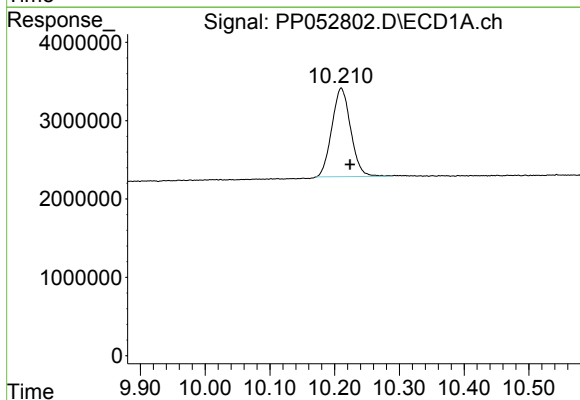


#2 Decachlorobiphenyl

R.T.: 10.210 min
Delta R.T.: -0.013 min
Response: 22896582
Conc: 18.04 ng/ml

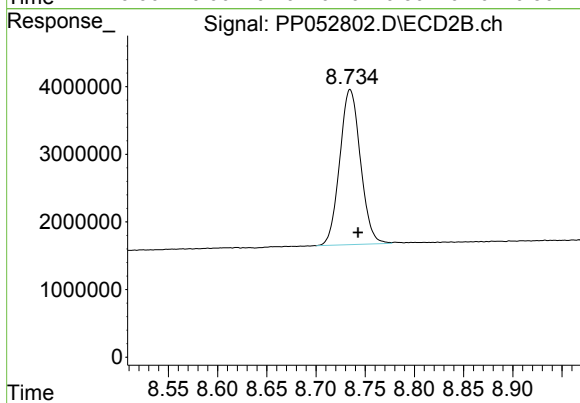

#2 Decachlorobiphenyl


R.T.: 8.735 min
Delta R.T.: -0.008 min
Response: 33502937
Conc: 19.98 ng/ml

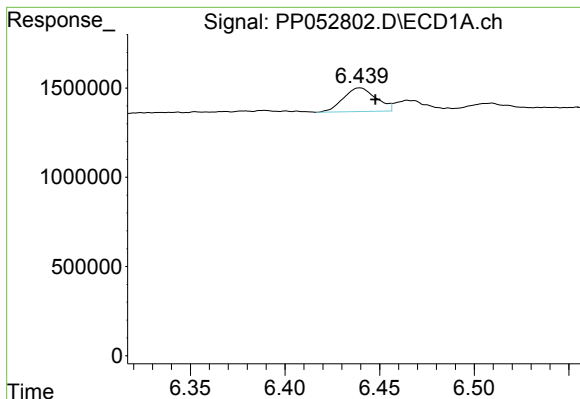

#26 AR-1254-1


R.T.: 6.440 min
Delta R.T.: -0.008 min
Response: 1593228
Conc: 20.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

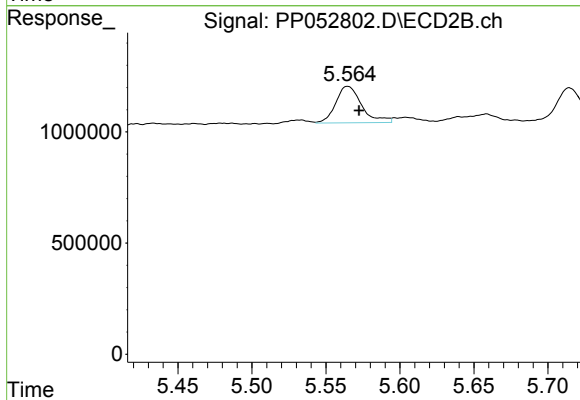


#26 AR-1254-1

R.T.: 5.565 min
Delta R.T.: -0.008 min
Response: 2004108
Conc: 18.66 ng/ml

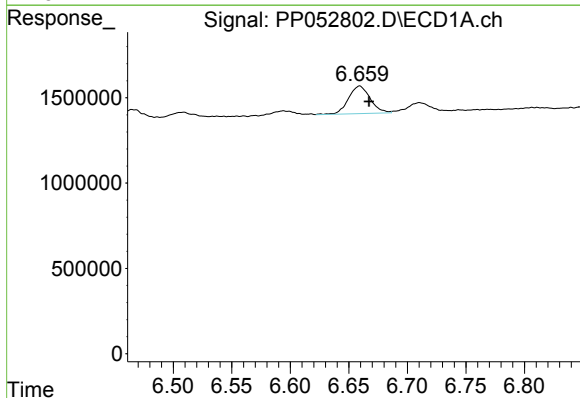


#27 AR-1254-2

R.T.: 6.659 min
Delta R.T.: -0.008 min
Response: 2099016
Conc: 18.78 ng/ml

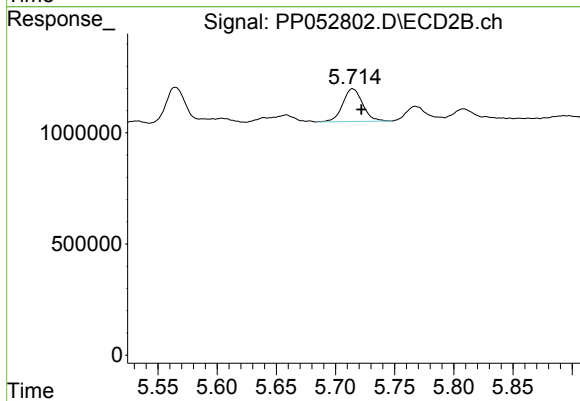

#27 AR-1254-2


R.T.: 5.714 min
Delta R.T.: -0.007 min
Response: 1725979
Conc: 18.06 ng/ml

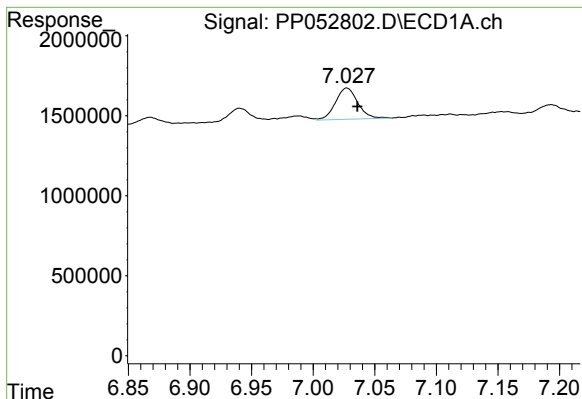

#28 AR-1254-3


R.T.: 7.027 min
Delta R.T.: -0.009 min
Response: 2460150
Conc: 22.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

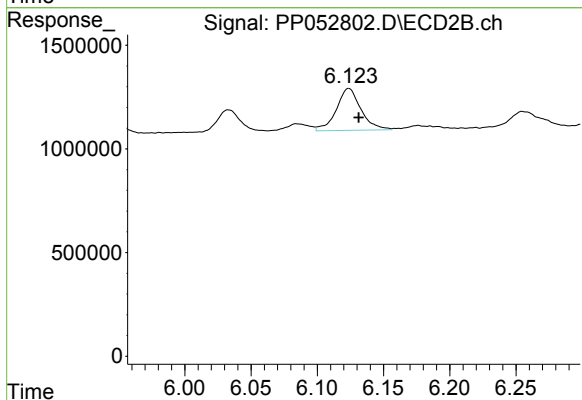


#28 AR-1254-3

R.T.: 6.124 min
Delta R.T.: -0.008 min
Response: 2610617
Conc: 17.09 ng/ml

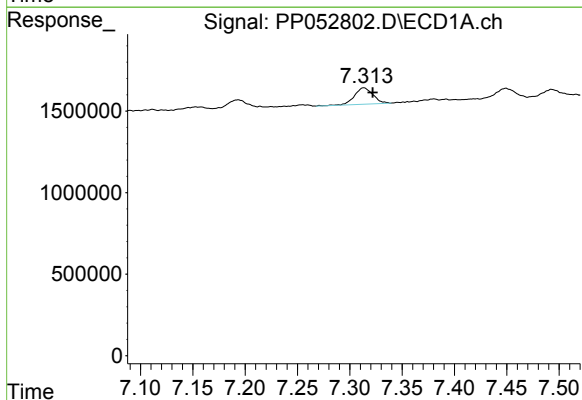


#29 AR-1254-4

R.T.: 7.314 min
Delta R.T.: -0.008 min
Response: 1249462
Conc: 17.74 ng/ml

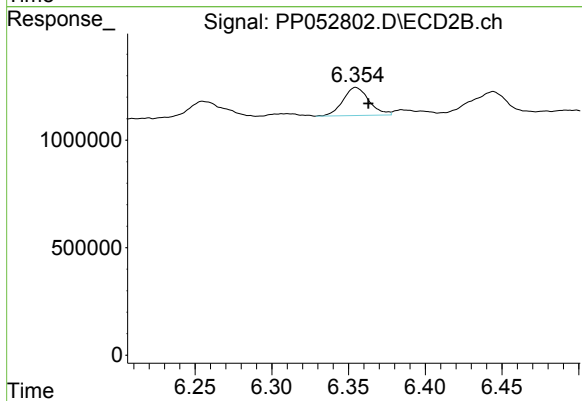

#29 AR-1254-4


R.T.: 6.355 min
Delta R.T.: -0.008 min
Response: 1543255
Conc: 17.00 ng/ml

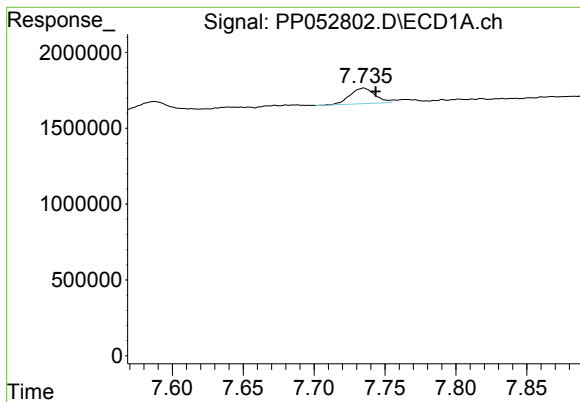

#30 AR-1254-5

R.T.: 7.735 min
Delta R.T.: -0.009 min
Response: 1270651
Conc: 16.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

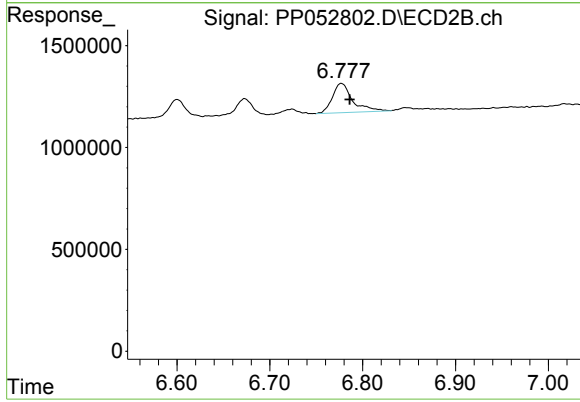

#30 AR-1254-5

R.T.: 6.777 min
Delta R.T.: -0.009 min
Response: 2182862
Conc: 15.69 ng/ml