

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
 Data File : PP052804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 11:34
 Operator : YP\AJ
 Sample : N4955-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:04:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.406	3.651	36316115	33750592	16.435	17.960
2) SA Decachlor...	10.210	8.735	26574397	34584624	20.936	20.621
Target Compounds						
41) L9 AR-1268-1	8.675	7.607	3399954	5384426	18.076	17.565
42) L9 AR-1268-2	8.771	7.672	3134942	4747729	19.154	17.505
43) L9 AR-1268-3	9.004	7.880	2841156	4358434	18.751	18.592
44) L9 AR-1268-4	9.439	8.172	1118027	1760188	21.984	20.722
45) L9 AR-1268-5	9.862	8.472	7560495	11093923	17.599	16.918



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
Data File : PP052804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 11:34
Operator : YP\AJ
Sample : N4955-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:04:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

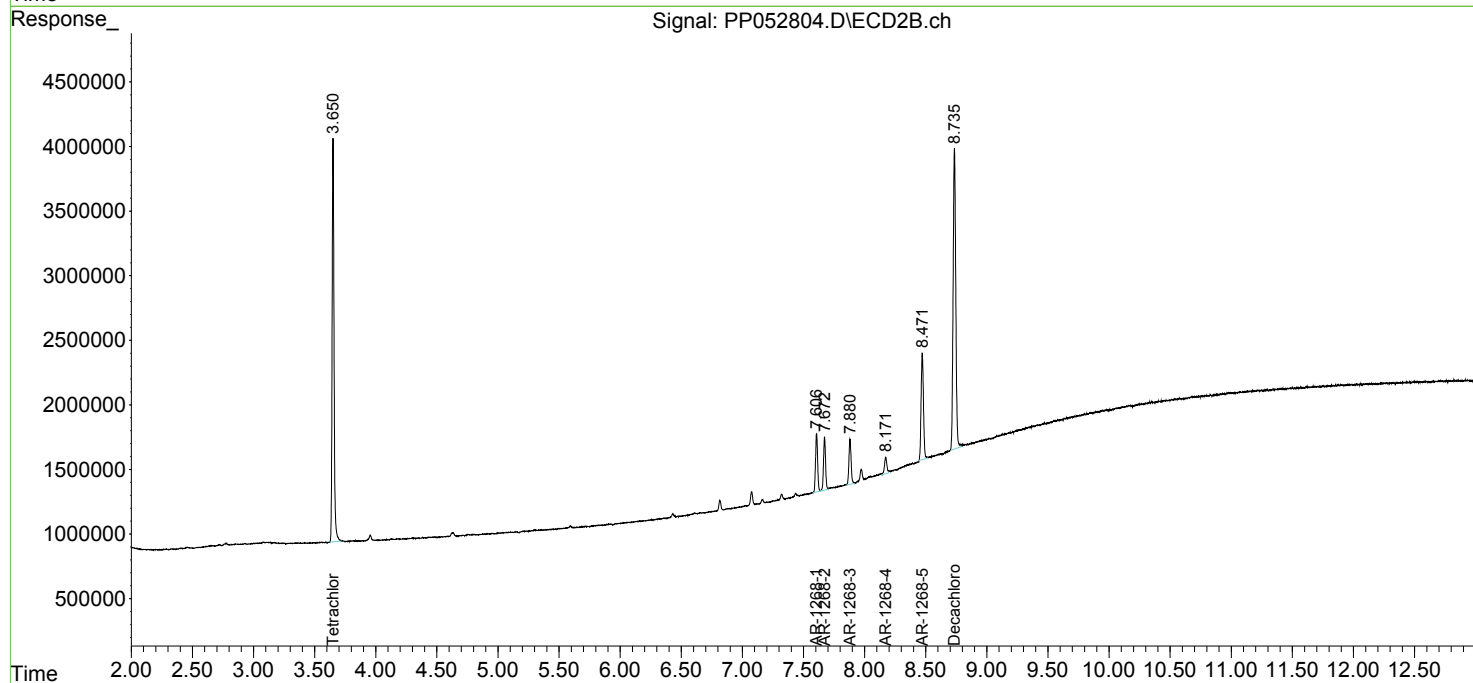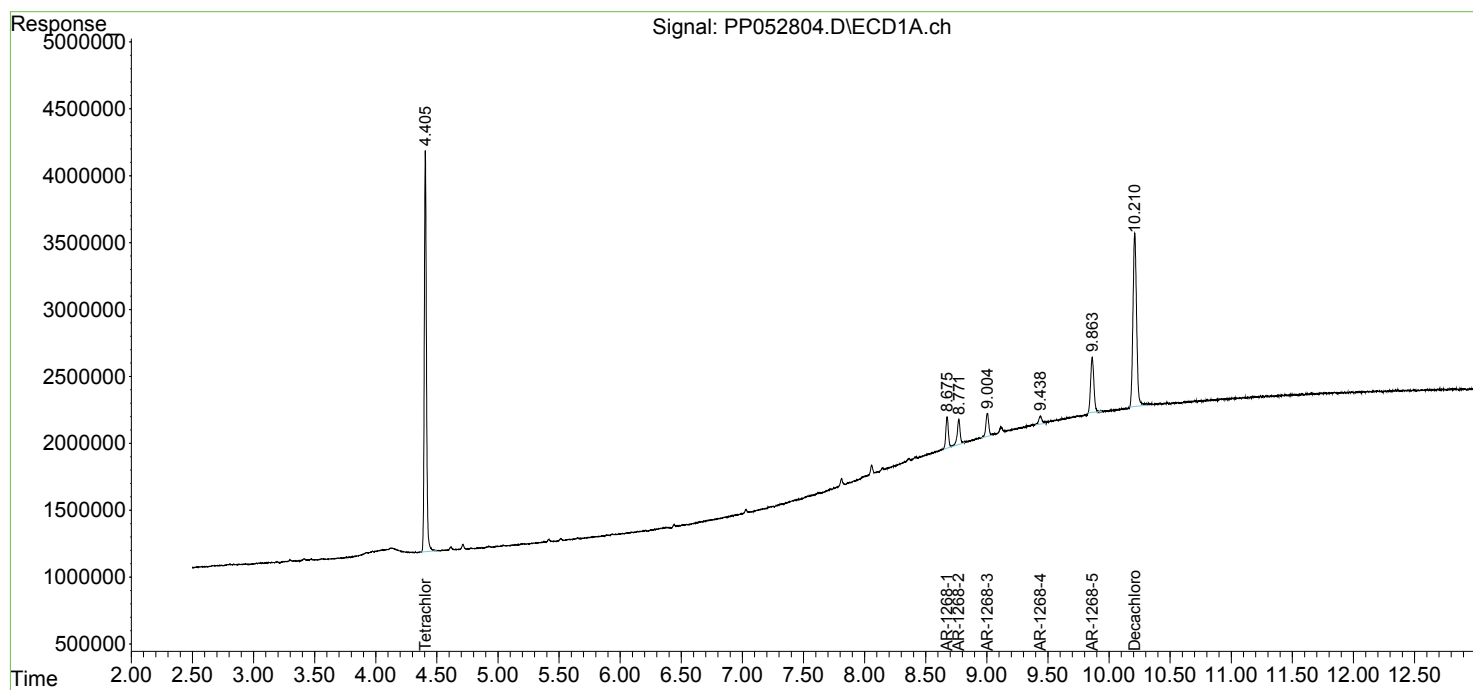


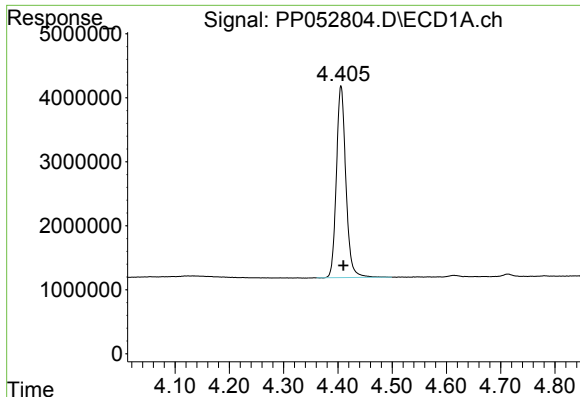

#1 Tetrachloro-m-xylene


R.T.: 4.406 min
Delta R.T.: -0.004 min
Response: 36316115
Conc: 16.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

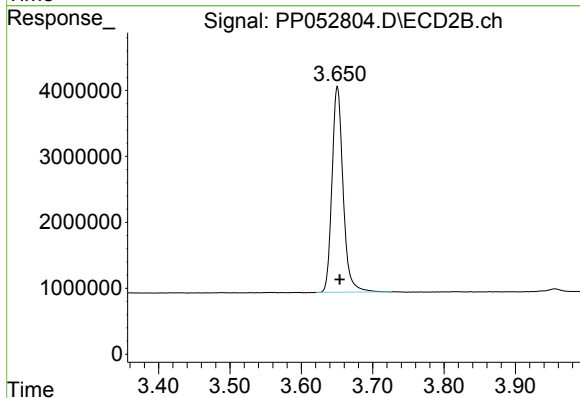


#1 Tetrachloro-m-xylene

R.T.: 3.651 min
Delta R.T.: -0.003 min
Response: 33750592
Conc: 17.96 ng/ml

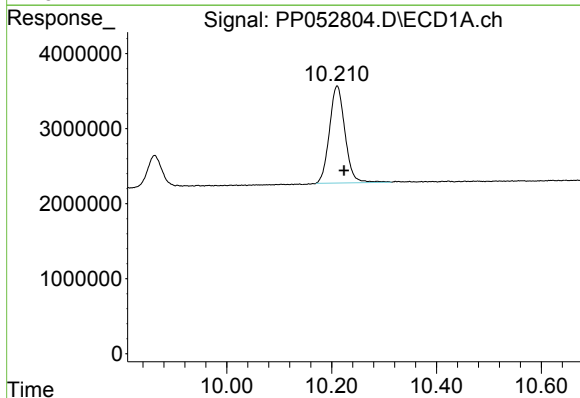


#2 Decachlorobiphenyl

R.T.: 10.210 min
Delta R.T.: -0.013 min
Response: 26574397
Conc: 20.94 ng/ml

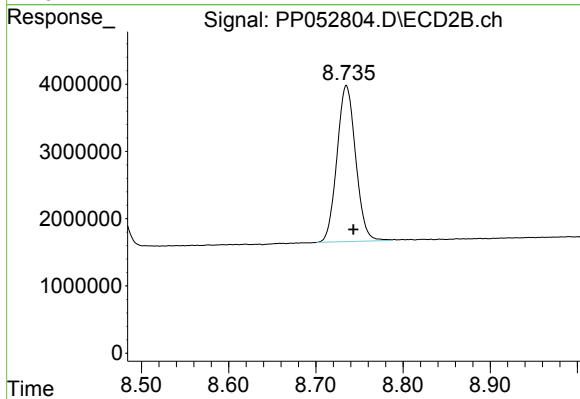

#2 Decachlorobiphenyl


R.T.: 8.735 min
Delta R.T.: -0.008 min
Response: 34584624
Conc: 20.62 ng/ml

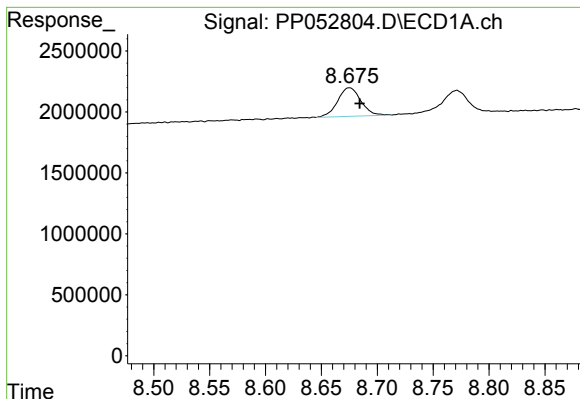

#41 AR-1268-1


R.T.: 8.675 min
Delta R.T.: -0.009 min
Response: 3399954
Conc: 18.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

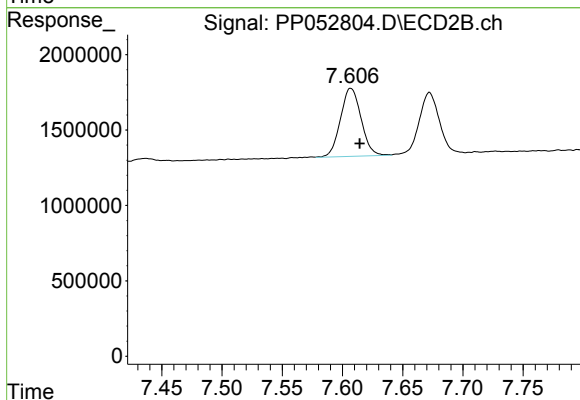


#41 AR-1268-1

R.T.: 7.607 min
Delta R.T.: -0.007 min
Response: 5384426
Conc: 17.57 ng/ml

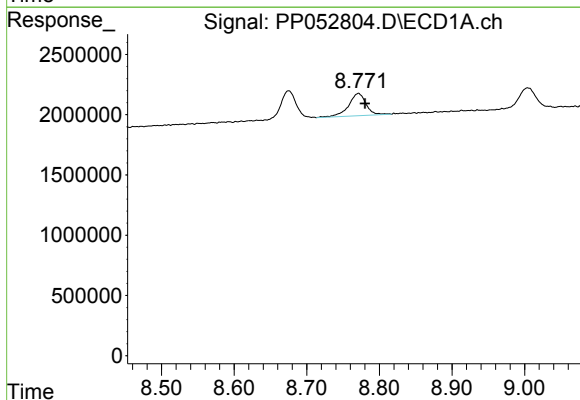


#42 AR-1268-2

R.T.: 8.771 min
Delta R.T.: -0.009 min
Response: 3134942
Conc: 19.15 ng/ml

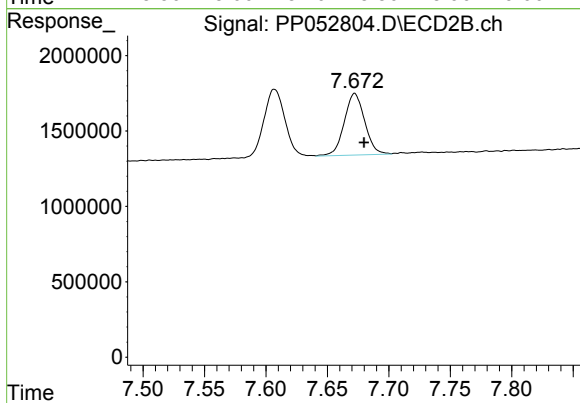

#42 AR-1268-2


R.T.: 7.672 min
Delta R.T.: -0.008 min
Response: 4747729
Conc: 17.50 ng/ml

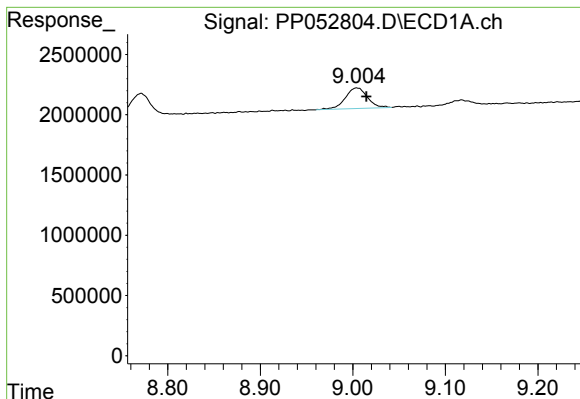

#43 AR-1268-3


R.T.: 9.004 min
Delta R.T.: -0.011 min
Response: 2841156
Conc: 18.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

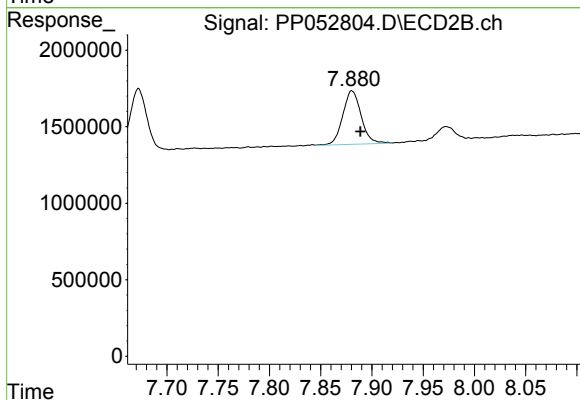


#43 AR-1268-3

R.T.: 7.880 min
Delta R.T.: -0.008 min
Response: 4358434
Conc: 18.59 ng/ml

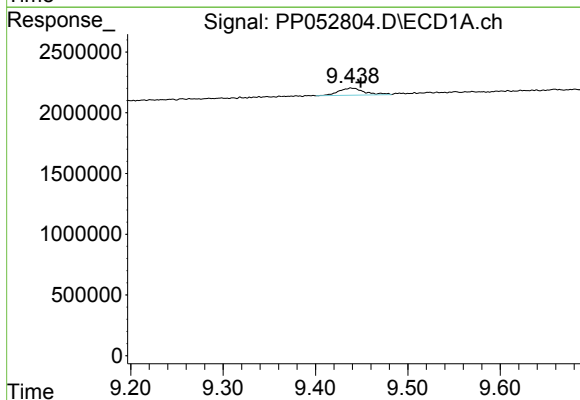


#44 AR-1268-4

R.T.: 9.439 min
Delta R.T.: -0.010 min
Response: 1118027
Conc: 21.98 ng/ml

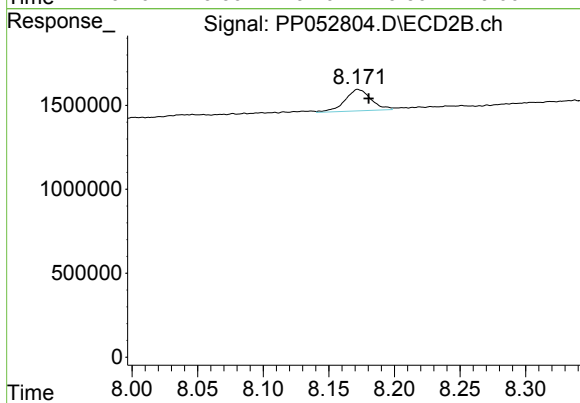

#44 AR-1268-4


R.T.: 8.172 min
Delta R.T.: -0.008 min
Response: 1760188
Conc: 20.72 ng/ml

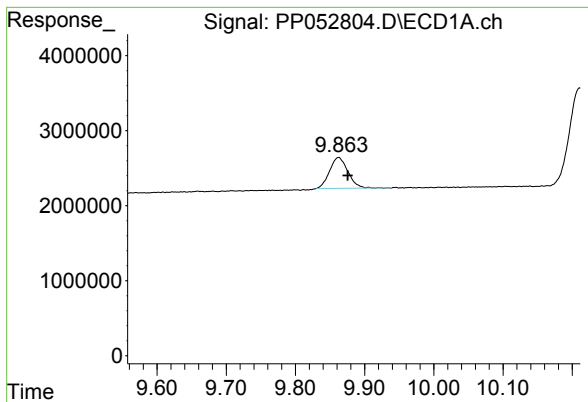

#45 AR-1268-5

R.T.: 9.862 min
Delta R.T.: -0.014 min
Response: 7560495
Conc: 17.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2022

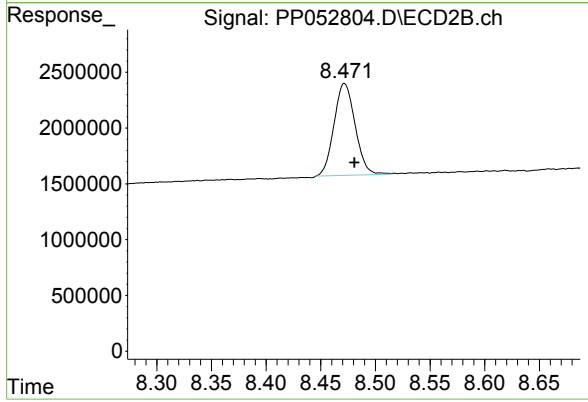

#45 AR-1268-5

R.T.: 8.472 min
Delta R.T.: -0.009 min
Response: 11093923
Conc: 16.92 ng/ml