

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
 Data File : PP052828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 18:10
 Operator : YP\AJ
 Sample : N5339-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NB-07-102722

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/31/2022
 Supervised By :Ankita Jodhani 10/31/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 09:16:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.406	3.651	40091710	36059798	18.144	19.189m
2) SA Decachlor...	10.212	8.735	24346076	28108009	19.181	16.760

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
Data File : PP052828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 18:10
Operator : YP\AJ
Sample : N5339-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NB-07-102722


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/31/2022
Supervised By :Ankita Jodhani 10/31/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 09:16:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

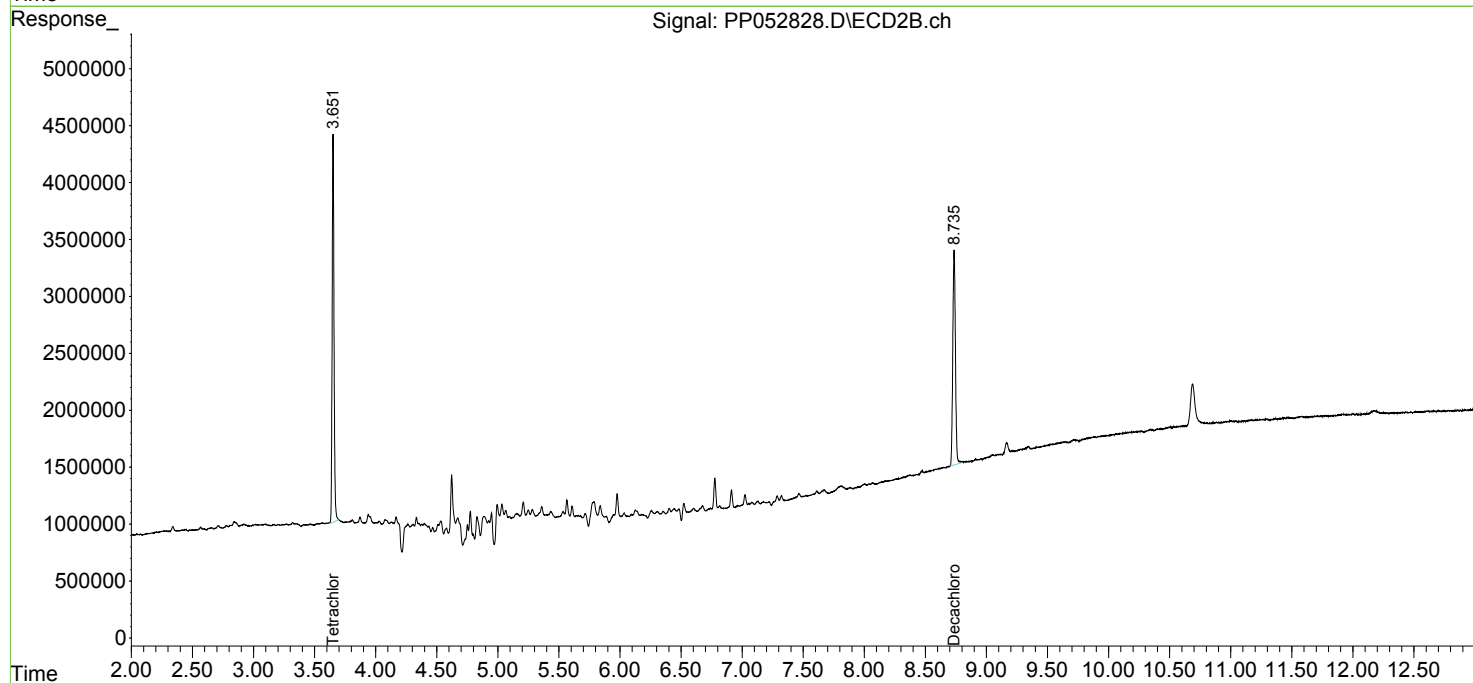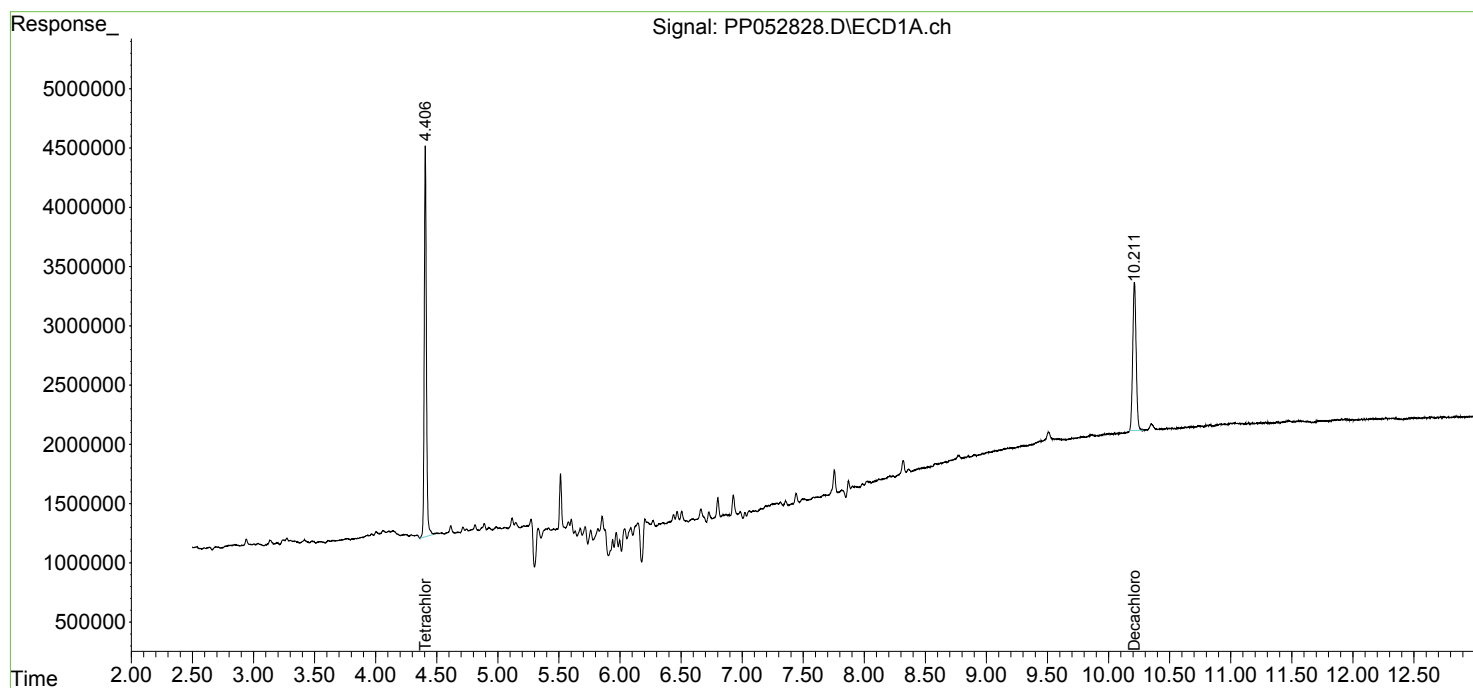

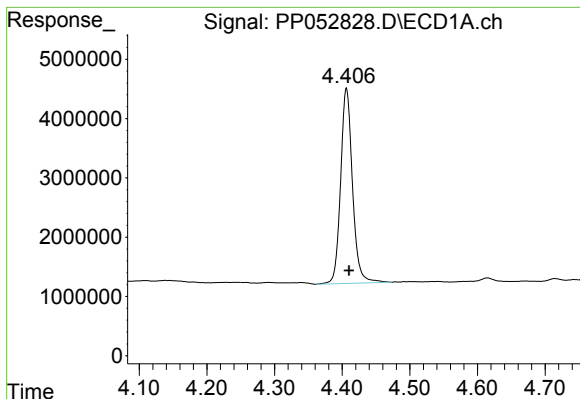

#1 Tetrachloro-m-xylene

R.T.: 4.406 min
Delta R.T.: -0.004 min
Response: 40091710
Conc: 18.14 ng/ml

Instrument :

ECD_P


ClientSampleId :

NB-07-102722

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/31/2022
Supervised By :Ankita Jodhani 10/31/2022

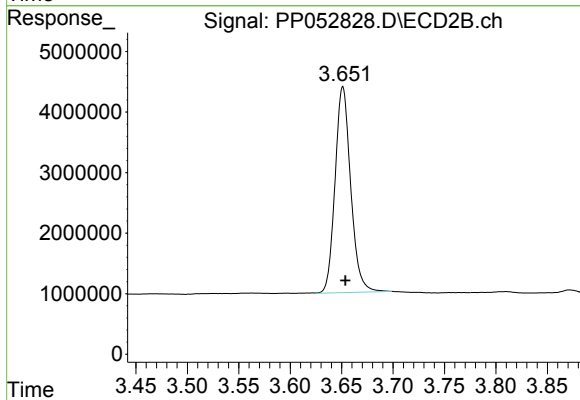


#1 Tetrachloro-m-xylene

R.T.: 3.651 min
Delta R.T.: -0.003 min
Response: 36059798
Conc: 19.19 ng/ml m

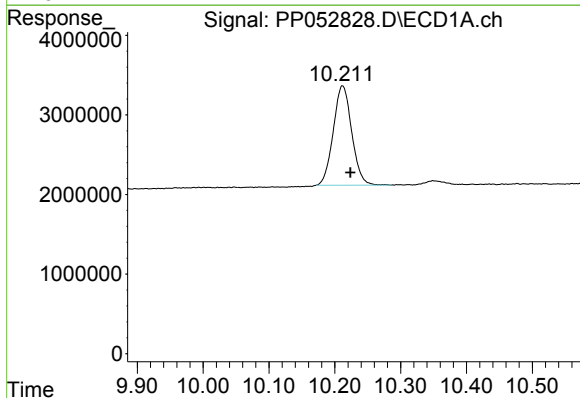

#2 Decachlorobiphenyl

R.T.: 10.212 min
Delta R.T.: -0.012 min
Response: 24346076
Conc: 19.18 ng/ml

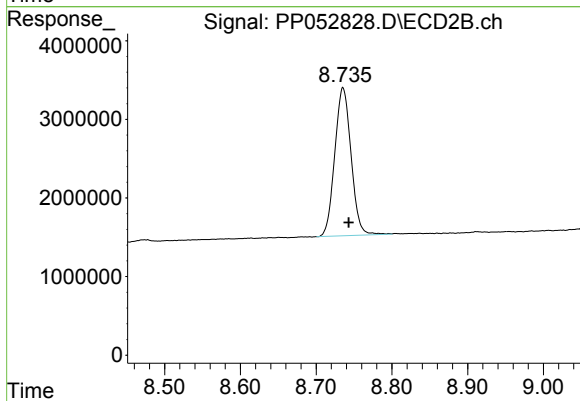

#2 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.007 min
Response: 28108009
Conc: 16.76 ng/ml