

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
Data File : PP052854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2022 02:40
Operator : YP\AJ
Sample : N5266-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20221100-204.1-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 09:33:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.406	3.651	33499204	31558366	15.160	16.793
2) SA Decachlor...	10.208	8.733	19248372	25196631	15.164	15.024

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
Data File : PP052854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2022 02:40
Operator : YP\AJ
Sample : N5266-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20221100-204.1-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 09:33:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

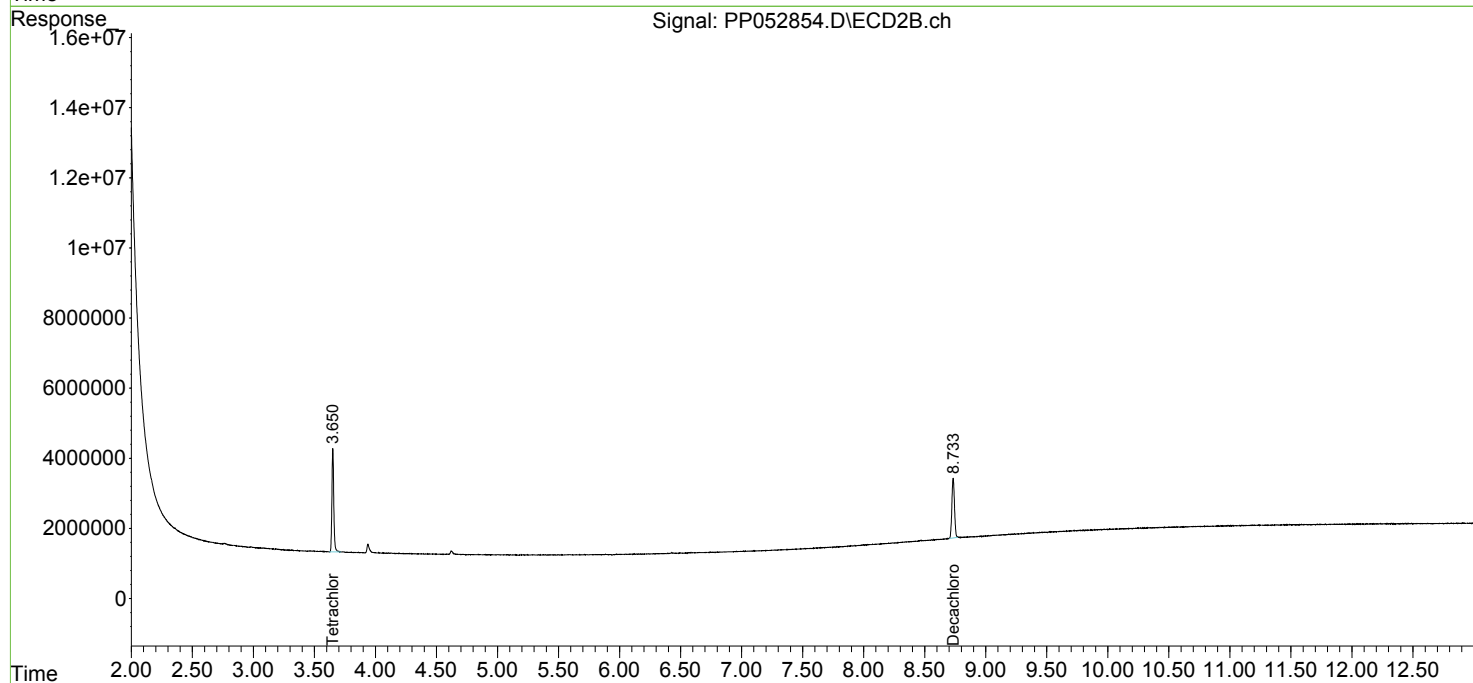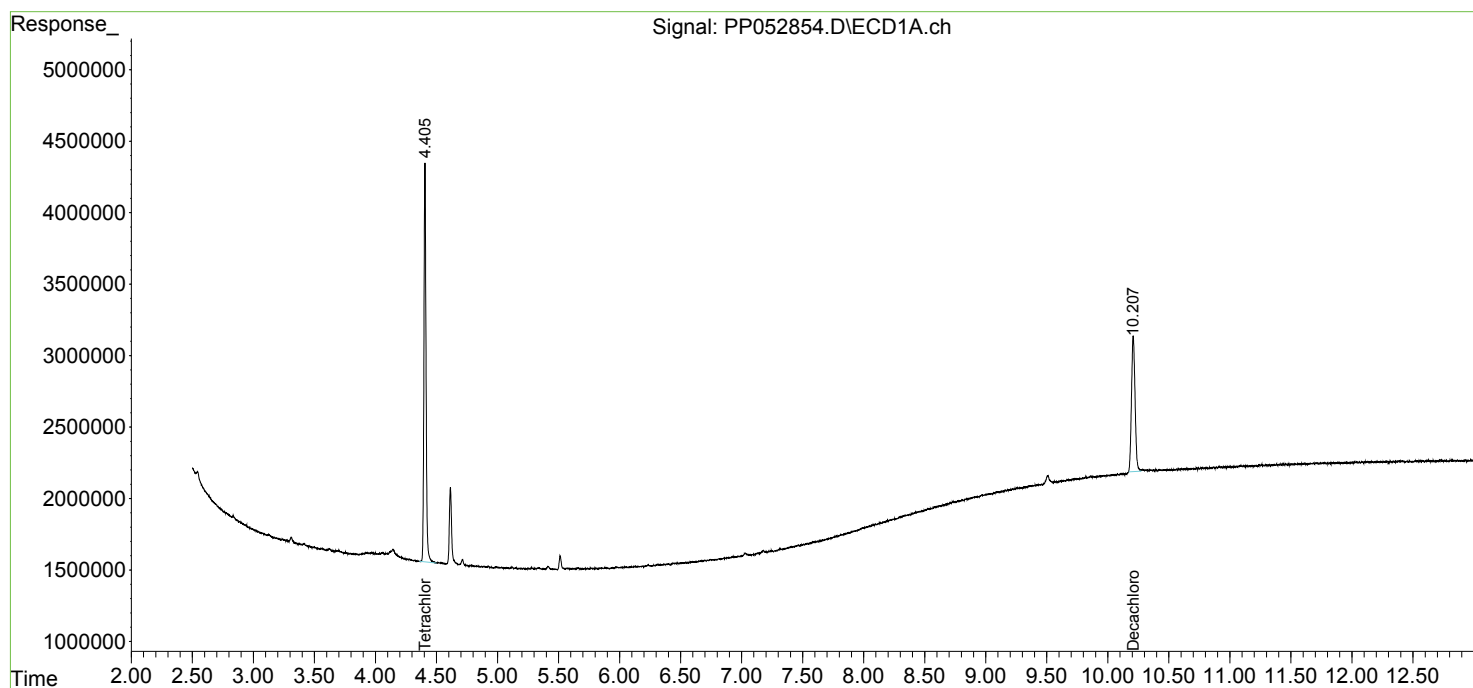


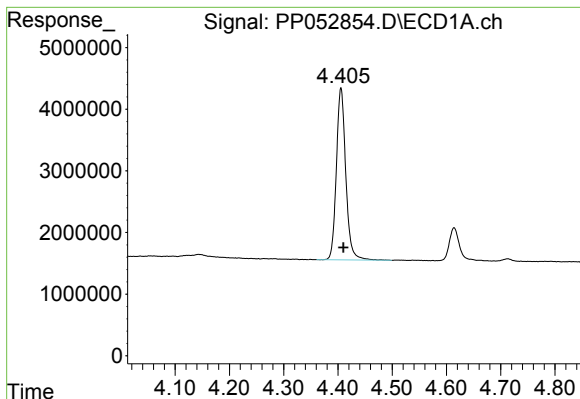

#1 Tetrachloro-m-xylene


R.T.: 4.406 min
Delta R.T.: -0.004 min
Response: 33499204
Conc: 15.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
20221100-204.1-SITE-WATER

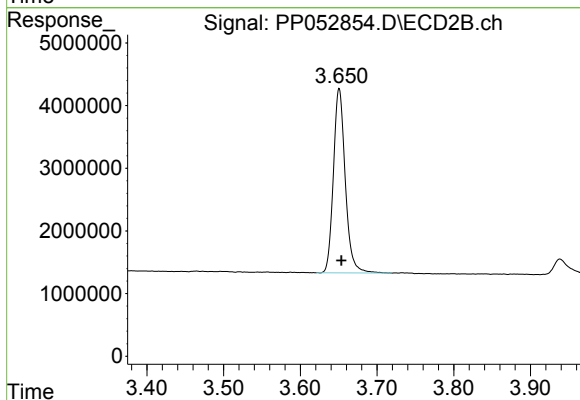


#1 Tetrachloro-m-xylene

R.T.: 3.651 min
Delta R.T.: -0.003 min
Response: 31558366
Conc: 16.79 ng/ml

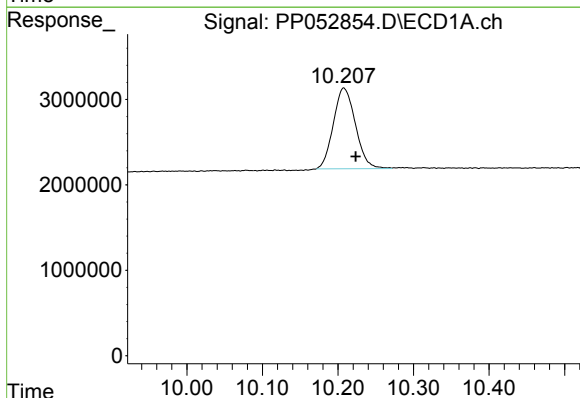

#2 Decachlorobiphenyl

R.T.: 10.208 min
Delta R.T.: -0.016 min
Response: 19248372
Conc: 15.16 ng/ml

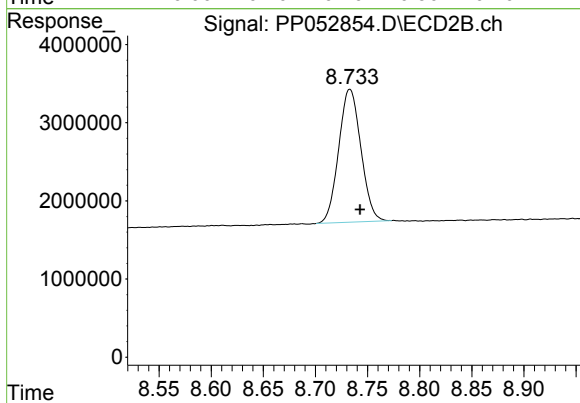

#2 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.010 min
Response: 25196631
Conc: 15.02 ng/ml