

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
 Data File : PP052866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2022 05:57
 Operator : YP\AJ
 Sample : N5316-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMPOSITE-NE-QUARTER

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/31/2022
 Supervised By :Ankita Jodhani 10/31/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 09:42:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 27 04:46:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.650	37226295	35251424	16.847	18.758
2) SA Decachlor...	10.208	8.732	20319008	26013968	16.008	15.511

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102822\
Data File : PP052866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2022 05:57
Operator : YP\AJ
Sample : N5316-01
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMPOSITE-NE-QUARTER


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/31/2022
Supervised By :Ankita Jodhani 10/31/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 09:42:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102622.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 27 04:46:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

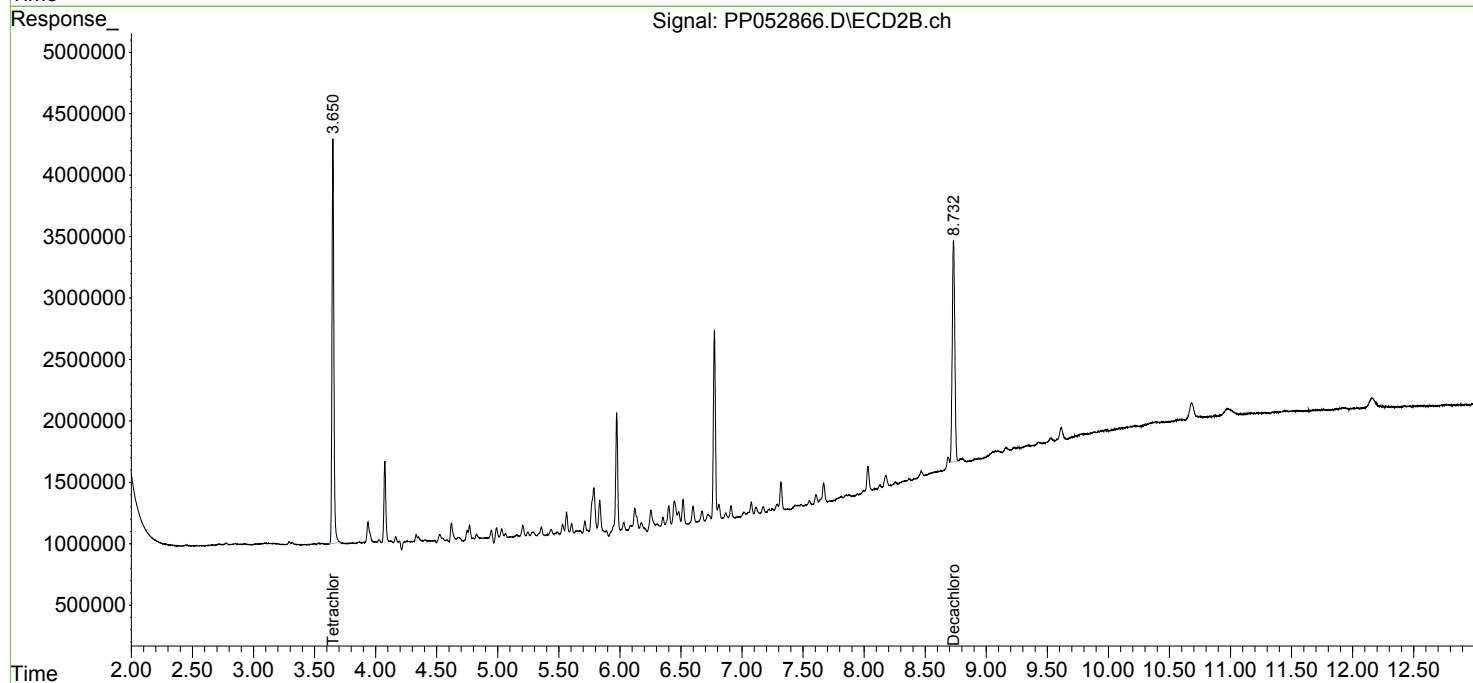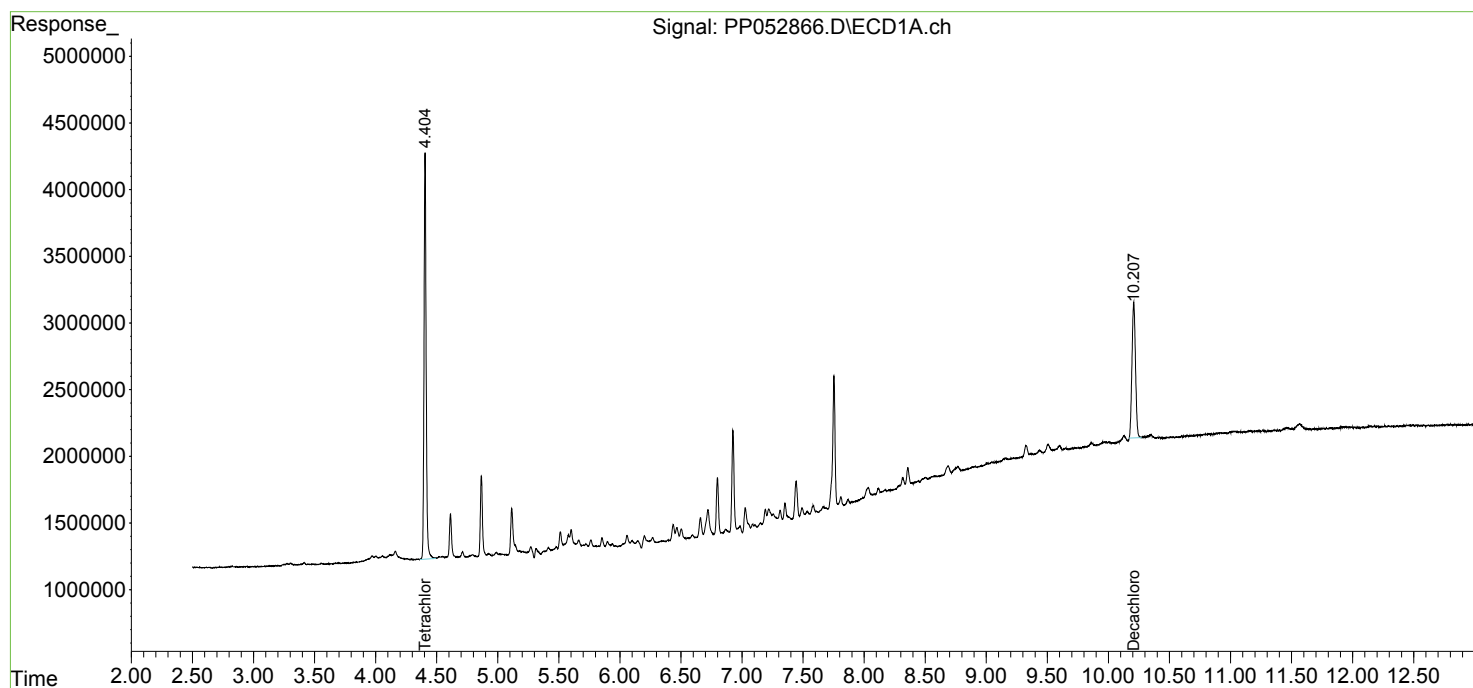

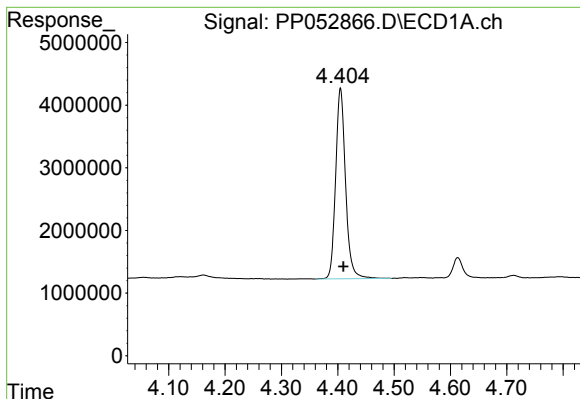


#1 Tetrachloro-m-xylene

R.T.: 4.405 min
Delta R.T.: -0.005 min
Response: 37226295
Conc: 16.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMPOSITE-NE-QUARTER


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/31/2022
Supervised By :Ankita Jodhani 10/31/2022

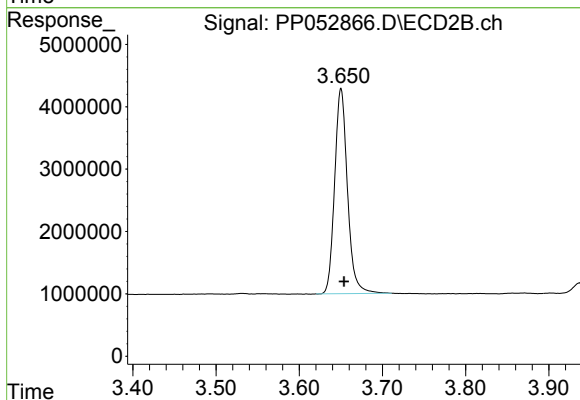


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.003 min
Response: 35251424
Conc: 18.76 ng/ml

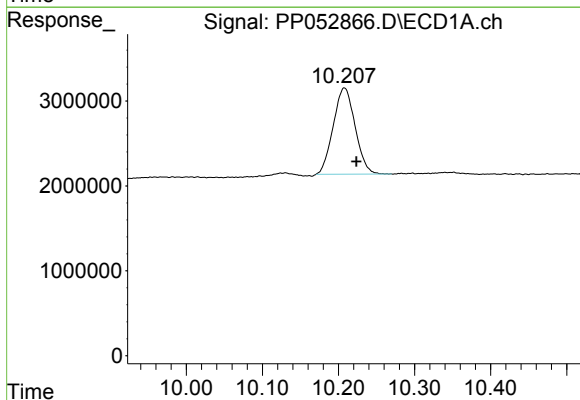

#2 Decachlorobiphenyl

R.T.: 10.208 min
Delta R.T.: -0.016 min
Response: 20319008
Conc: 16.01 ng/ml

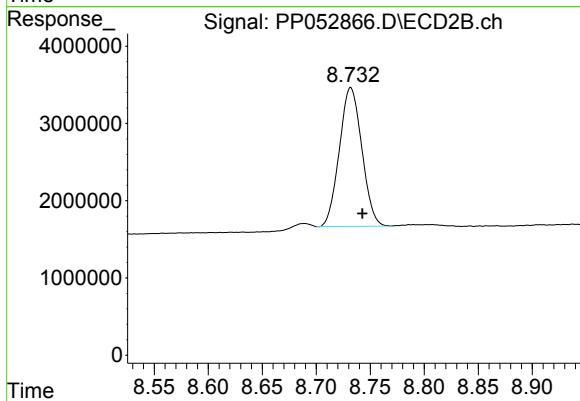

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.011 min
Response: 26013968
Conc: 15.51 ng/ml