

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102824\  
 Data File : PP068271.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 28 Oct 2024 15:57  
 Operator : YP\AJ  
 Sample : P4563-11  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 FITTING-1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 29 03:07:47 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP100824.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Oct 09 05:48:32 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

|                    |        |       |          |          |        |        |
|--------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlo... | 4.754  | 4.048 | 19312536 | 19598832 | 20.864 | 19.397 |
| 2) SA Decachlor... | 10.663 | 9.202 | 25569137 | 23646406 | 22.209 | 21.085 |

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102824\  
Data File : PP068271.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 Oct 2024 15:57  
Operator : YP\AJ  
Sample : P4563-11  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
FITTING-1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 29 03:07:47 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP100824.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Oct 09 05:48:32 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

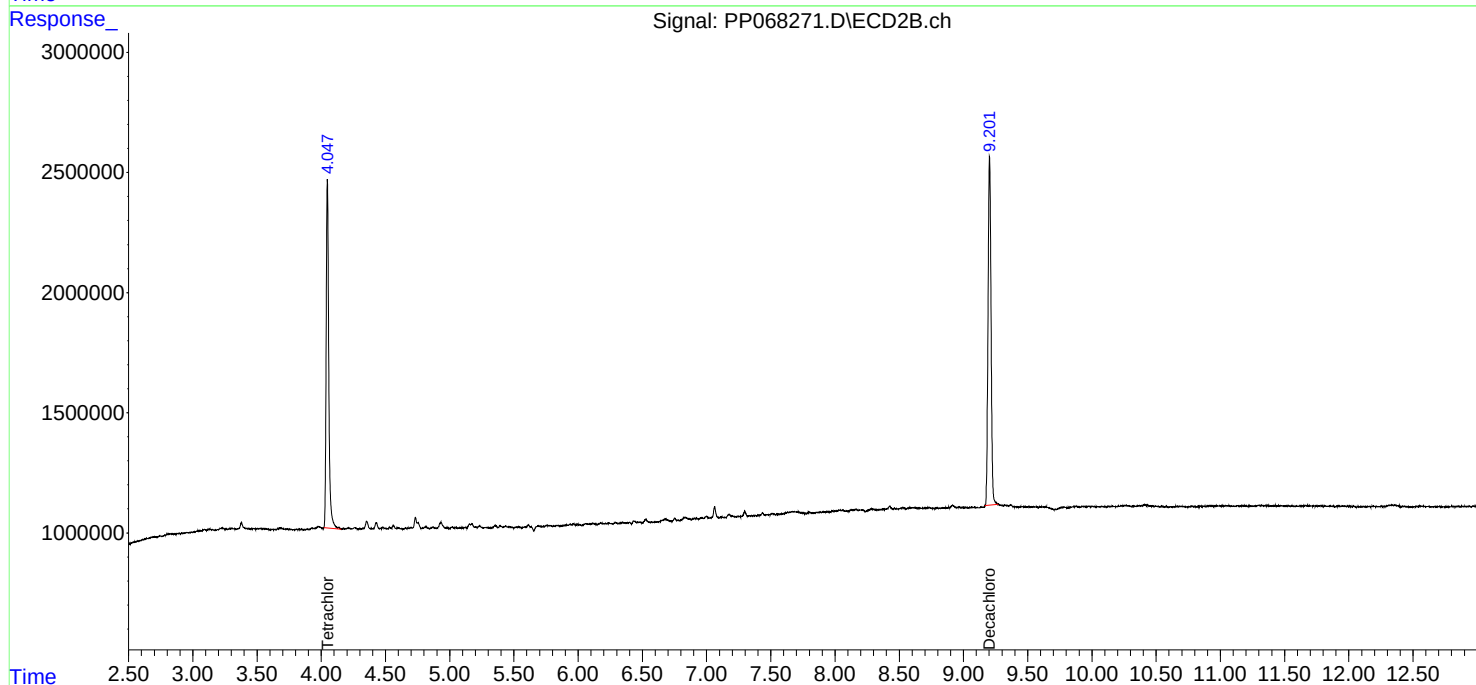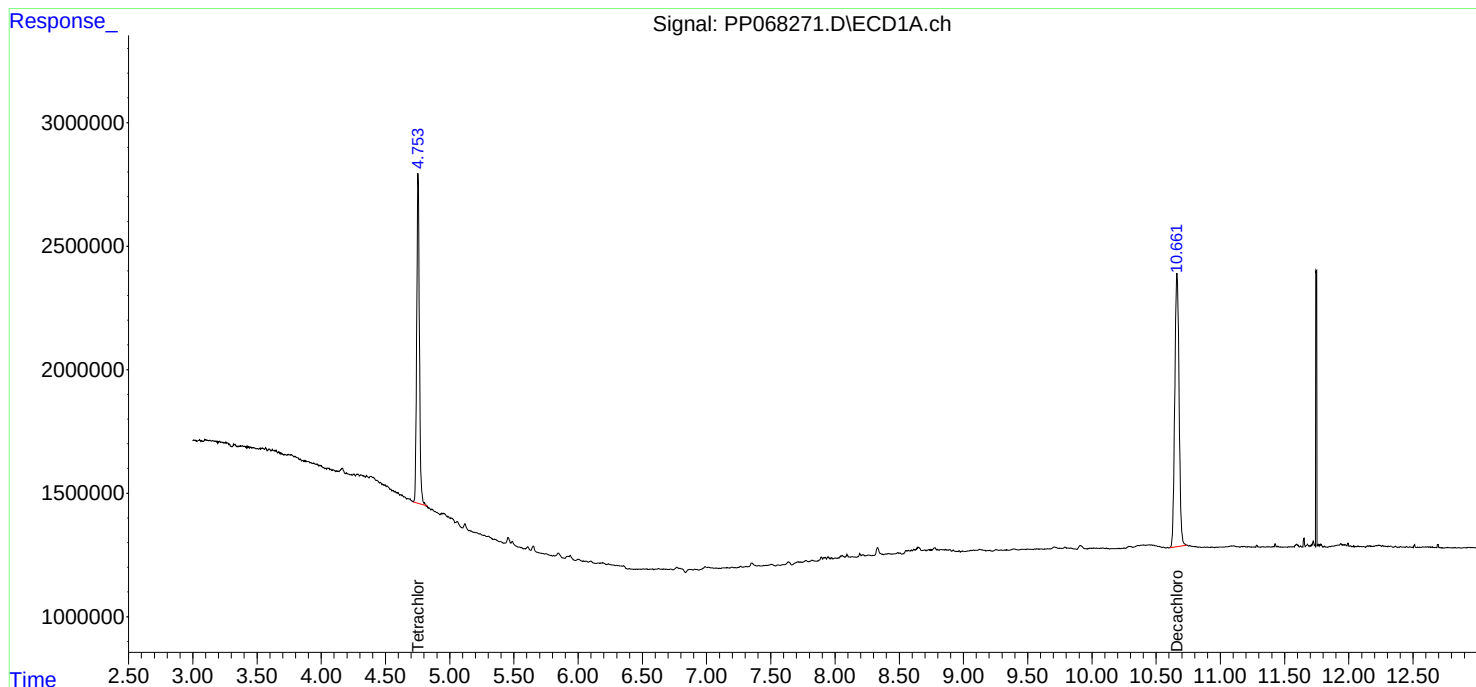


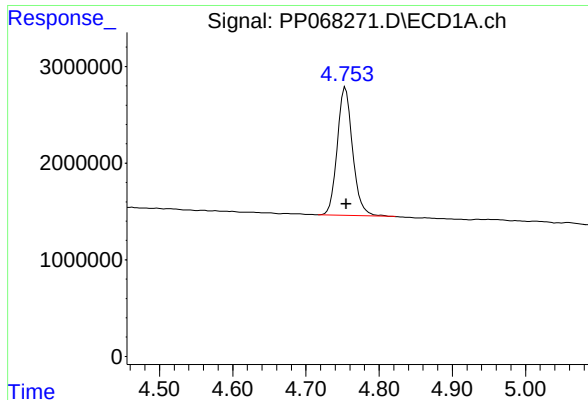

#1 Tetrachloro-m-xylene


R.T.: 4.754 min  
Delta R.T.: 0.000 min  
Response: 19312536  
Conc: 20.86 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
FITTING-1

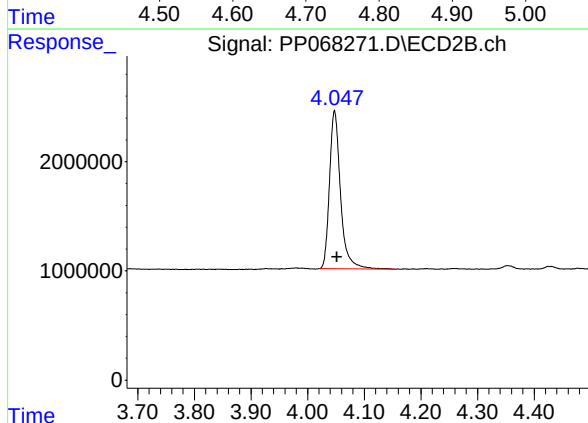


#1 Tetrachloro-m-xylene

R.T.: 4.048 min  
Delta R.T.: -0.004 min  
Response: 19598832  
Conc: 19.40 ng/ml

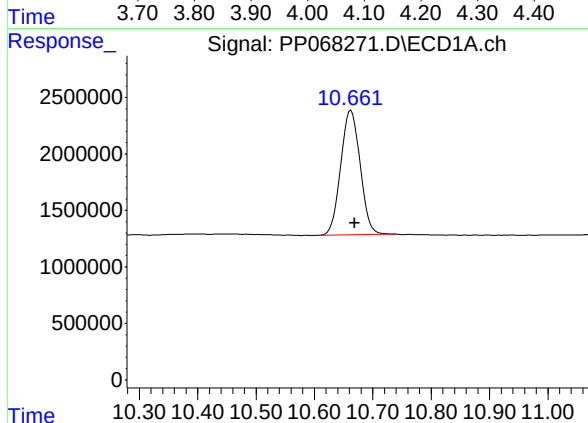

#2 Decachlorobiphenyl

R.T.: 10.663 min  
Delta R.T.: -0.006 min  
Response: 25569137  
Conc: 22.21 ng/ml

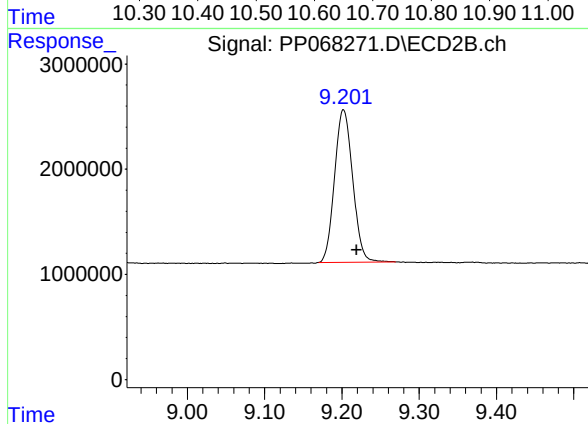

#2 Decachlorobiphenyl

R.T.: 9.202 min  
Delta R.T.: -0.017 min  
Response: 23646406  
Conc: 21.09 ng/ml