

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102825\
 Data File : PP076121.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 12:26
 Operator : YP\AJ
 Sample : Q3472-10 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/29/2025
 Supervised By :Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 14:05:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.639	3.786	2900493	3219677	2.030	0.486m#
2) SA Decachlor...	10.404	8.778	2122336	10617426	1.971m	1.291 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102825\
Data File : PP076121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 12:26
Operator : YP\AJ
Sample : Q3472-10 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 14:05:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

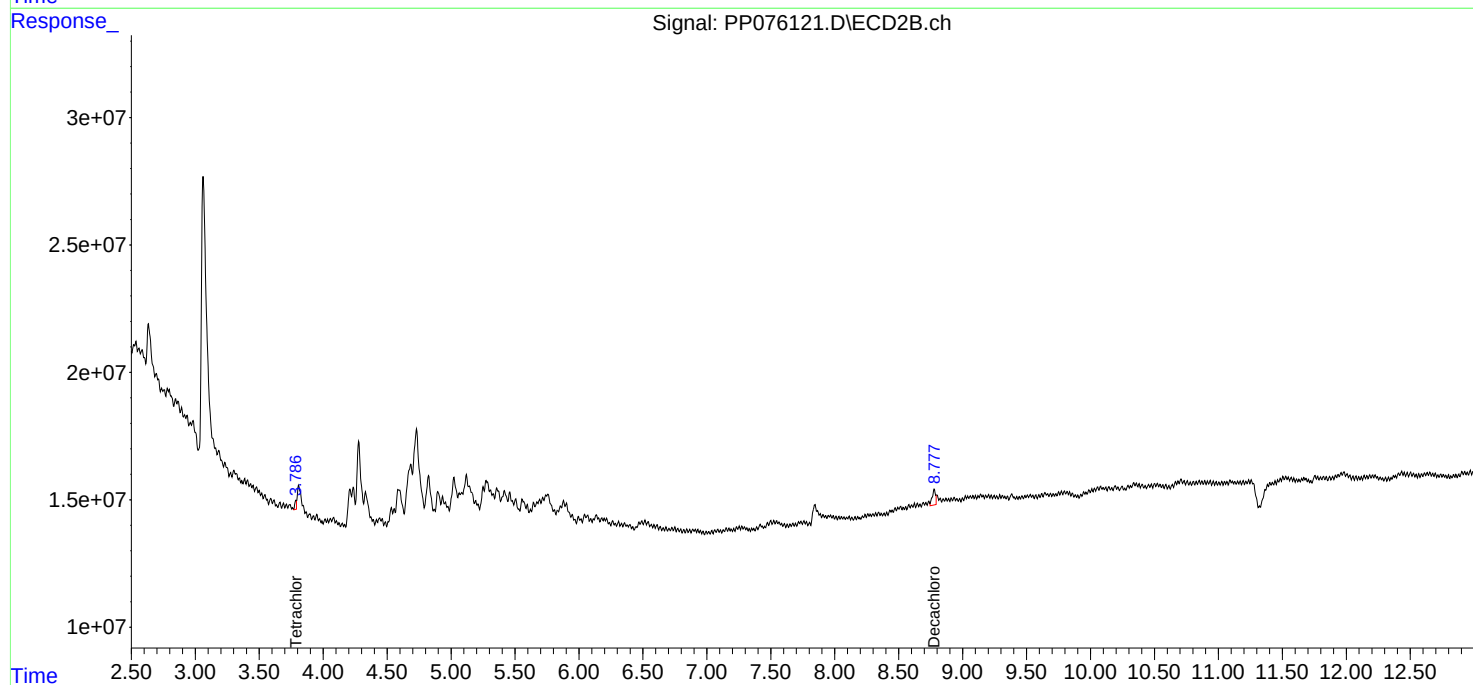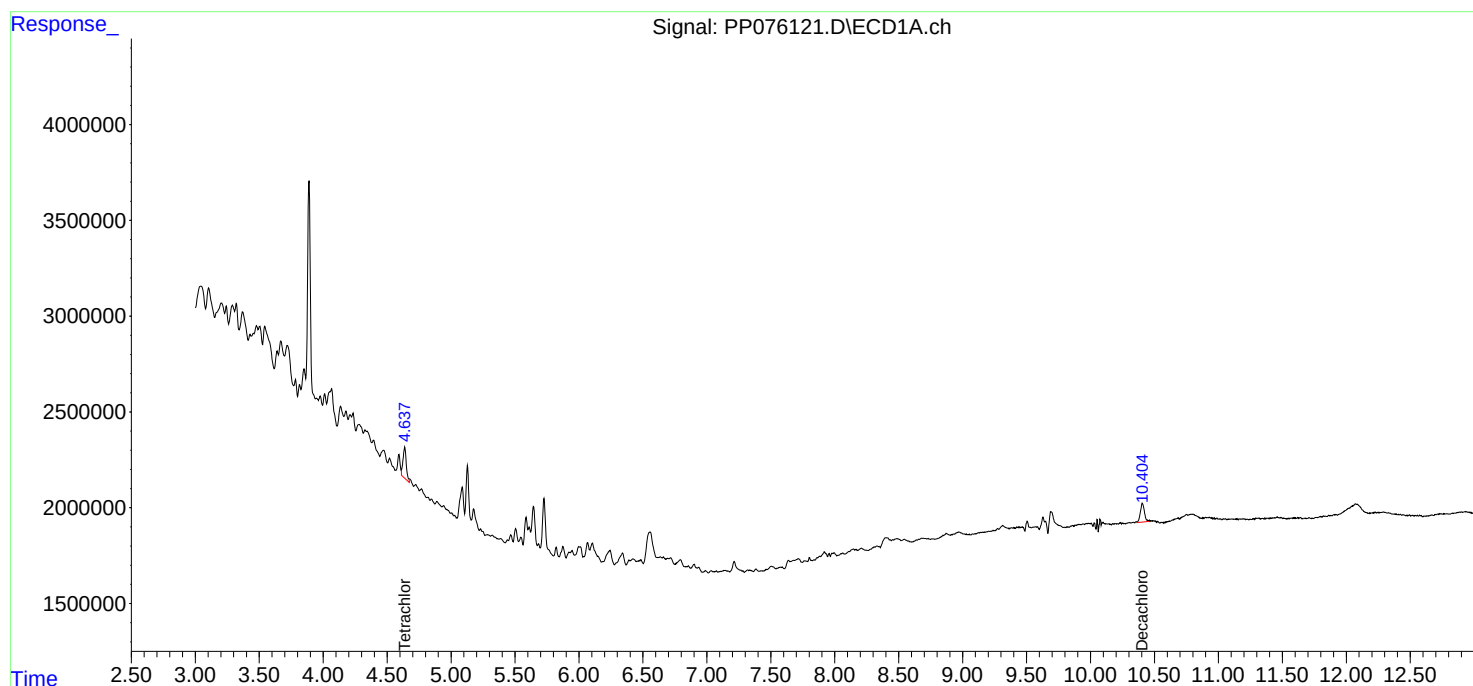

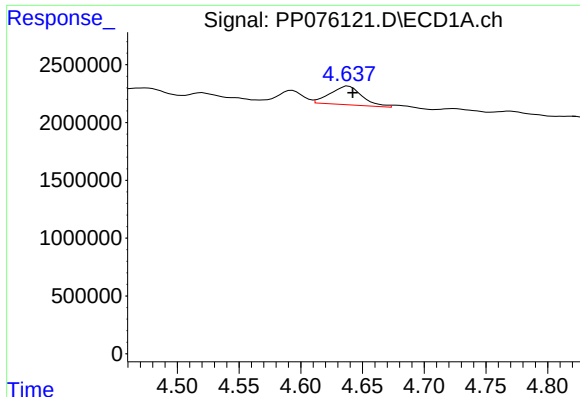


#1 Tetrachloro-m-xylene

R.T.: 4.639 min
Delta R.T.: -0.003 min
Response: 2900493
Conc: 2.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

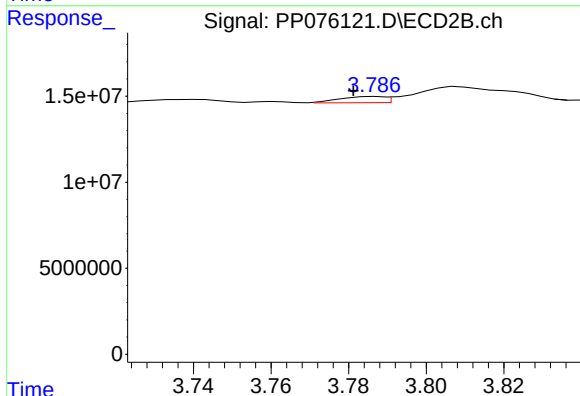


#1 Tetrachloro-m-xylene

R.T.: 3.786 min
Delta R.T.: 0.005 min
Response: 3219677
Conc: 0.49 ng/ml m

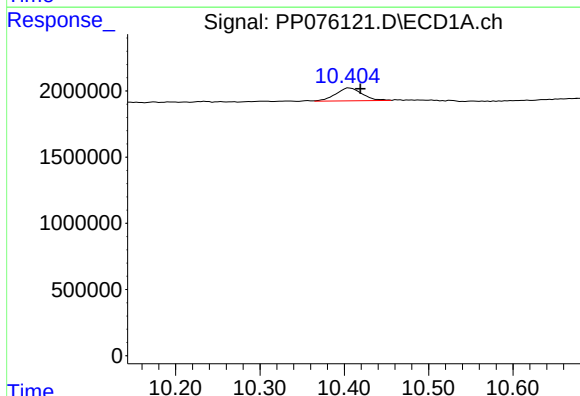

#2 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.015 min
Response: 2122336
Conc: 1.97 ng/ml m

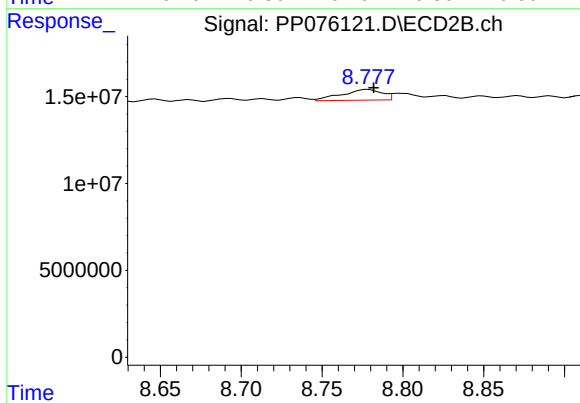

#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: -0.004 min
Response: 10617426
Conc: 1.29 ng/ml