

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102825\
 Data File : PP076123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 12:58
 Operator : YP\AJ
 Sample : Q3472-14 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 155

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/29/2025
 Supervised By :Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 14:06:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.637	3.790	2498958	11458130	1.749m	1.731
2) SA Decachlor...	10.405	8.778	2135933	4636471	1.984m	0.564m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102825\
Data File : PP076123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 12:58
Operator : YP\AJ
Sample : Q3472-14 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
155


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 14:06:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

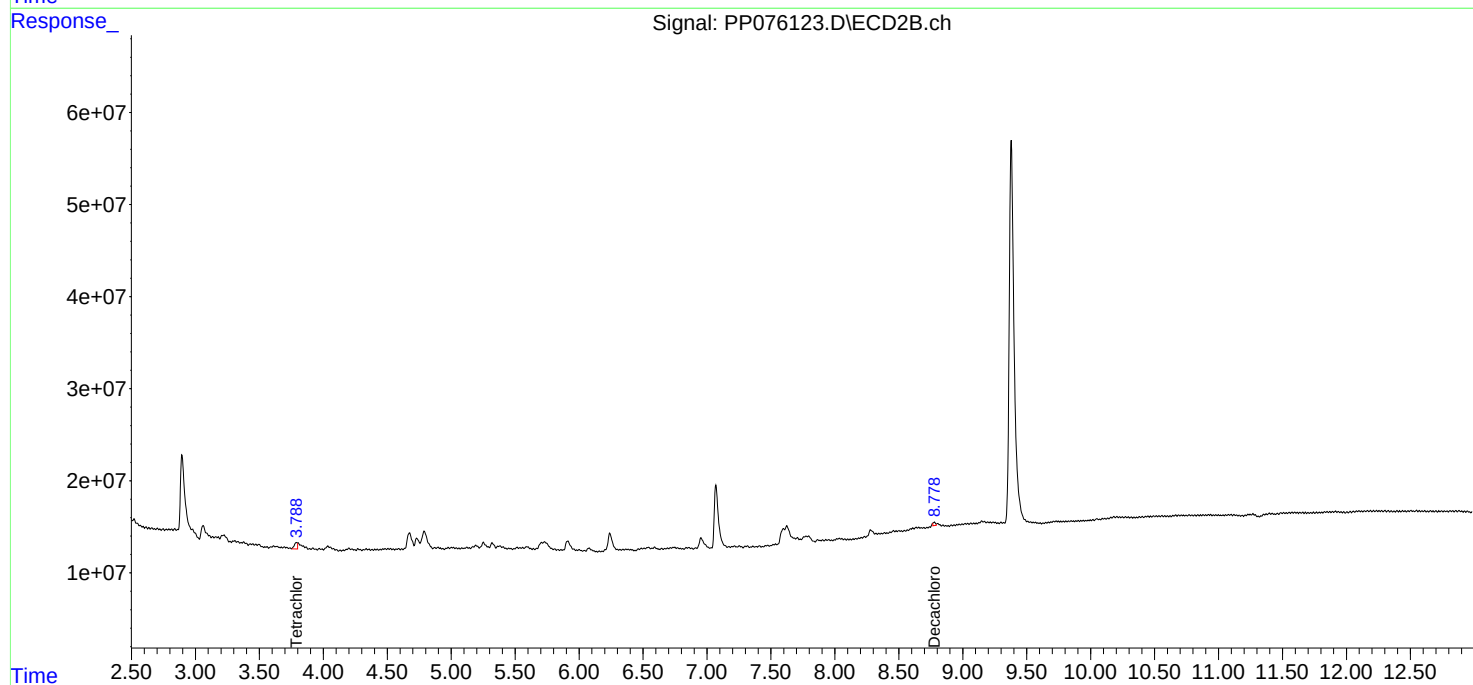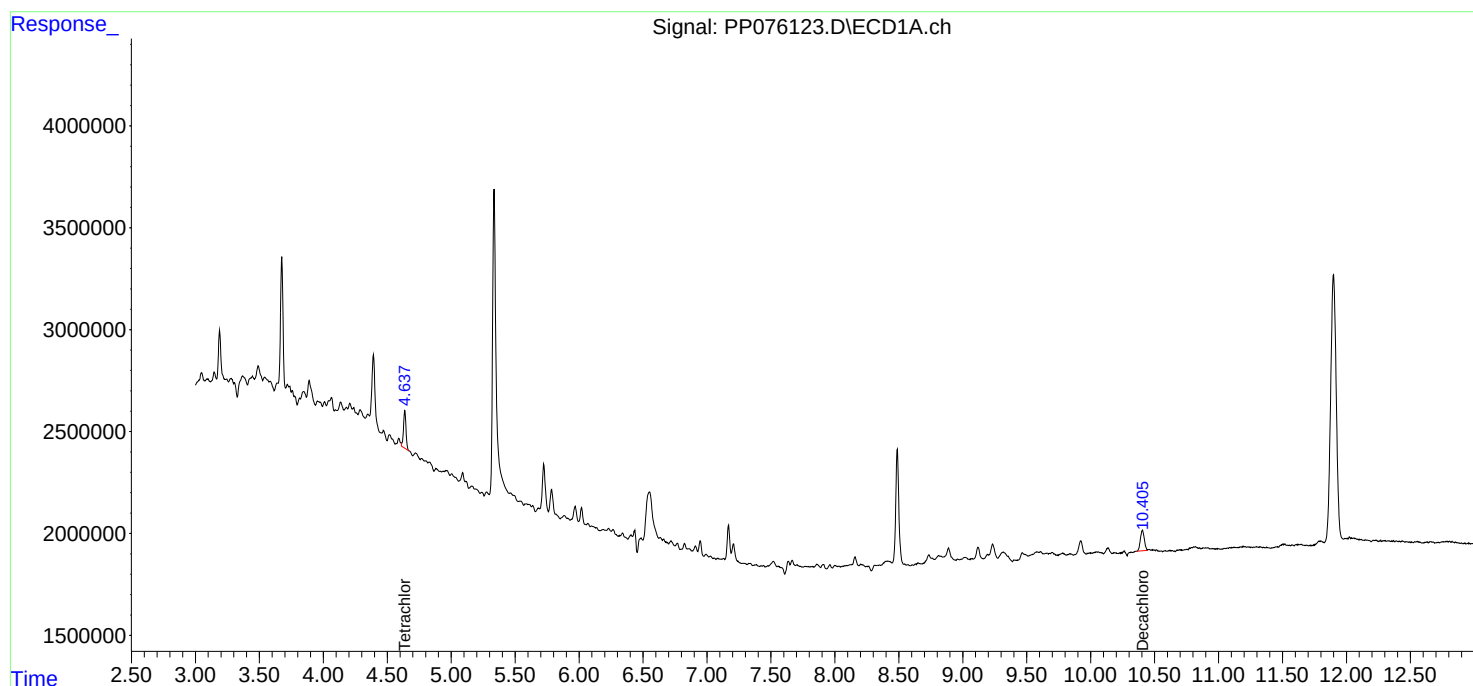

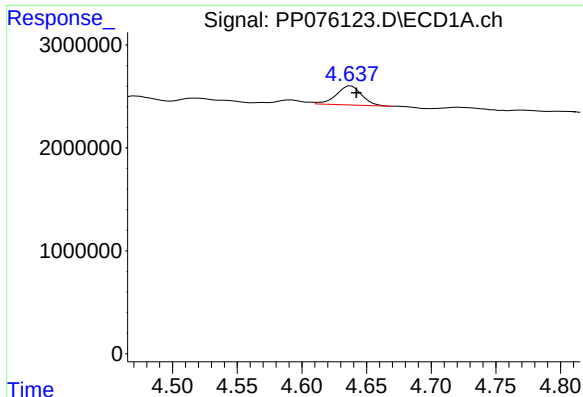


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: -0.005 min
Response: 2498958
Conc: 1.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
155


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

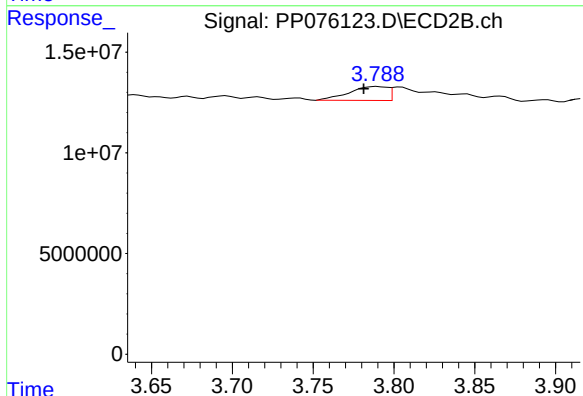


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.008 min
Response: 11458130
Conc: 1.73 ng/ml

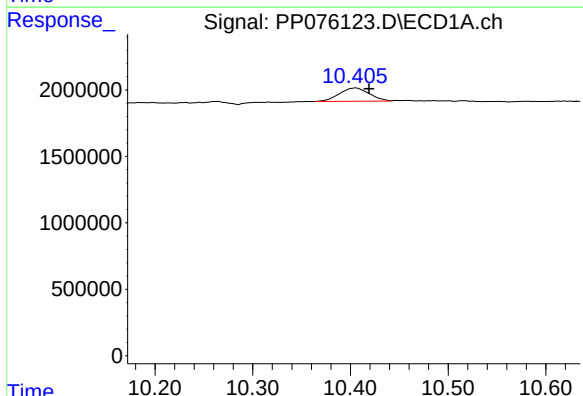

#2 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.014 min
Response: 2135933
Conc: 1.98 ng/ml m

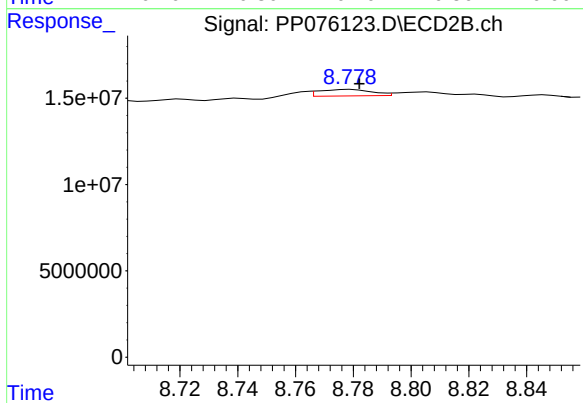

#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: -0.004 min
Response: 4636471
Conc: 0.56 ng/ml m