

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102920\
 Data File : PP030927.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2020 18:47
 Operator : DD\AJ
 Sample : MDL-PCB-BL-S-2
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-S-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 10:04:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1248PP102920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 28 16:58:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.803	4.080	1124717	1019593	18.865	18.904
2) SA Decachlor...	10.690	9.414	675268	709554	19.853	19.476

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102920\
Data File : PP030927.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2020 18:47
Operator : DD\AJ
Sample : MDL-PCB-BL-S-2
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 10:04:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1248PP102920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 28 16:58:01 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

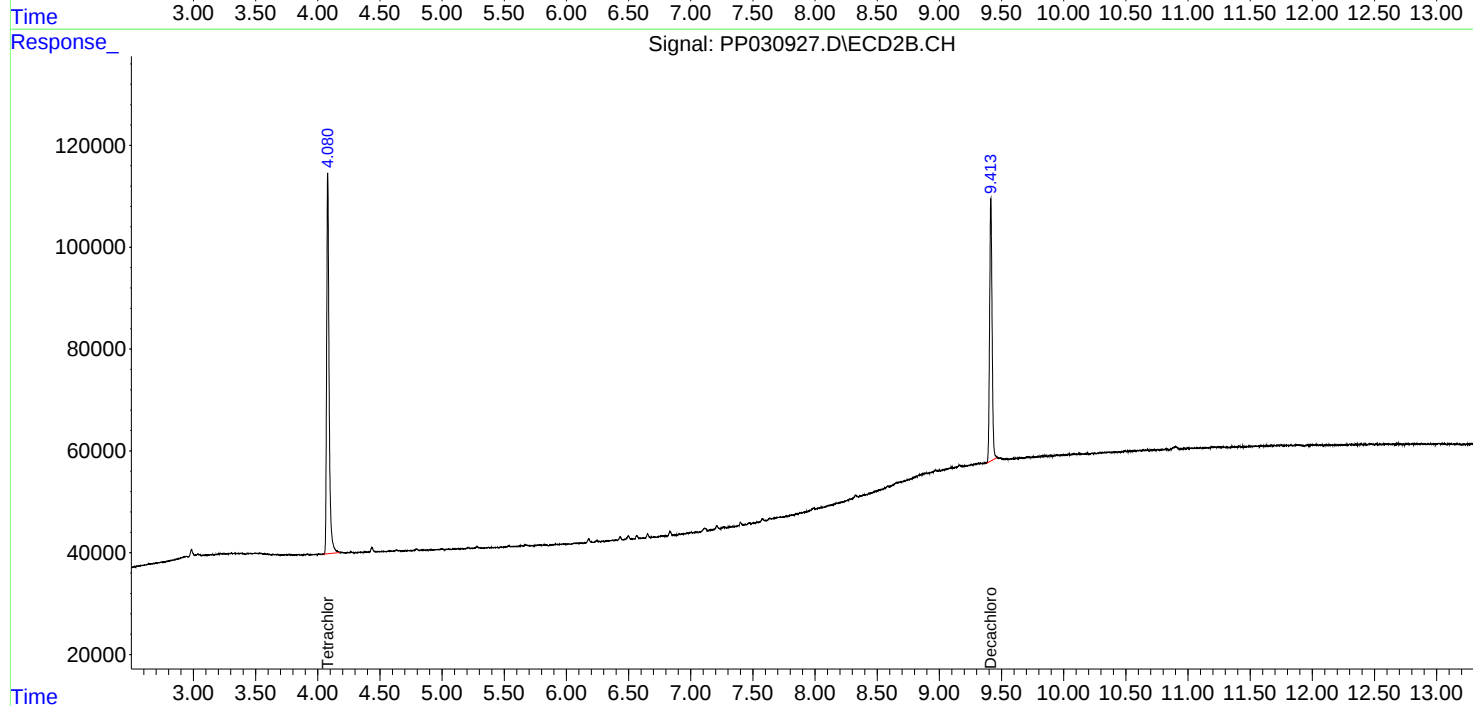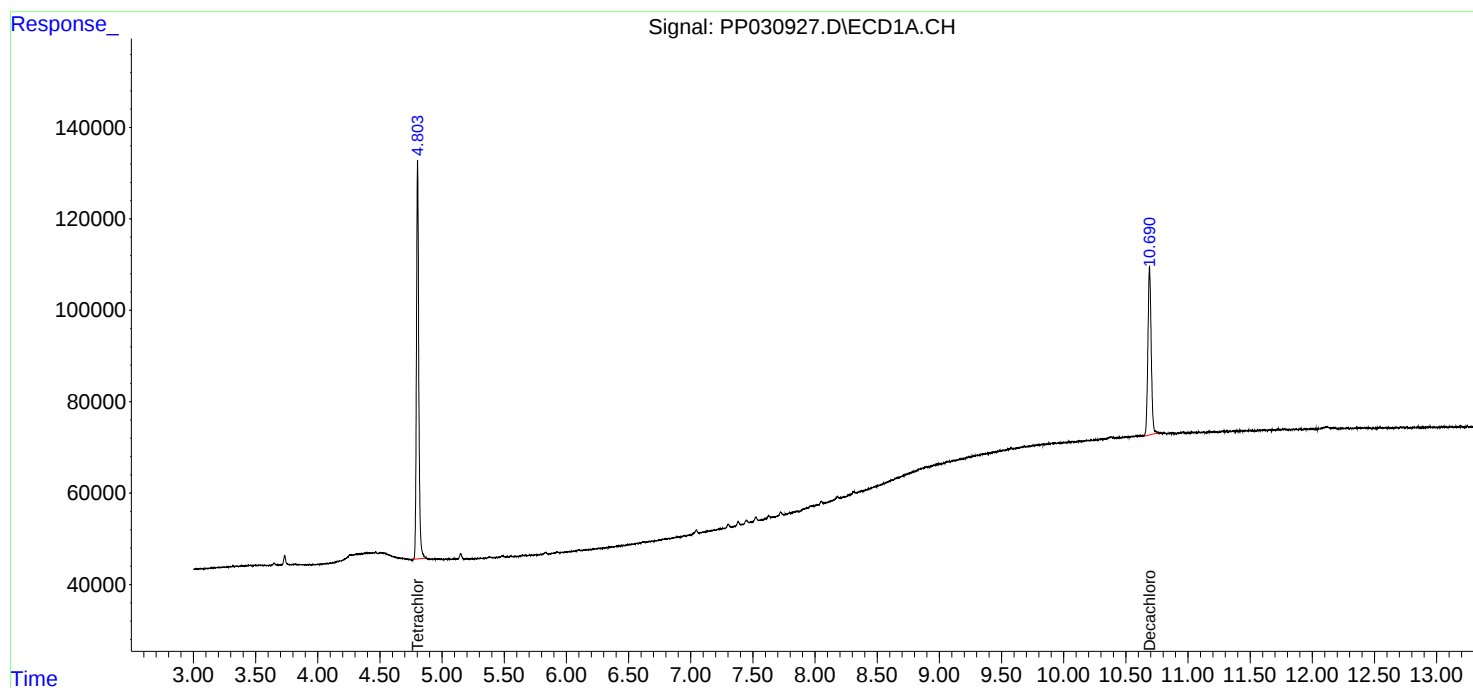


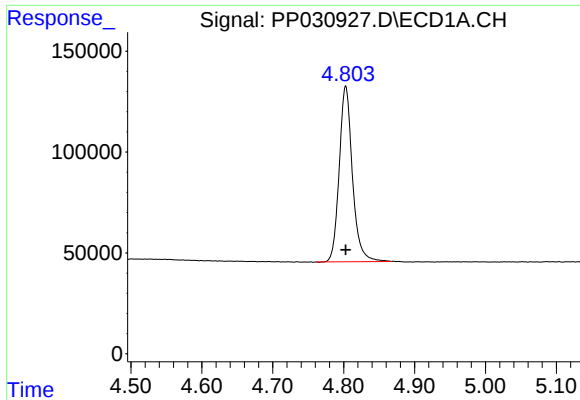

#1 Tetrachloro-m-xylene


R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 1124717
Conc: 18.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-2

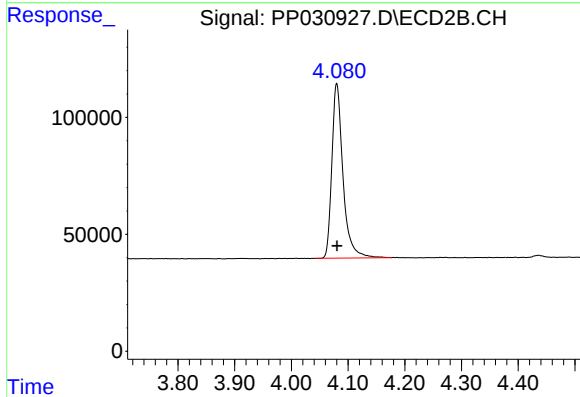


#1 Tetrachloro-m-xylene

R.T.: 4.080 min
Delta R.T.: 0.000 min
Response: 1019593
Conc: 18.90 ng/ml

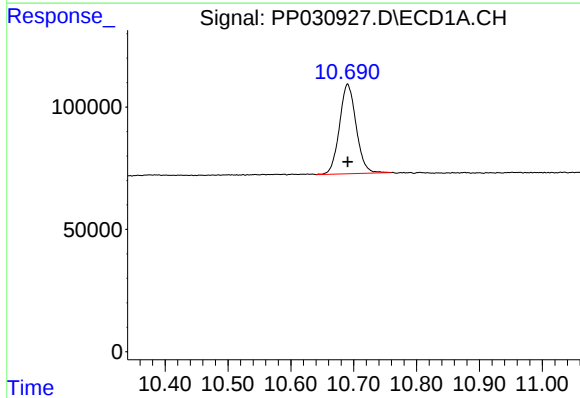

#2 Decachlorobiphenyl

R.T.: 10.690 min
Delta R.T.: 0.000 min
Response: 675268
Conc: 19.85 ng/ml

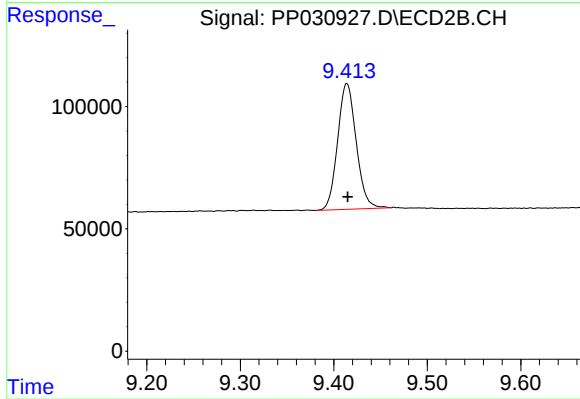

#2 Decachlorobiphenyl

R.T.: 9.414 min
Delta R.T.: 0.000 min
Response: 709554
Conc: 19.48 ng/ml