

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102920\
 Data File : PP030937.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2020 21:33
 Operator : DD\AJ
 Sample : MDL-PCB-BL-W-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-W-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 10:07:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1248PP102920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 28 16:58:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.802	4.079	1139991	1014525	19.121	18.810
2) SA Decachlor...	10.689	9.414	662934	726832	19.491	19.950

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102920\
Data File : PP030937.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2020 21:33
Operator : DD\AJ
Sample : MDL-PCB-BL-W-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-W-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 10:07:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1248PP102920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 28 16:58:01 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

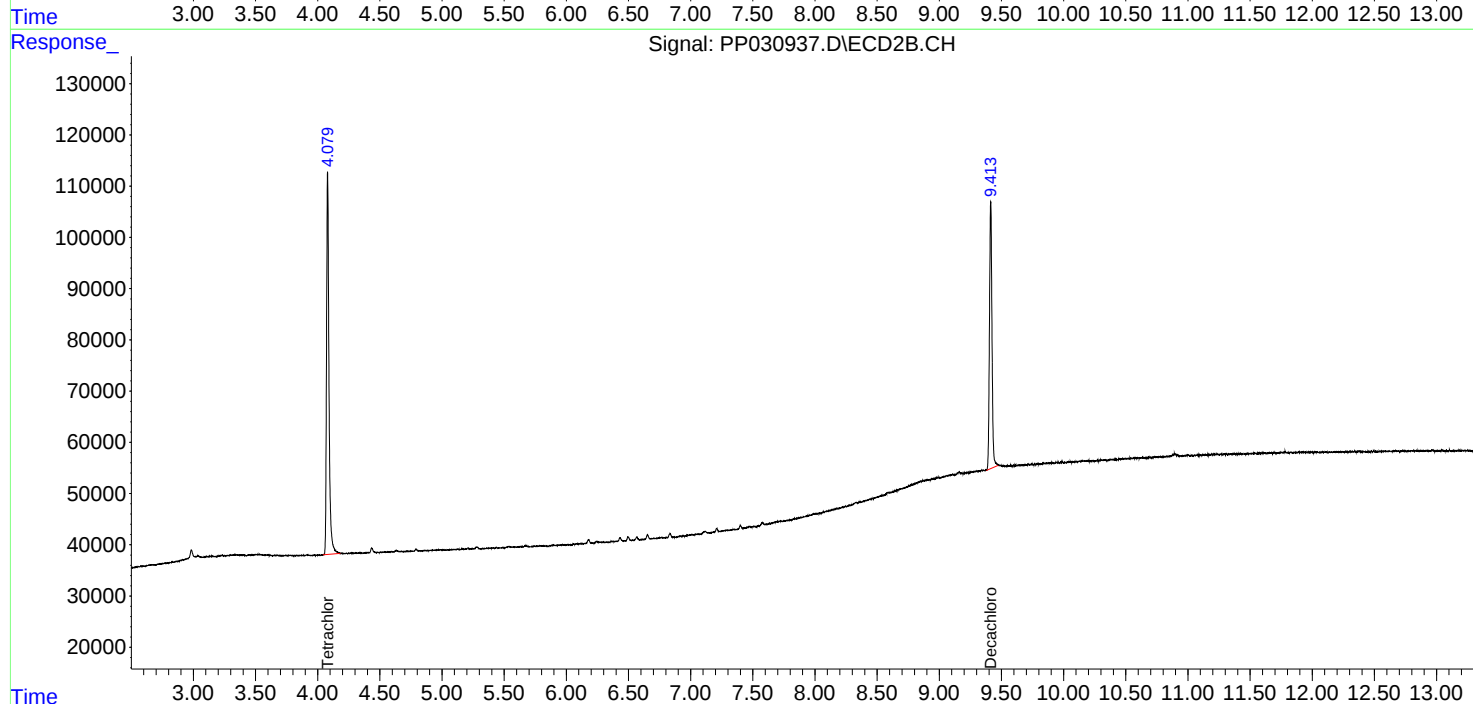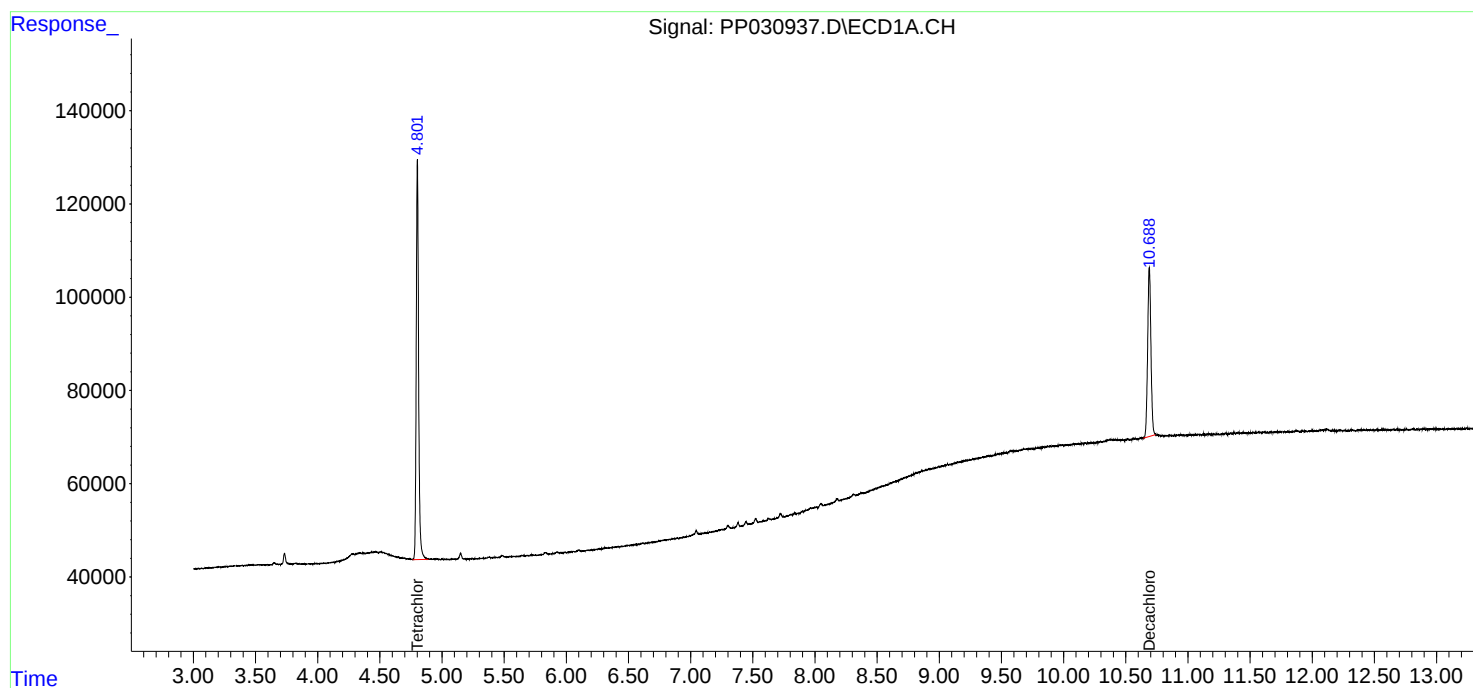


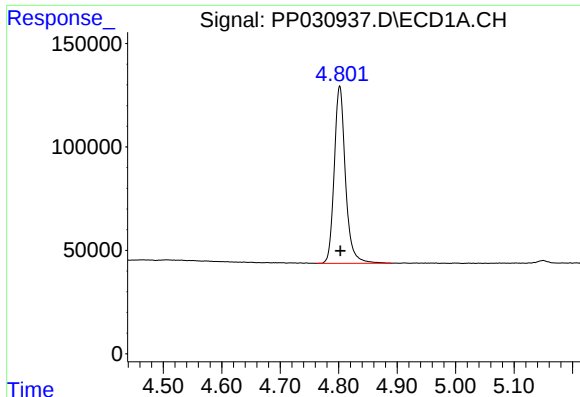

#1 Tetrachloro-m-xylene


R.T.: 4.802 min
Delta R.T.: -0.001 min
Response: 1139991
Conc: 19.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-W-10

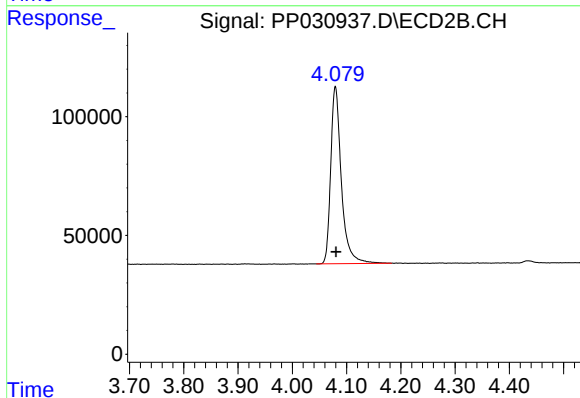


#1 Tetrachloro-m-xylene

R.T.: 4.079 min
Delta R.T.: -0.001 min
Response: 1014525
Conc: 18.81 ng/ml

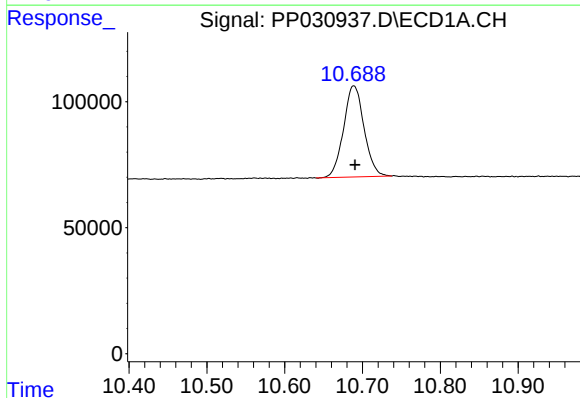

#2 Decachlorobiphenyl

R.T.: 10.689 min
Delta R.T.: -0.002 min
Response: 662934
Conc: 19.49 ng/ml

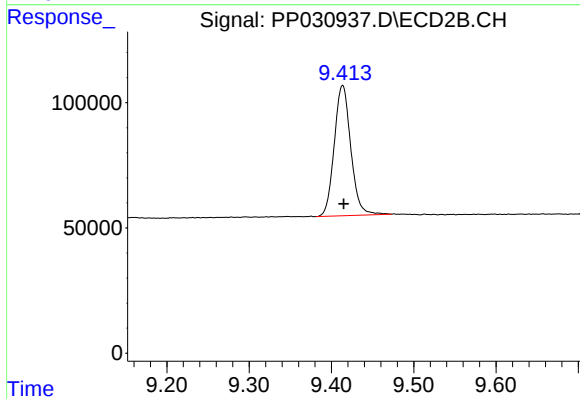

#2 Decachlorobiphenyl

R.T.: 9.414 min
Delta R.T.: -0.001 min
Response: 726832
Conc: 19.95 ng/ml