

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
 Data File : PP040591.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2021 22:13
 Operator : AJ\MA
 Sample : PB140359BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:26:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 28 08:58:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.750	3.770	904784	505628	22.214	18.560
2)	SA Decachlor...	10.683	9.054	645806	581596	21.317	20.730
Target Compounds							
8)	L2 AR-1221-1	4.997	0.000	46531	0	96.010	N.D. #
9)	L2 AR-1221-2	5.101	0.000	14097	0	41.530	N.D. #
10)	L2 AR-1221-3	0.000	4.214	0	9707	N.D.	11.414 #
11)	L3 AR-1232-1	0.000	4.214	0	9707	N.D.	13.745 #
38)	L8 AR-1262-3	0.000	8.002	0	6227	N.D.	4.861 #
41)	L9 AR-1268-1	0.000	8.002	0	6227	N.D.	1.761 #
45)	L9 AR-1268-5	0.000	8.826	0	4646	N.D.	0.517 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
Data File : PP040591.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 22:13
Operator : AJ\MA
Sample : PB140359BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:26:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

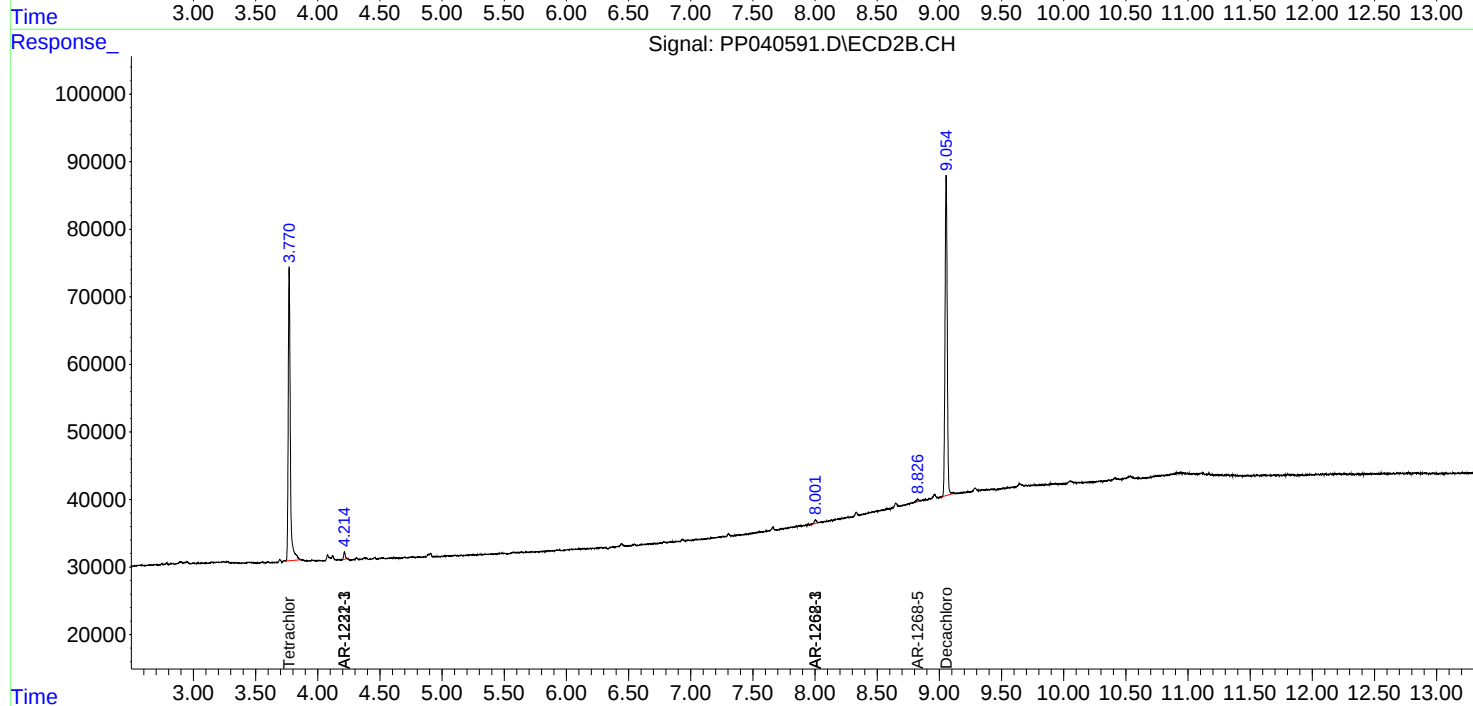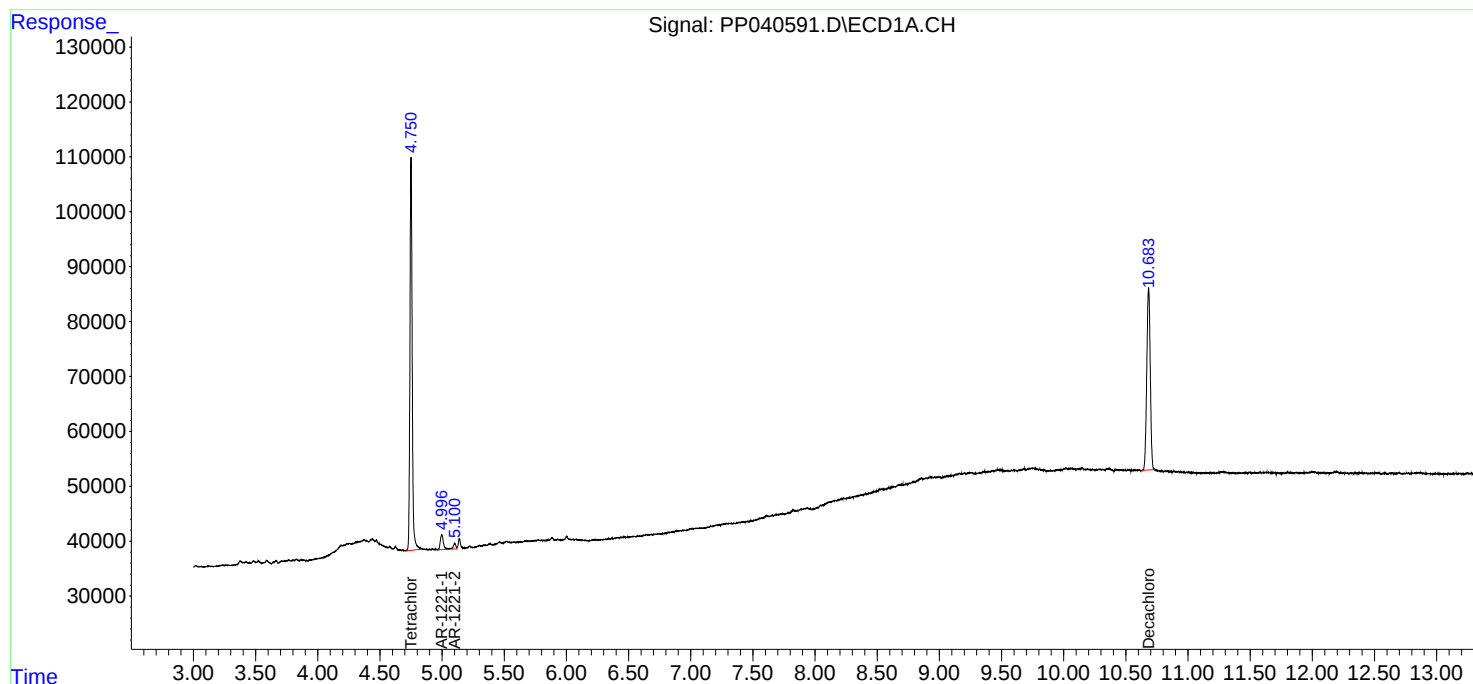


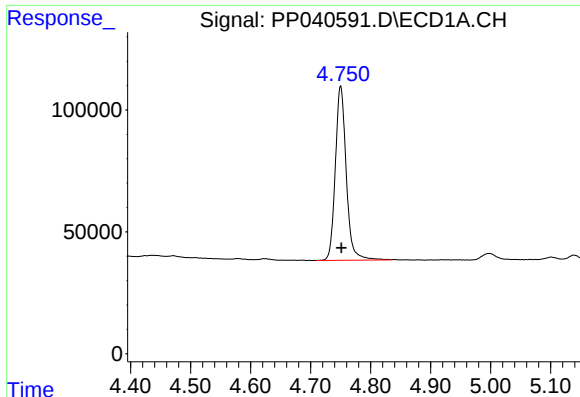

#1 Tetrachloro-m-xylene


R.T.: 4.750 min
Delta R.T.: 0.000 min
Response: 904784
Conc: 22.21 ng/ml

Instrument :
ECD_P
ClientSampleId :

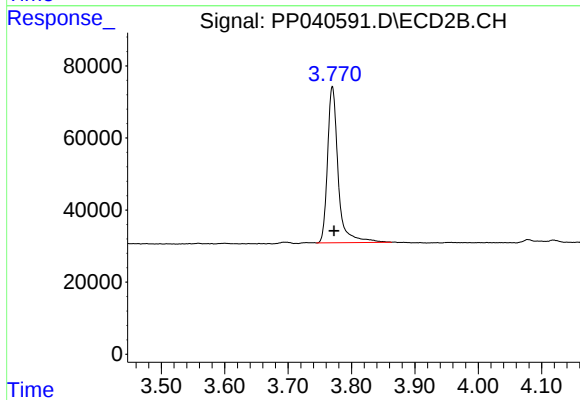


#1 Tetrachloro-m-xylene

R.T.: 3.770 min
Delta R.T.: -0.003 min
Response: 505628
Conc: 18.56 ng/ml

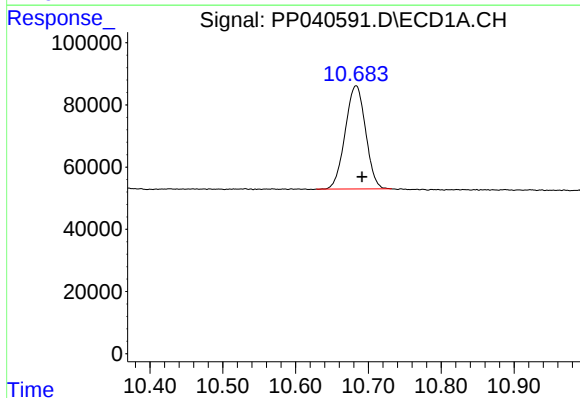


#2 Decachlorobiphenyl

R.T.: 10.683 min
Delta R.T.: -0.008 min
Response: 645806
Conc: 21.32 ng/ml

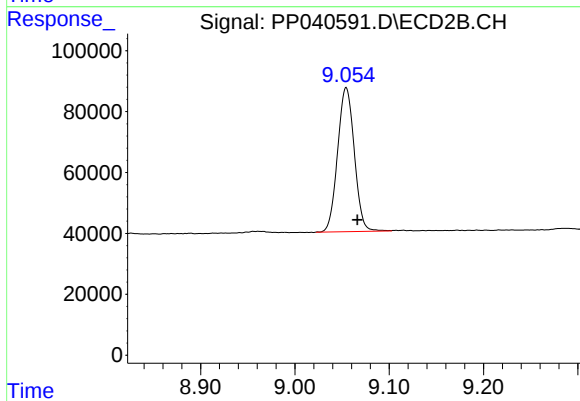

#2 Decachlorobiphenyl


R.T.: 9.054 min
Delta R.T.: -0.012 min
Response: 581596
Conc: 20.73 ng/ml

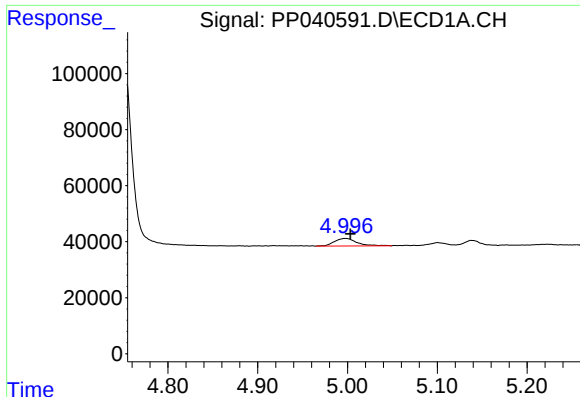

#8 AR-1221-1


R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 46531
Conc: 96.01 ng/ml

Instrument :
ECD_P
ClientSampleId :

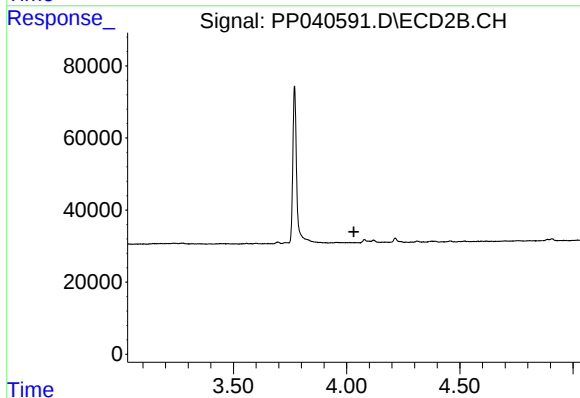


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.032 min
Response: 0
Conc: N.D.

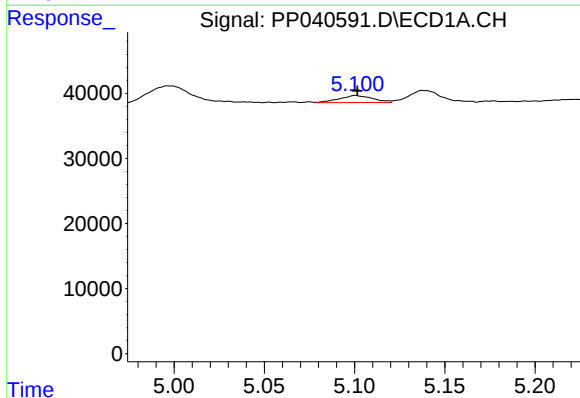


#9 AR-1221-2

R.T.: 5.101 min
Delta R.T.: -0.001 min
Response: 14097
Conc: 41.53 ng/ml

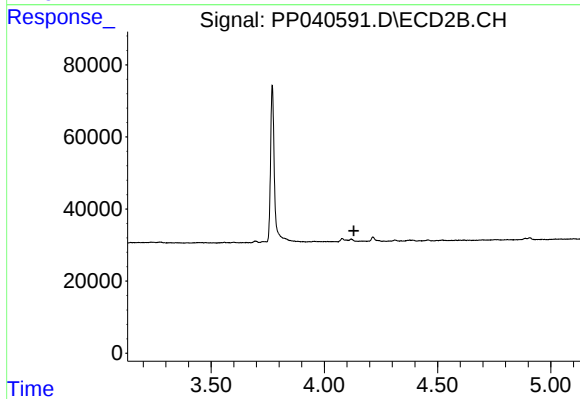

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.131 min
Response: 0
Conc: N.D.

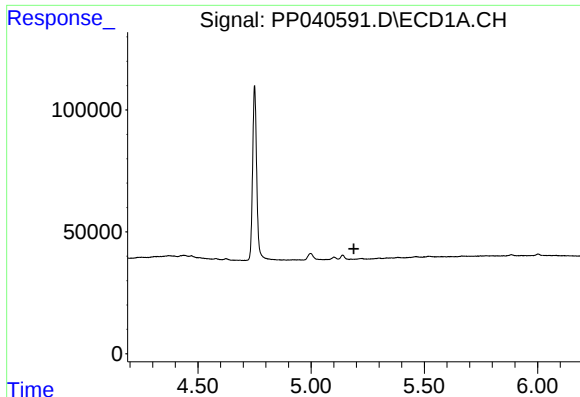

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.189 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

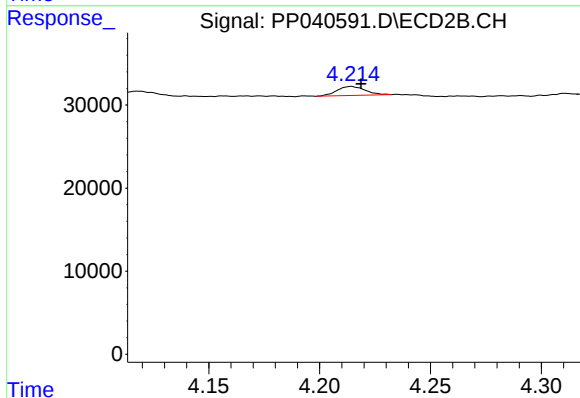


#10 AR-1221-3

R.T.: 4.214 min
Delta R.T.: -0.004 min
Response: 9707
Conc: 11.41 ng/ml

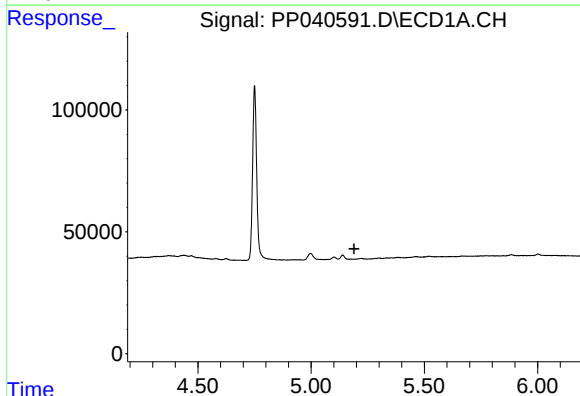


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.189 min
Response: 0
Conc: N.D.

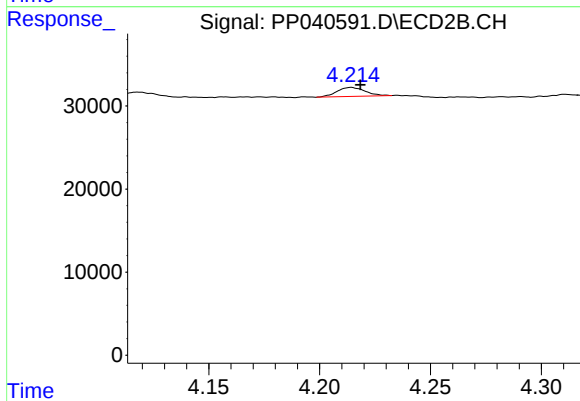

#11 AR-1232-1


R.T.: 4.214 min
Delta R.T.: -0.004 min
Response: 9707
Conc: 13.74 ng/ml

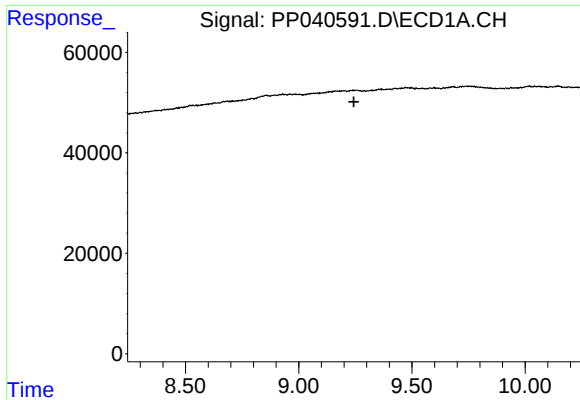

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

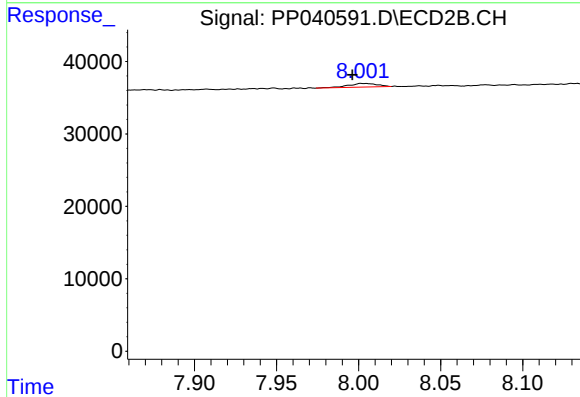


#38 AR-1262-3

R.T.: 8.002 min
Delta R.T.: 0.005 min
Response: 6227
Conc: 4.86 ng/ml

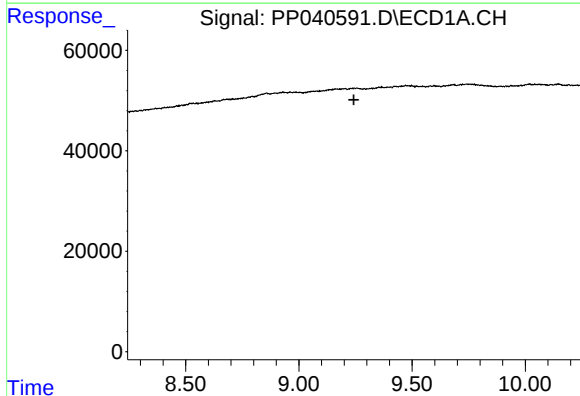


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.243 min
Response: 0
Conc: N.D.

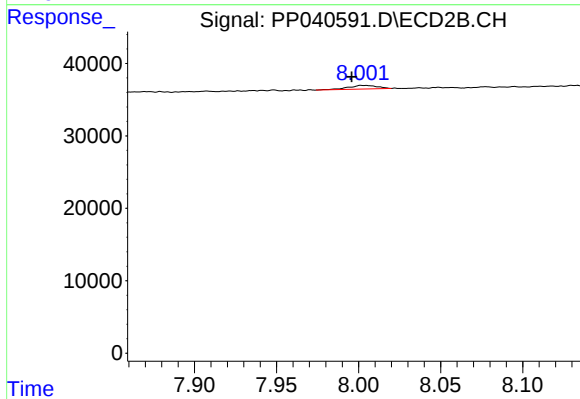

#41 AR-1268-1


R.T.: 8.002 min
Delta R.T.: 0.006 min
Response: 6227
Conc: 1.76 ng/ml

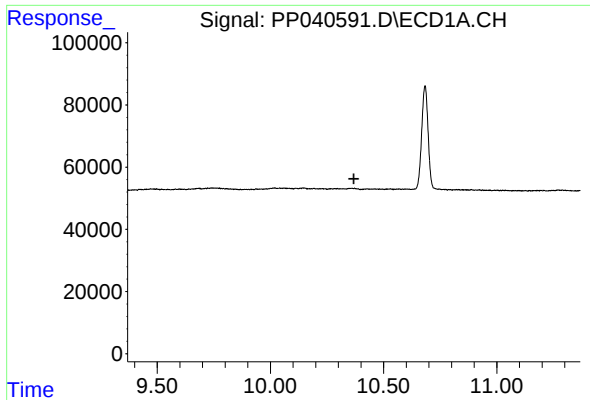

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

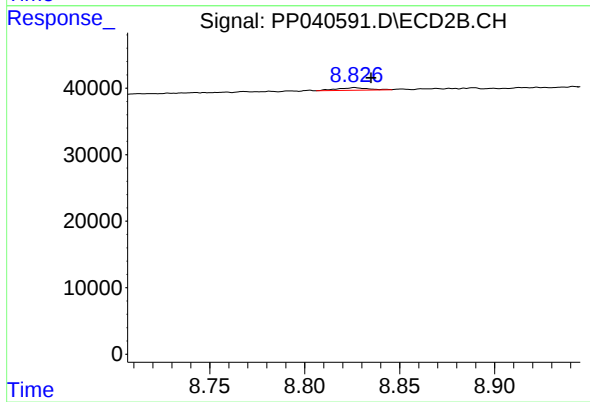

#45 AR-1268-5

R.T.: 8.826 min
Delta R.T.: -0.009 min
Response: 4646
Conc: 0.52 ng/ml