

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
Data File : PP040562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 13:10
Operator : AJ\MA
Sample : PB140337BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB140337BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:17:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.749	3.770	853942	485401	20.966	17.818
2) SA Decachlor...	10.677	9.053	629067	560259	20.764	19.970

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
Data File : PP040562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 13:10
Operator : AJ\MA
Sample : PB140337BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB140337BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:17:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

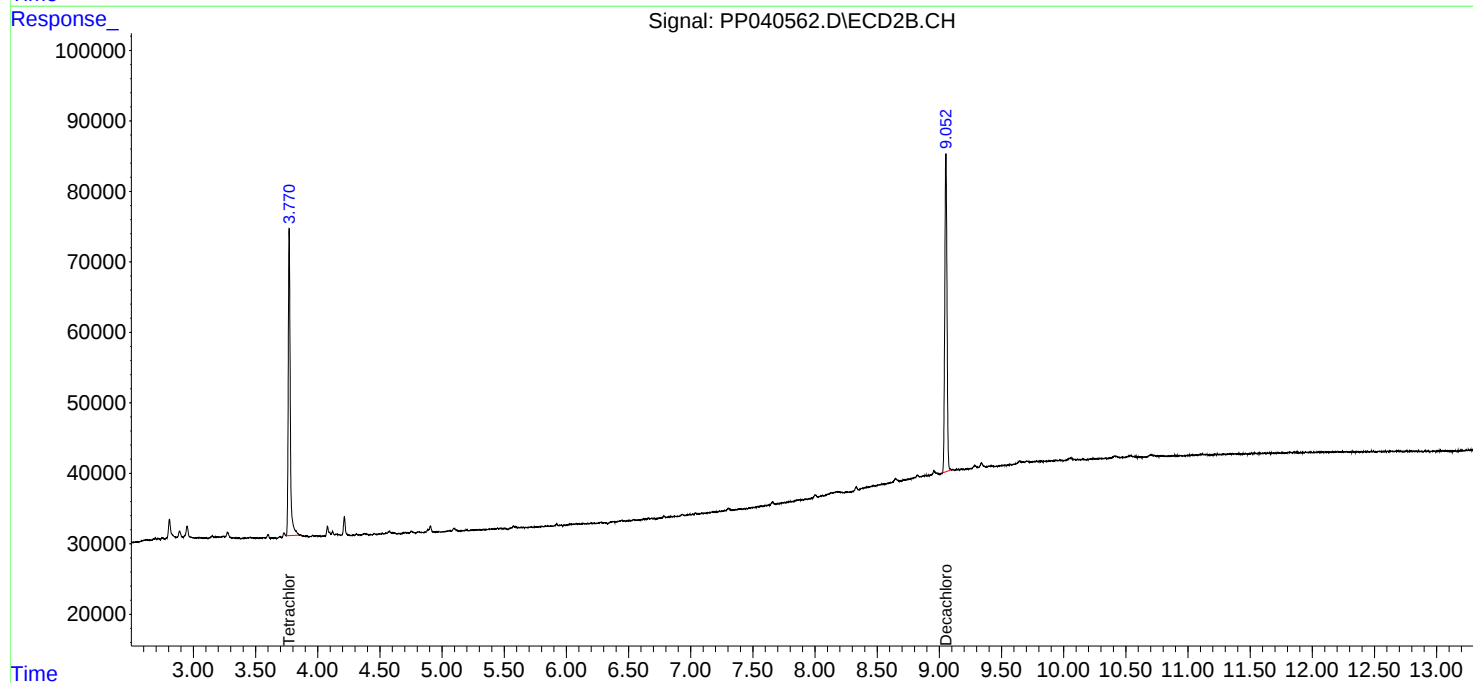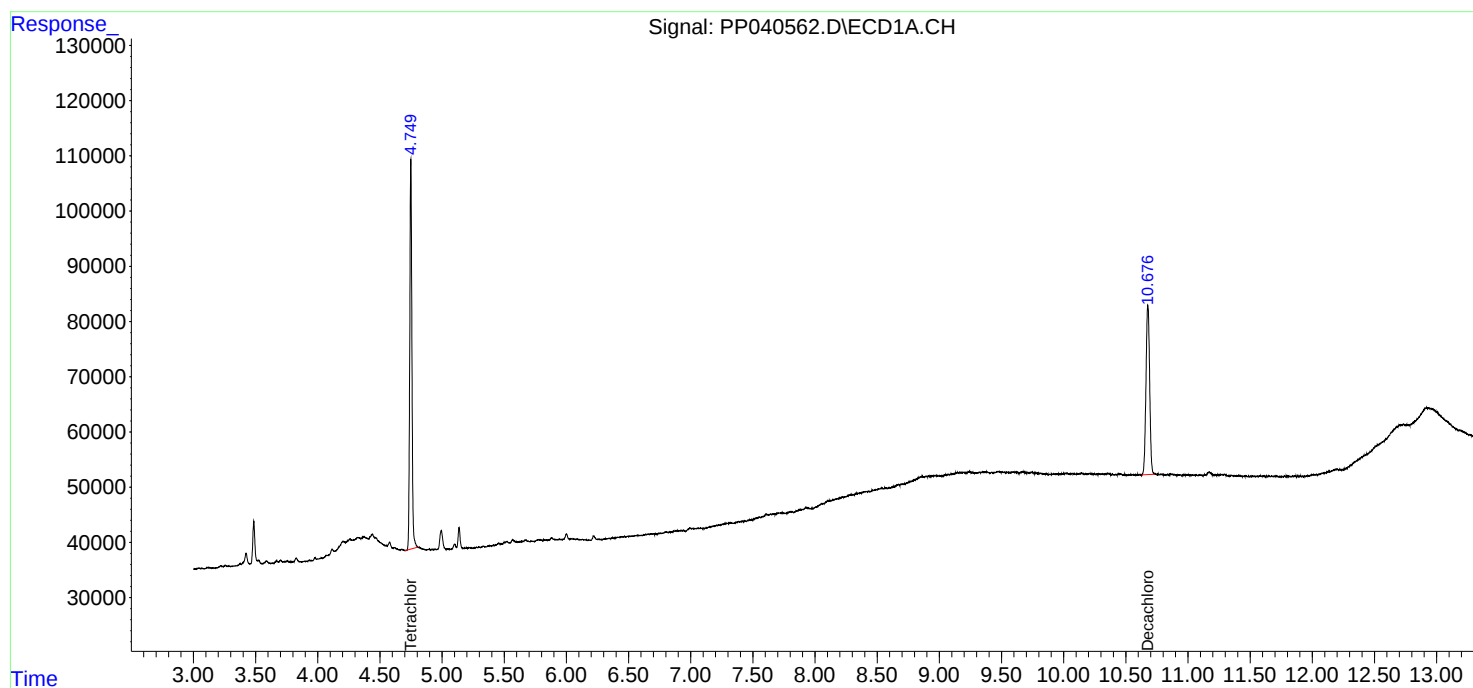


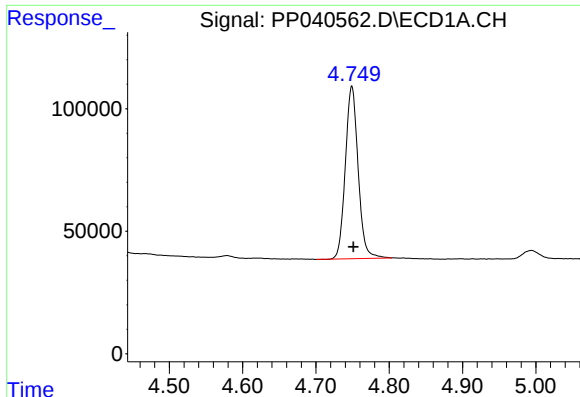

#1 Tetrachloro-m-xylene


R.T.: 4.749 min
Delta R.T.: -0.002 min
Response: 853942
Conc: 20.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB140337BL

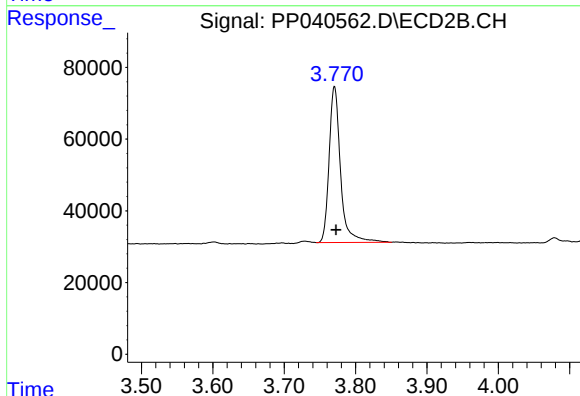


#1 Tetrachloro-m-xylene

R.T.: 3.770 min
Delta R.T.: -0.002 min
Response: 485401
Conc: 17.82 ng/ml

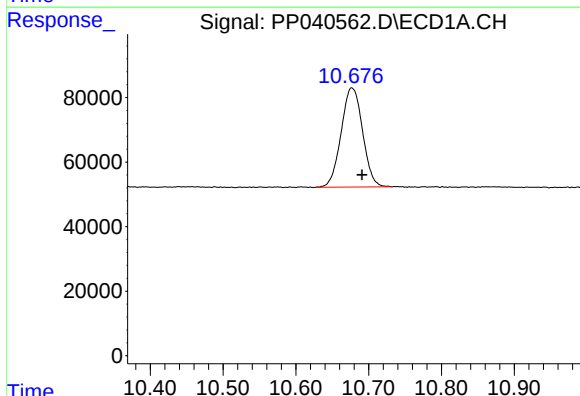

#2 Decachlorobiphenyl

R.T.: 10.677 min
Delta R.T.: -0.015 min
Response: 629067
Conc: 20.76 ng/ml

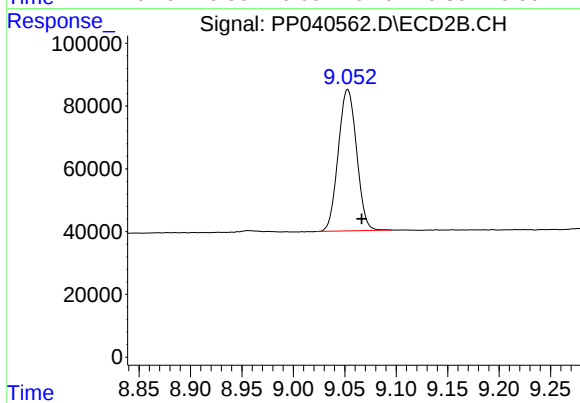

#2 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.014 min
Response: 560259
Conc: 19.97 ng/ml