

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
 Data File : PP040568.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2021 14:50
 Operator : AJ\MA
 Sample : M4402-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EO-01-102821

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:19:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 28 08:58:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.749	3.770	901750	530699	22.139	19.480
2)	SA Decachlor...	10.679	9.054	575674	483008	19.002	17.216

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
Data File : PP040568.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 14:50
Operator : AJ\MA
Sample : M4402-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
EO-01-102821

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:19:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

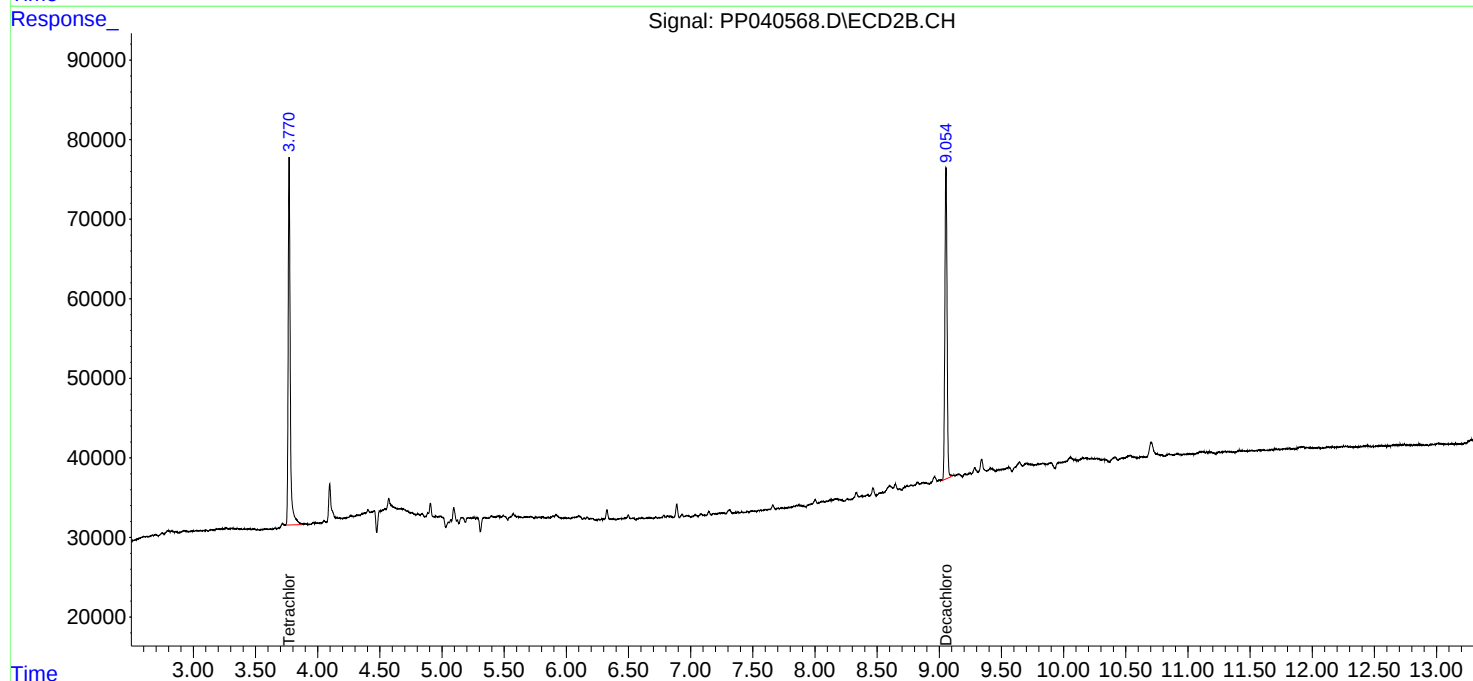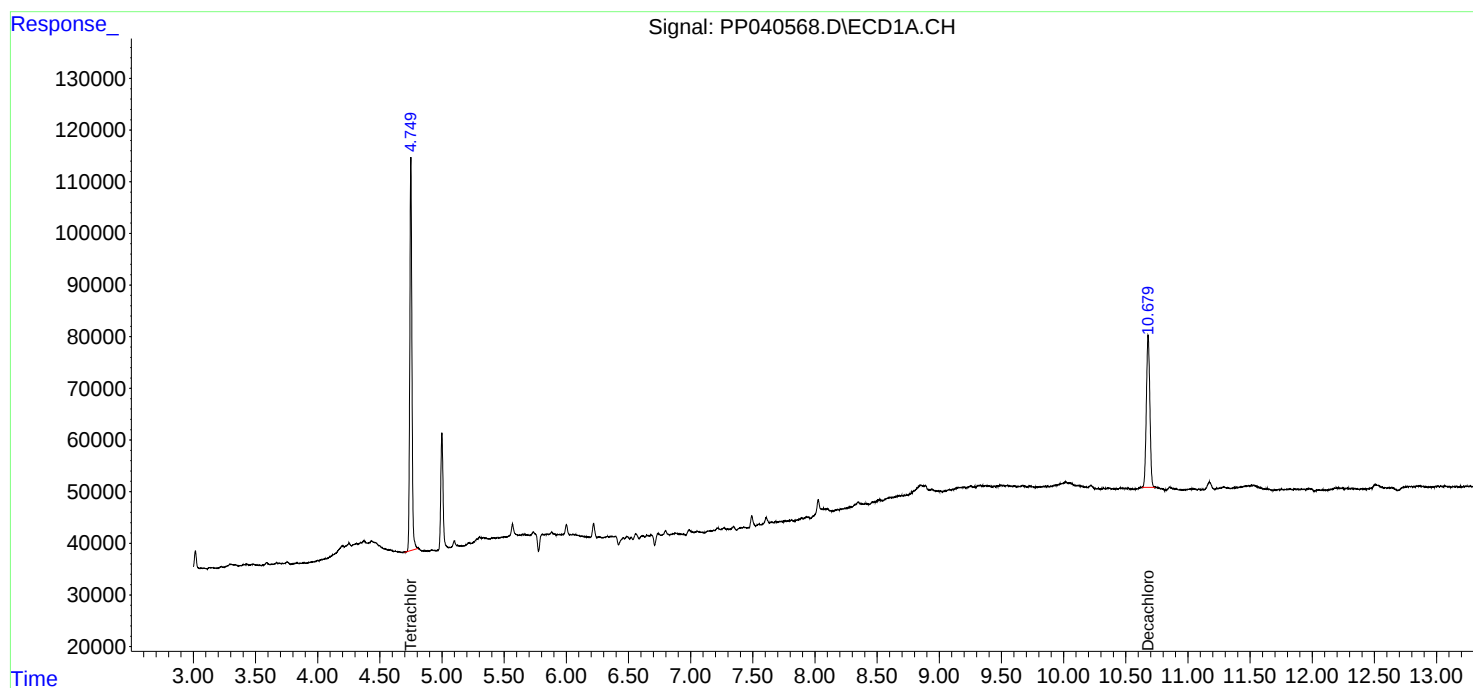


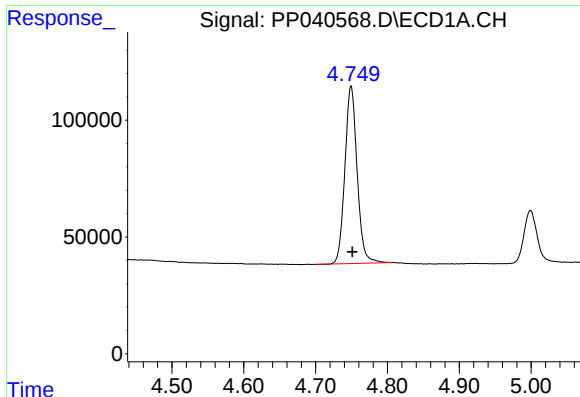

#1 Tetrachloro-m-xylene


R.T.: 4.749 min
Delta R.T.: -0.002 min
Response: 901750
Conc: 22.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
EO-01-102821

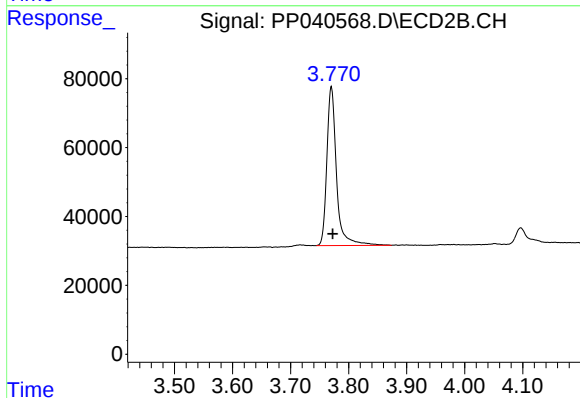


#1 Tetrachloro-m-xylene

R.T.: 3.770 min
Delta R.T.: -0.002 min
Response: 530699
Conc: 19.48 ng/ml

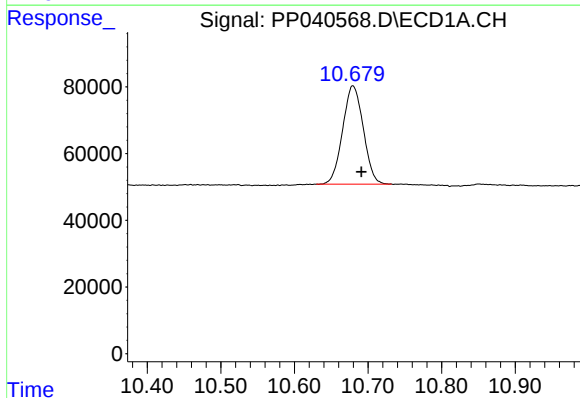

#2 Decachlorobiphenyl

R.T.: 10.679 min
Delta R.T.: -0.012 min
Response: 575674
Conc: 19.00 ng/ml

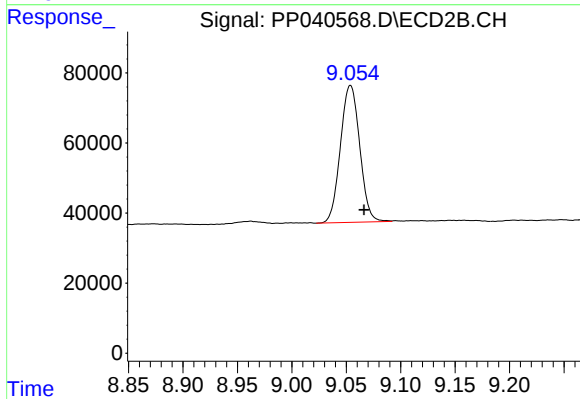

#2 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.013 min
Response: 483008
Conc: 17.22 ng/ml