

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
Data File : PP040571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 15:41
Operator : AJ\MA
Sample : M4406-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
280243

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:20:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.751	3.773	688991	374928	16.916	13.763
2) SA Decachlor...	10.680	9.054	641868	574838	21.187	20.489

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
Data File : PP040571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 15:41
Operator : AJ\MA
Sample : M4406-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
280243

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:20:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

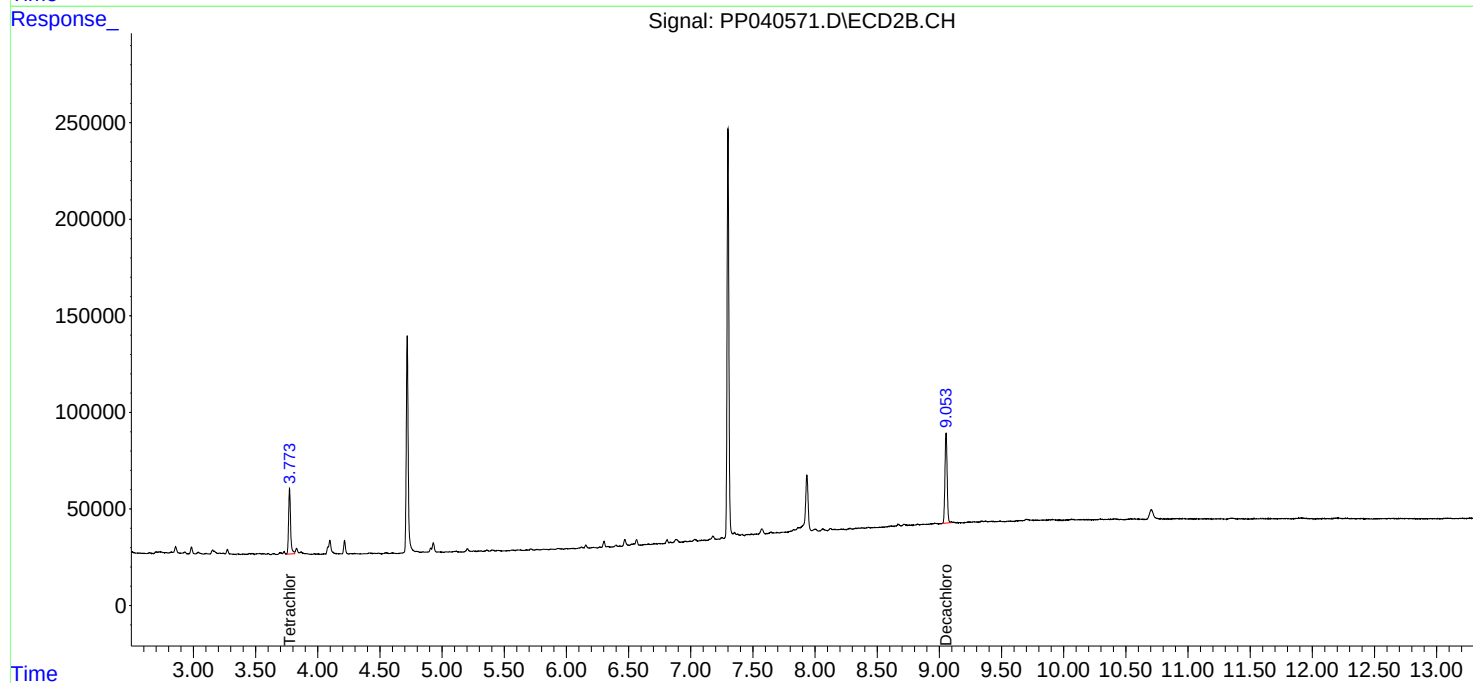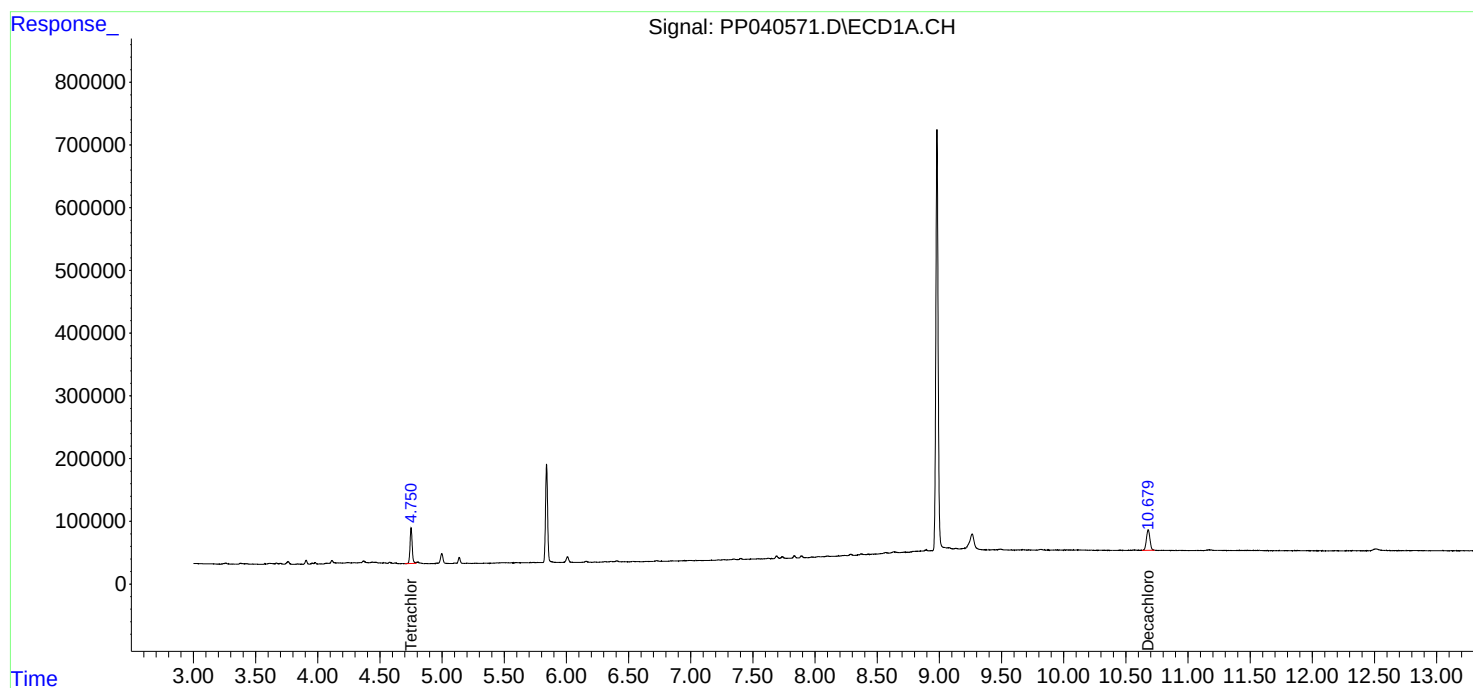


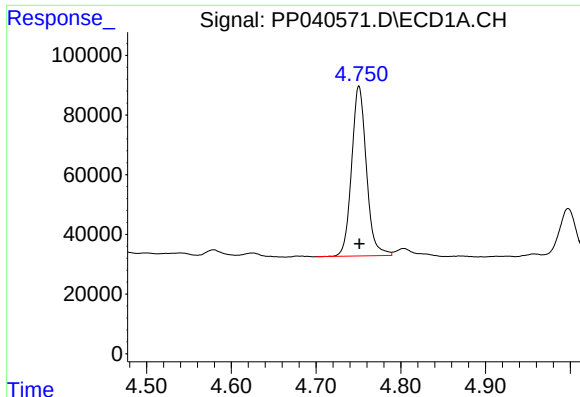

#1 Tetrachloro-m-xylene


R.T.: 4.751 min
Delta R.T.: 0.000 min
Response: 688991
Conc: 16.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
280243

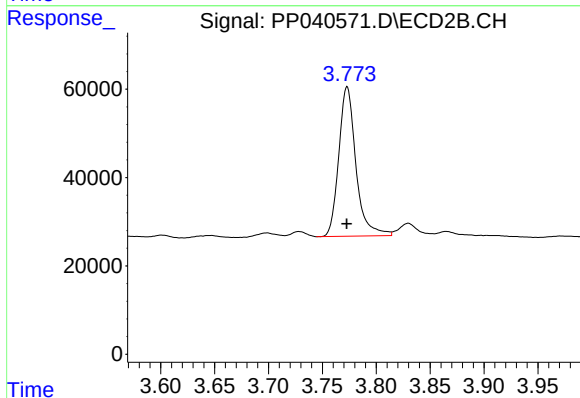


#1 Tetrachloro-m-xylene

R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 374928
Conc: 13.76 ng/ml

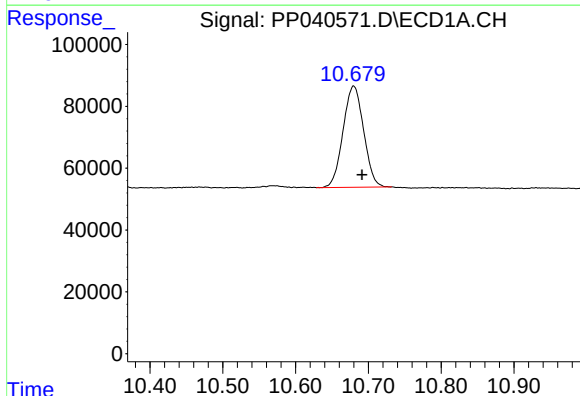

#2 Decachlorobiphenyl

R.T.: 10.680 min
Delta R.T.: -0.011 min
Response: 641868
Conc: 21.19 ng/ml

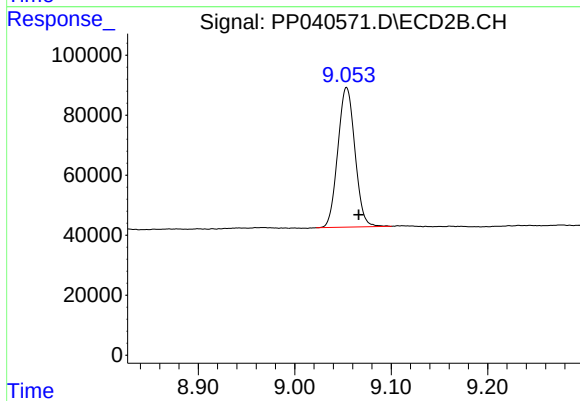

#2 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.013 min
Response: 574838
Conc: 20.49 ng/ml