

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
 Data File : PP040580.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2021 18:25
 Operator : AJ\MA
 Sample : M4407-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FDR-BH-1-20211028-5.5-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:23:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 28 08:58:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.749	3.770	842402	474290	20.682	17.410
2) SA Decachlor...	10.679	9.053	421464	375036	13.912	13.368

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102921\
Data File : PP040580.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 18:25
Operator : AJ\MA
Sample : M4407-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FDR-BH-1-20211028-5.5-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:23:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 28 08:58:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

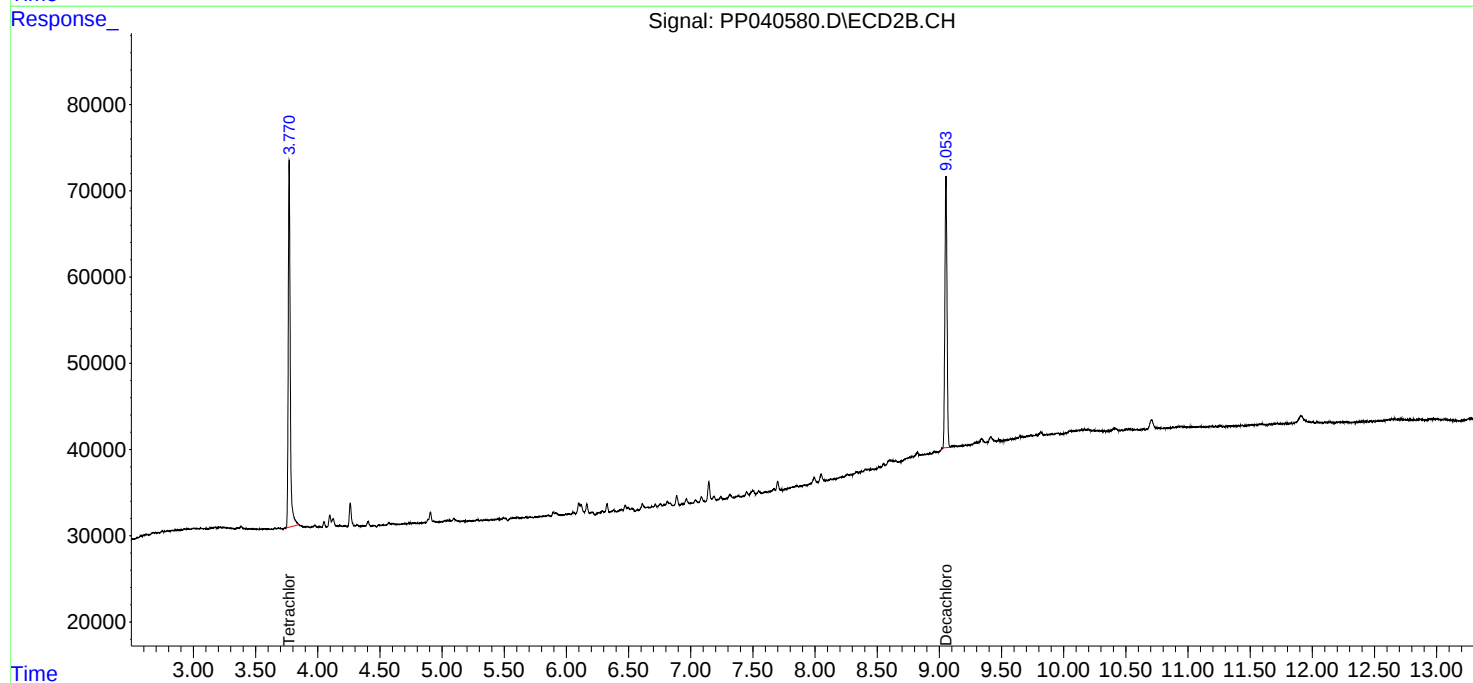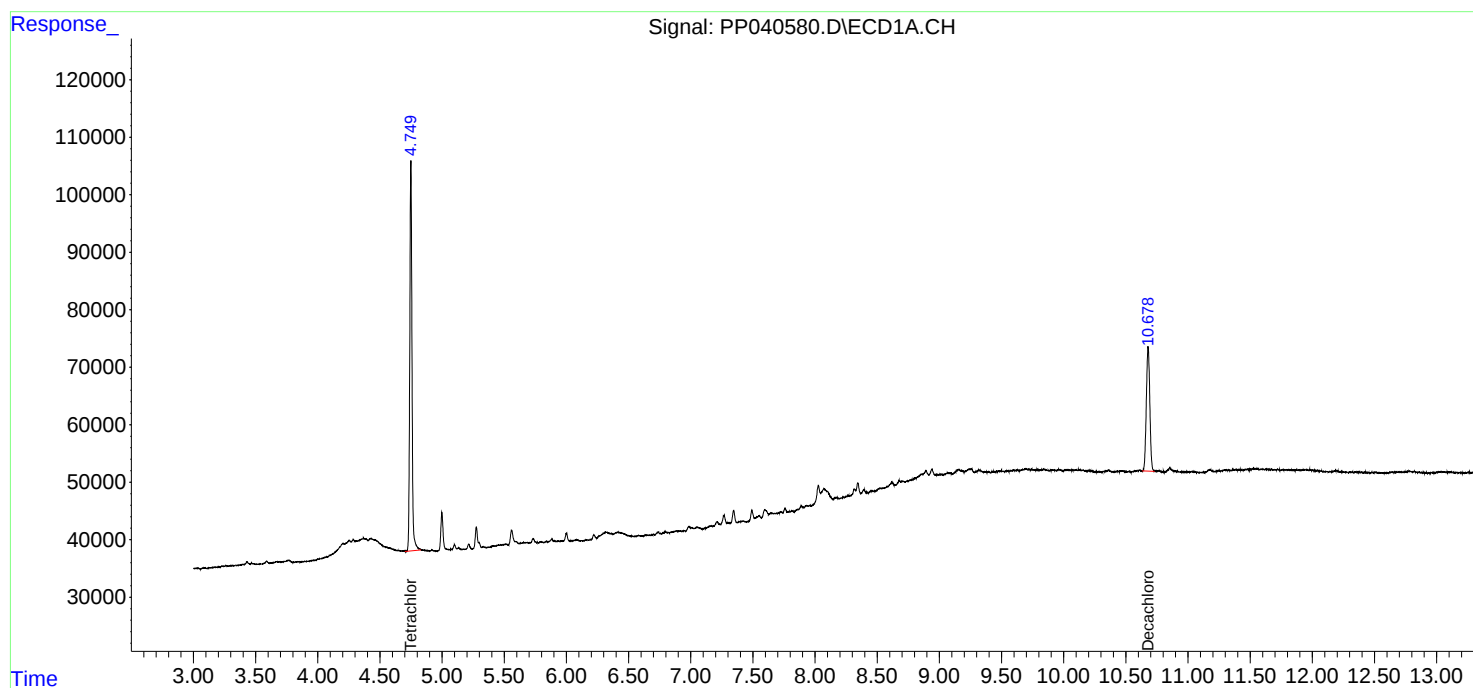


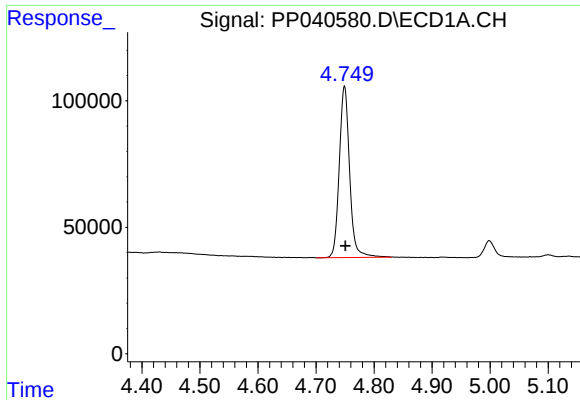

#1 Tetrachloro-m-xylene


R.T.: 4.749 min
Delta R.T.: -0.002 min
Response: 842402
Conc: 20.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDR-BH-1-20211028-5.5-6

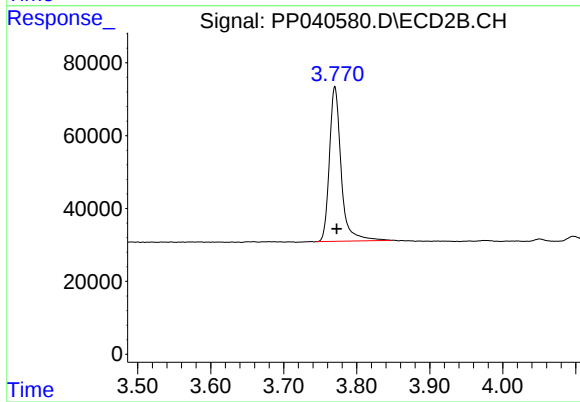


#1 Tetrachloro-m-xylene

R.T.: 3.770 min
Delta R.T.: -0.002 min
Response: 474290
Conc: 17.41 ng/ml

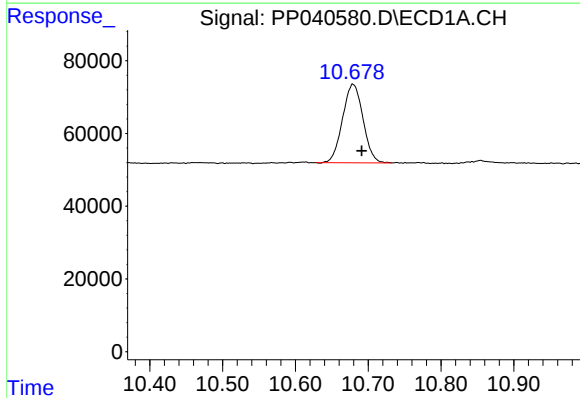

#2 Decachlorobiphenyl

R.T.: 10.679 min
Delta R.T.: -0.013 min
Response: 421464
Conc: 13.91 ng/ml

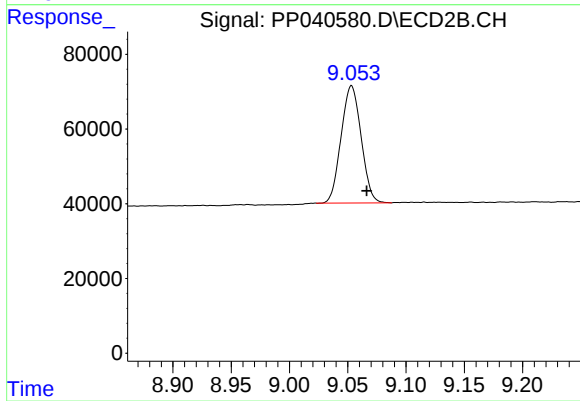

#2 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.013 min
Response: 375036
Conc: 13.37 ng/ml