

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102924\
 Data File : PP068307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 16:05
 Operator : YP\AJ
 Sample : P4564-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 100324

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/30/2024
 Supervised By :Ankita Jodhani 10/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 16:36:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.762	4.041	5755450	67070745	6.218m	66.380m#
2) SA Decachlor...	10.673	9.210	11871266	11739215	10.311m	10.468m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102924\
Data File : PP068307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 16:05
Operator : YP\AJ
Sample : P4564-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
100324


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/30/2024
Supervised By :Ankita Jodhani 10/30/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 16:36:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

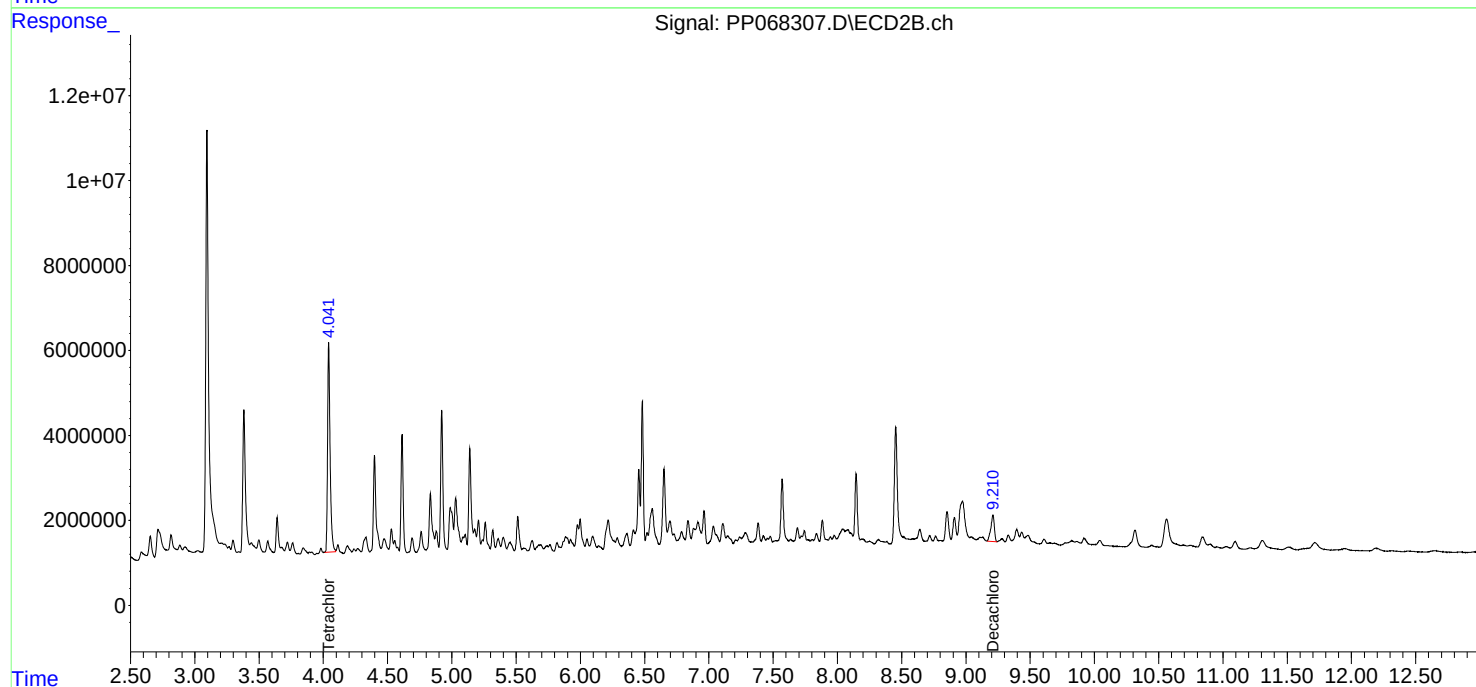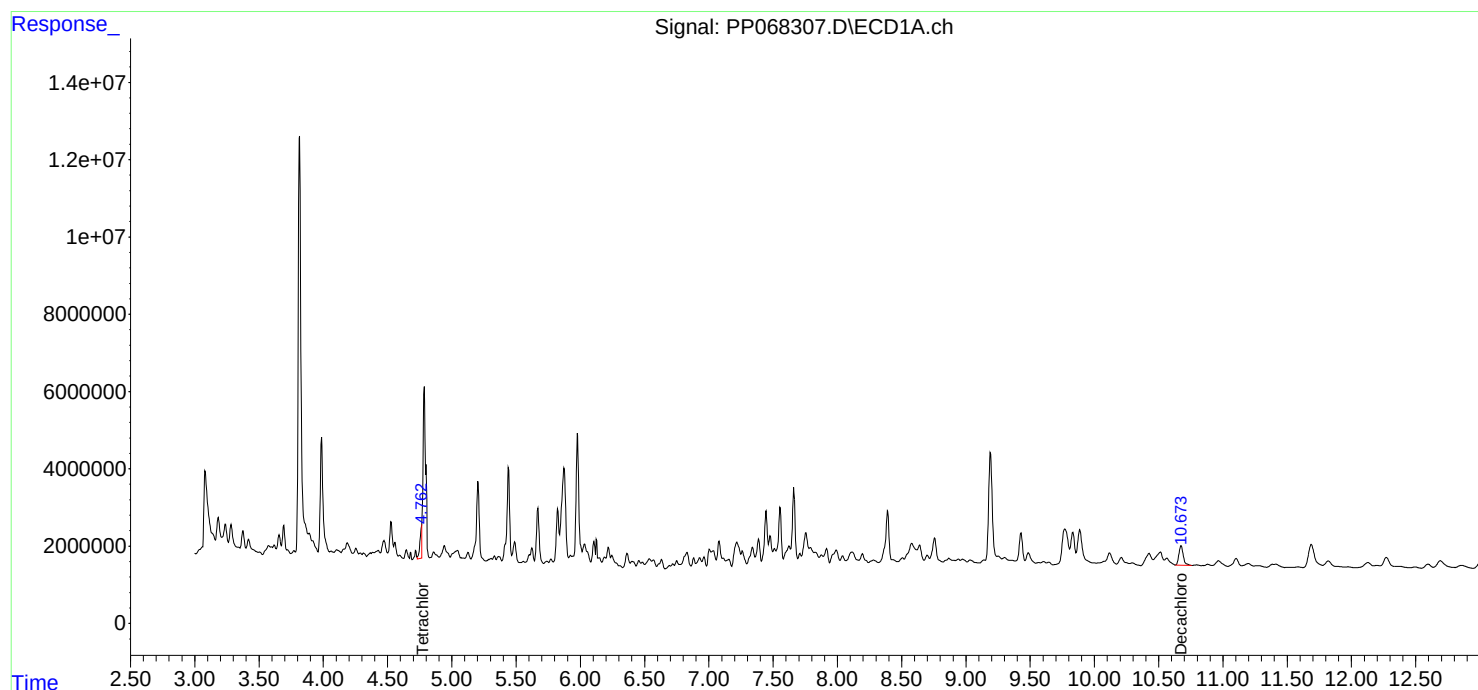

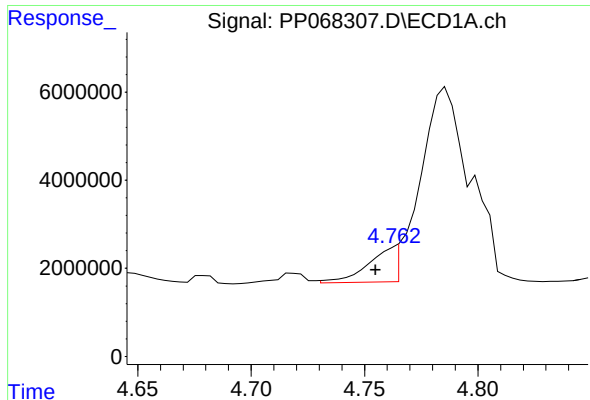


#1 Tetrachloro-m-xylene

R.T.: 4.762 min
Delta R.T.: 0.007 min
Response: 5755450
Conc: 6.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
100324


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/30/2024
Supervised By :Ankita Jodhani 10/30/2024

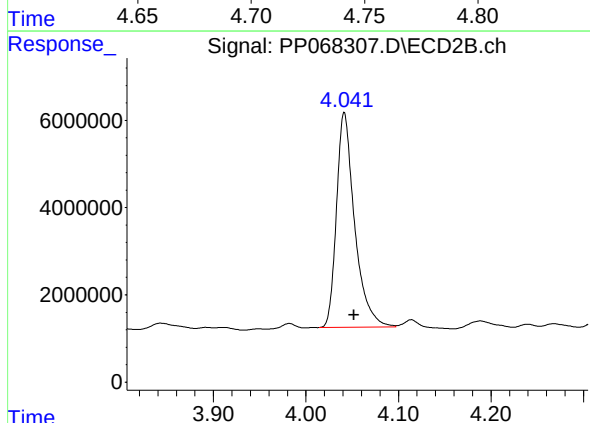


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.011 min
Response: 67070745
Conc: 66.38 ng/ml m

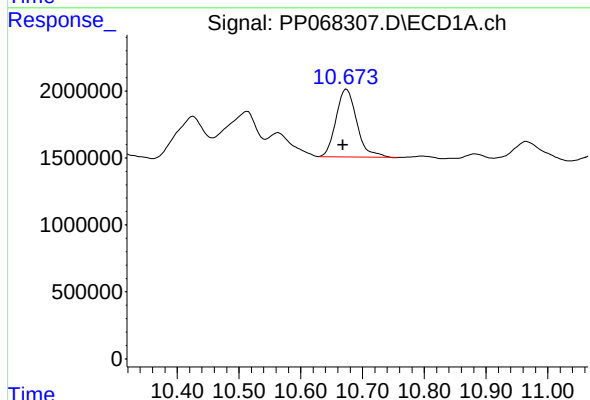

#2 Decachlorobiphenyl

R.T.: 10.673 min
Delta R.T.: 0.004 min
Response: 11871266
Conc: 10.31 ng/ml m

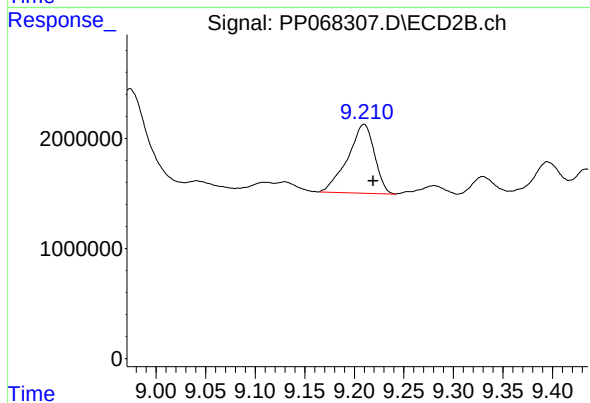

#2 Decachlorobiphenyl

R.T.: 9.210 min
Delta R.T.: -0.009 min
Response: 11739215
Conc: 10.47 ng/ml m