

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102925\
 Data File : PP076171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2025 17:09
 Operator : YP\AJ
 Sample : Q3472-03 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/30/2025
 Supervised By :Sohil Jodhani 10/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:27:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.641	3.776	2225677	4573063	1.557m	0.691m#
2) SA Decachlor...	10.411	8.779	1968357	9508256	1.828m	1.156 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102925\
Data File : PP076171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2025 17:09
Operator : YP\AJ
Sample : Q3472-03 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-7


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/30/2025
Supervised By :Sohil Jodhani 10/30/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:27:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

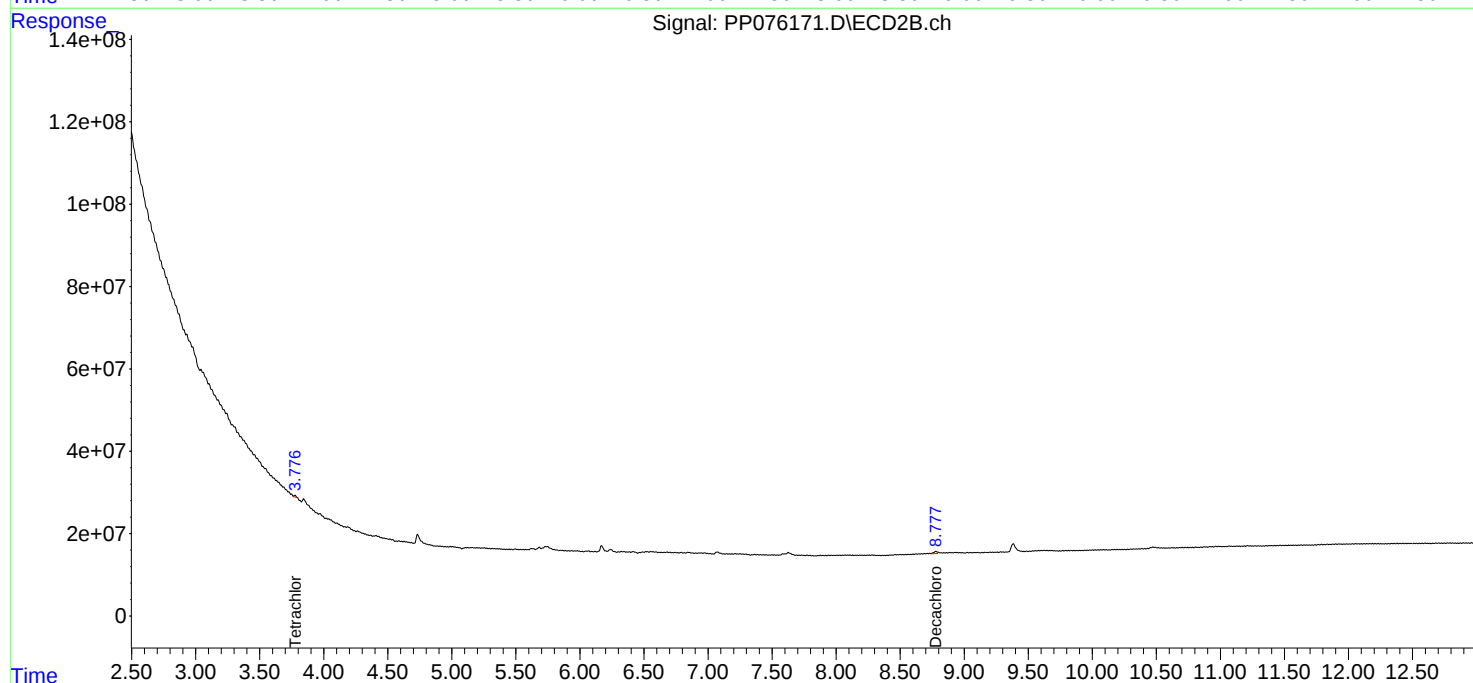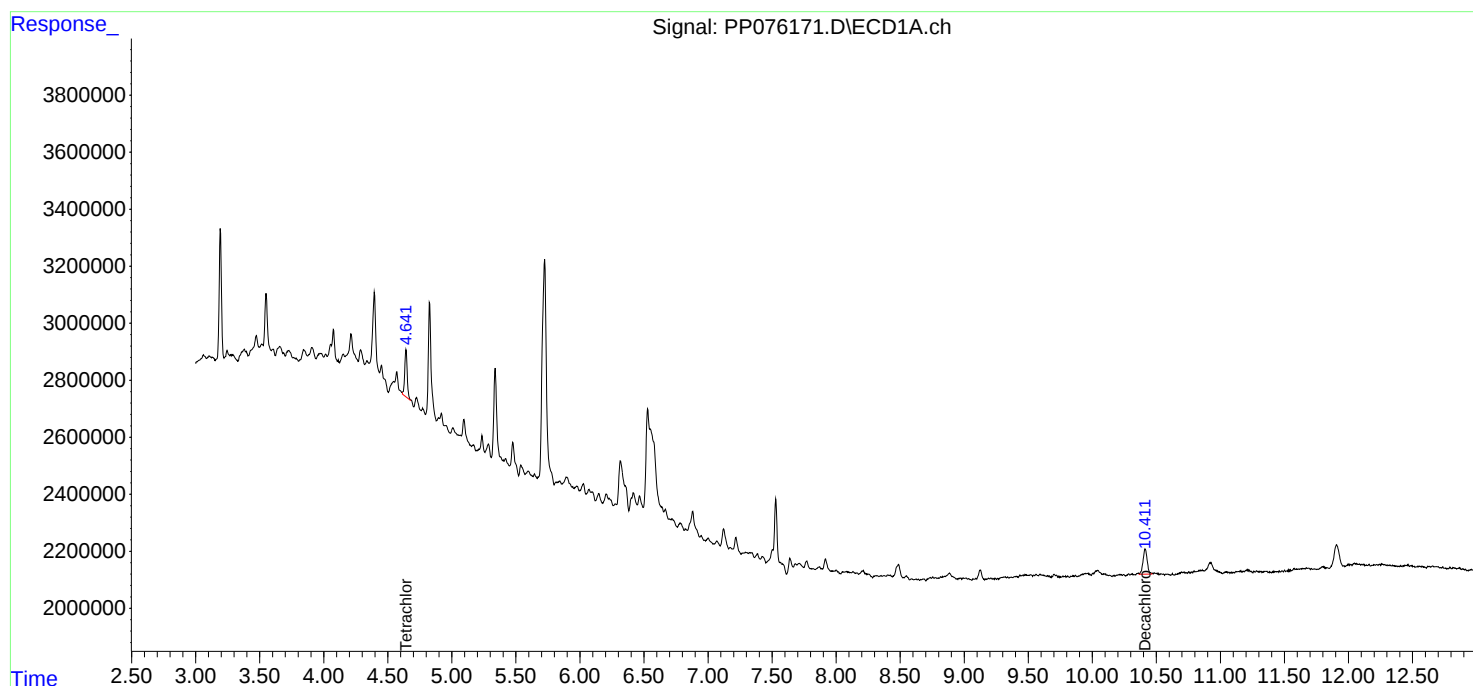

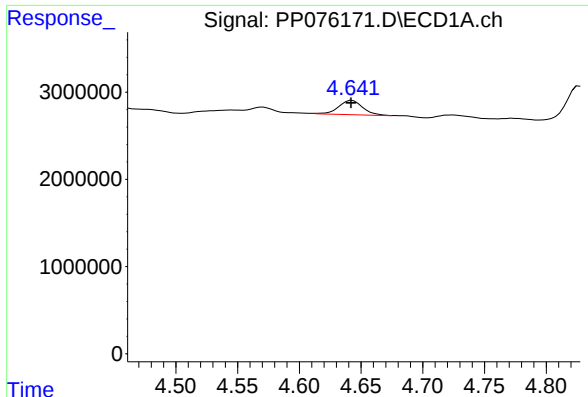


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 2225677
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-7


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/30/2025
Supervised By :Sohil Jodhani 10/30/2025

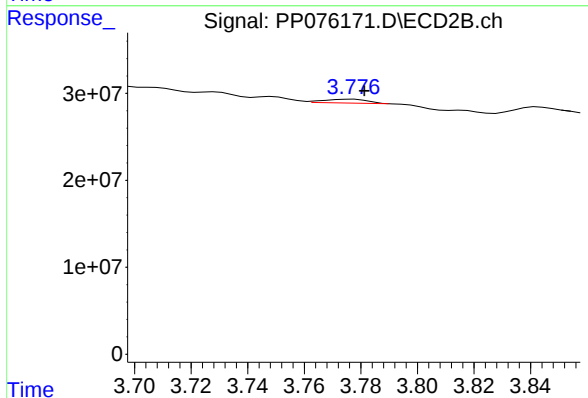


#1 Tetrachloro-m-xylene

R.T.: 3.776 min
Delta R.T.: -0.005 min
Response: 4573063
Conc: 0.69 ng/ml m

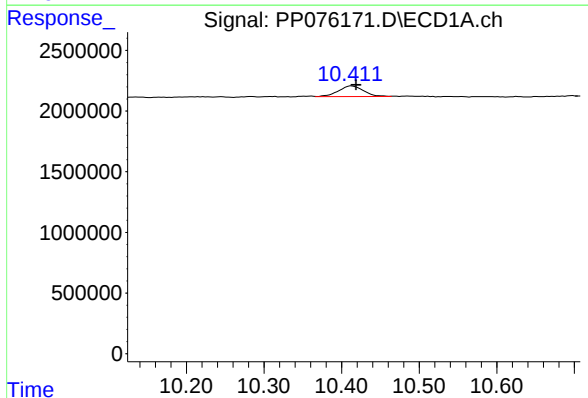

#2 Decachlorobiphenyl

R.T.: 10.411 min
Delta R.T.: -0.007 min
Response: 1968357
Conc: 1.83 ng/ml m

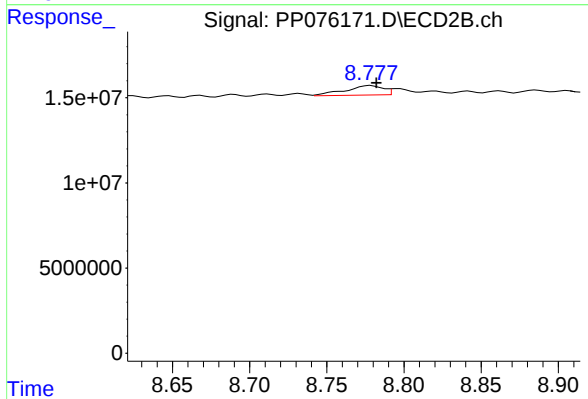

#2 Decachlorobiphenyl

R.T.: 8.779 min
Delta R.T.: -0.004 min
Response: 9508256
Conc: 1.16 ng/ml