

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103018\
 Data File : PP027911.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2018 13:49
 Operator : EI\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 03:50:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102418.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 24 12:31:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	0.000	12.625	0 57292769	N.D.	36.119 #
16) T	DCPA	0.000	18.235	0 17635365	N.D.	5.482 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103018\
Data File : PP027911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2018 13:49
Operator : EI\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 03:50:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102418.M
Quant Title : 8080.M
QLast Update : Wed Oct 24 12:31:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

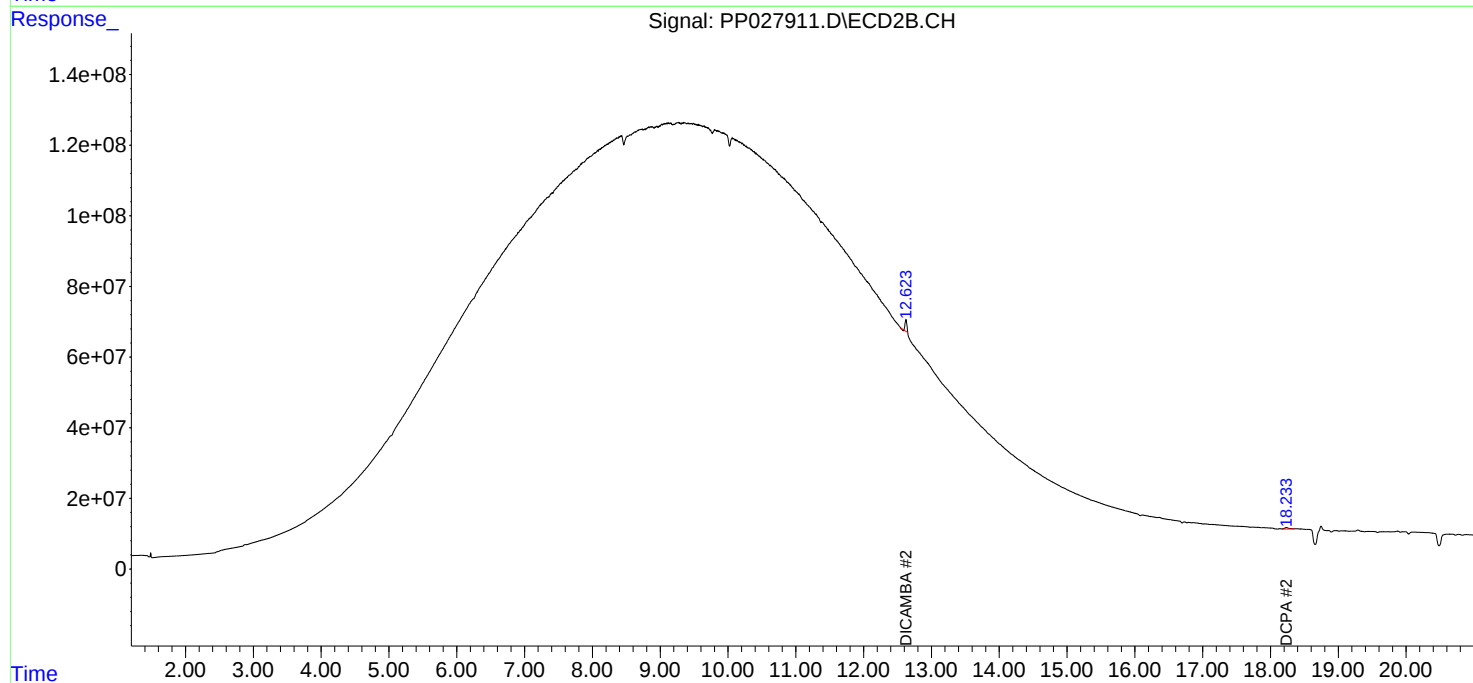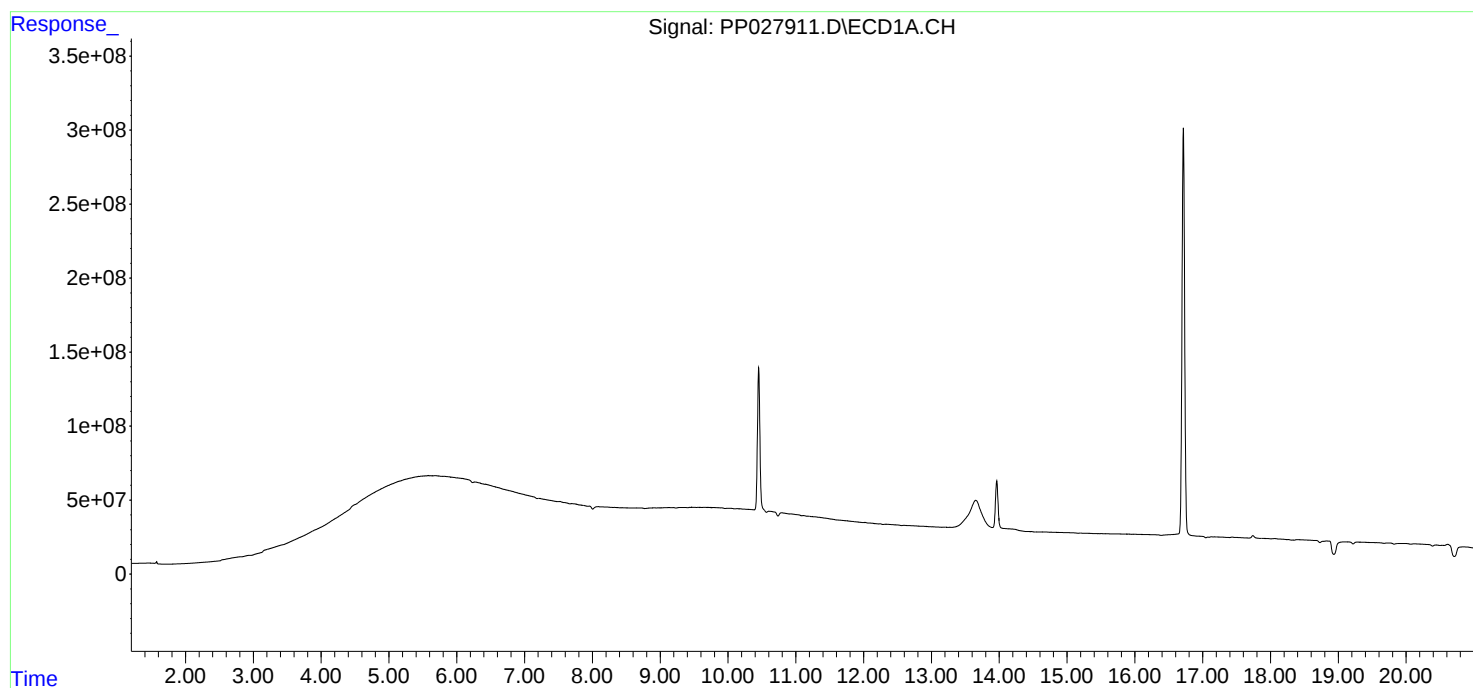


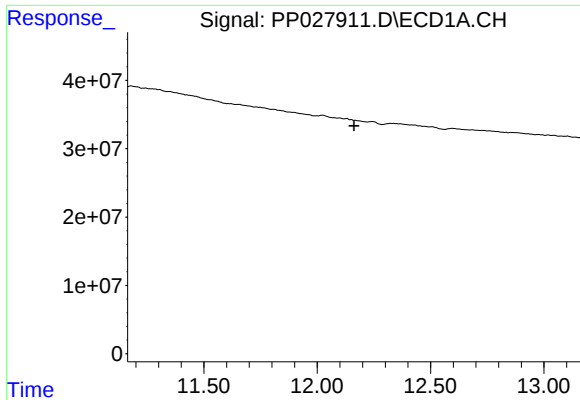

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

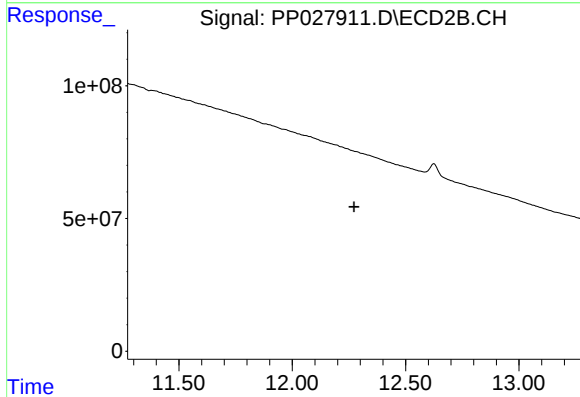


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 12.273 min
Response: 0
Conc: N.D.

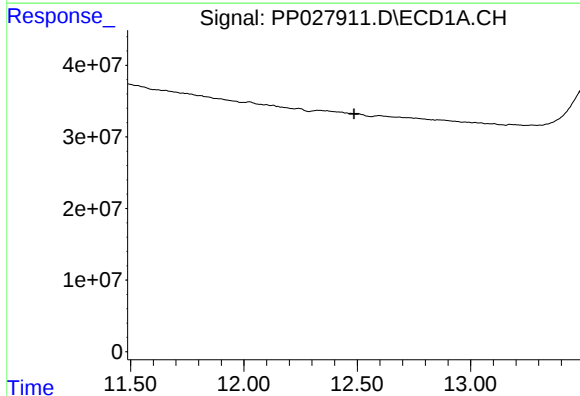


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.486 min
Response: 0
Conc: N.D.

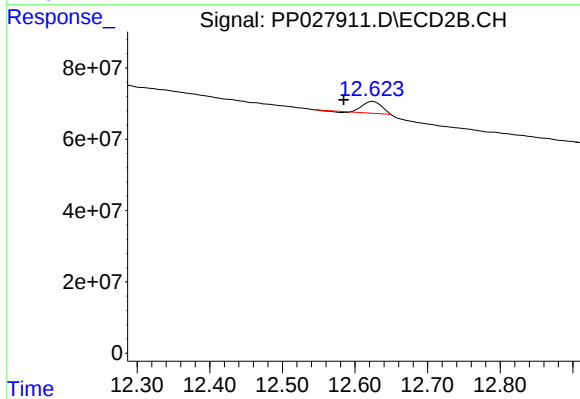

#5 DICAMBA


R.T.: 12.625 min
Delta R.T.: 0.040 min
Response: 57292769
Conc: 36.12 ng/ml

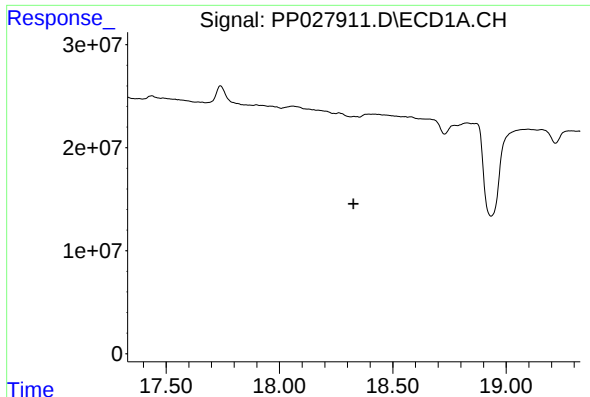

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

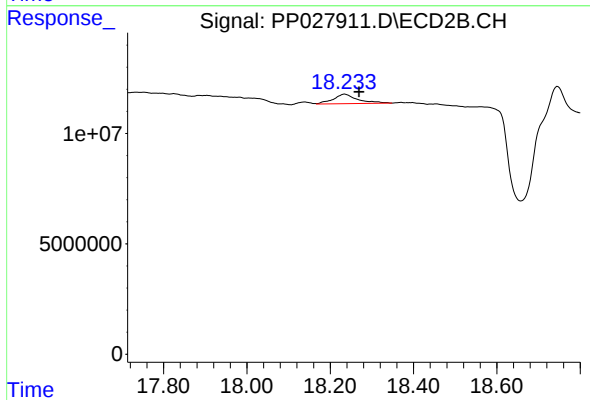

#16 DCPA

R.T.: 18.235 min
Delta R.T.: -0.035 min
Response: 17635365
Conc: 5.48 ng/ml