

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103020\
 Data File : PP030951.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2020 9:45
 Operator : DD\AJ
 Sample : MDL-PCB-BL-S-4
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-S-4

Manual Integrations
 APPROVED

Ankita
 10/30/2020 3:52:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 17:08:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1248PP102920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 28 16:58:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.803	4.080	1143178	1017015	19.175	18.856m
2) SA Decachlor...	10.691	9.415	674555	717141	19.832	19.684

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103020\
Data File : PP030951.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2020 9:45
Operator : DD\AJ
Sample : MDL-PCB-BL-S-4
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-4


Manual Integrations
APPROVED

Ankita
10/30/2020 3:52:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 17:08:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1248PP102920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 28 16:58:01 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

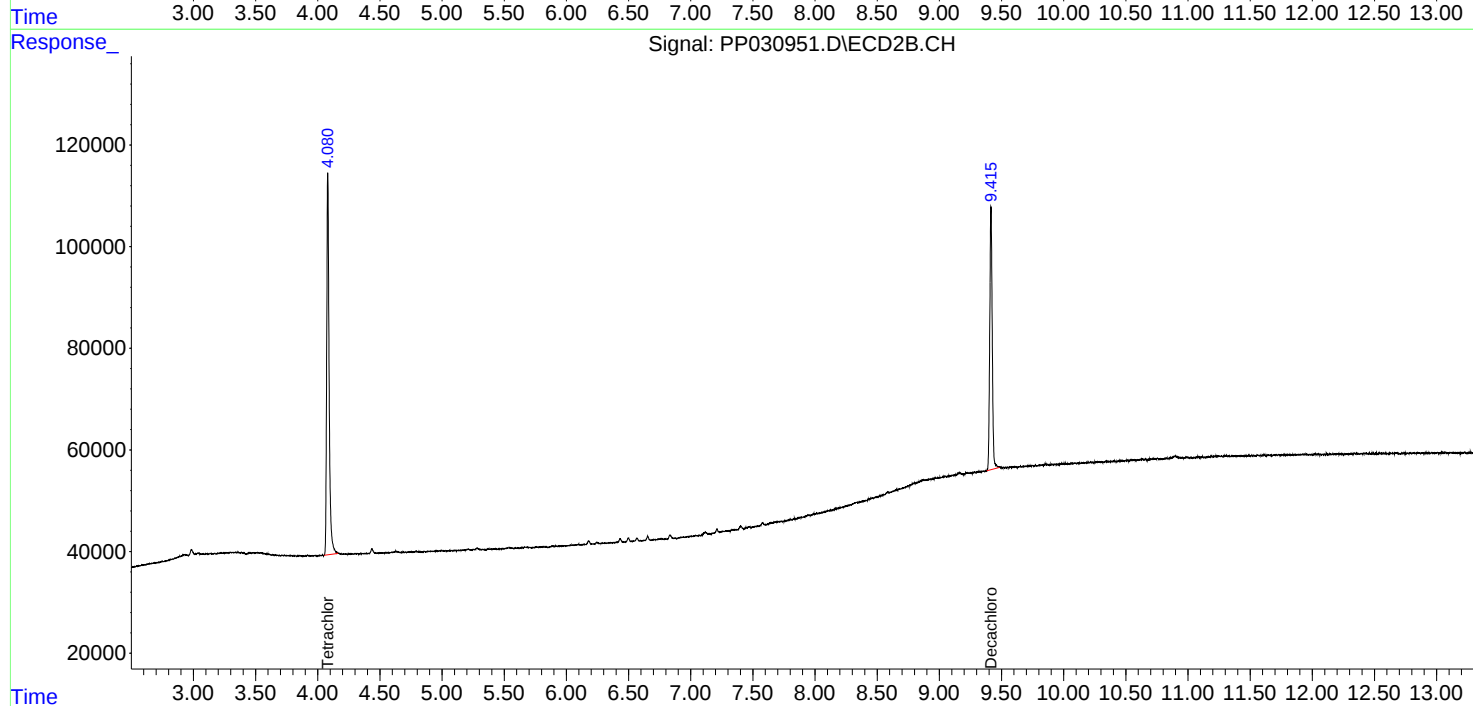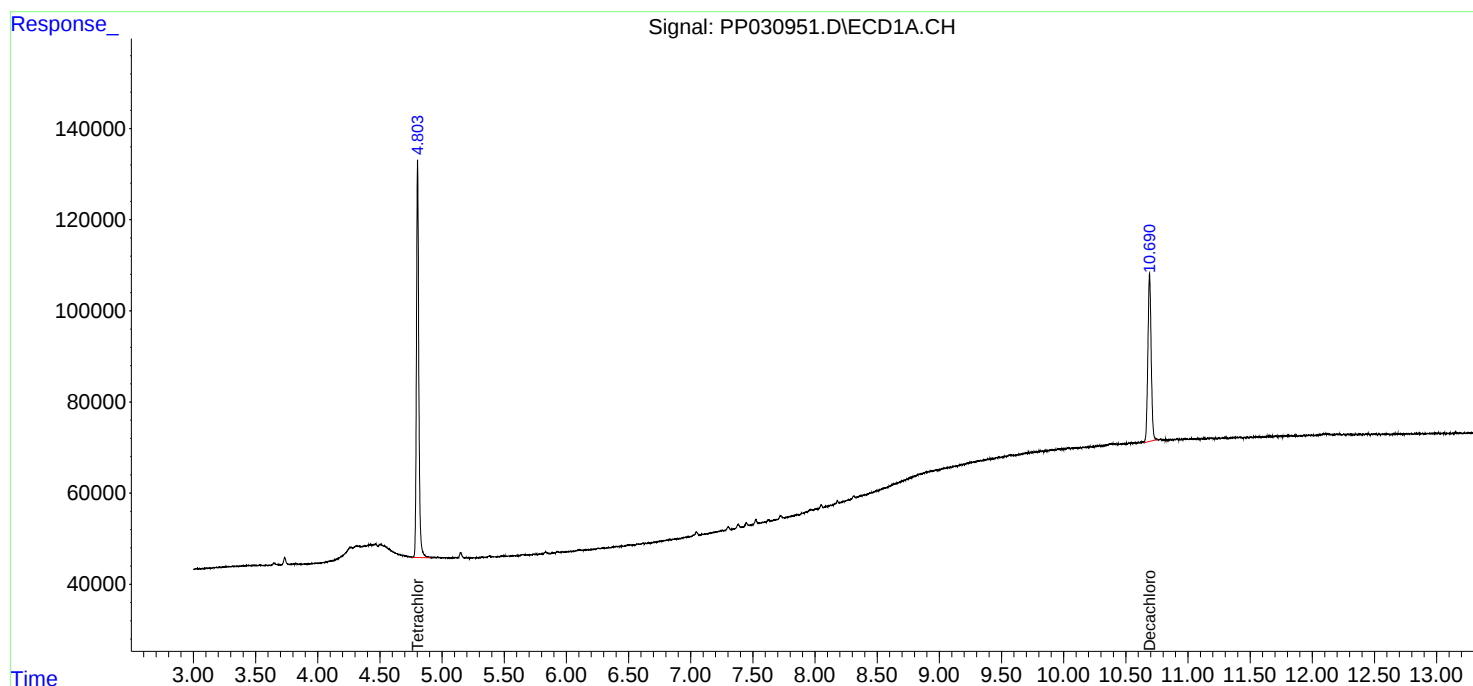

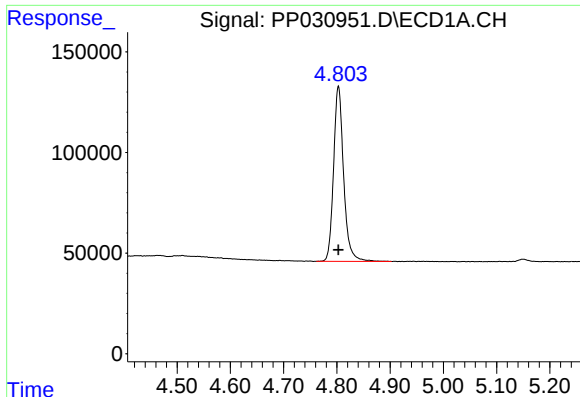


#1 Tetrachloro-m-xylene

R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 1143178
Conc: 19.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-4


Manual Integrations
APPROVED

Ankita
10/30/2020 3:52:27 PM

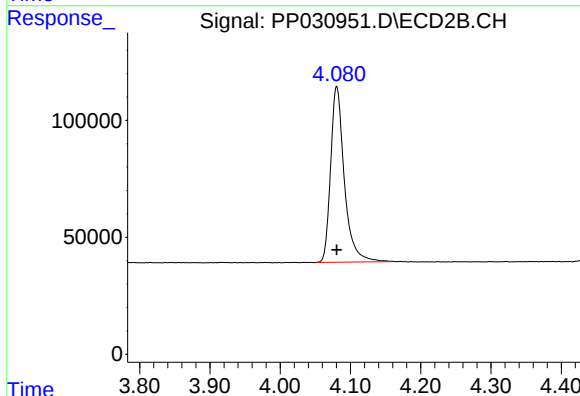


#1 Tetrachloro-m-xylene

R.T.: 4.080 min
Delta R.T.: 0.000 min
Response: 1017015
Conc: 18.86 ng/ml m

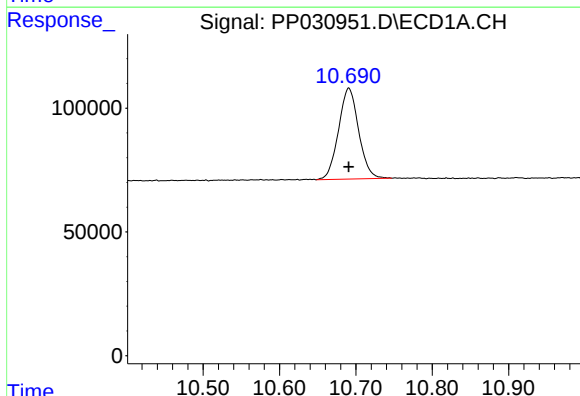

#2 Decachlorobiphenyl

R.T.: 10.691 min
Delta R.T.: 0.000 min
Response: 674555
Conc: 19.83 ng/ml

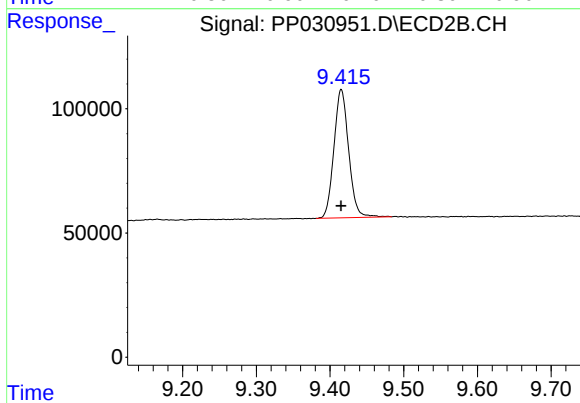

#2 Decachlorobiphenyl

R.T.: 9.415 min
Delta R.T.: 0.000 min
Response: 717141
Conc: 19.68 ng/ml