

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
 Data File : PL086382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2023 10:54
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 11:52:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 01 11:43:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.617	16153395	5840518	5.208	4.988
28)	SA Decachlor...	8.853	7.769	14611104	6614721	5.701	5.748
Target Compounds							
23)	Chlordane-1	4.510	3.607	7180523	1823844	51.892	52.164
24)	Chlordane-2	5.042	4.184	8706923	2571930	57.241	55.761
25)	Chlordane-3	5.754	4.813	28403527	5547308	49.281	46.376
26)	Chlordane-4	5.837	4.876	36157795	6757258	50.640	50.569
27)	Chlordane-5	6.683	5.545	6061400	1732285	53.760	49.834


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
Data File : PL086382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2023 10:54
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 11:52:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
Quant Title : GC Extractables
QLast Update : Wed Nov 01 11:43:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

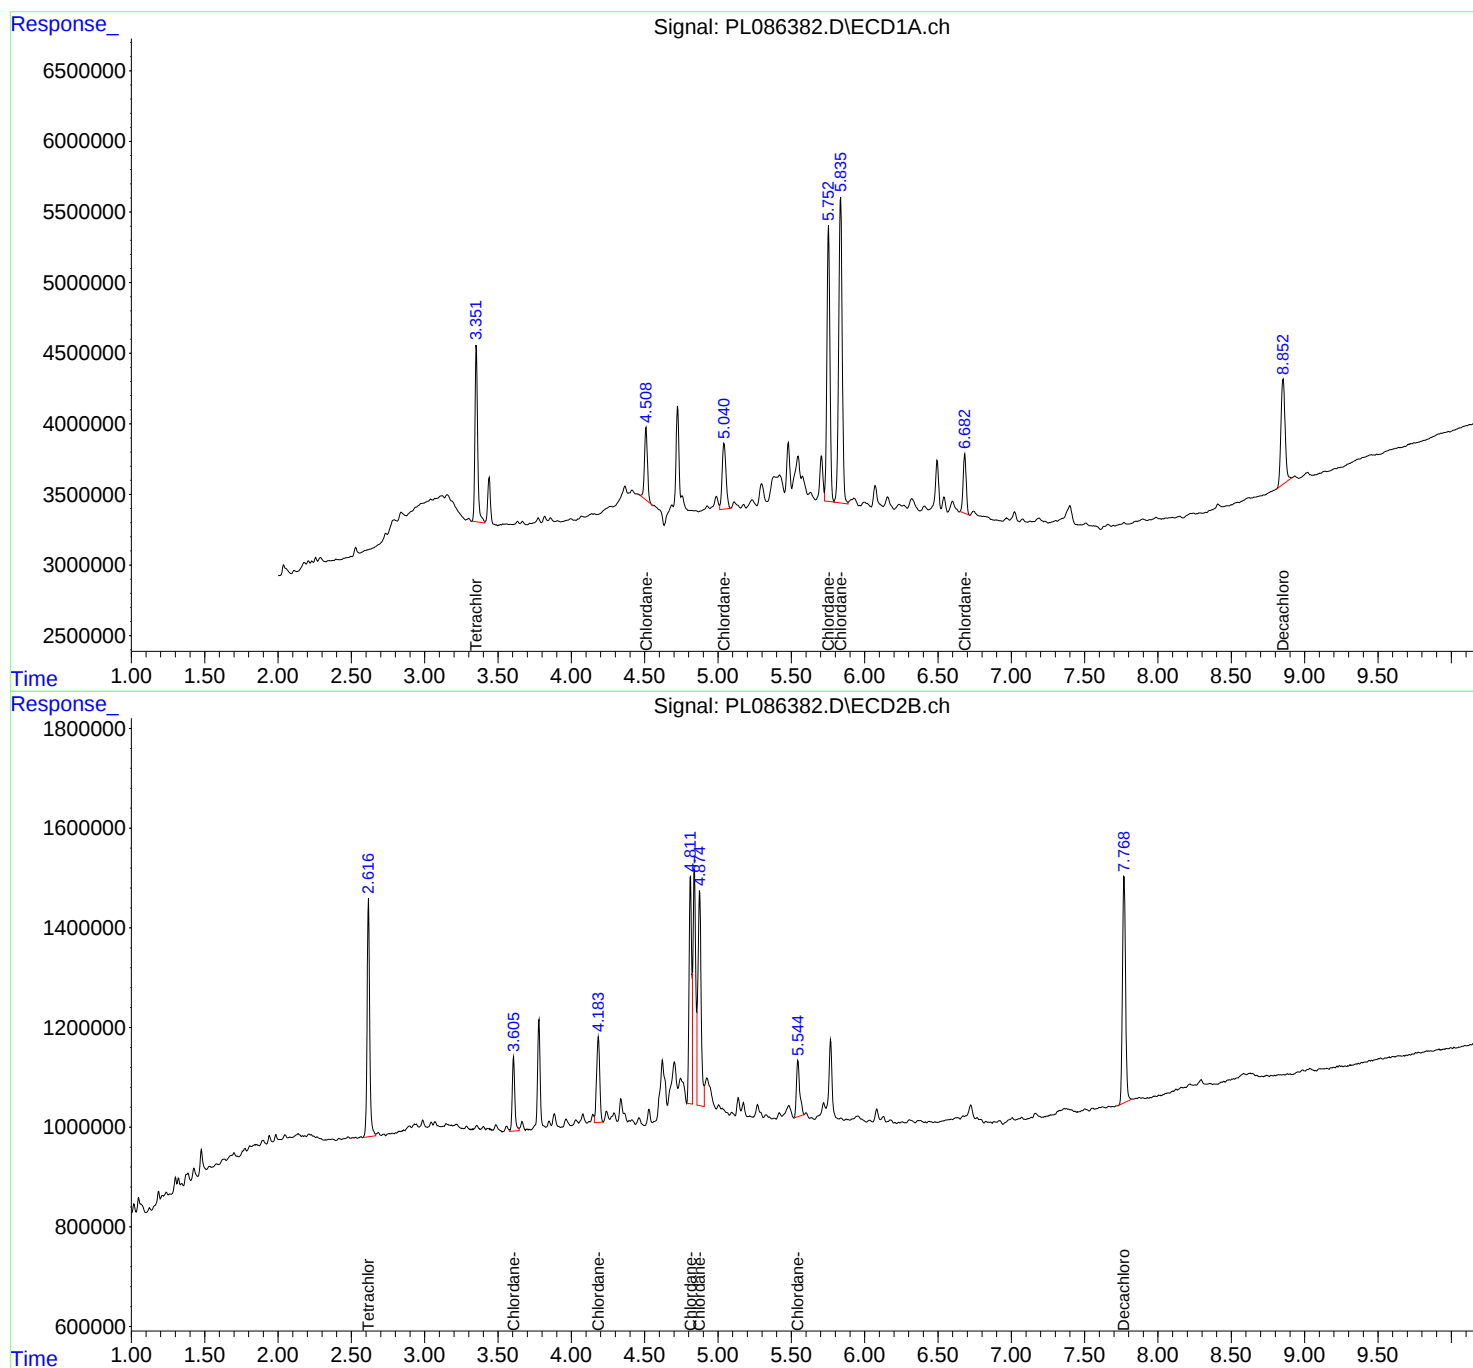


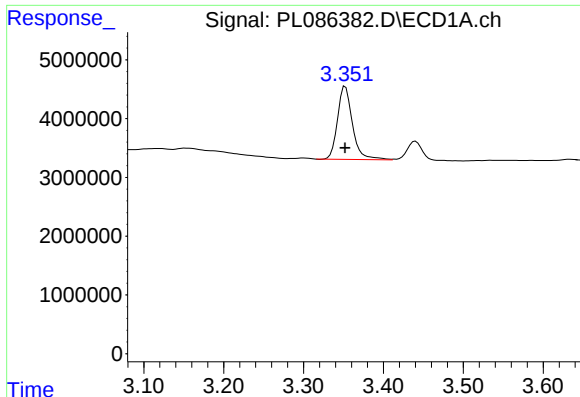

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 16153395
Conc: 5.21 ng/ml

Instrument :
ECD_P
ClientSampleId :

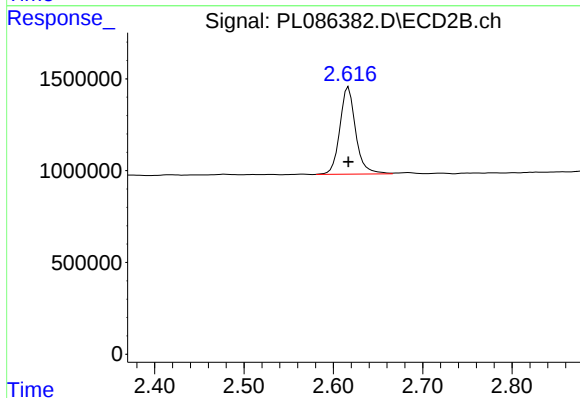


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 5840518
Conc: 4.99 ng/ml

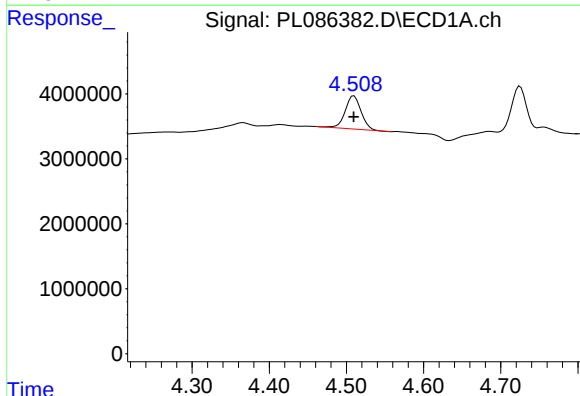


#23 Chlordane-1

R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 7180523
Conc: 51.89 ng/ml

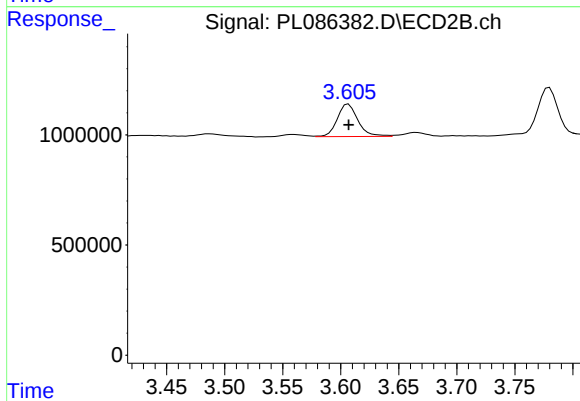

#23 Chlordane-1


R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 1823844
Conc: 52.16 ng/ml

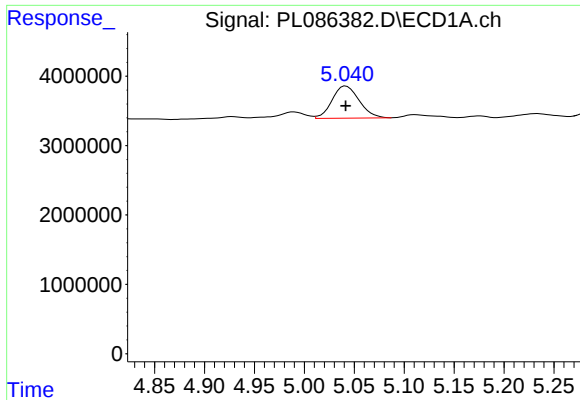

#24 Chlordane-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 8706923
Conc: 57.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

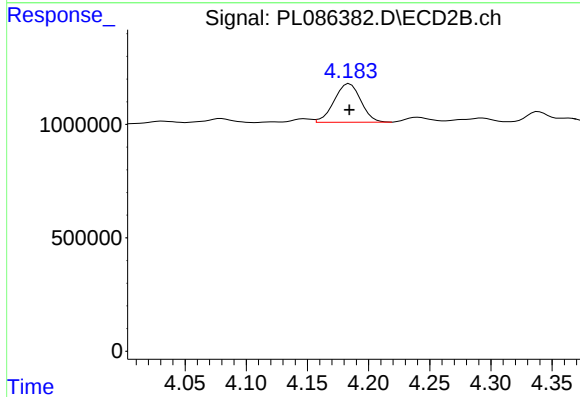


#24 Chlordane-2

R.T.: 4.184 min
Delta R.T.: 0.000 min
Response: 2571930
Conc: 55.76 ng/ml

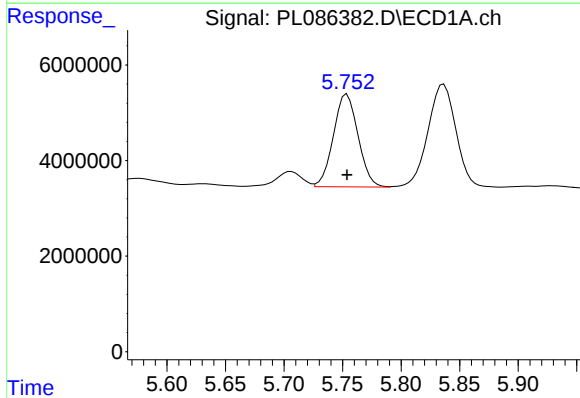


#25 Chlordane-3

R.T.: 5.754 min
Delta R.T.: 0.000 min
Response: 28403527
Conc: 49.28 ng/ml

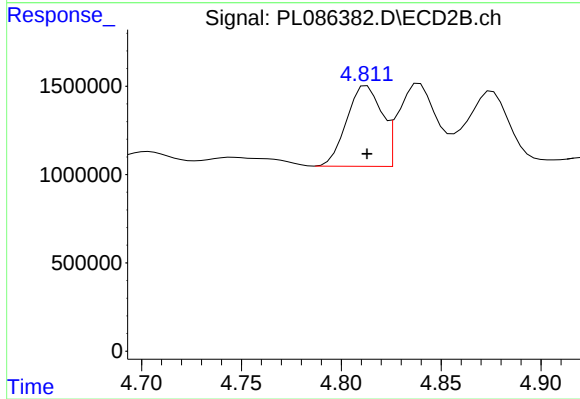

#25 Chlordane-3


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 5547308
Conc: 46.38 ng/ml

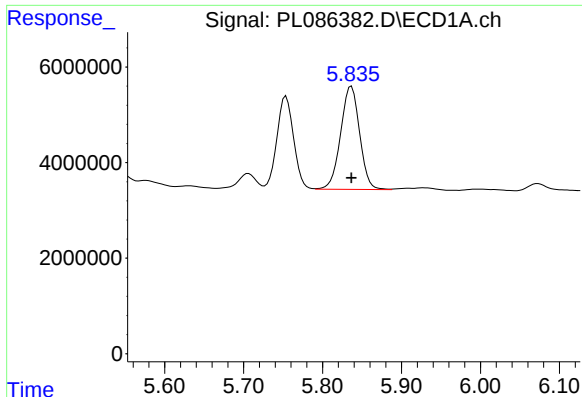

#26 Chlordane-4


R.T.: 5.837 min
Delta R.T.: 0.000 min
Response: 36157795
Conc: 50.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

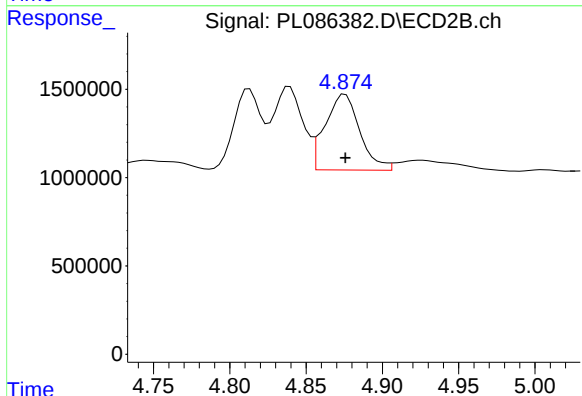


#26 Chlordane-4

R.T.: 4.876 min
Delta R.T.: 0.000 min
Response: 6757258
Conc: 50.57 ng/ml

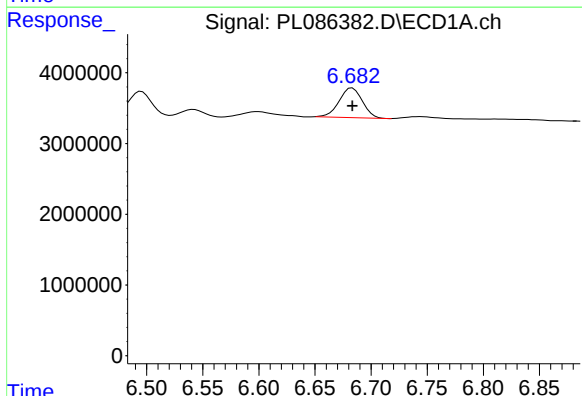


#27 Chlordane-5

R.T.: 6.683 min
Delta R.T.: 0.000 min
Response: 6061400
Conc: 53.76 ng/ml

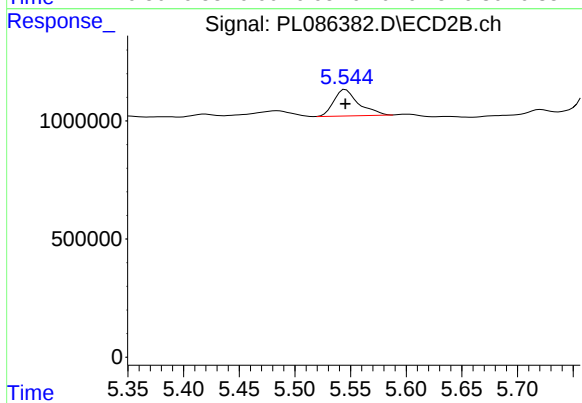

#27 Chlordane-5


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 1732285
Conc: 49.83 ng/ml

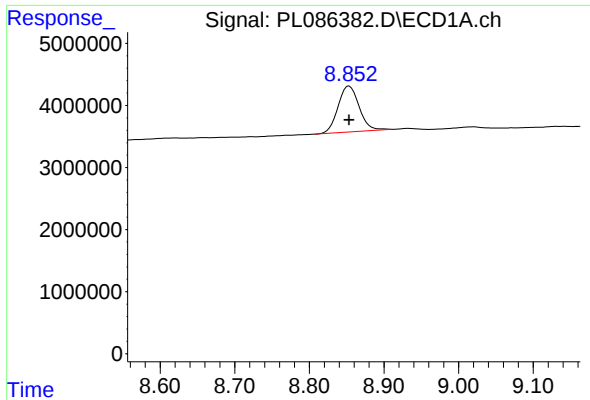

#28 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: 0.000 min
Response: 14611104
Conc: 5.70 ng/ml

Instrument :
ECD_P
ClientSampleId :

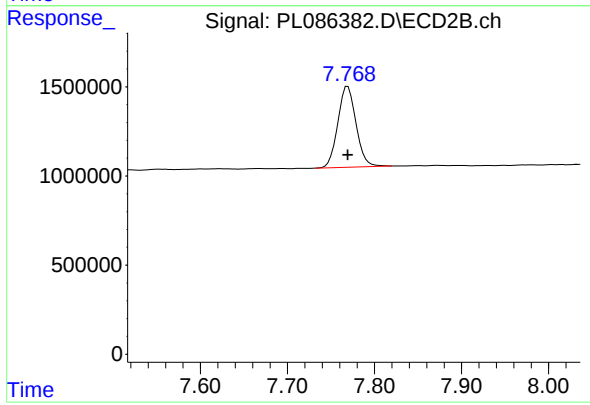

#28 Decachlorobiphenyl

R.T.: 7.769 min
Delta R.T.: 0.000 min
Response: 6614721
Conc: 5.75 ng/ml