

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103023\
 Data File : PP061327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 12:21
 Operator : YP\AJ
 Sample : 05144-04 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH4000-END-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 13:23:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 27 18:44:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	3.690	4428041	3367186	1.793	2.253 #
2)	SA Decachlor...	10.533	8.761	4585520	2776155	2.432	1.808 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103023\
Data File : PP061327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 12:21
Operator : YP\AJ
Sample : 05144-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KMH4000-END-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 13:23:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 27 18:44:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

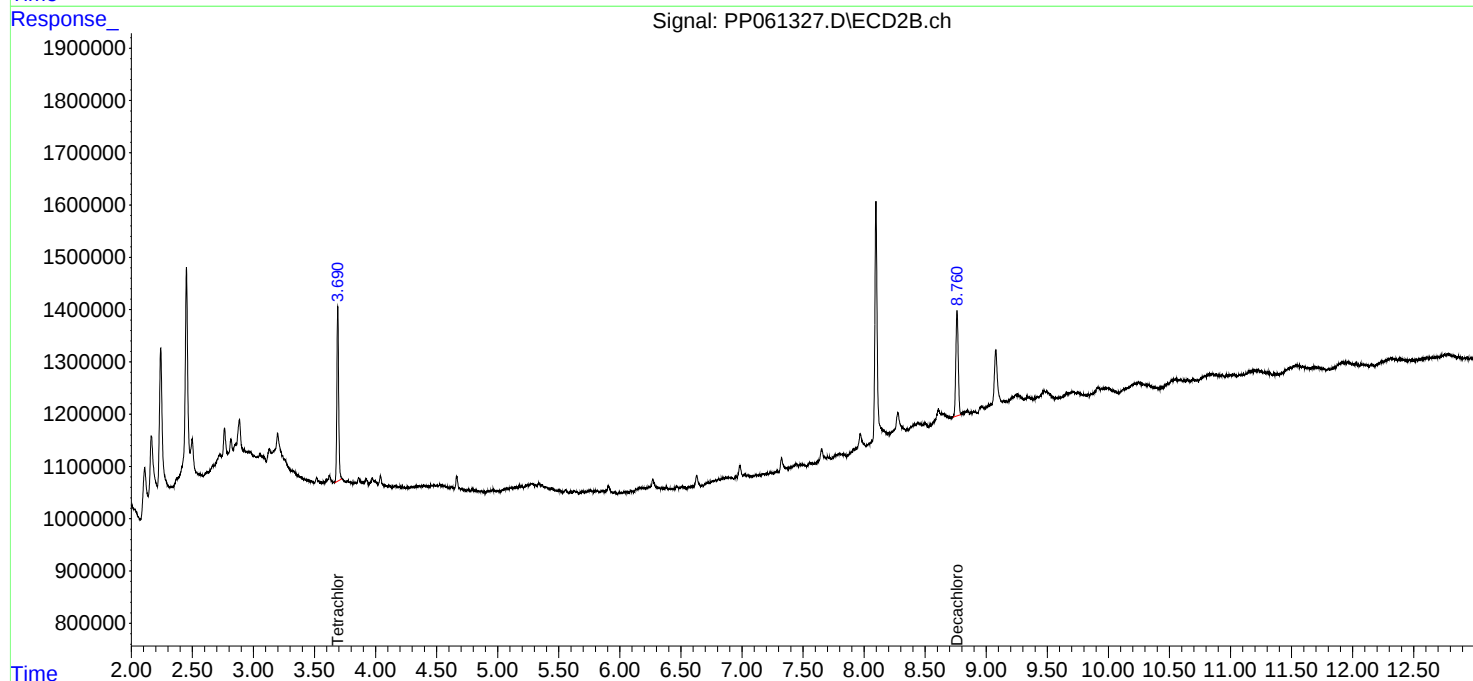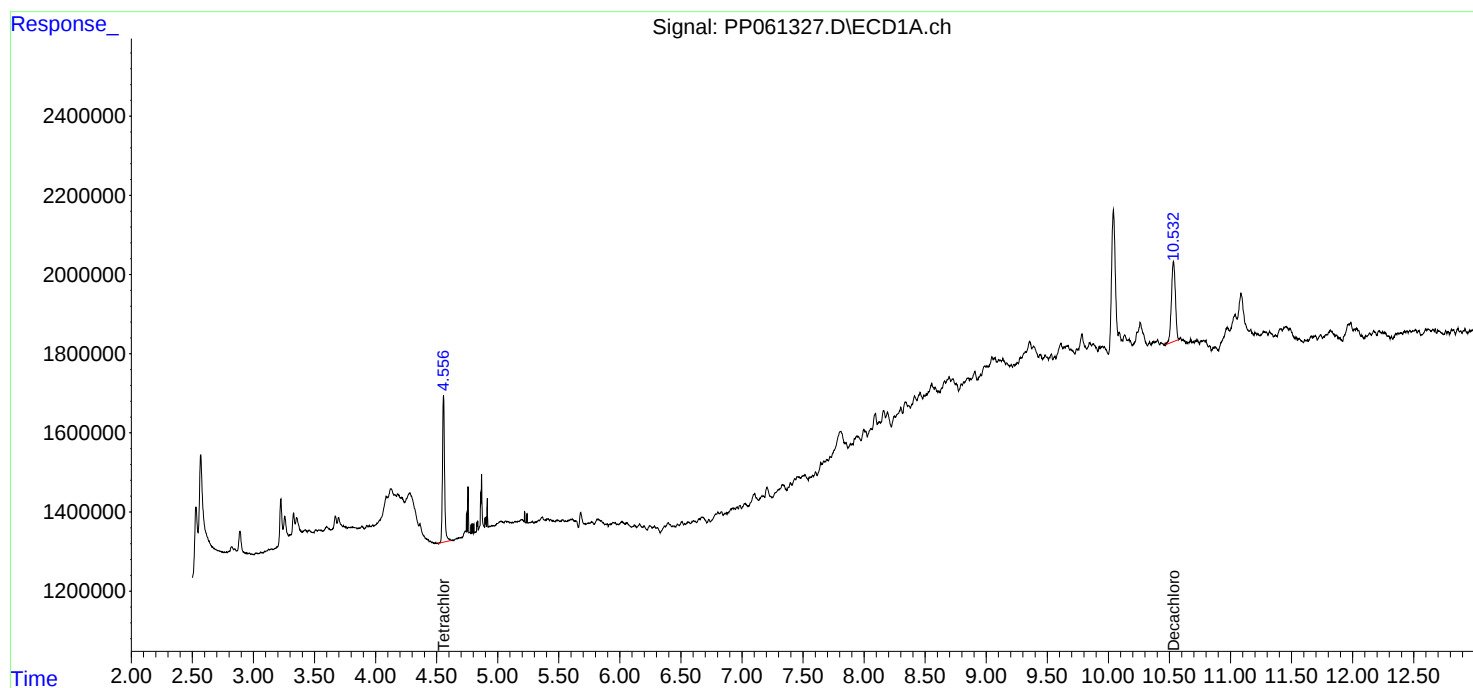


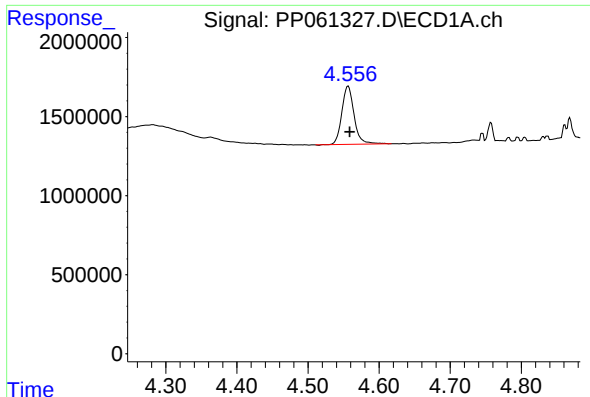

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.003 min
Response: 4428041
Conc: 1.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
KMH4000-END-1-2

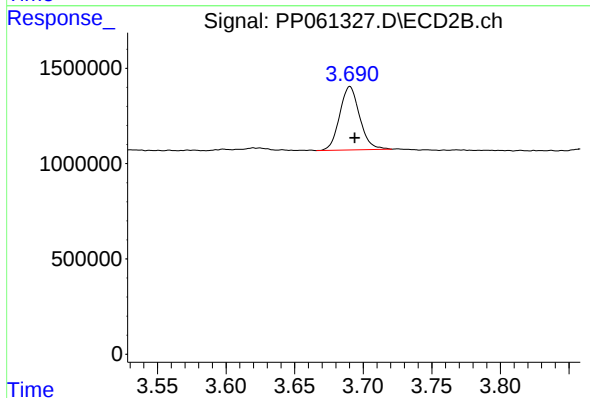


#1 Tetrachloro-m-xylene

R.T.: 3.690 min
Delta R.T.: -0.003 min
Response: 3367186
Conc: 2.25 ng/ml

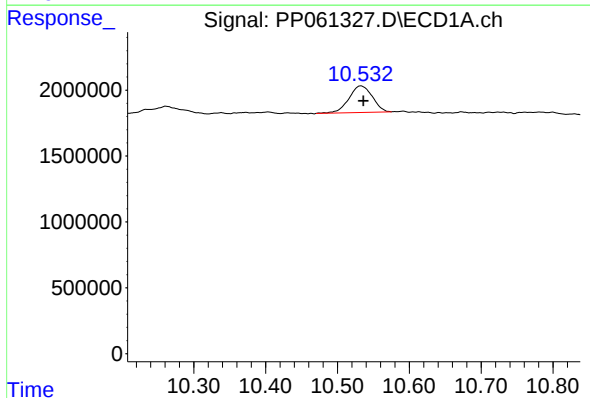

#2 Decachlorobiphenyl

R.T.: 10.533 min
Delta R.T.: -0.003 min
Response: 4585520
Conc: 2.43 ng/ml

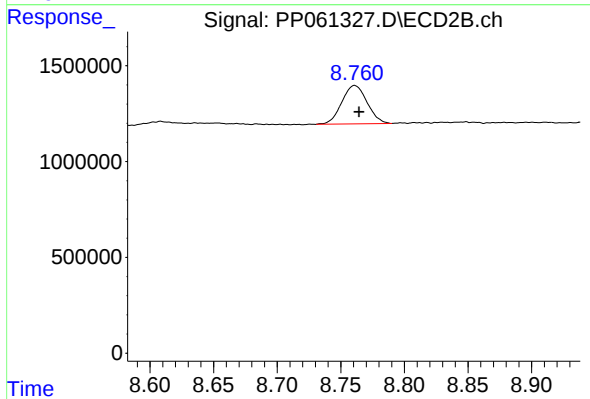

#2 Decachlorobiphenyl

R.T.: 8.761 min
Delta R.T.: -0.003 min
Response: 2776155
Conc: 1.81 ng/ml