

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103023\
 Data File : PP061361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 23:12
 Operator : YP\AJ
 Sample : 05134-03 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 60195

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 03:05:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 27 18:44:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.560	3.694	5168432	4282928	2.092m	2.866 #
2) SA Decachlor...	10.550	8.778	4949636	3496251	2.625m	2.277

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103023\
Data File : PP061361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 23:12
Operator : YP\AJ
Sample : 05134-03 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
60195


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/02/2023
Supervised By :mohammad ahmed 11/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 03:05:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 27 18:44:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

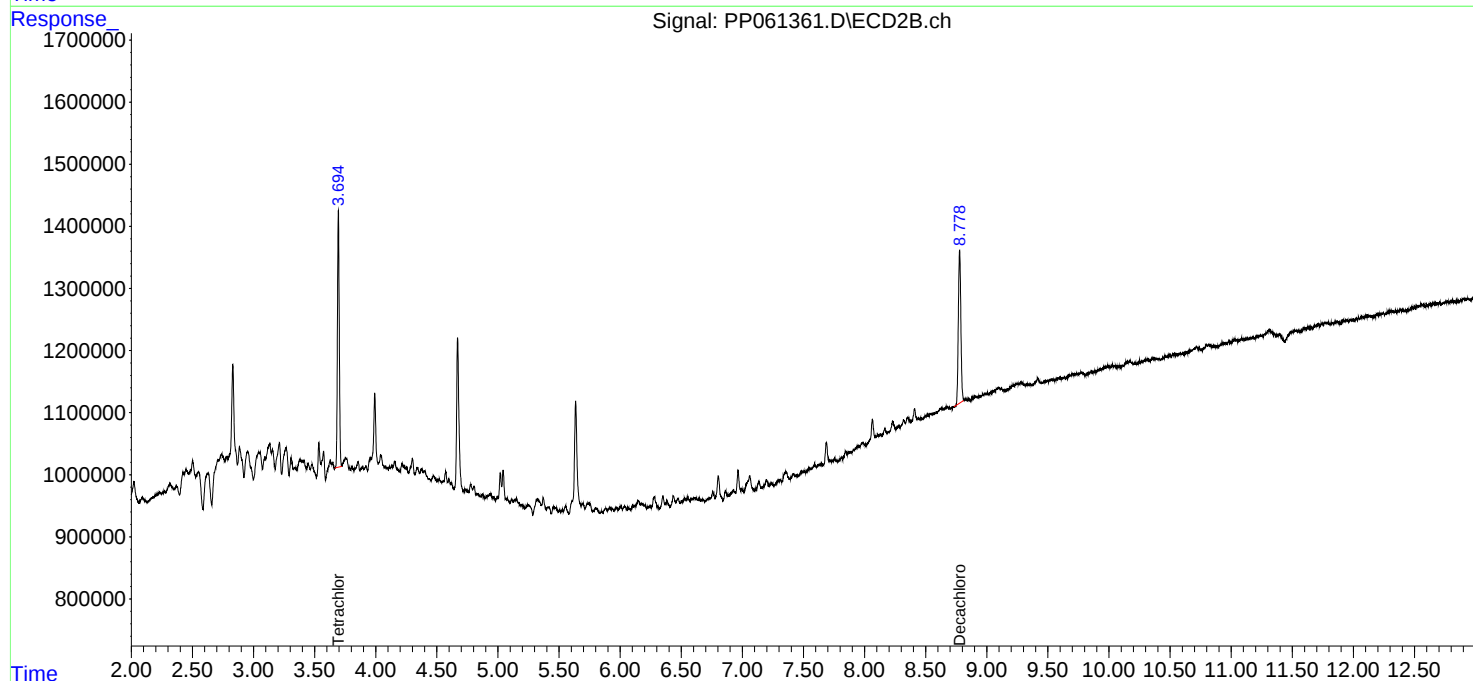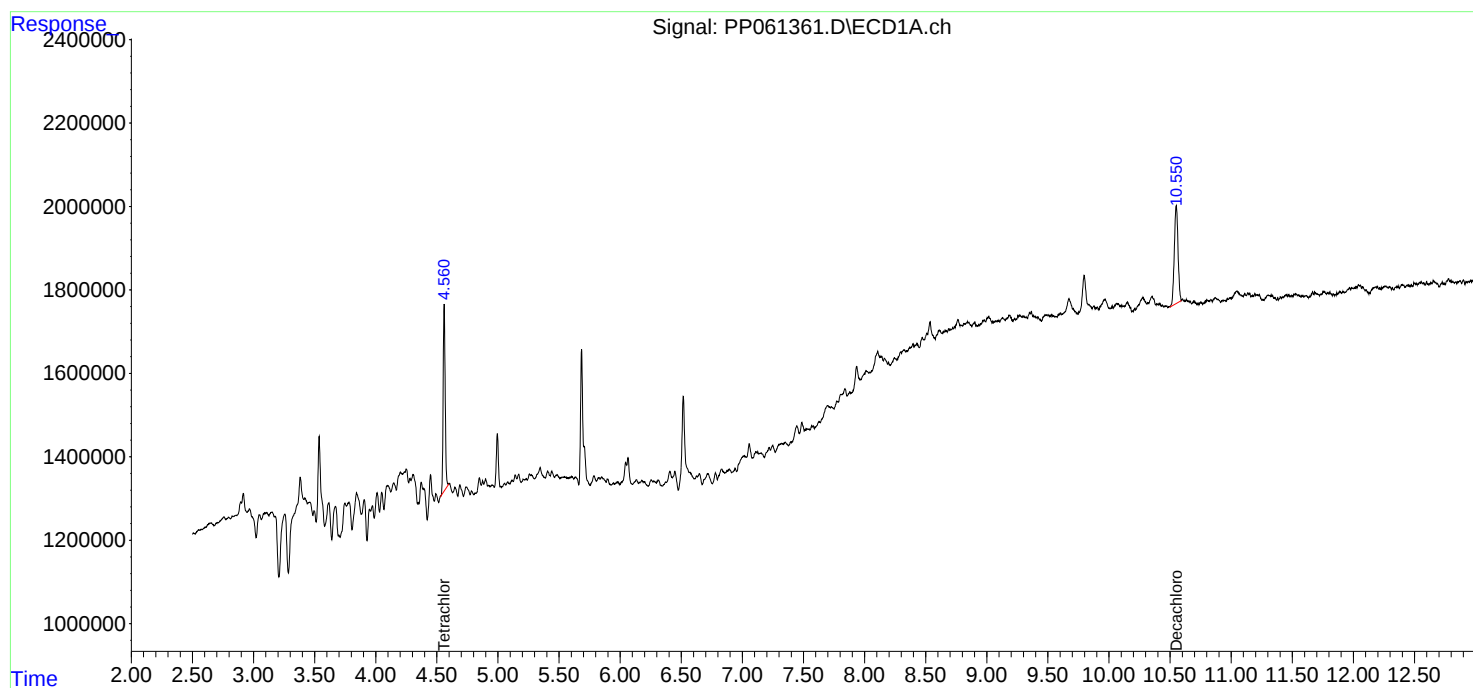

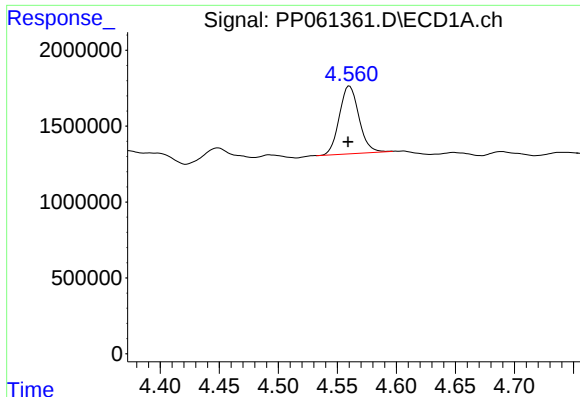


#1 Tetrachloro-m-xylene

R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 5168432
Conc: 2.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
60195


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/02/2023
Supervised By :mohammad ahmed 11/02/2023

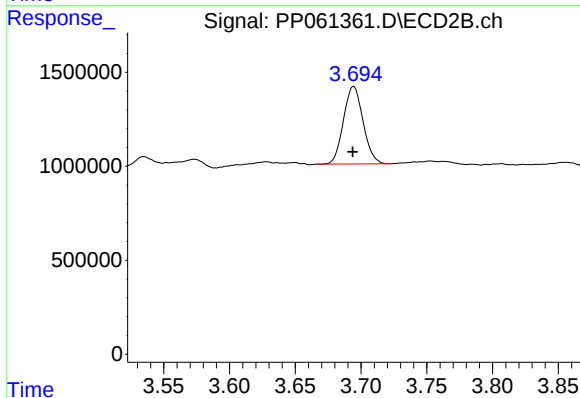


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: 0.000 min
Response: 4282928
Conc: 2.87 ng/ml

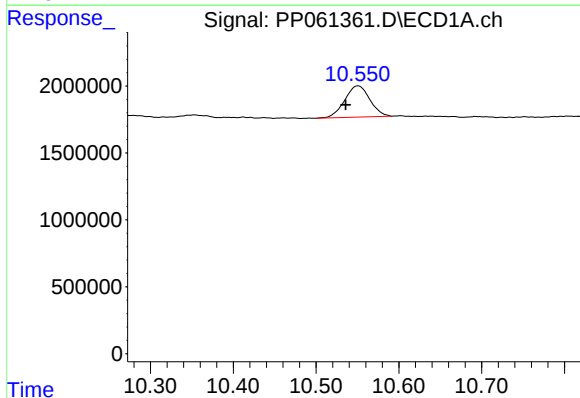

#2 Decachlorobiphenyl

R.T.: 10.550 min
Delta R.T.: 0.014 min
Response: 4949636
Conc: 2.62 ng/ml m

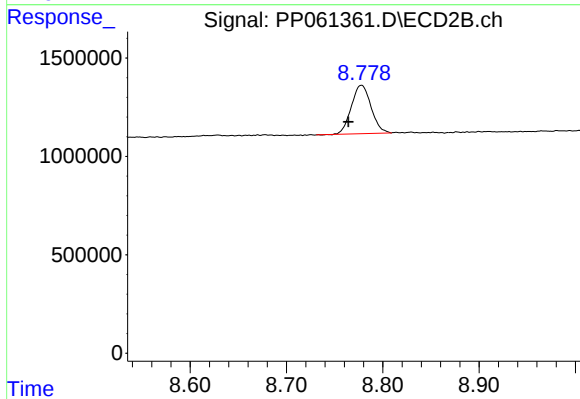

#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: 0.014 min
Response: 3496251
Conc: 2.28 ng/ml