

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103023\
 Data File : PP061386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 07:46
 Operator : YP\AJ
 Sample : PB156751BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB156751BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/31/2023
 Supervised By :mohammad ahmed 10/31/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 09:33:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 27 18:44:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.565	3.699	50061414	32484506	20.266	21.736
2) SA Decachlor...	10.549	8.773	39351491	31135509	20.868m	20.275

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103023\
Data File : PP061386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2023 07:46
Operator : YP\AJ
Sample : PB156751BL
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB156751BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/31/2023
Supervised By :mohammad ahmed 10/31/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 09:33:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 27 18:44:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

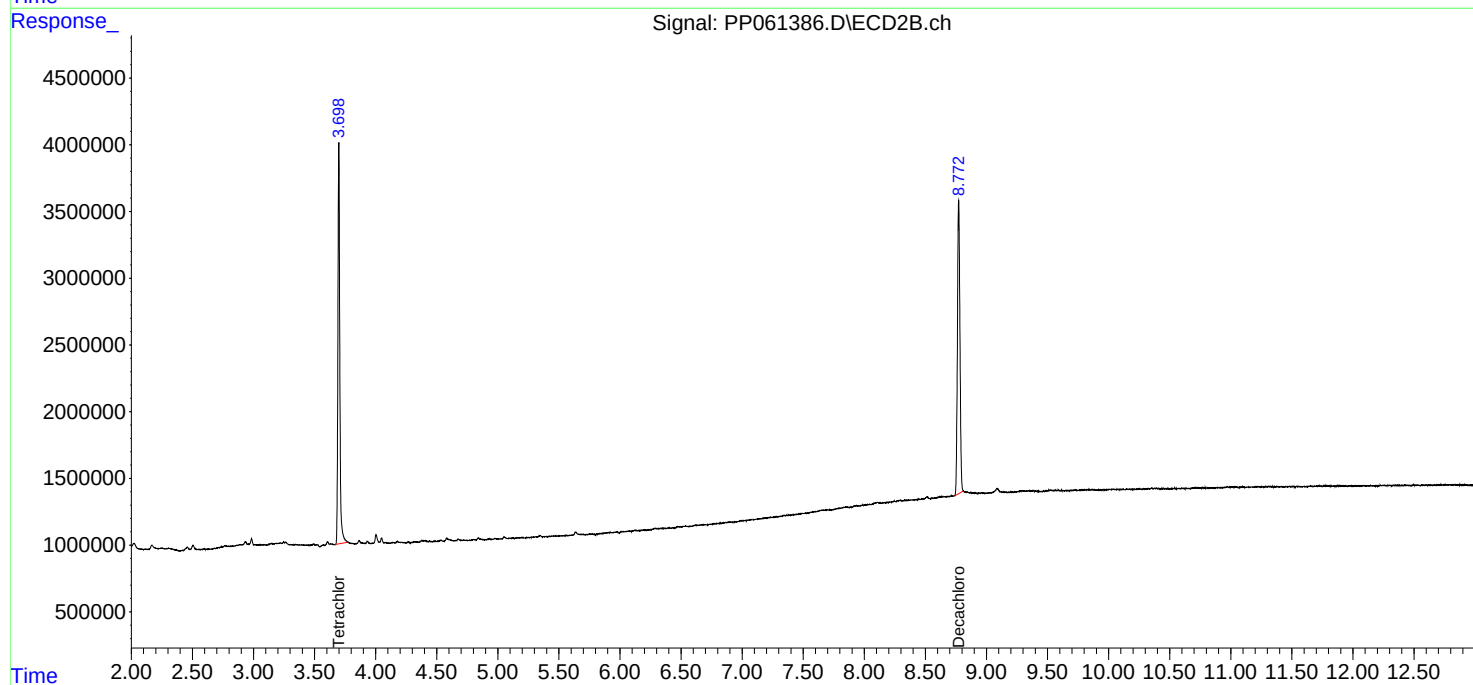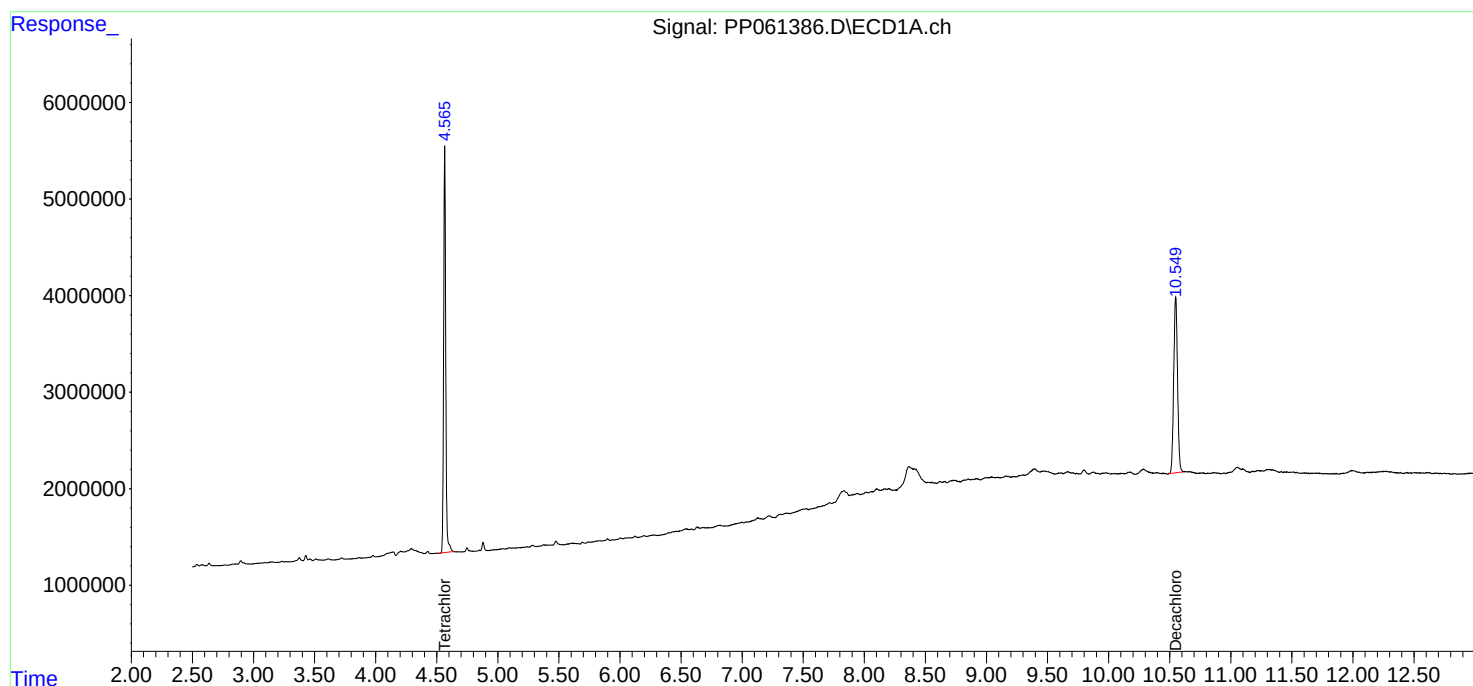

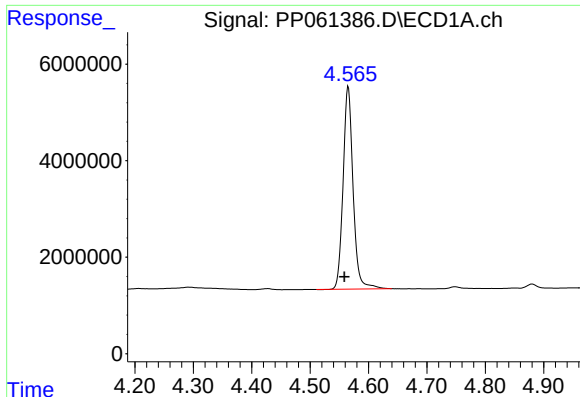


#1 Tetrachloro-m-xylene

R.T.: 4.565 min
Delta R.T.: 0.006 min
Response: 50061414
Conc: 20.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB156751BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/31/2023
Supervised By :mohammad ahmed 10/31/2023

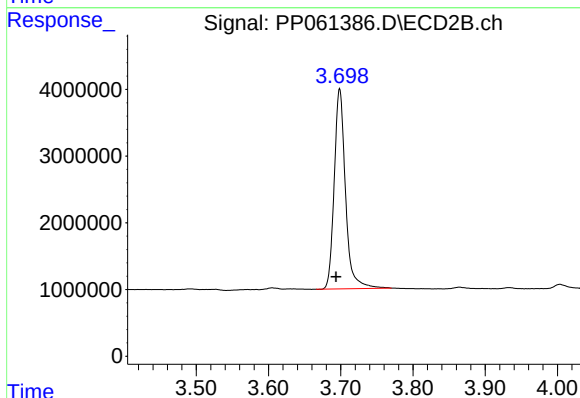


#1 Tetrachloro-m-xylene

R.T.: 3.699 min
Delta R.T.: 0.005 min
Response: 32484506
Conc: 21.74 ng/ml

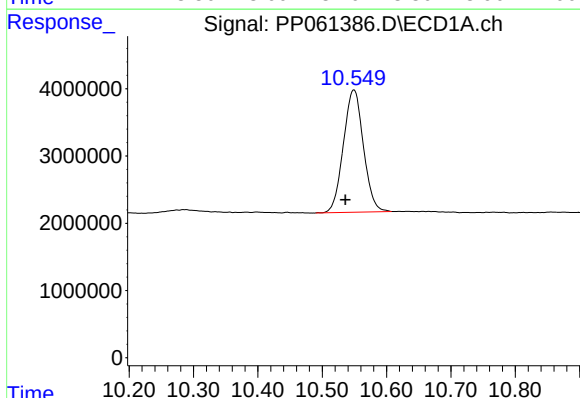

#2 Decachlorobiphenyl

R.T.: 10.549 min
Delta R.T.: 0.013 min
Response: 39351491
Conc: 20.87 ng/ml m

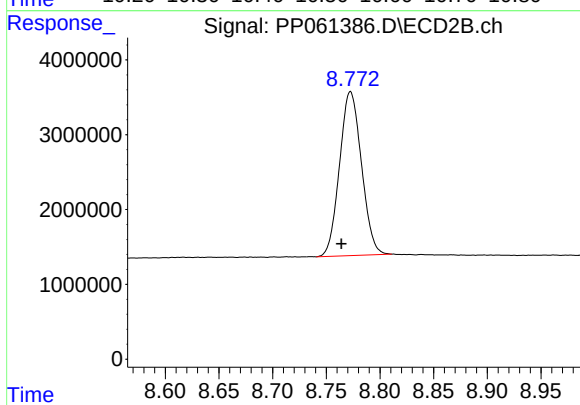

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.008 min
Response: 31135509
Conc: 20.27 ng/ml