

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103025\
 Data File : PP076193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2025 14:53
 Operator : YP\AJ
 Sample : Q3486-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP5

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 10/31/2025
 Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 23:24:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.643	3.784	26366832	67228419	18.450m	10.158m#
2) SA Decachlor...	10.420	8.782	19546634	110.4E6	18.157m	13.429 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103025\
Data File : PP076193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2025 14:53
Operator : YP\AJ
Sample : Q3486-05
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP5


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 23:24:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

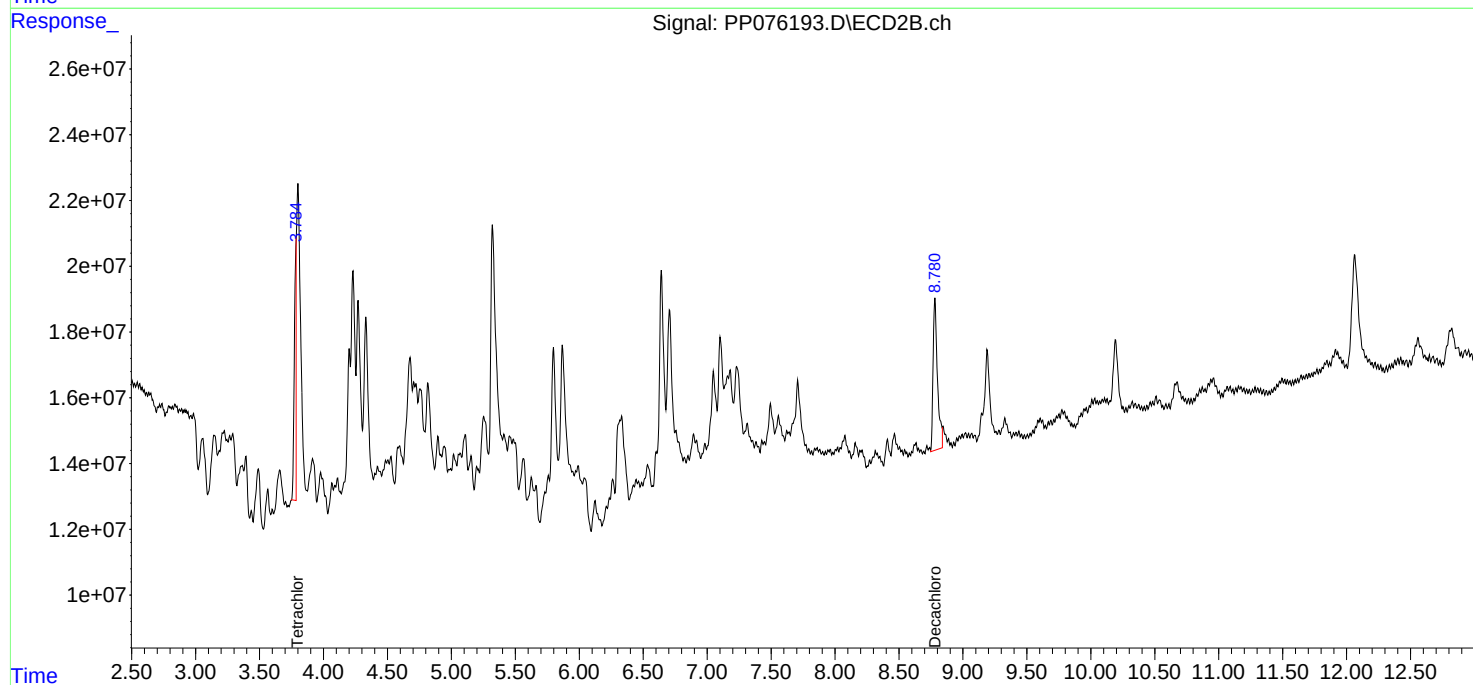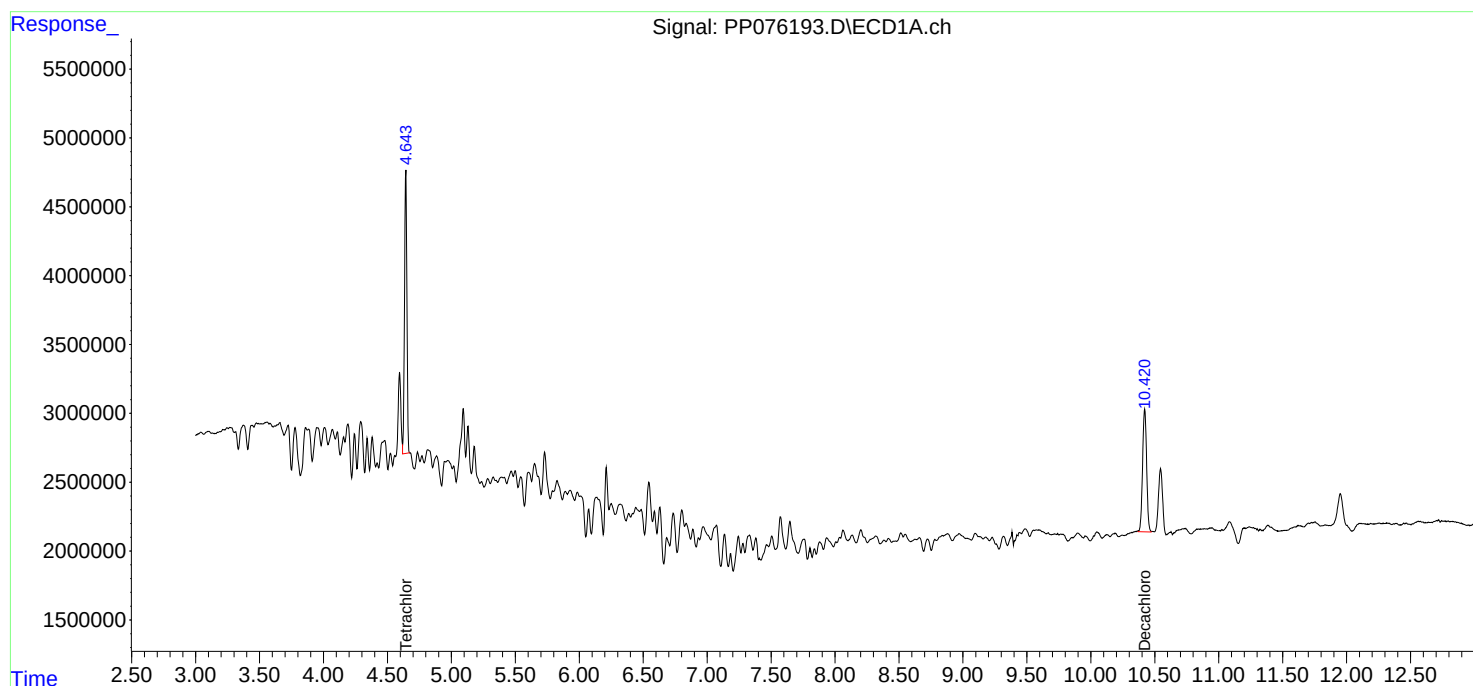

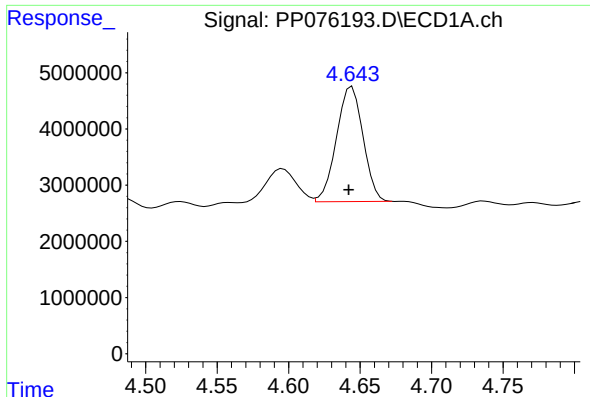


#1 Tetrachloro-m-xylene

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 26366832
Conc: 18.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP5


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

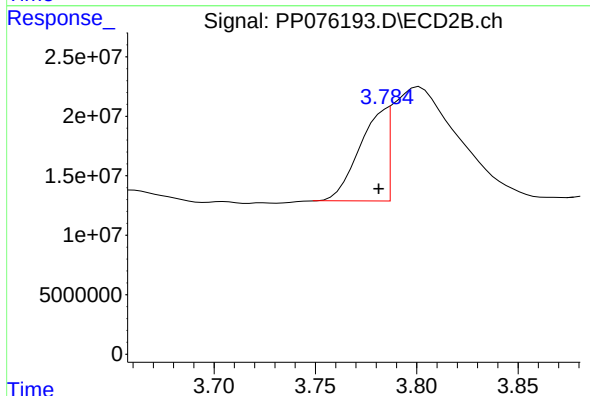


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: 0.003 min
Response: 67228419
Conc: 10.16 ng/ml m

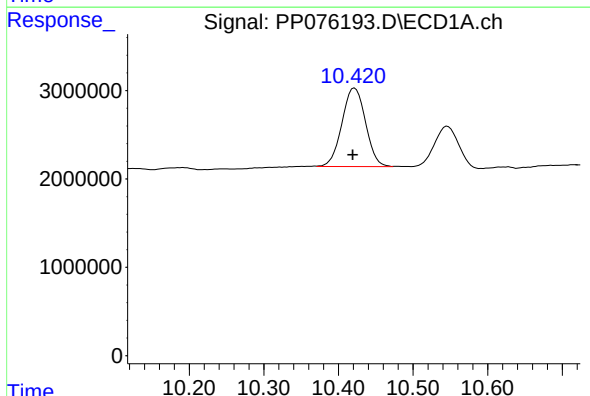

#2 Decachlorobiphenyl

R.T.: 10.420 min
Delta R.T.: 0.001 min
Response: 19546634
Conc: 18.16 ng/ml m

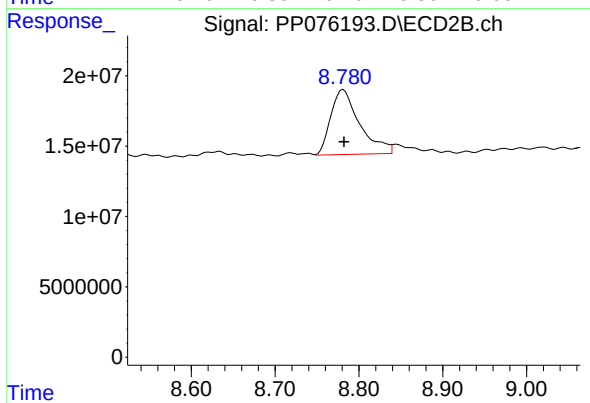

#2 Decachlorobiphenyl

R.T.: 8.782 min
Delta R.T.: 0.000 min
Response: 110426007
Conc: 13.43 ng/ml