

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103025\
 Data File : PP076218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2025 23:51
 Operator : YP\AJ
 Sample : Q3489-26 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 L65-B

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 10/31/2025
 Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 09:53:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.643	3.779	2344370	8483893	1.640m	1.282
2) SA Decachlor...	10.425	8.778	2254442	6746173	2.094	0.820m#
Target Compounds						
26) L6 AR-1254-1	6.645	0.000	1793947	0	22.454m	N.D. d#
27) L6 AR-1254-2	6.864	0.000	2537579	0	25.380	N.D. d#
28) L6 AR-1254-3	7.225	0.000	2129800	0	20.488	N.D. d#
29) L6 AR-1254-4	7.508	0.000	1448489	0	17.324	N.D. d#
30) L6 AR-1254-5	7.924	0.000	914718	0	9.989	N.D. d#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103025\
Data File : PP076218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2025 23:51
Operator : YP\AJ
Sample : Q3489-26 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
L65-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 09:53:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

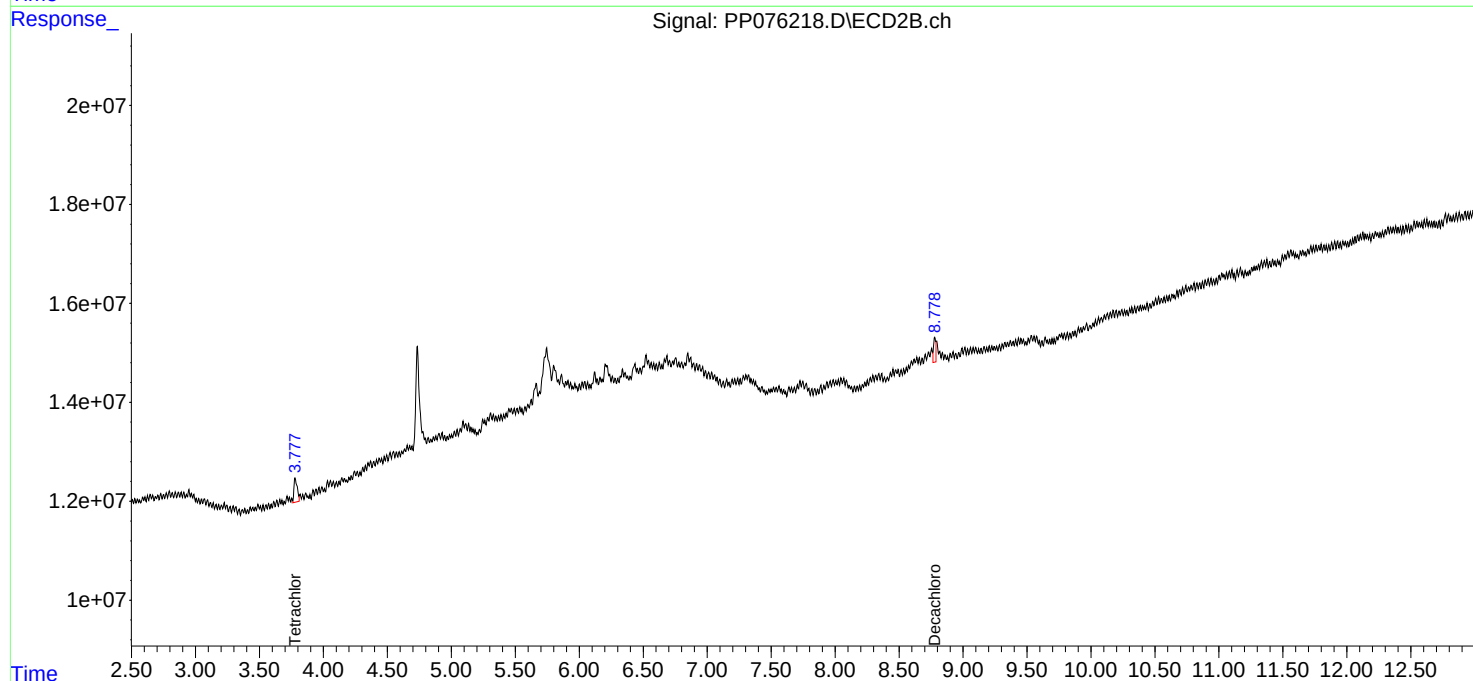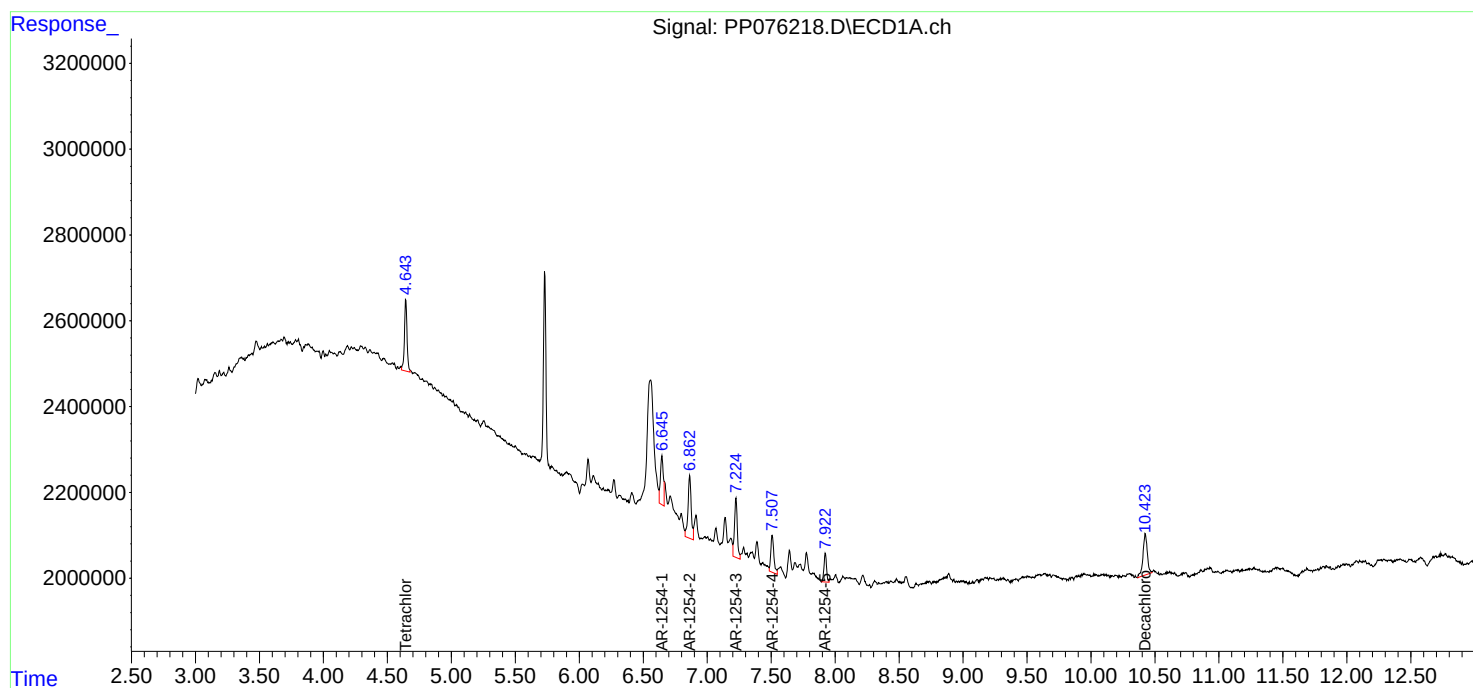

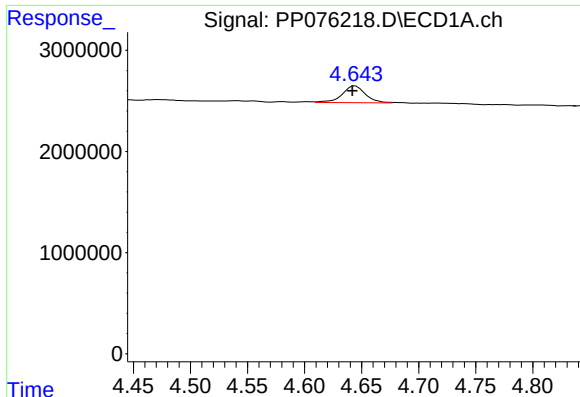


#1 Tetrachloro-m-xylene

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 2344370
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
L65-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

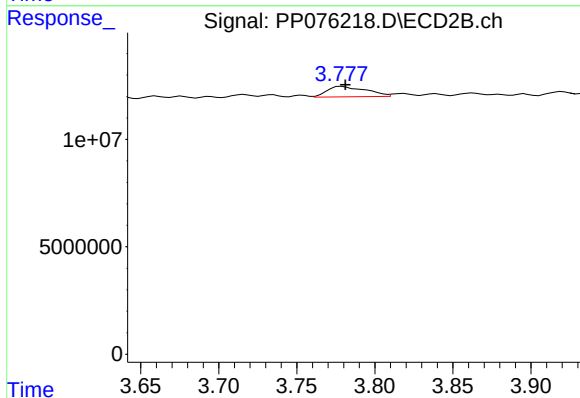


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: -0.002 min
Response: 8483893
Conc: 1.28 ng/ml

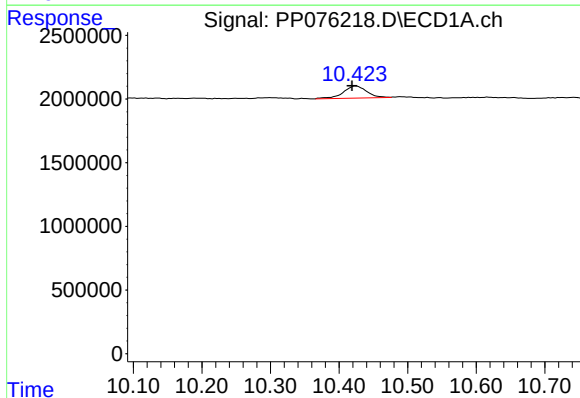

#2 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: 0.006 min
Response: 2254442
Conc: 2.09 ng/ml

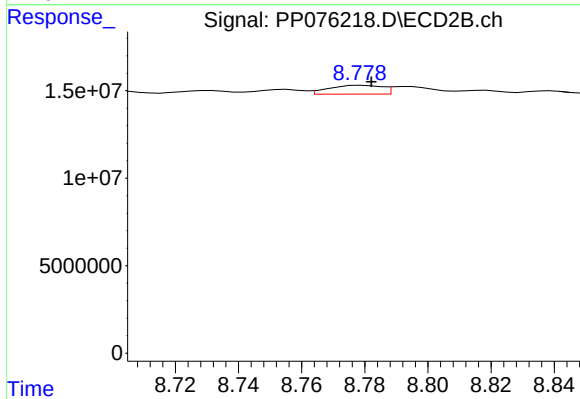

#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: -0.005 min
Response: 6746173
Conc: 0.82 ng/ml m