

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103025\
 Data File : PP076221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 00:40
 Operator : YP\AJ
 Sample : Q3489-29 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 STF24-A

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 10/31/2025
 Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 03:04:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.648	3.789	1427870	5875031	0.999m	0.888
2) SA Decachlor...	10.429	8.789	1970428	5927548	1.830	0.721m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103025\
Data File : PP076221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 00:40
Operator : YP\AJ
Sample : Q3489-29 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
STF24-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 03:04:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

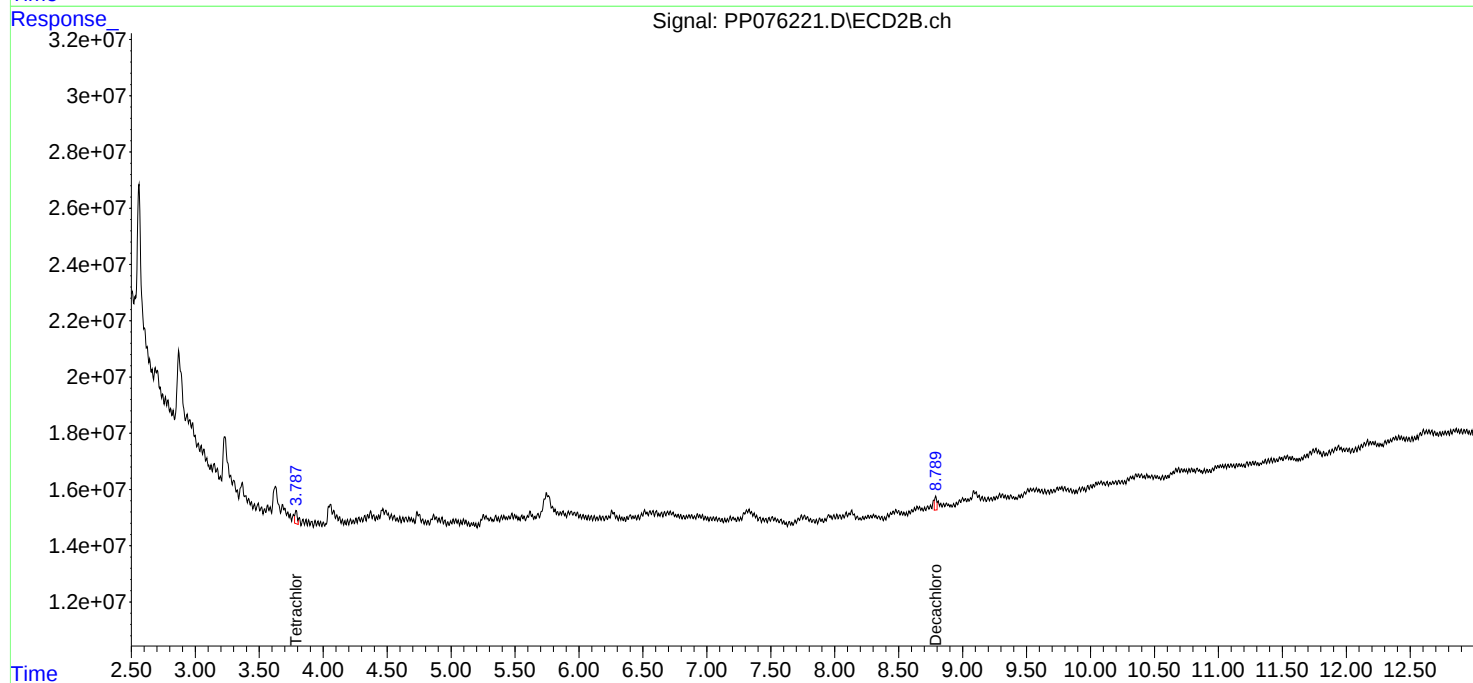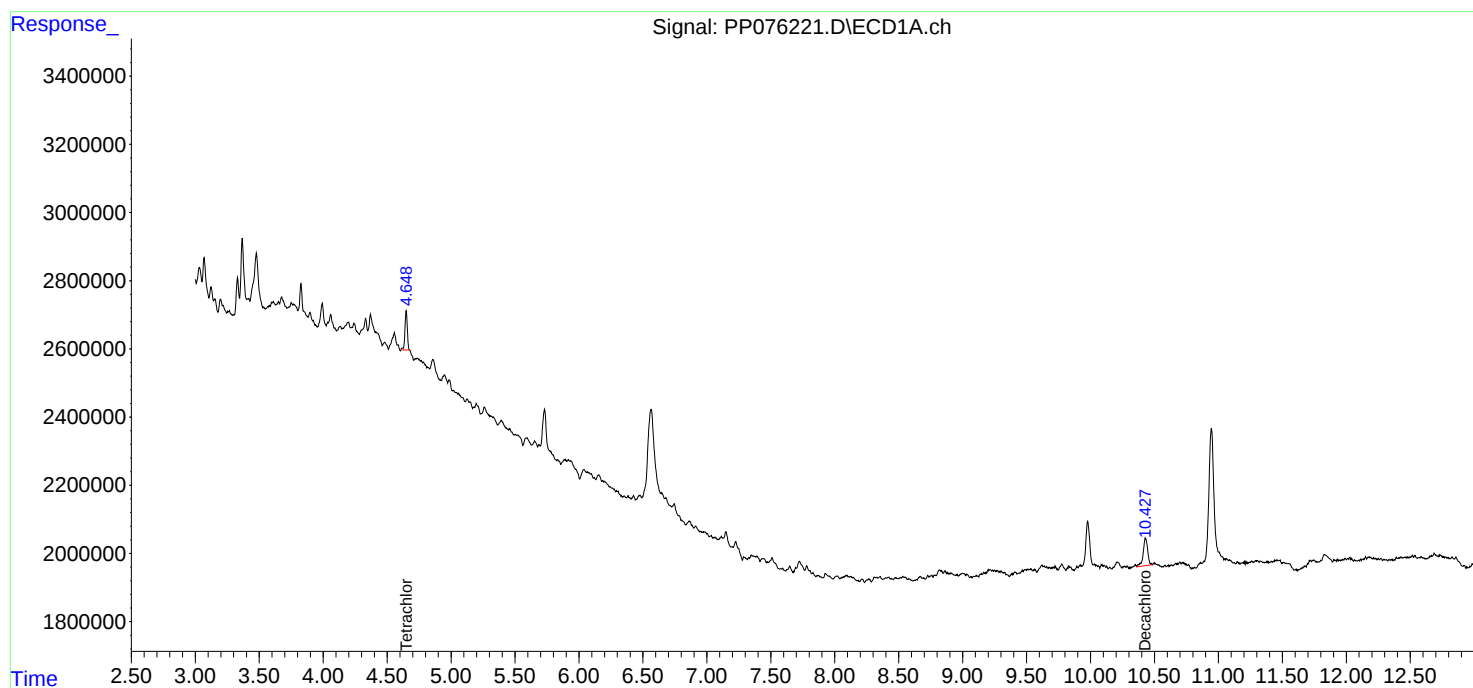

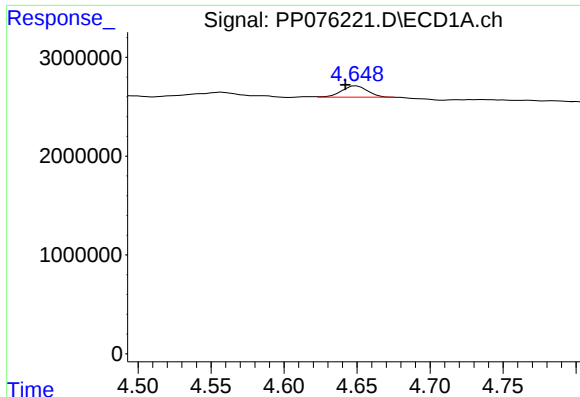


#1 Tetrachloro-m-xylene

R.T.: 4.648 min
Delta R.T.: 0.006 min
Response: 1427870
Conc: 1.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
STF24-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

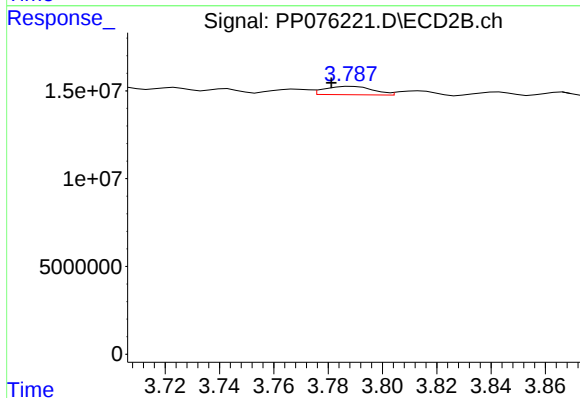


#1 Tetrachloro-m-xylene

R.T.: 3.789 min
Delta R.T.: 0.008 min
Response: 5875031
Conc: 0.89 ng/ml

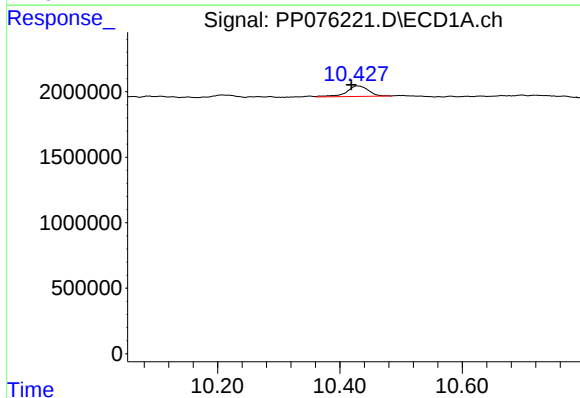

#2 Decachlorobiphenyl

R.T.: 10.429 min
Delta R.T.: 0.010 min
Response: 1970428
Conc: 1.83 ng/ml

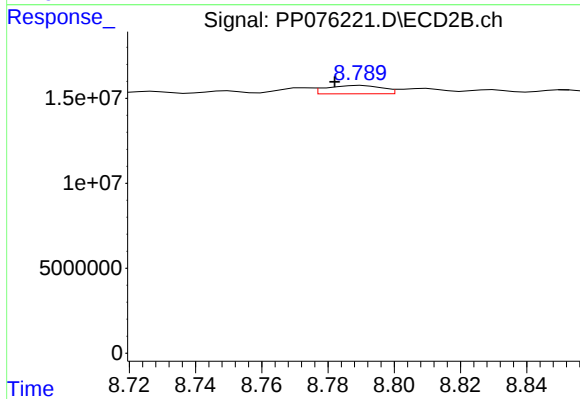

#2 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: 0.007 min
Response: 5927548
Conc: 0.72 ng/ml m