

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103025\
 Data File : PP076222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 00:56
 Operator : YP\AJ
 Sample : Q3489-30 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 STF24-B

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 10/31/2025
 Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 09:50:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.644	3.779	1636982	7566758	1.145m	1.143
2) SA Decachlor...	10.427	8.780	2683914	8756057	2.493	1.065m#
Target Compounds						
26) L6 AR-1254-1	6.645	0.000	1211810	0	15.168m	N.D. d#
27) L6 AR-1254-2	6.863	0.000	1084123	0	10.843	N.D. d#
28) L6 AR-1254-3	7.225	0.000	1564158	0	15.047	N.D. d#
29) L6 AR-1254-4	7.509	0.000	1347233	0	16.113	N.D. d#
30) L6 AR-1254-5	7.925	0.000	1101796	0	12.032	N.D. d#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103025\
Data File : PP076222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 00:56
Operator : YP\AJ
Sample : Q3489-30 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
STF24-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 09:50:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

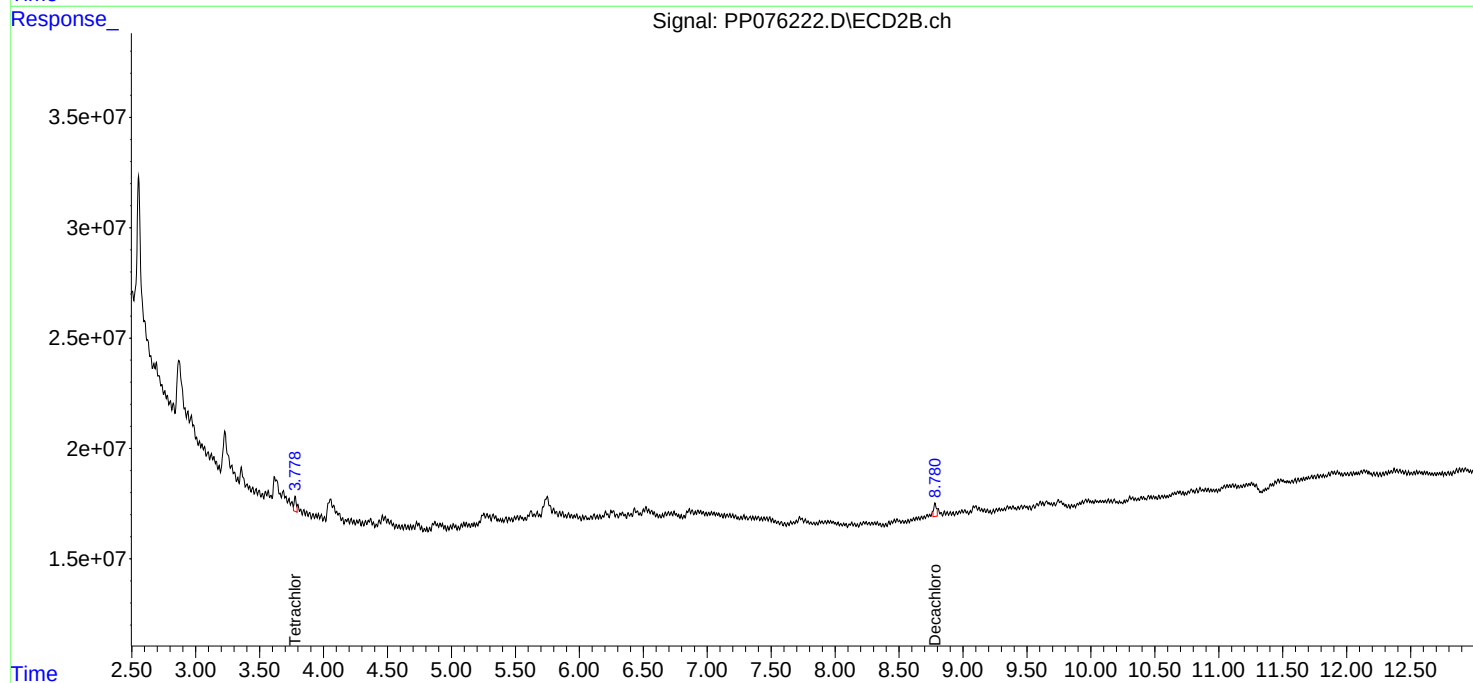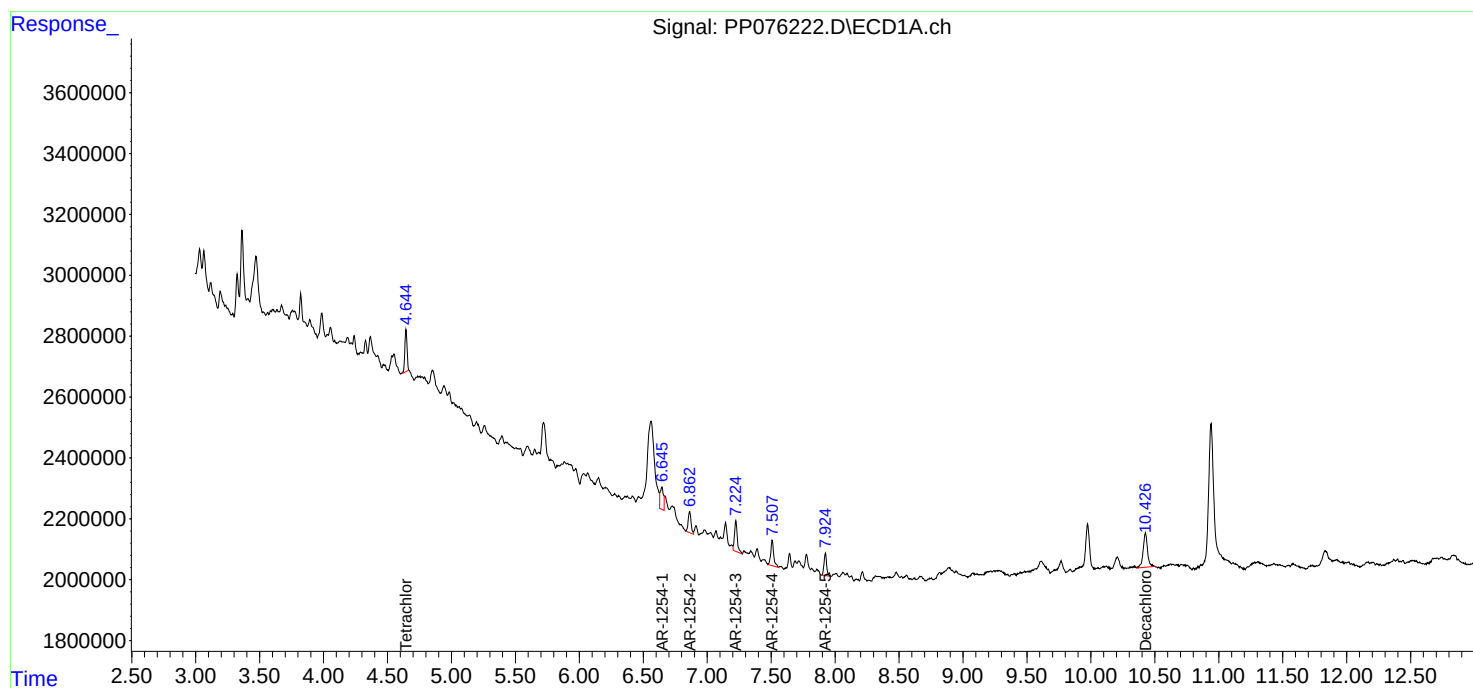

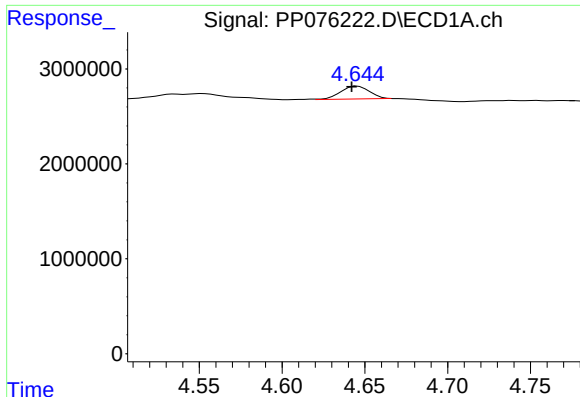


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: 0.002 min
Response: 1636982
Conc: 1.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
STF24-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

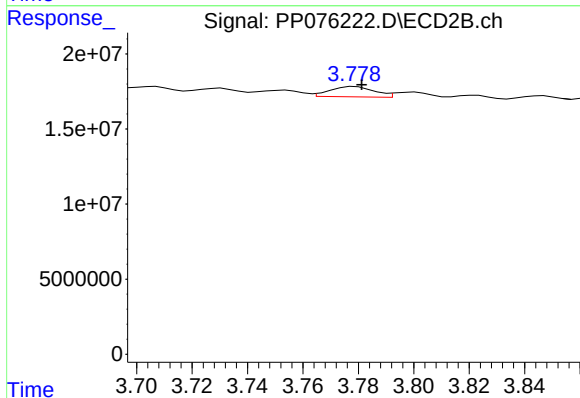


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: -0.002 min
Response: 7566758
Conc: 1.14 ng/ml

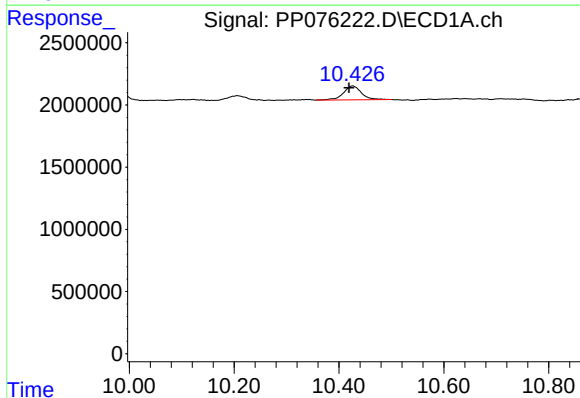

#2 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: 0.008 min
Response: 2683914
Conc: 2.49 ng/ml

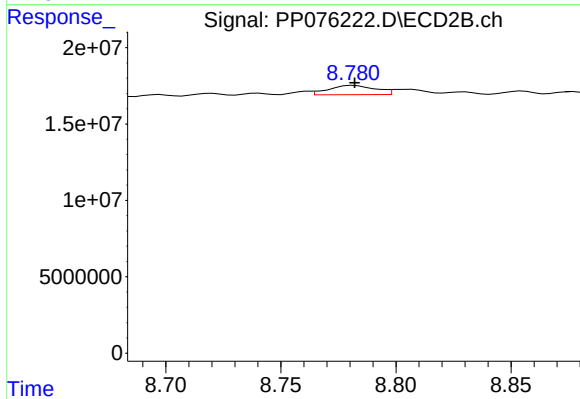

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.002 min
Response: 8756057
Conc: 1.06 ng/ml m